

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 03:59
 Operator : SM\AJ
 Sample : K4044-09
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 7/31/2019 3:30:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 04:50:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	229.6E6	59842496	22.851	20.974
28)	SA Decachlor...	7.979	8.959	198.2E6	55682348	19.572	19.690
Target Compounds							
12)	B 4,4'-DDE	5.423	6.253	7658345	1194426	0.511m	0.331m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 03:59
Operator : SM\AJ
Sample : K4044-09
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
7/31/2019 3:30:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 04:50:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

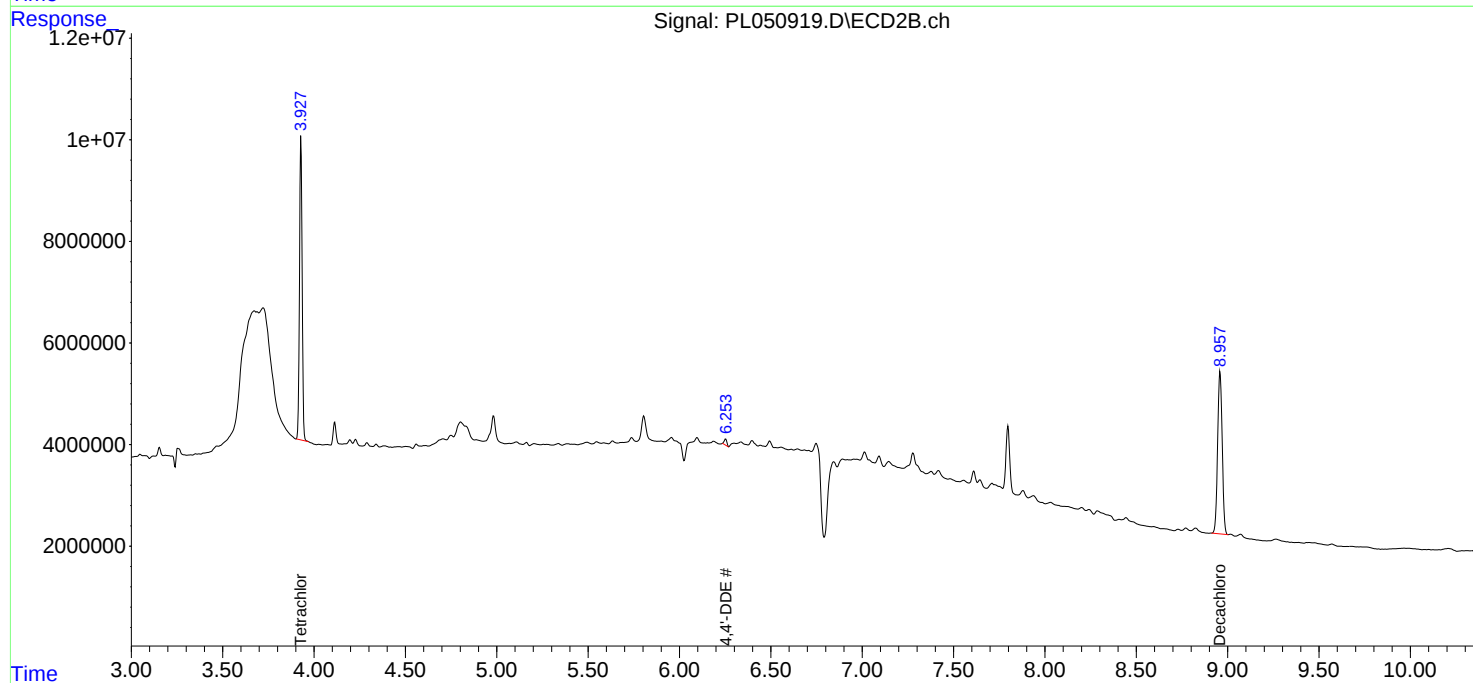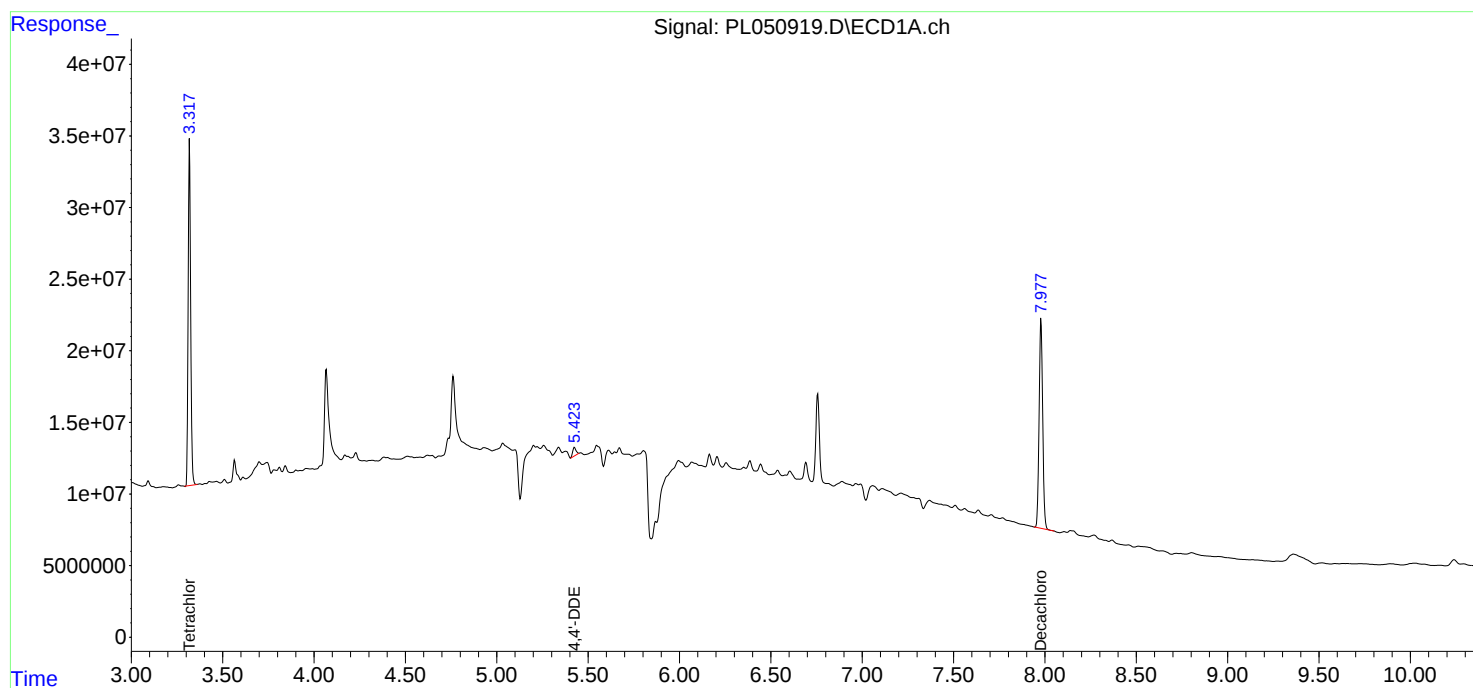

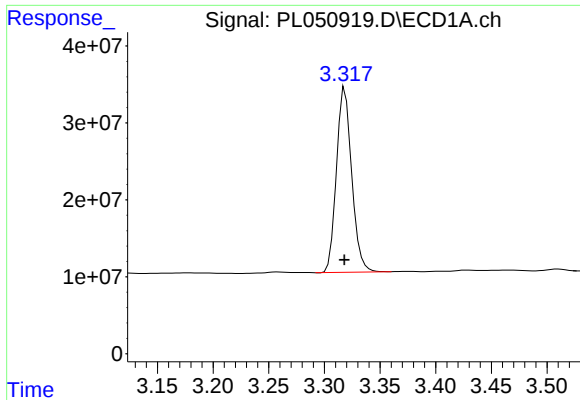


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 229606120
Conc: 22.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
7/31/2019 3:30:39 PM

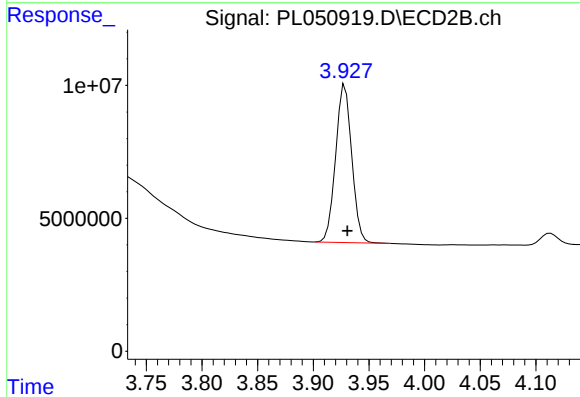


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 59842496
Conc: 20.97 ng/ml

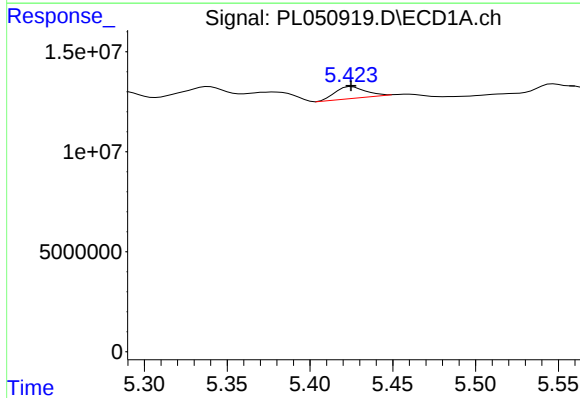


#12 4,4'-DDE

R.T.: 5.423 min
Delta R.T.: -0.002 min
Response: 7658345
Conc: 0.51 ng/ml m

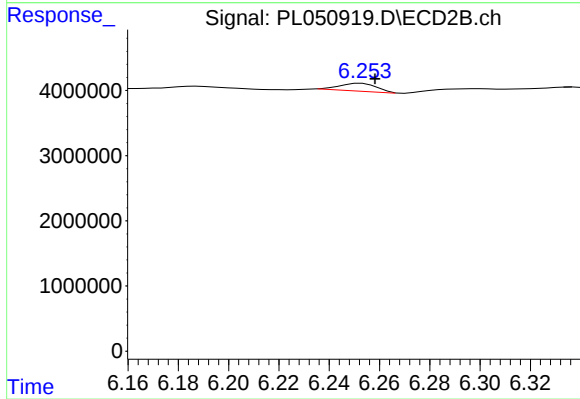

#12 4,4'-DDE

R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 1194426
Conc: 0.33 ng/ml m

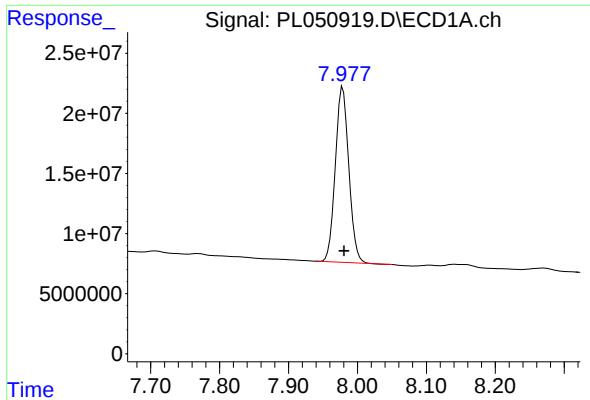


#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 198173633
Conc: 19.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
7/31/2019 3:30:39 PM

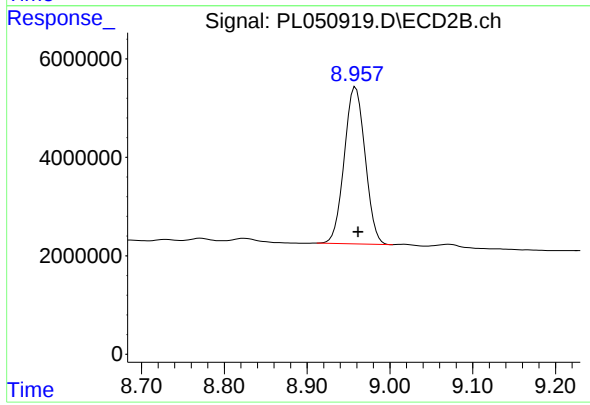

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 55682348
Conc: 19.69 ng/ml