

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073020\
 Data File : PL060360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 07:34
 Operator : DD\AJ
 Sample : L3436-11RE 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 11RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 09:43:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.882	0	12535685	N.D.	5.173 #
12) B	4,4'-DDE	0.000	6.355	0	9768642	N.D.	3.693 #
13) MA	Dieldrin	5.755	0.000	16458820	0	9.299	N.D. #
14) MA	Endrin	0.000	6.717	0	16354014	N.D.	6.983 #
15) B	Endosulfa...	6.277	0.000	6646324	0	3.915	N.D. #
16) A	4,4'-DDD	0.000	6.854	0	4072916	N.D.	1.955 #
17) MA	4,4'-DDT	6.382	7.121f	14888880	30416396	10.899	15.040 #
27)	Chlordane-5	6.277f	0.000	6646324	0	117.469	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073020\
Data File : PL060360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 07:34
Operator : DD\AJ
Sample : L3436-11RE 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
11RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 09:43:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

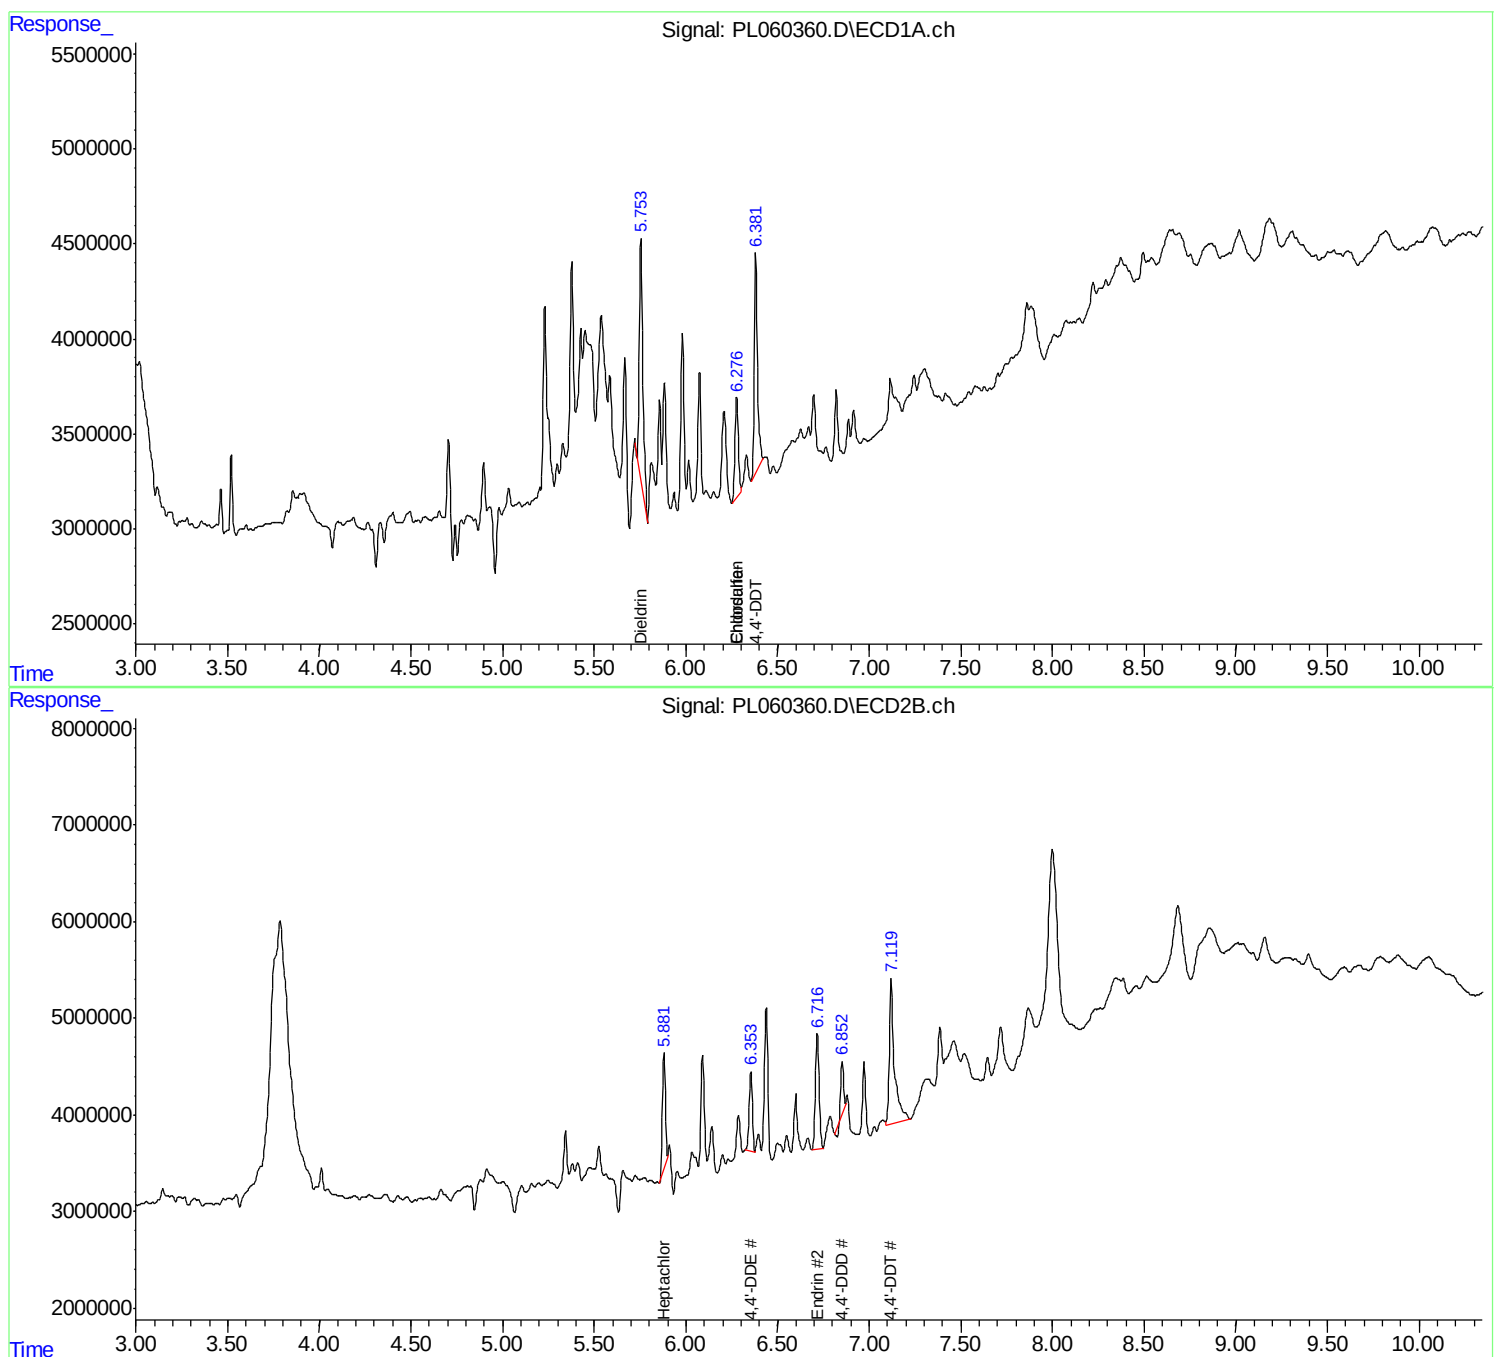


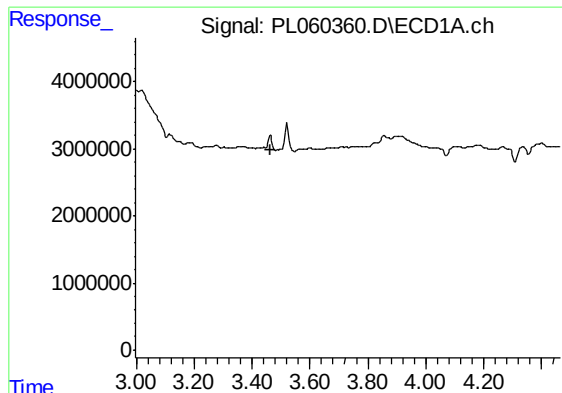

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
11RE

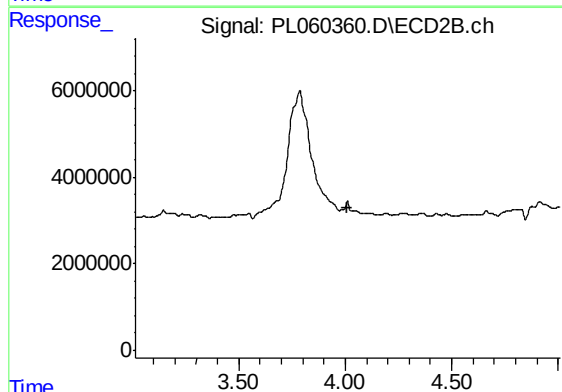


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.013 min
Response: 0
Conc: N.D.

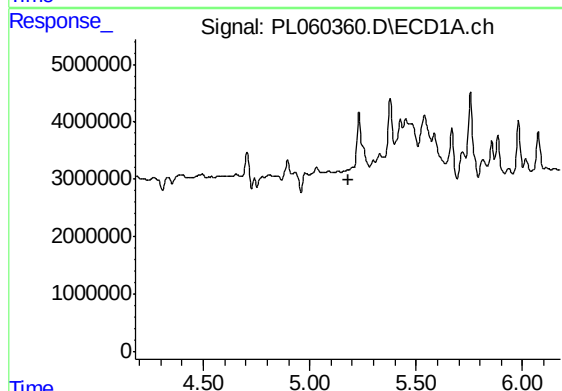


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.180 min
Response: 0
Conc: N.D.

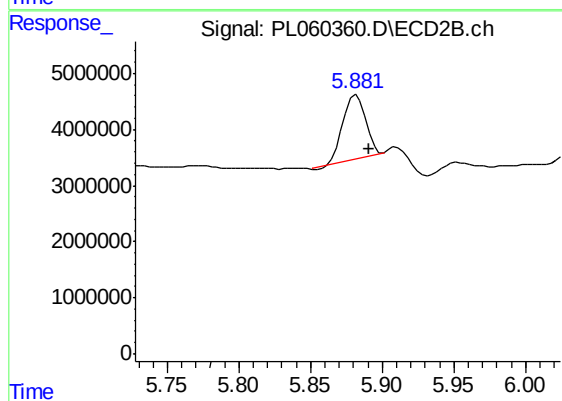

#8 Heptachlor epoxide


R.T.: 5.882 min
Delta R.T.: -0.009 min
Response: 12535685
Conc: 5.17 ng/ml

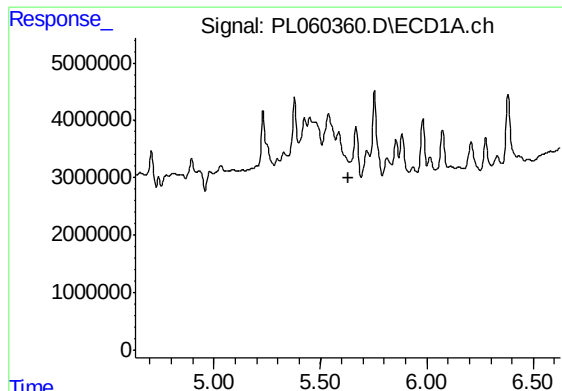

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.630 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
11RE

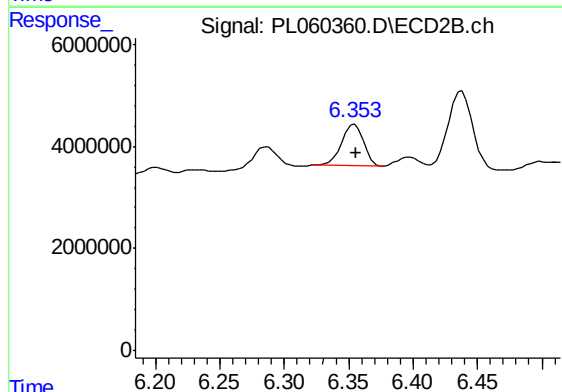


#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 9768642
Conc: 3.69 ng/ml

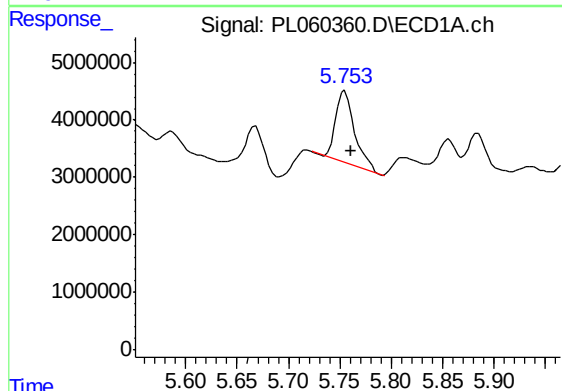


#13 Dieldrin

R.T.: 5.755 min
Delta R.T.: -0.007 min
Response: 16458820
Conc: 9.30 ng/ml

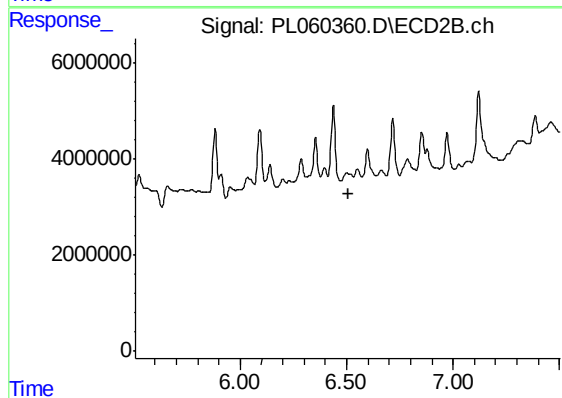

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.506 min
Response: 0
Conc: N.D.

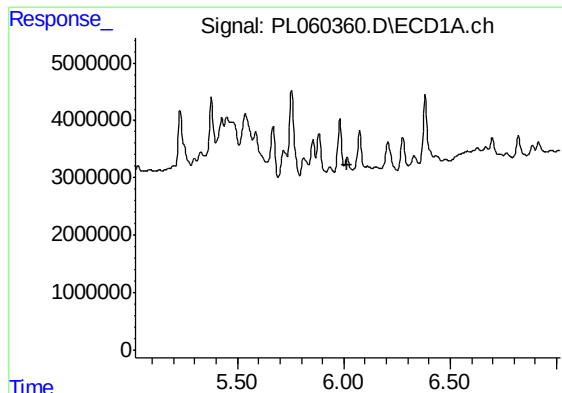

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
11RE

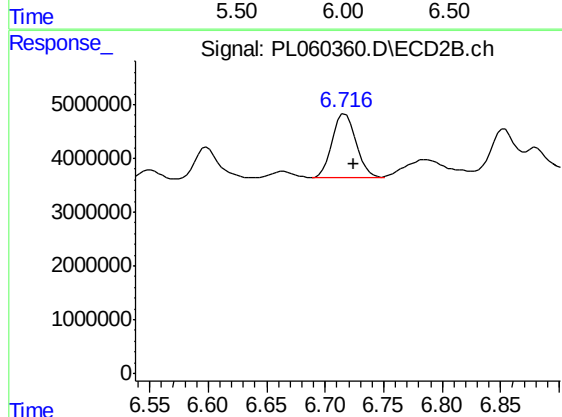


#14 Endrin

R.T.: 6.717 min
Delta R.T.: -0.008 min
Response: 16354014
Conc: 6.98 ng/ml

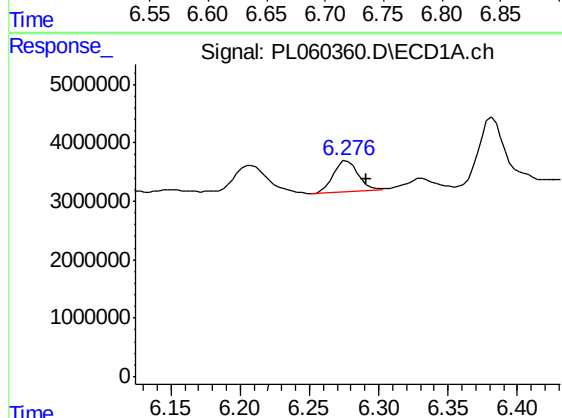


#15 Endosulfan II

R.T.: 6.277 min
Delta R.T.: -0.014 min
Response: 6646324
Conc: 3.91 ng/ml

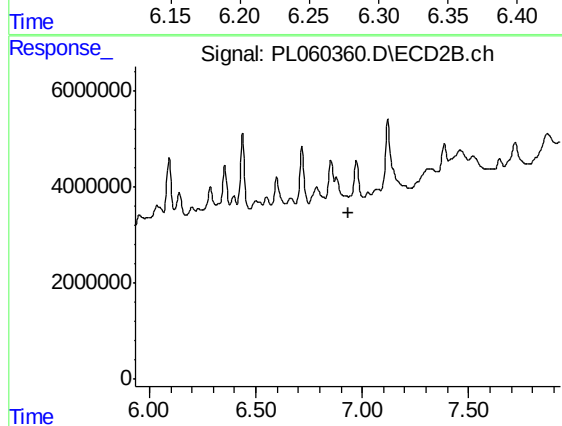

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

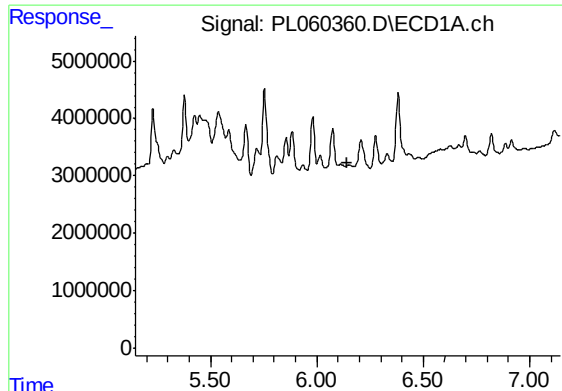

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
11RE

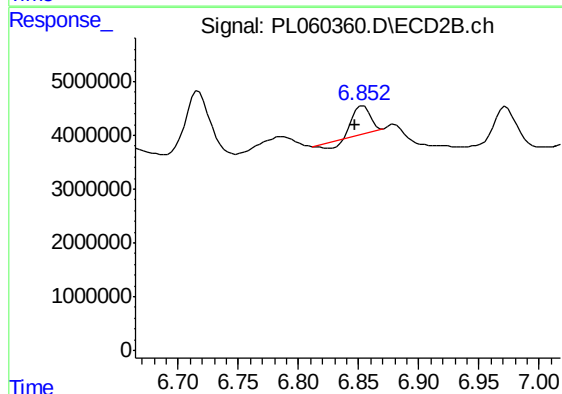


#16 4,4'-DDD

R.T.: 6.854 min
Delta R.T.: 0.007 min
Response: 4072916
Conc: 1.96 ng/ml

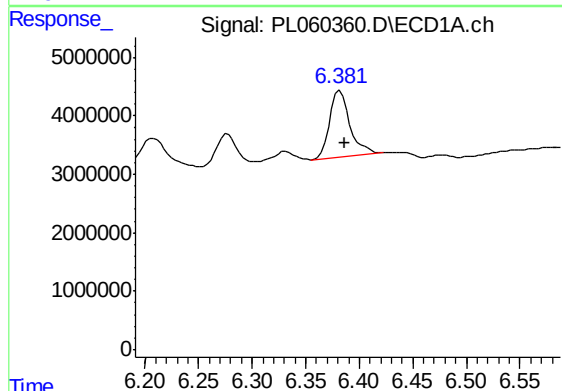


#17 4,4'-DDT

R.T.: 6.382 min
Delta R.T.: -0.004 min
Response: 14888880
Conc: 10.90 ng/ml

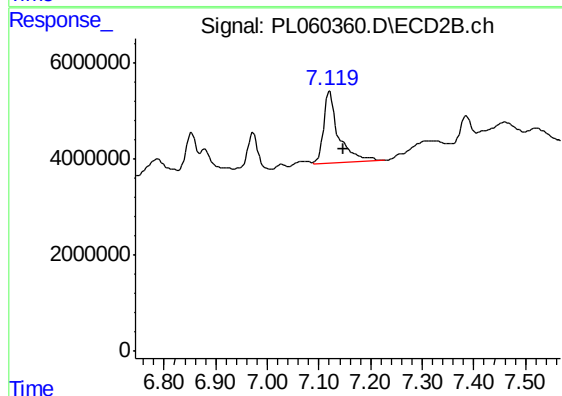

#17 4,4'-DDT


R.T.: 7.121 min
Delta R.T.: -0.026 min
Response: 30416396
Conc: 15.04 ng/ml

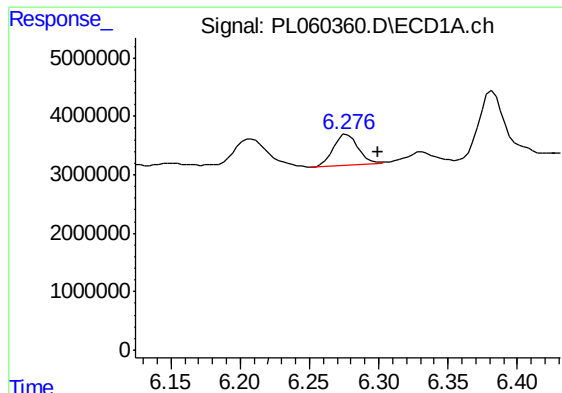

#27 Chlordane-5


R.T.: 6.277 min
Delta R.T.: -0.022 min
Response: 6646324
Conc: 117.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
11RE

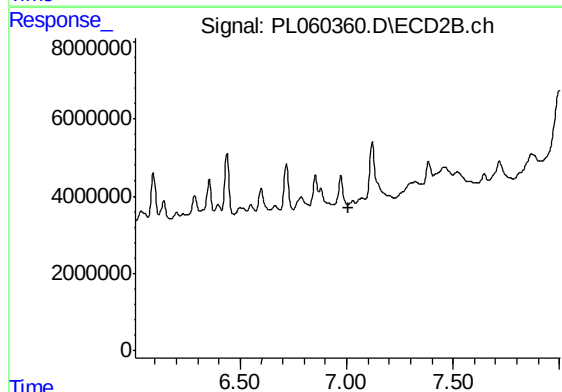


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

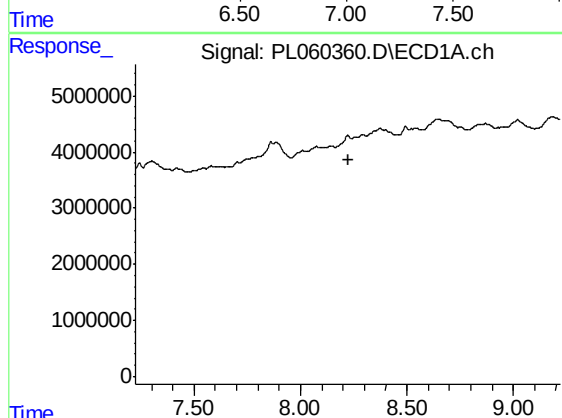

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.223 min
Response: 0
Conc: N.D.

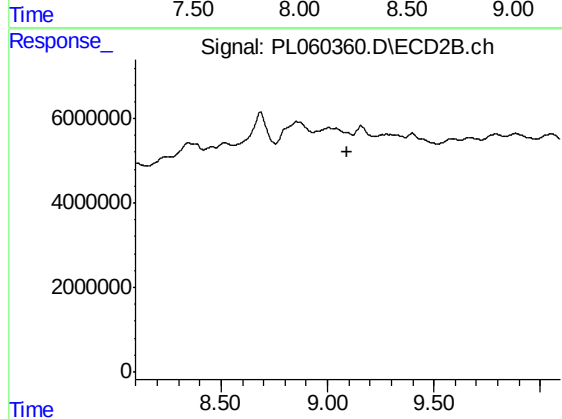

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.