

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073020\
 Data File : PL060343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2020 19:18
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 03:39:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 03:39:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.013	115.4E6	133.0E6	50.000	50.000
28)	SA Decachlor...	8.222	9.095	75922982	89342452	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.336	5.009	30024212	47510039	500.000	500.000
24)	Chlordane-2	4.838	5.477	30574748	50878428	500.000	500.000
25)	Chlordane-3	5.407	6.126	83581785	184.0E6	500.000	500.000
26)	Chlordane-4	5.465	6.201	68872224	228.3E6	500.000	500.000
27)	Chlordane-5	6.300	7.007	28289765	37363016	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073020\
Data File : PL060343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2020 19:18
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 03:39:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 03:39:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

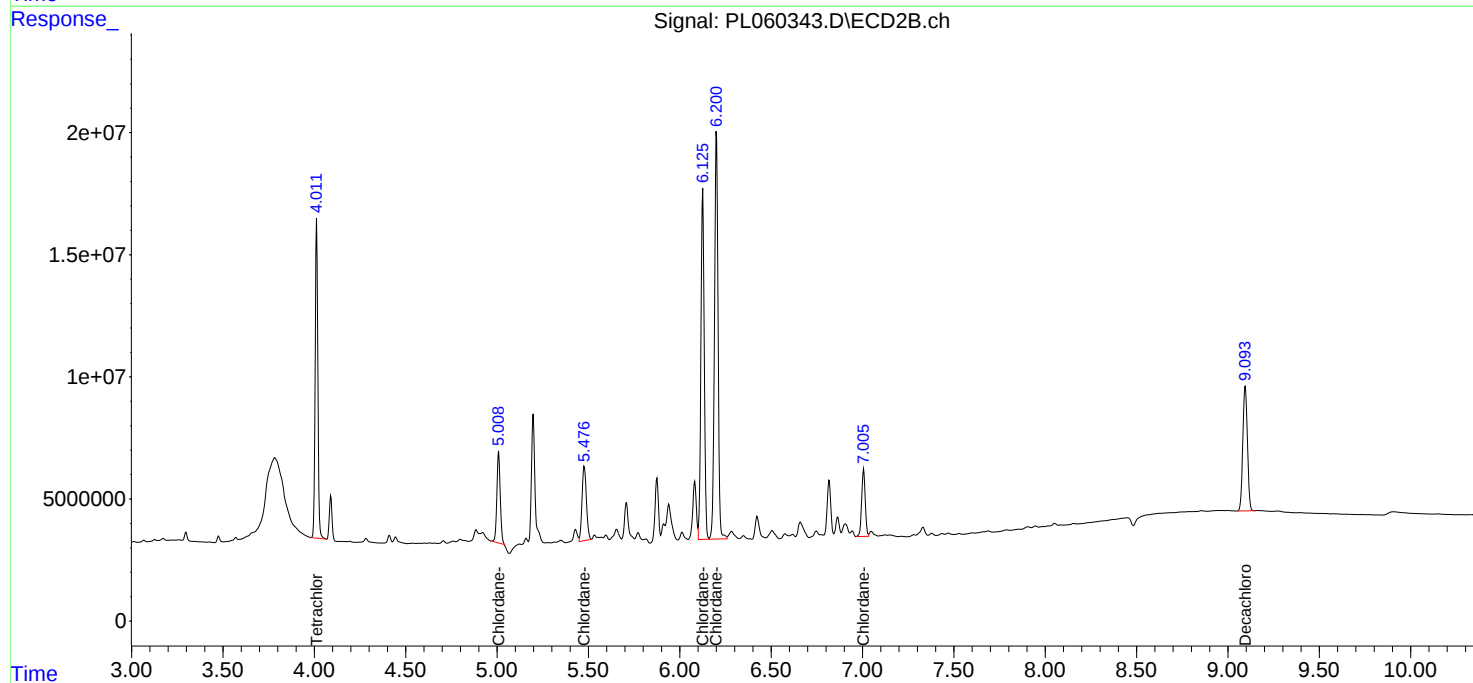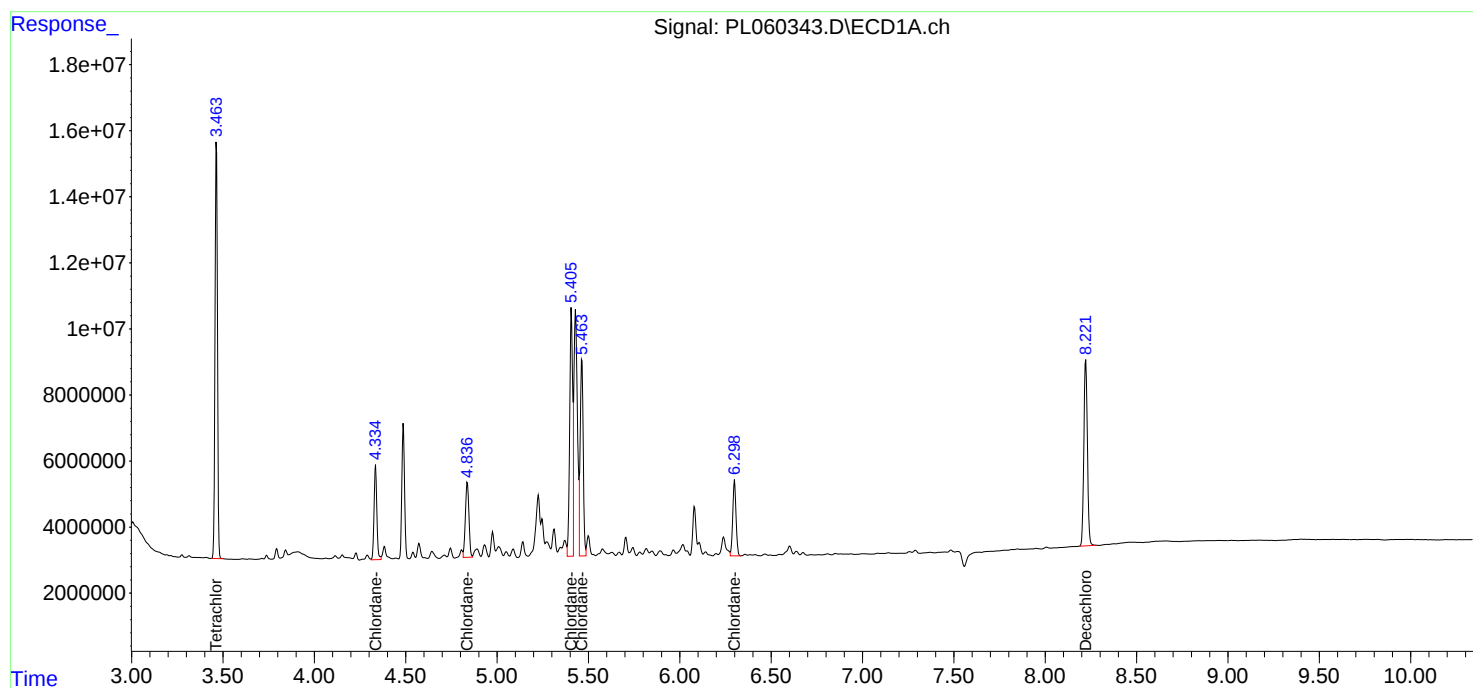


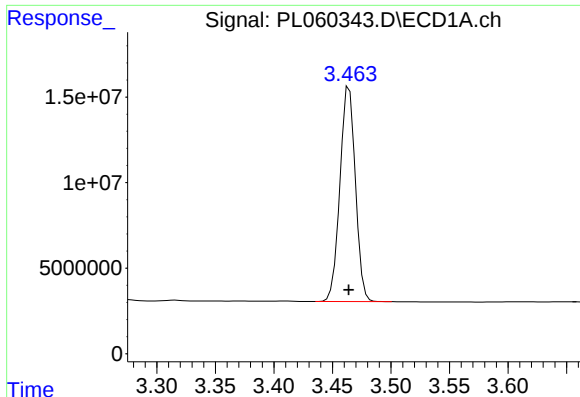

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 115427875
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

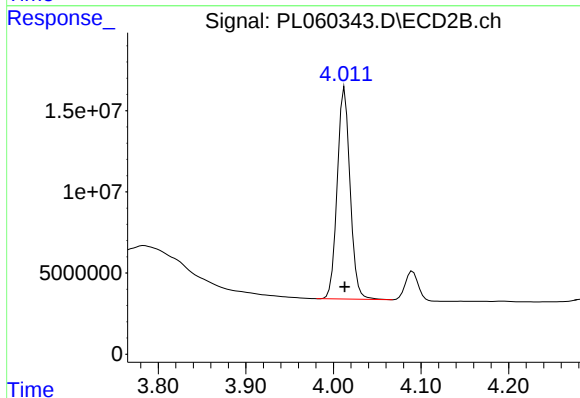


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 133009965
Conc: 50.00 ng/ml

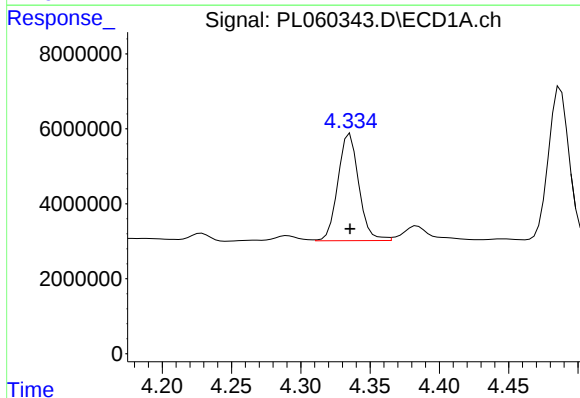


#23 Chlordane-1

R.T.: 4.336 min
Delta R.T.: 0.000 min
Response: 30024212
Conc: 500.00 ng/ml

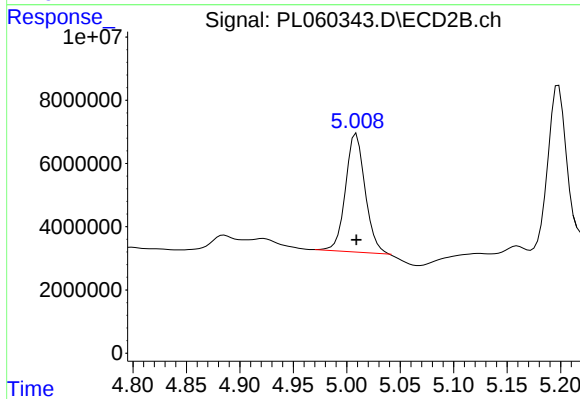

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 47510039
Conc: 500.00 ng/ml

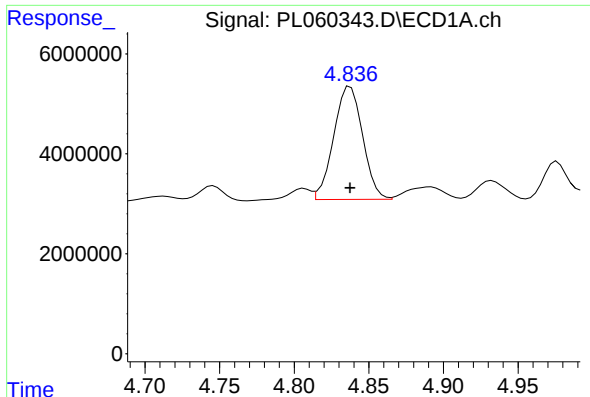

#24 Chlordane-2


R.T.: 4.838 min
Delta R.T.: 0.000 min
Response: 30574748
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

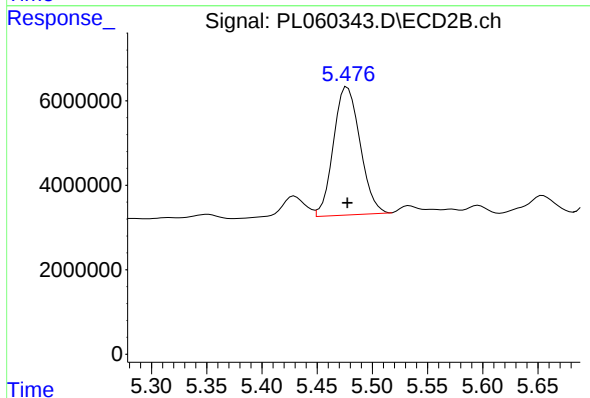


#24 Chlordane-2

R.T.: 5.477 min
Delta R.T.: 0.000 min
Response: 50878428
Conc: 500.00 ng/ml

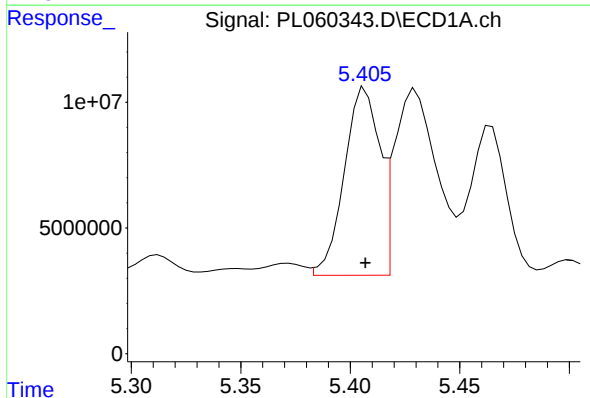


#25 Chlordane-3

R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 83581785
Conc: 500.00 ng/ml

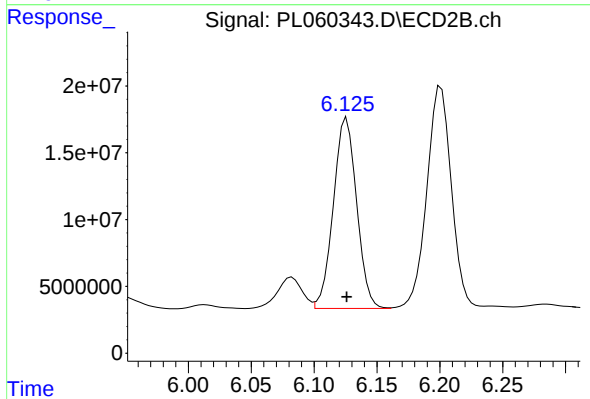

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 183978027
Conc: 500.00 ng/ml

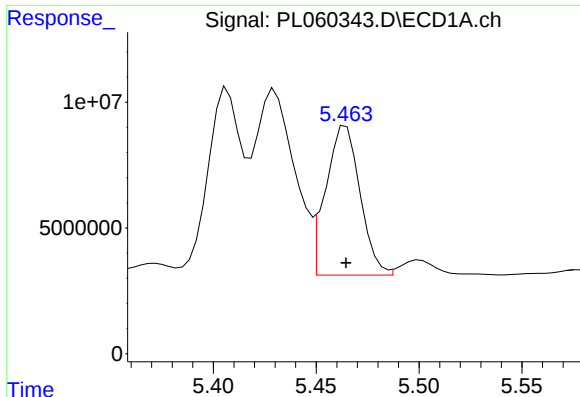

#26 Chlordane-4


R.T.: 5.465 min
Delta R.T.: 0.000 min
Response: 68872224
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

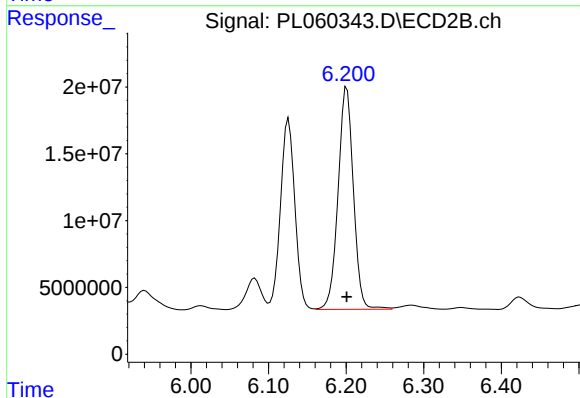


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 228263744
Conc: 500.00 ng/ml

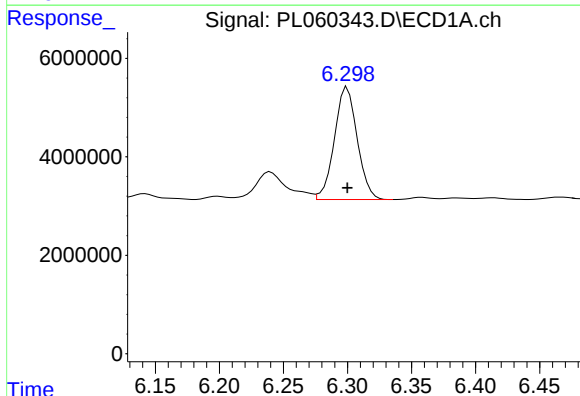


#27 Chlordane-5

R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 28289765
Conc: 500.00 ng/ml

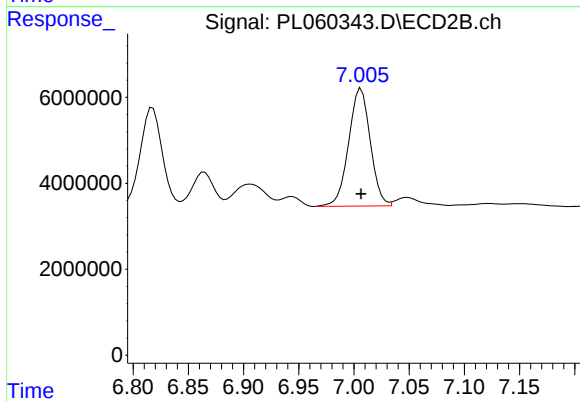

#27 Chlordane-5


R.T.: 7.007 min
Delta R.T.: 0.000 min
Response: 37363016
Conc: 500.00 ng/ml

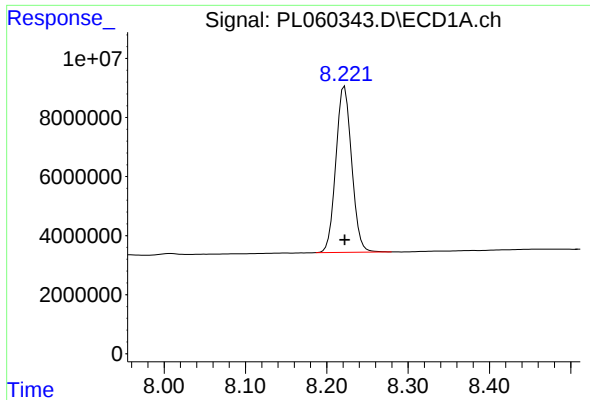

#28 Decachlorobiphenyl

R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 75922982
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

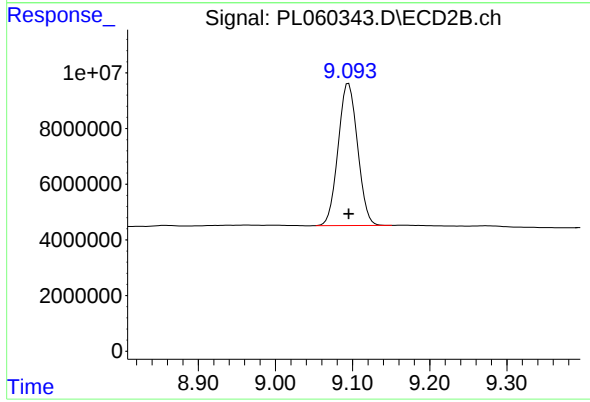

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 89342452
Conc: 50.00 ng/ml