

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073021\
 Data File : PL068627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 22:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:23:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.570	9210563	23791855	21.461	23.316
28)	SA Decachlor...	10.413	11.492	12299588	20916512	21.869	23.449
Target Compounds							
6)	B beta-BHC	6.157	0.000	1484456	0	5.073	N.D. #
8)	B Heptachlo...	0.000	8.039	0	109930	N.D.	0.097 #
9)	A Endosulfan I	0.000	8.421f	0	81138	N.D.	0.079 #
13)	MA Dieldrin	0.000	8.726	0	143853	N.D.	0.136 #
14)	MA Endrin	8.085	8.969	506002	451479	1.012	0.505 #
15)	B Endosulfa...	0.000	9.217f	0	2202878	N.D.	2.430 #
19)	B Endosulfa...	0.000	9.566	0	101278	N.D.	0.112 #
20)	A Methoxychlor	0.000	9.913	0	249639	N.D.	0.491 #
21)	B Endrin ke...	0.000	10.090f	0	215219	N.D.	0.216 #
22)	Mirex	0.000	10.560f	0	319132	N.D.	0.413 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073021\
Data File : PL068627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 22:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 03:23:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

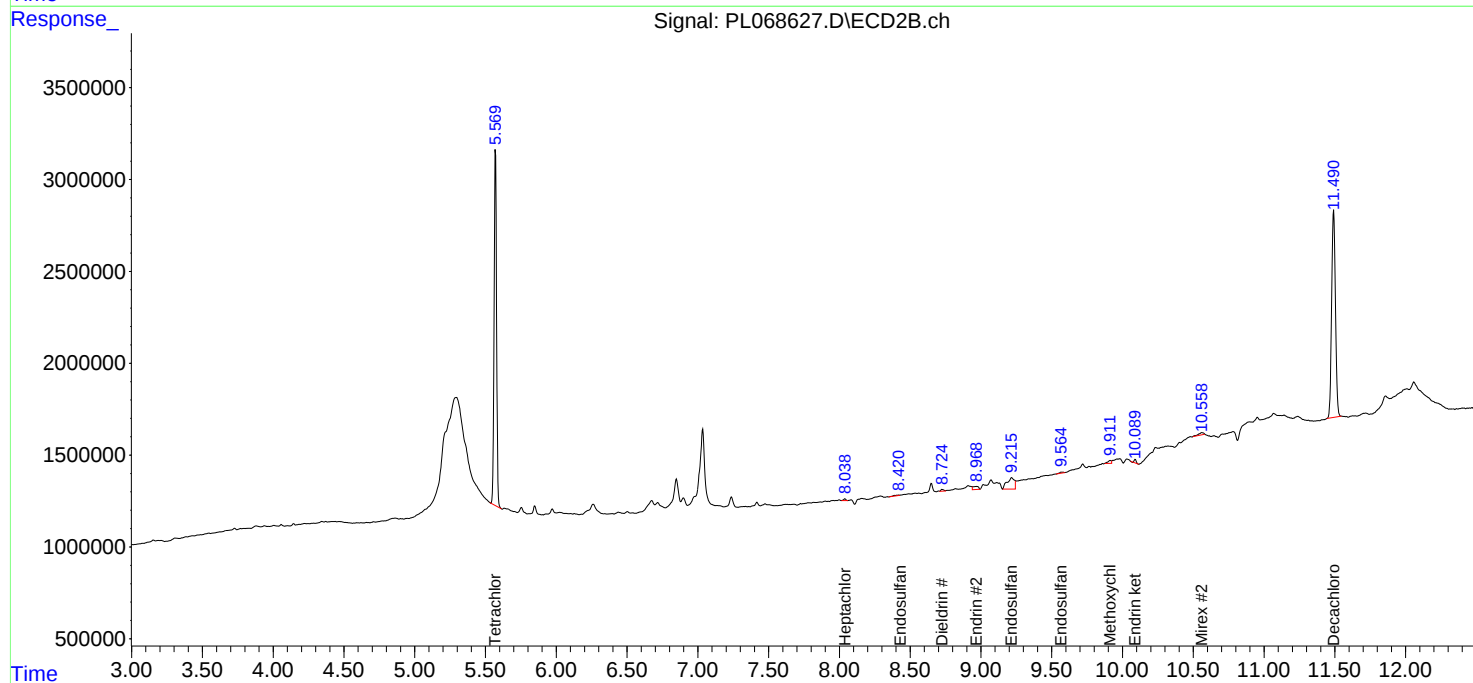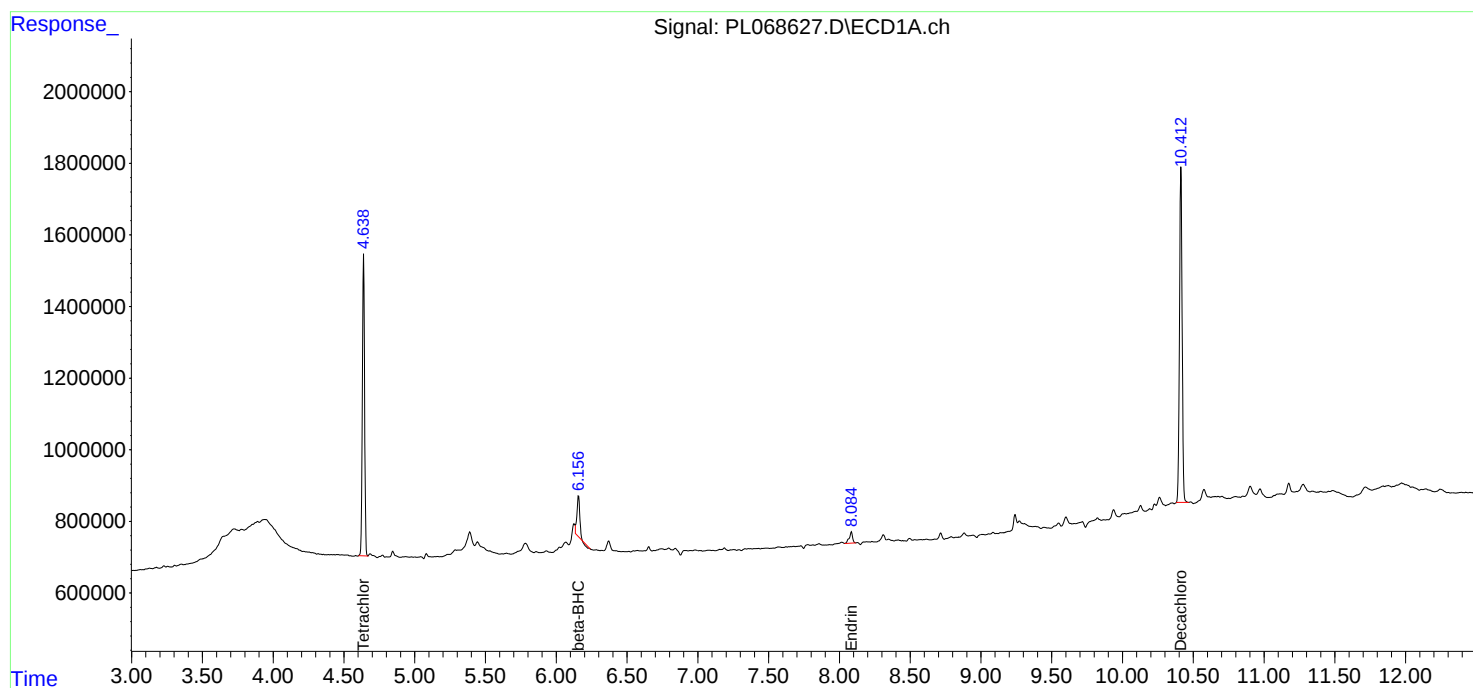


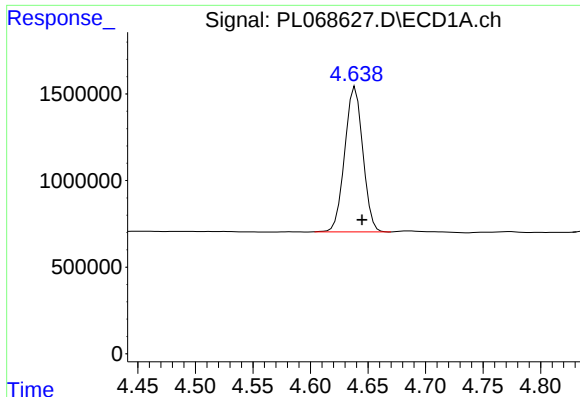

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: -0.006 min
Response: 9210563
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

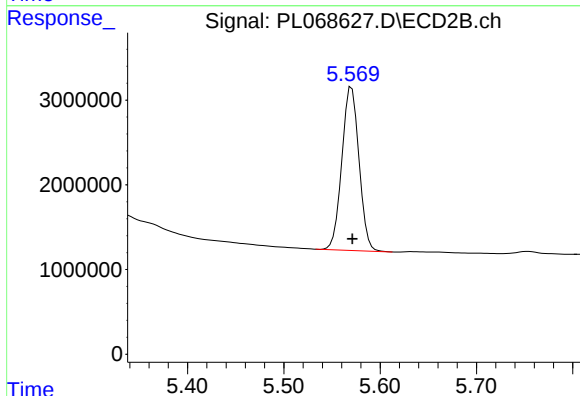


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 23791855
Conc: 23.32 ng/ml

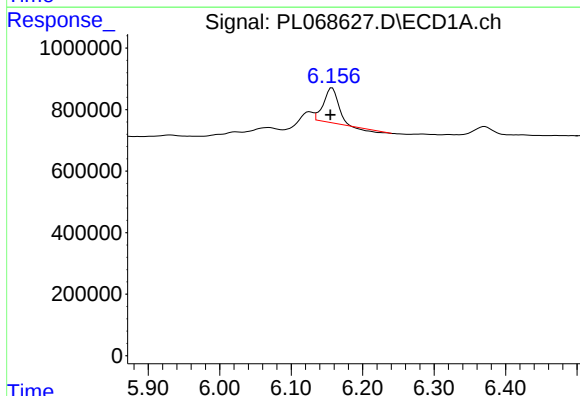


#6 beta-BHC

R.T.: 6.157 min
Delta R.T.: 0.002 min
Response: 1484456
Conc: 5.07 ng/ml

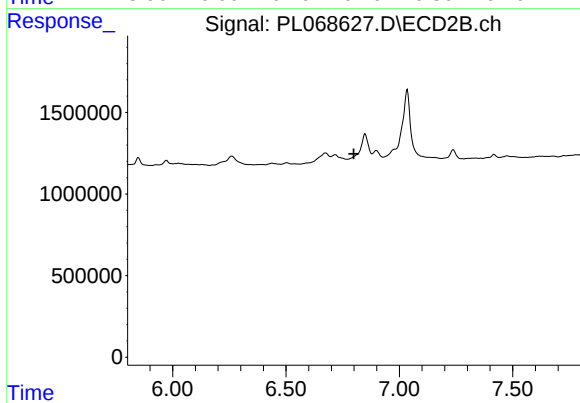

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

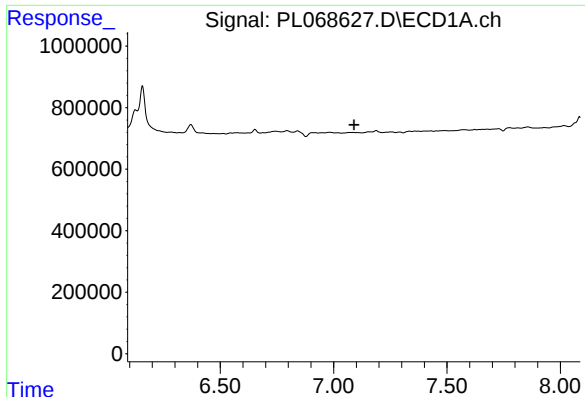

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

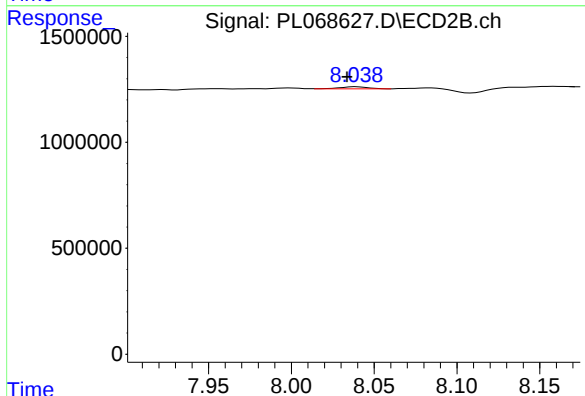


#8 Heptachlor epoxide

R.T.: 8.039 min
Delta R.T.: 0.005 min
Response: 109930
Conc: 0.10 ng/ml

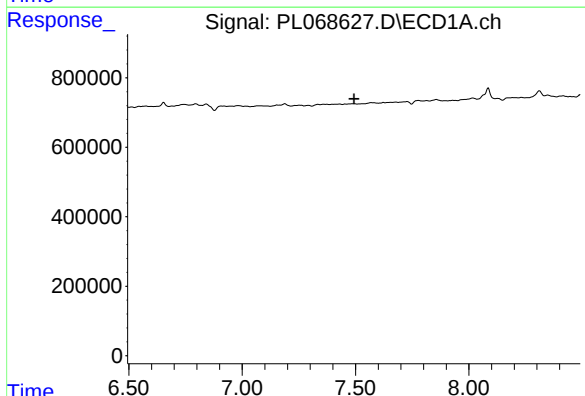


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

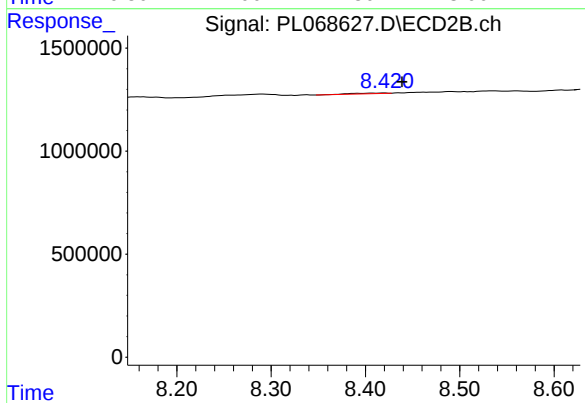

#9 Endosulfan I


R.T.: 8.421 min
Delta R.T.: -0.018 min
Response: 81138
Conc: 0.08 ng/ml

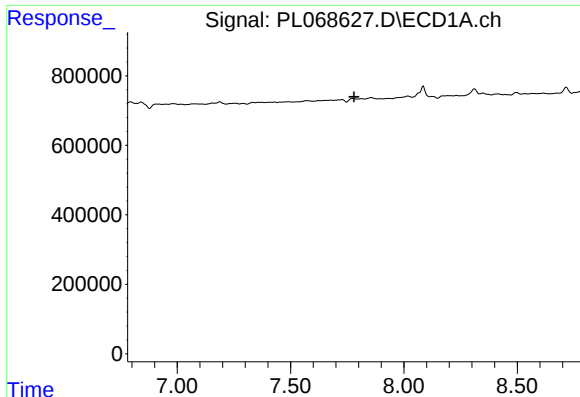

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

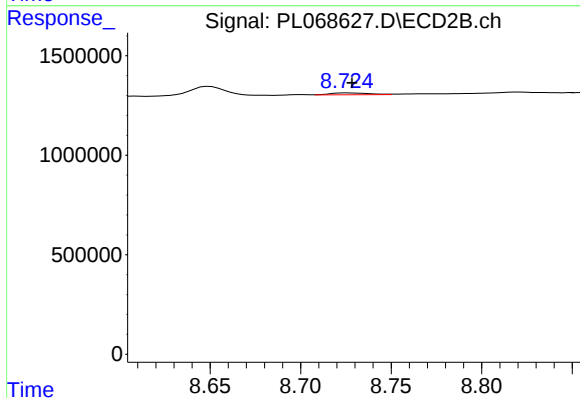


#13 Dieldrin

R.T.: 8.726 min
Delta R.T.: -0.003 min
Response: 143853
Conc: 0.14 ng/ml

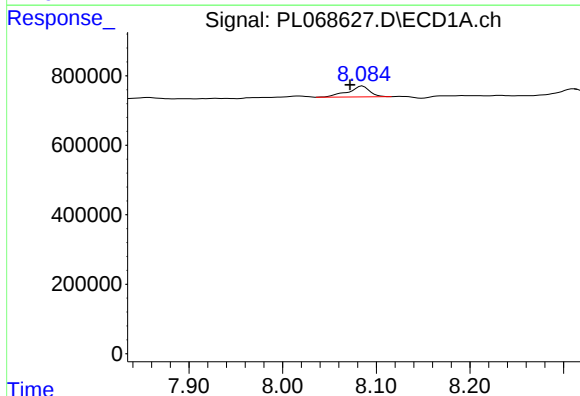


#14 Endrin

R.T.: 8.085 min
Delta R.T.: 0.013 min
Response: 506002
Conc: 1.01 ng/ml

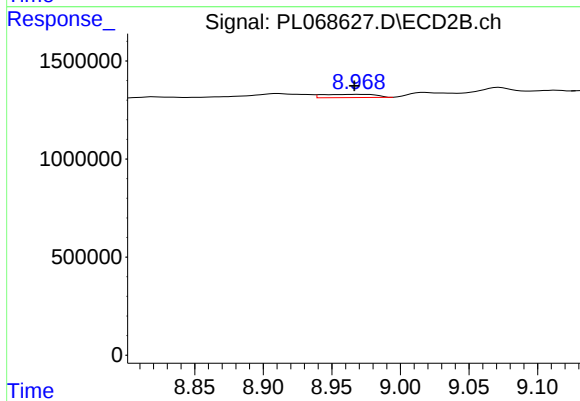

#14 Endrin


R.T.: 8.969 min
Delta R.T.: 0.002 min
Response: 451479
Conc: 0.50 ng/ml

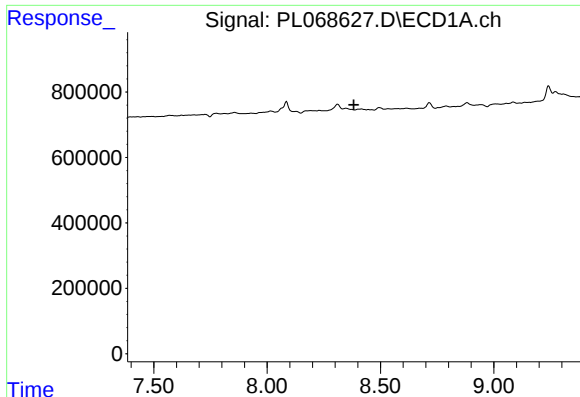

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

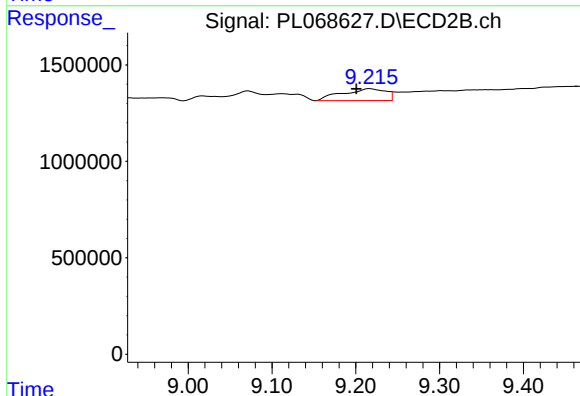


#15 Endosulfan II

R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 2202878
Conc: 2.43 ng/ml

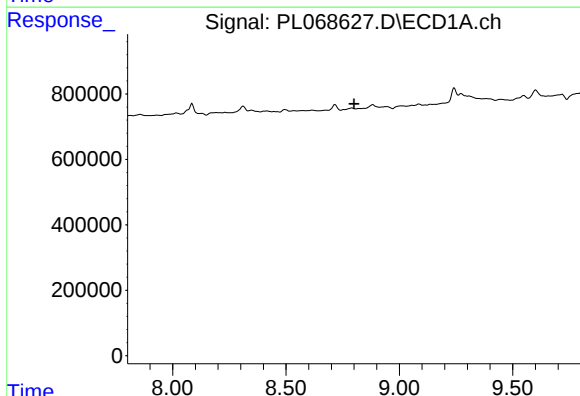


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

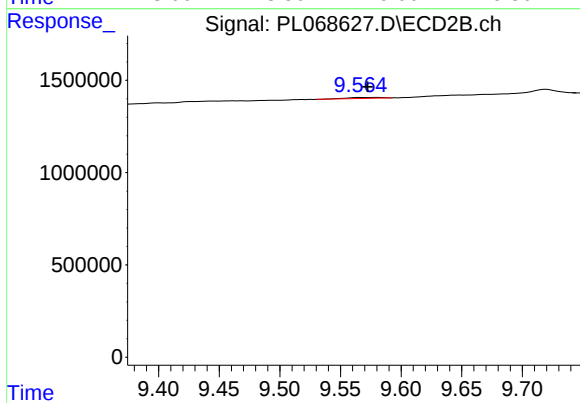

#19 Endosulfan Sulfate


R.T.: 9.566 min
Delta R.T.: -0.006 min
Response: 101278
Conc: 0.11 ng/ml

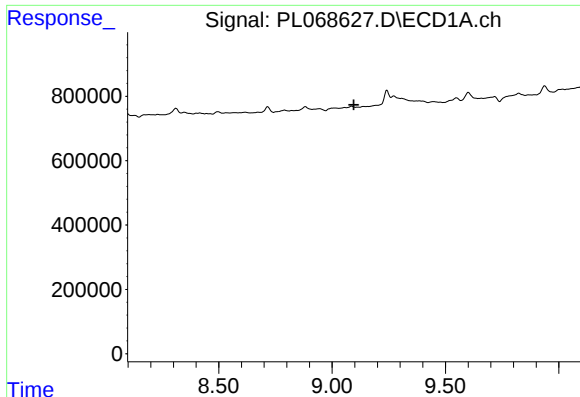

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

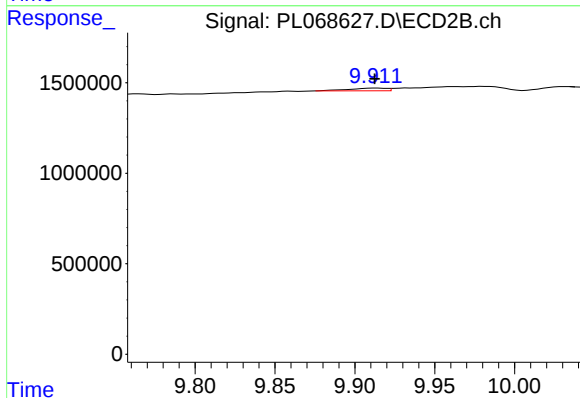


#20 Methoxychlor

R.T.: 9.913 min
Delta R.T.: 0.000 min
Response: 249639
Conc: 0.49 ng/ml

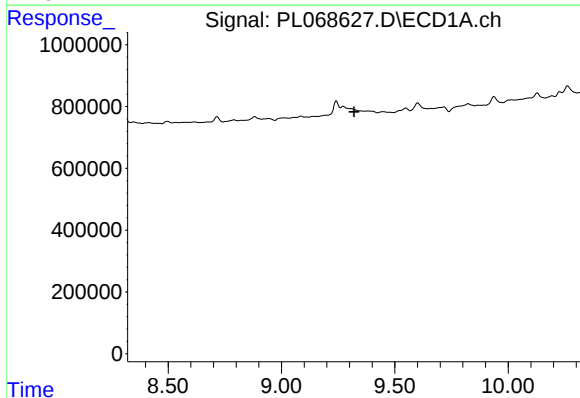


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.320 min
Response: 0
Conc: N.D.

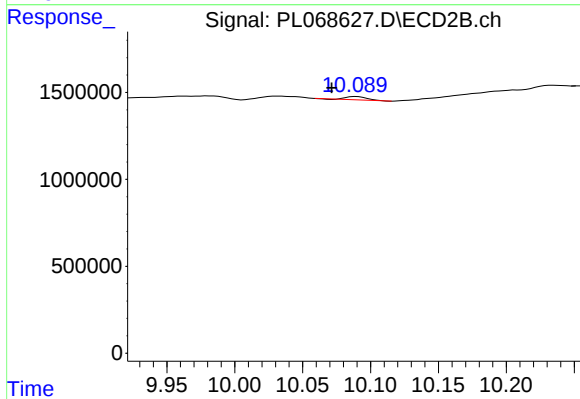

#21 Endrin ketone


R.T.: 10.090 min
Delta R.T.: 0.019 min
Response: 215219
Conc: 0.22 ng/ml

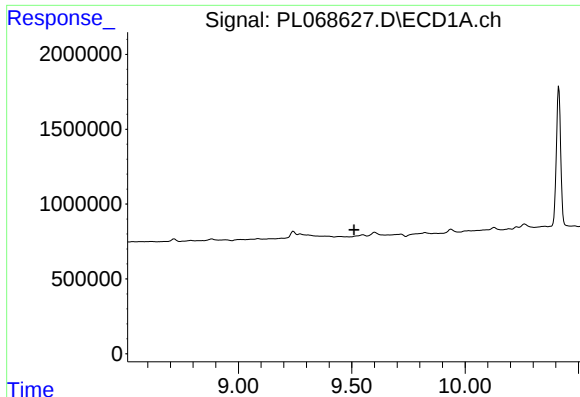

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

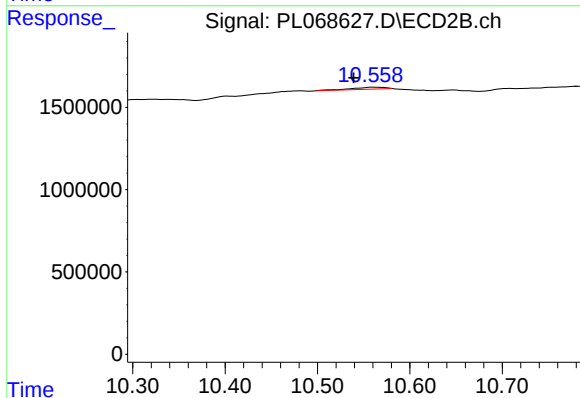


#22 Mirex

R.T.: 10.560 min
Delta R.T.: 0.021 min
Response: 319132
Conc: 0.41 ng/ml

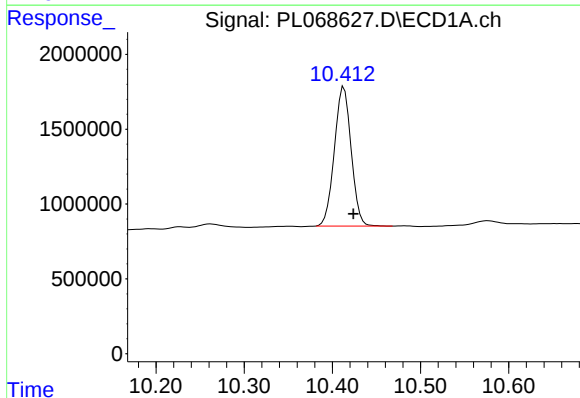

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: -0.011 min
Response: 12299588
Conc: 21.87 ng/ml

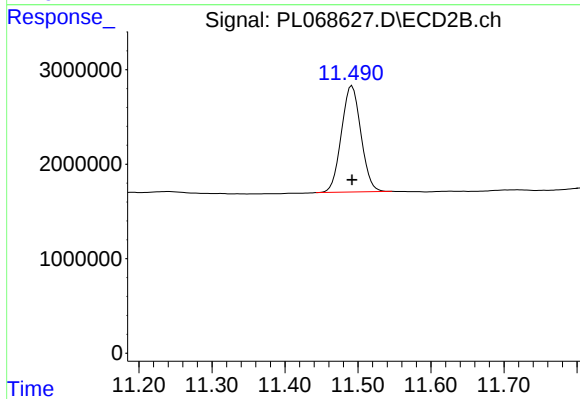

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 20916512
Conc: 23.45 ng/ml