

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073021\
 Data File : PL068613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 18:41
 Operator : AR\AJ
 Sample : M3235-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MH-457-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 11:29:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.570	6436655	16537979	14.997	16.207
28)	SA Decachlor...	10.416	11.493	9286164	15936514	16.511	17.866
Target Compounds							
10)	B gamma-Chl...	7.361	8.302	147224	416135	0.257m	0.370 #
11)	B alpha-Chl...	7.430	8.385	376868	1173626	0.656m	1.043 #
12)	B 4,4'-DDE	7.645	8.566	118753	236257	0.236m	0.229
17)	MA 4,4'-DDT	8.490	9.428	161792	243188	0.323m	0.258



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073021\
Data File : PL068613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 18:41
Operator : AR\AJ
Sample : M3235-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
MH-457-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 11:29:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

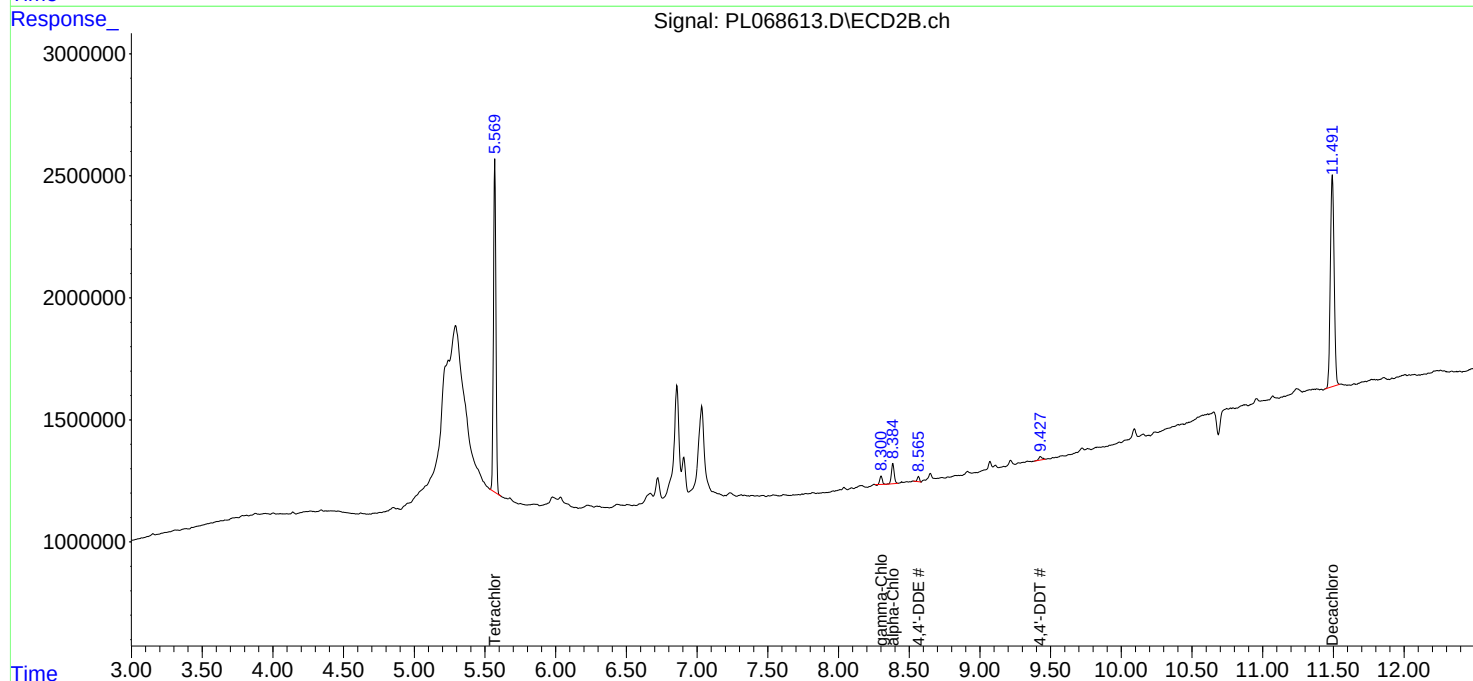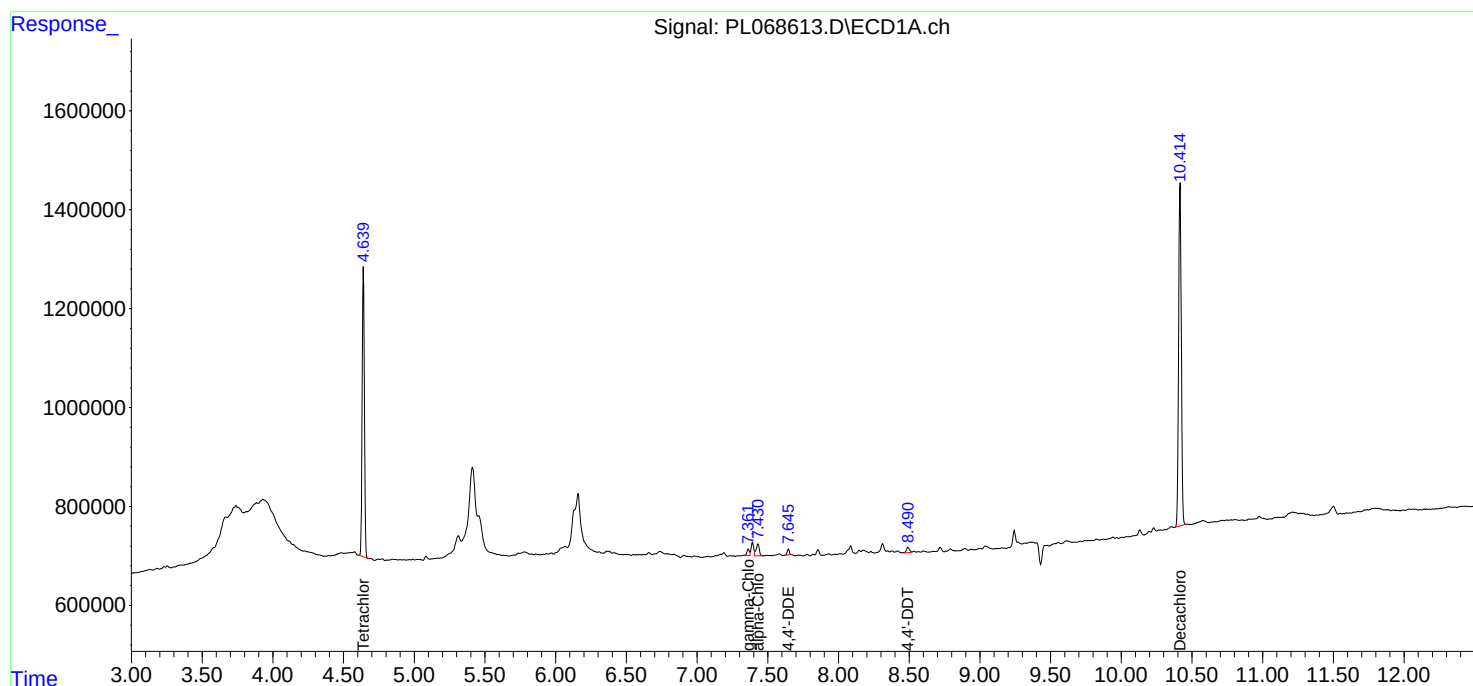


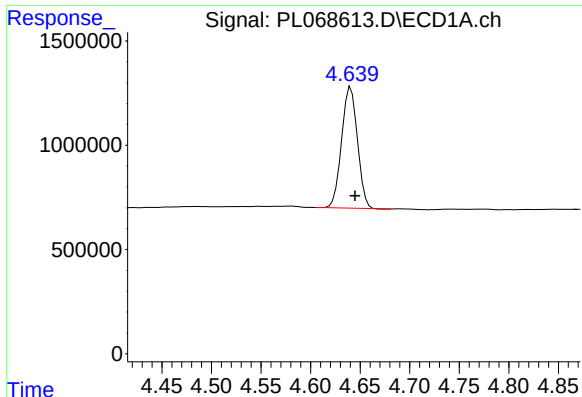

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 6436655
Conc: 15.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
MH-457-COMP

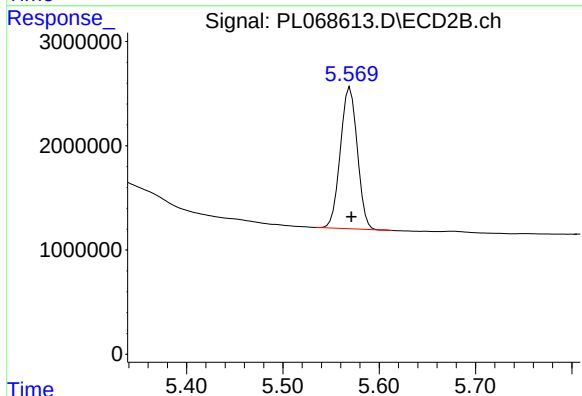


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 16537979
Conc: 16.21 ng/ml

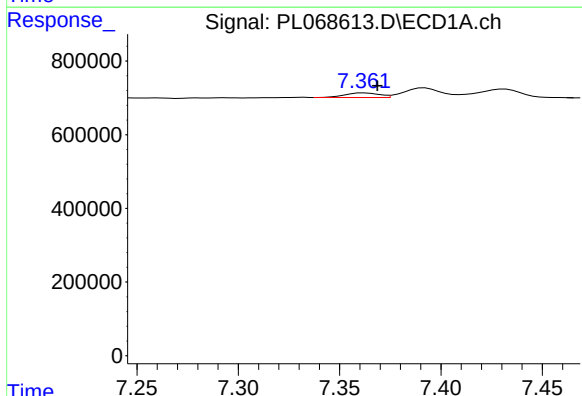


#10 gamma-Chlordane

R.T.: 7.361 min
Delta R.T.: -0.008 min
Response: 147224
Conc: 0.26 ng/ml m

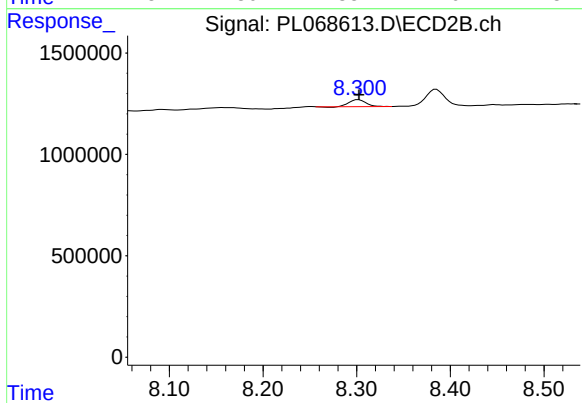

#10 gamma-Chlordane


R.T.: 8.302 min
Delta R.T.: 0.000 min
Response: 416135
Conc: 0.37 ng/ml

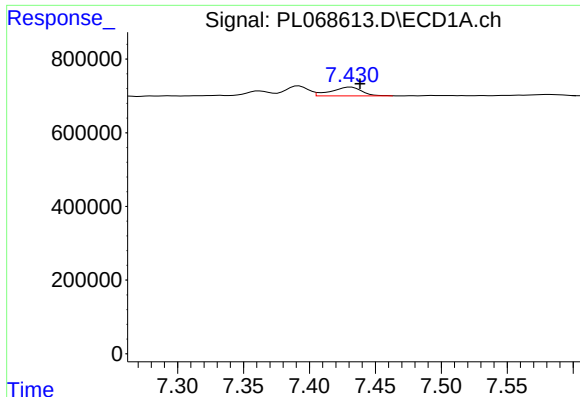

#11 alpha-Chlordane


R.T.: 7.430 min
Delta R.T.: -0.008 min
Response: 376868
Conc: 0.66 ng/ml m

Instrument :
ECD_L
ClientSampleId :
MH-457-COMP

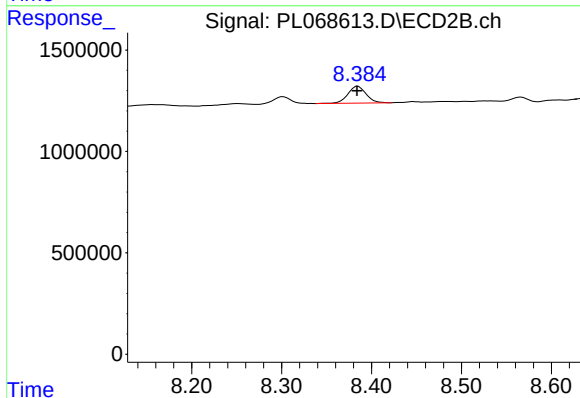


#11 alpha-Chlordane

R.T.: 8.385 min
Delta R.T.: 0.001 min
Response: 1173626
Conc: 1.04 ng/ml

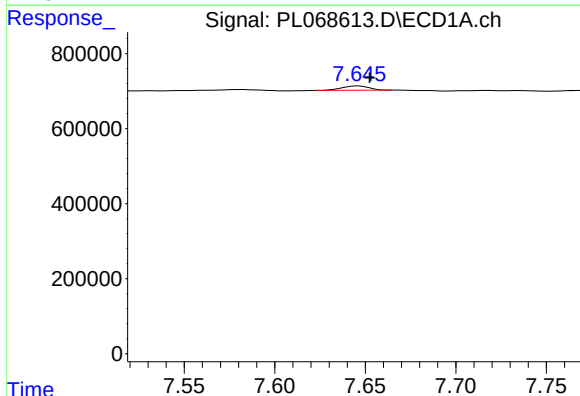


#12 4,4'-DDE

R.T.: 7.645 min
Delta R.T.: -0.007 min
Response: 118753
Conc: 0.24 ng/ml m

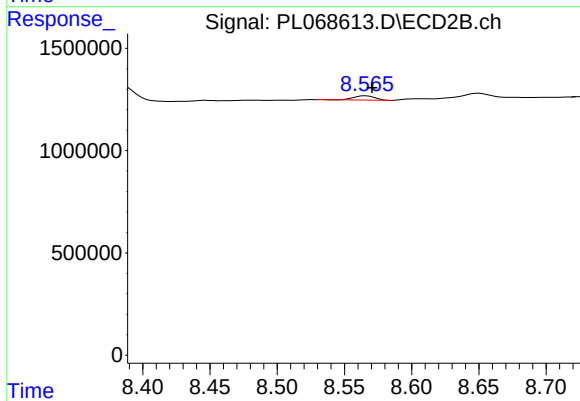

#12 4,4'-DDE


R.T.: 8.566 min
Delta R.T.: -0.005 min
Response: 236257
Conc: 0.23 ng/ml

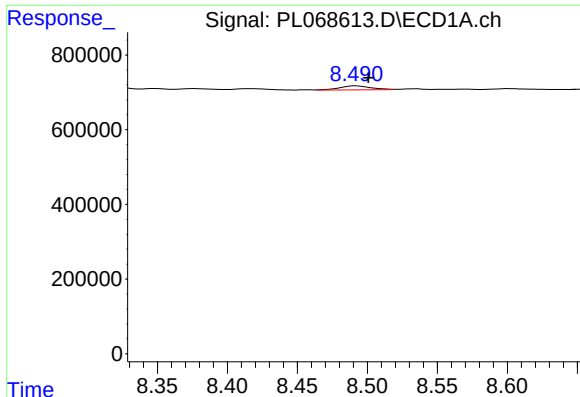

#17 4,4'-DDT


R.T.: 8.490 min
Delta R.T.: -0.010 min
Response: 161792
Conc: 0.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
MH-457-COMP

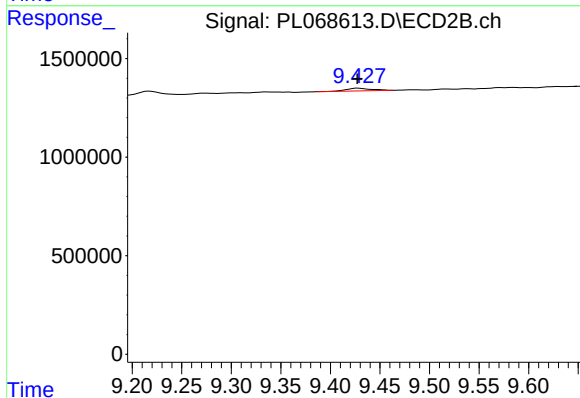


#17 4,4'-DDT

R.T.: 9.428 min
Delta R.T.: 0.001 min
Response: 243188
Conc: 0.26 ng/ml

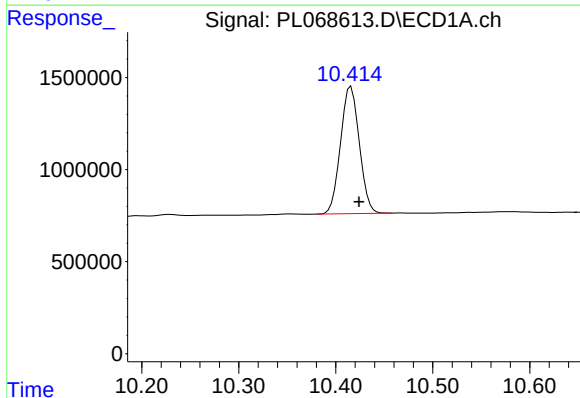

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.008 min
Response: 9286164
Conc: 16.51 ng/ml

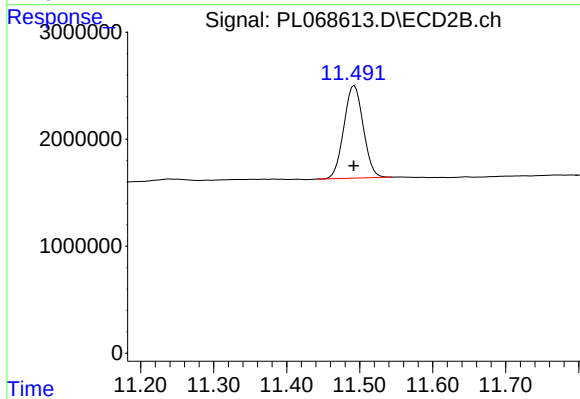

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 15936514
Conc: 17.87 ng/ml