

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073025\
 Data File : PL096650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2025 15:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 07:58:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.824	67868867	106.0E6	21.337	22.180
28)	SA Decachlor...	9.019	7.992	55983108	96778359	23.476	22.308
Target Compounds							
5)	MB Aldrin	5.228	0.000	2699102	0	0.628	N.D. #
8)	B Heptachlo...	5.655	0.000	40086267	0	10.394	N.D. #
13)	MA Dieldrin	0.000	5.423	0	32819103	N.D.	5.556 #
14)	MA Endrin	0.000	5.717	0	111.5E6	N.D.	20.628 #
16)	A 4,4'-DDD	6.671	0.000	11718099	0	4.635	N.D. #
22)	Mirex	8.086	0.000	6136055	0	2.475	N.D. #
24)	Chlordane-2	5.200	4.444f	7621763	59416588	43.551	244.925 #
27)	Chlordane-5	0.000	6.032f	0	37918568	N.D.	148.635 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073025\
Data File : PL096650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2025 15:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 07:58:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

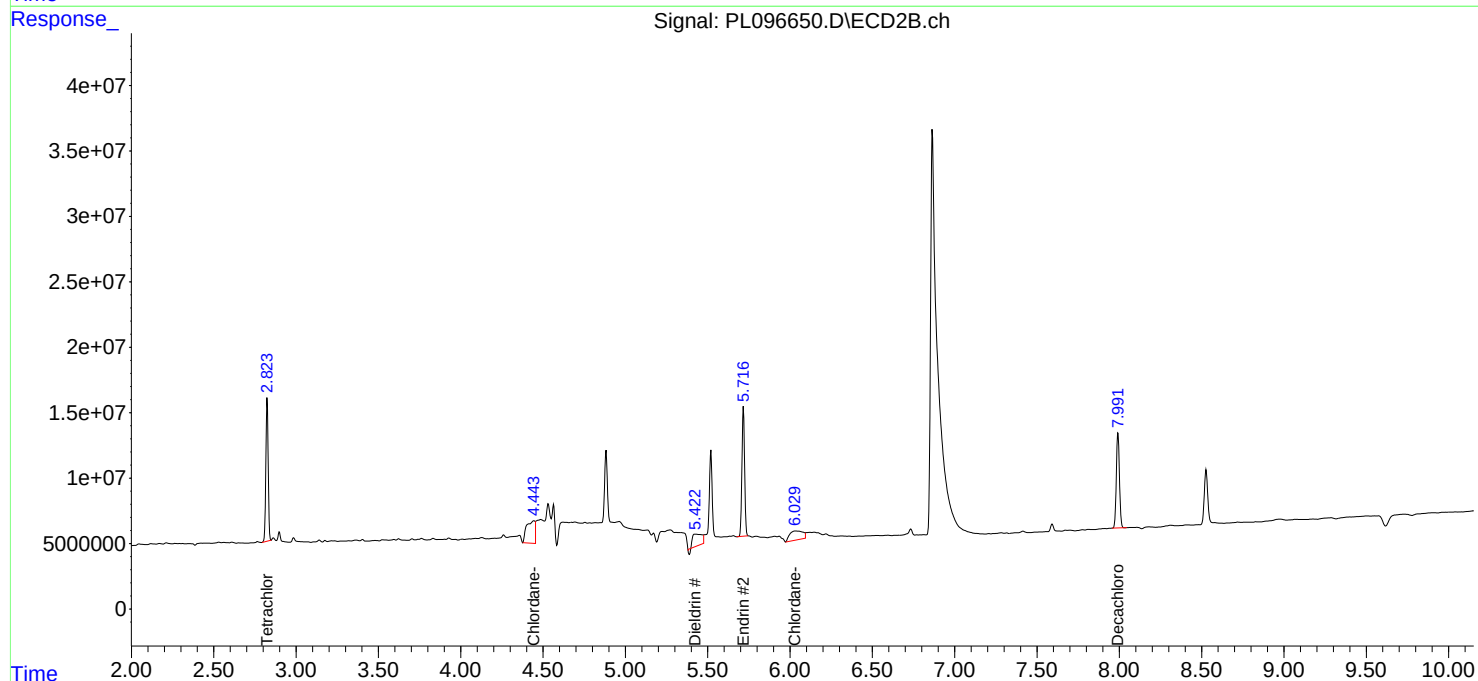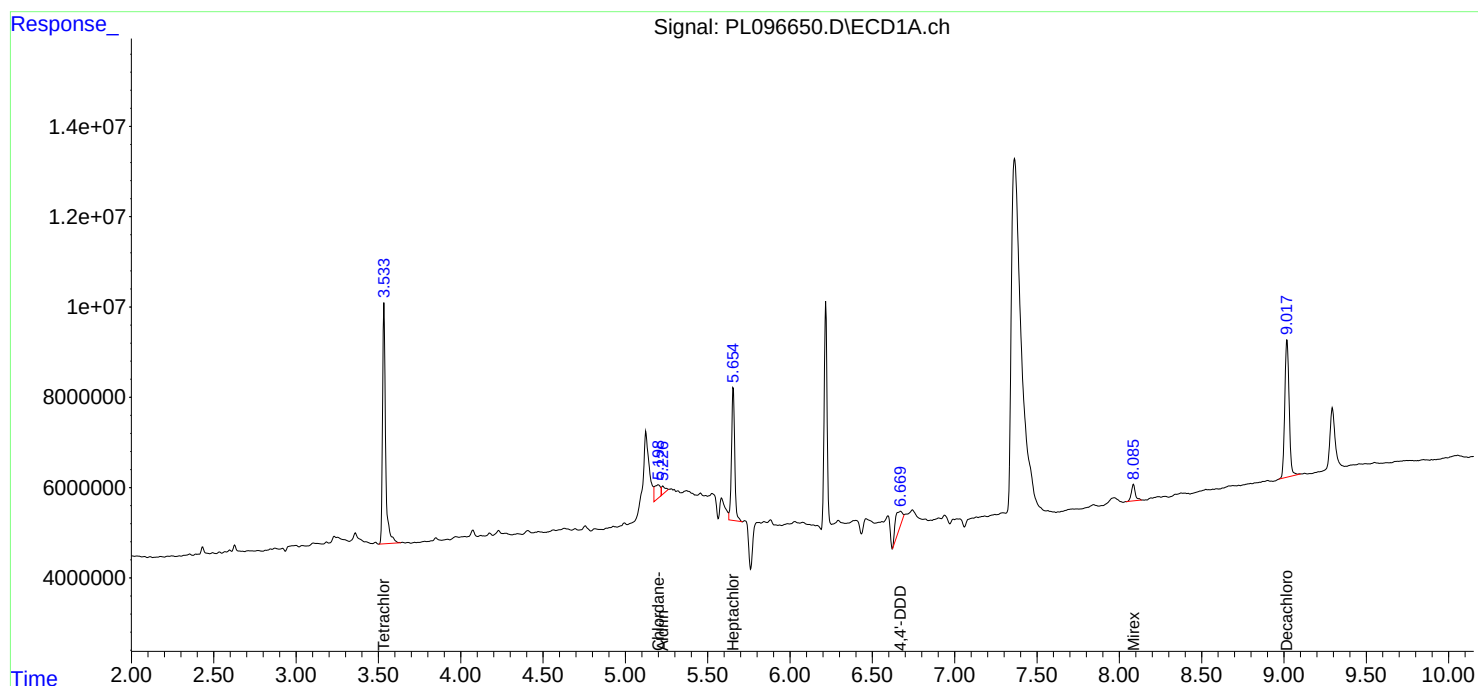


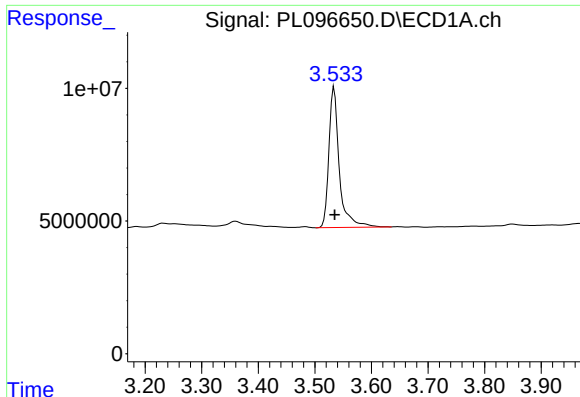

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: -0.001 min
Response: 67868867
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

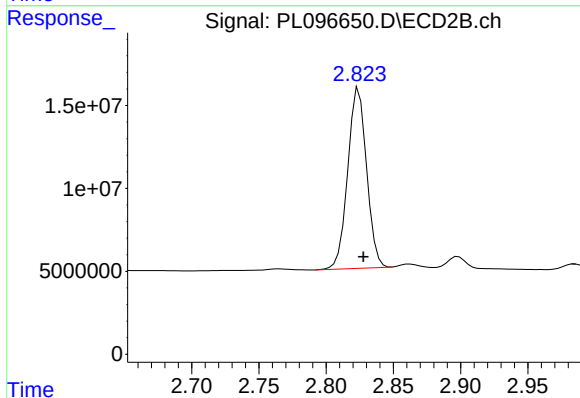


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: -0.003 min
Response: 105970112
Conc: 22.18 ng/ml

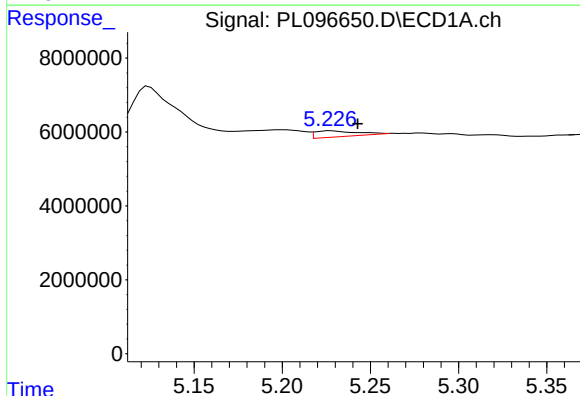


#5 Aldrin

R.T.: 5.228 min
Delta R.T.: -0.015 min
Response: 2699102
Conc: 0.63 ng/ml

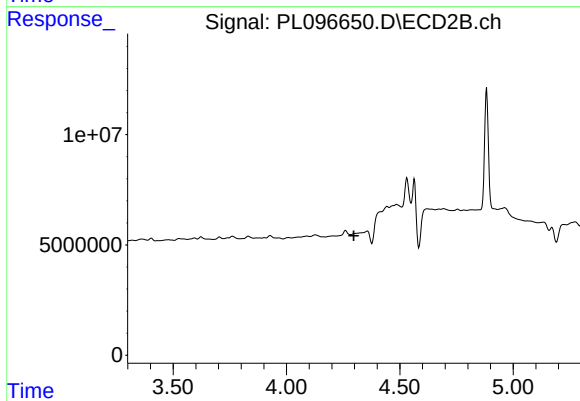

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.297 min
Response: 0
Conc: N.D.

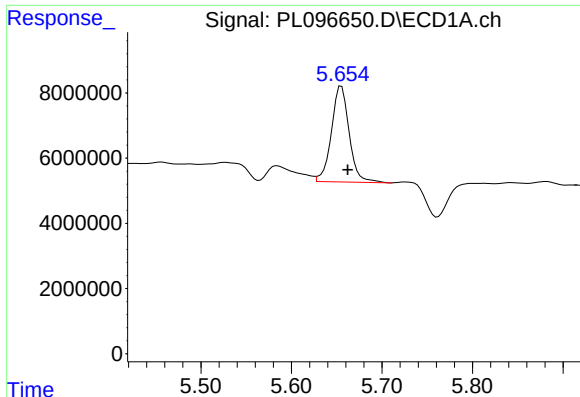

#8 Heptachlor epoxide


R.T.: 5.655 min
Delta R.T.: -0.007 min
Response: 40086267
Conc: 10.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

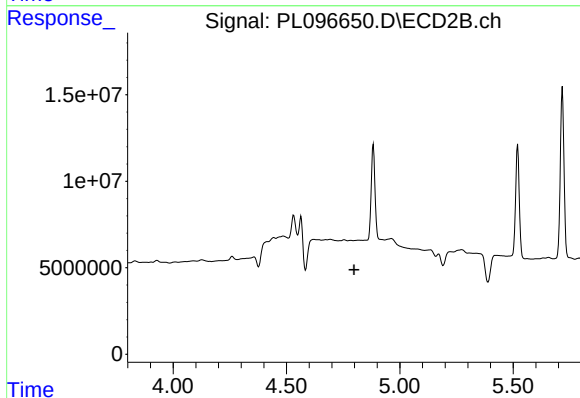


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

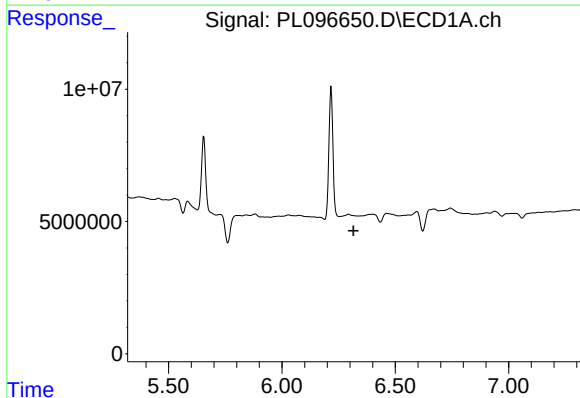


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

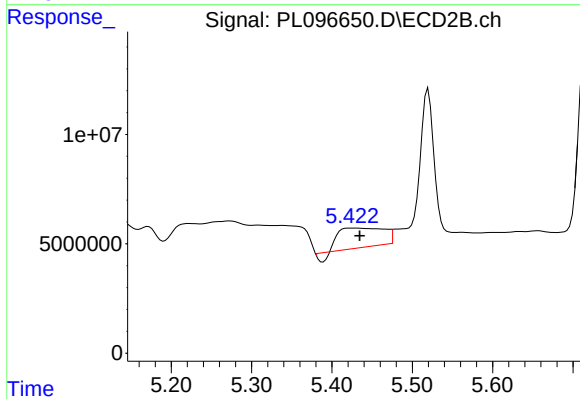

#13 Dieldrin


R.T.: 5.423 min
Delta R.T.: -0.011 min
Response: 32819103
Conc: 5.56 ng/ml

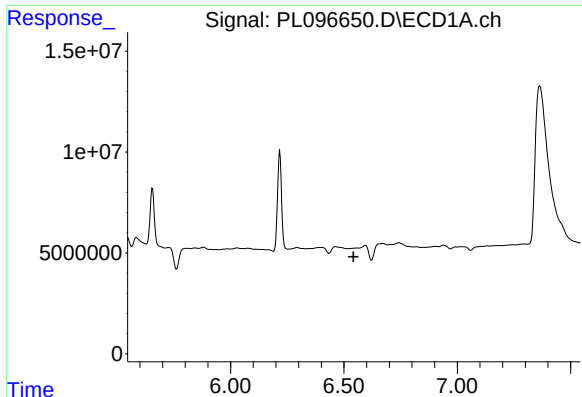

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

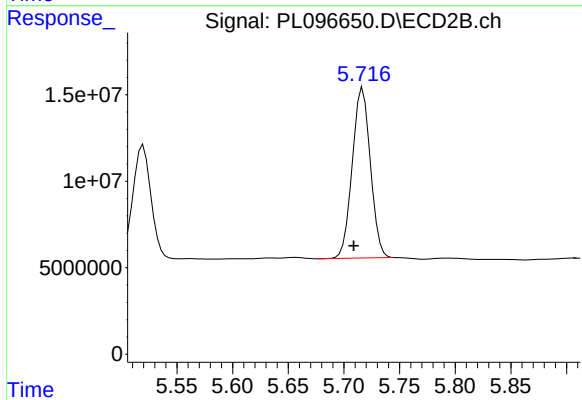


#14 Endrin

R.T.: 5.717 min
Delta R.T.: 0.008 min
Response: 111514878
Conc: 20.63 ng/ml

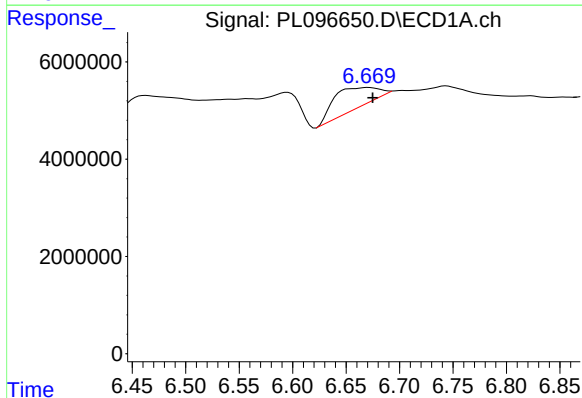


#16 4,4'-DDD

R.T.: 6.671 min
Delta R.T.: -0.004 min
Response: 11718099
Conc: 4.63 ng/ml

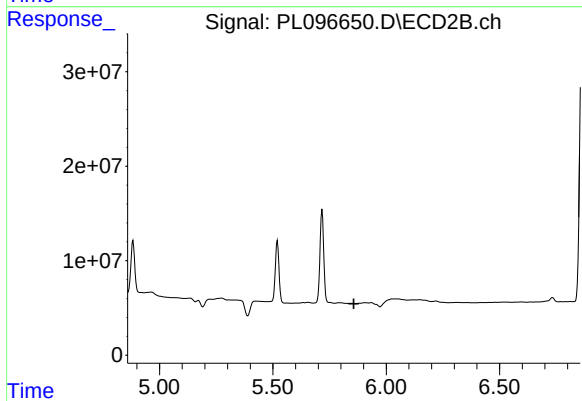

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.856 min
Response: 0
Conc: N.D.

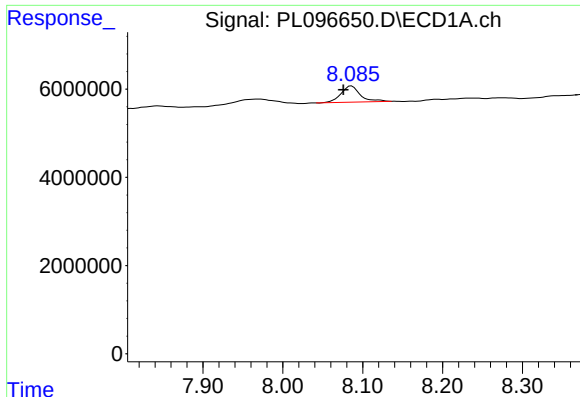

#22 Mirex


R.T.: 8.086 min
Delta R.T.: 0.010 min
Response: 6136055
Conc: 2.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

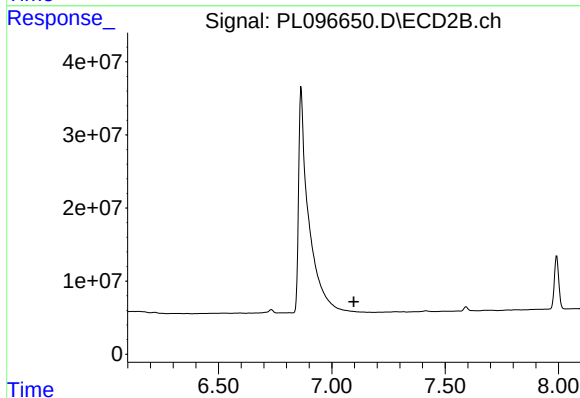


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.097 min
Response: 0
Conc: N.D.

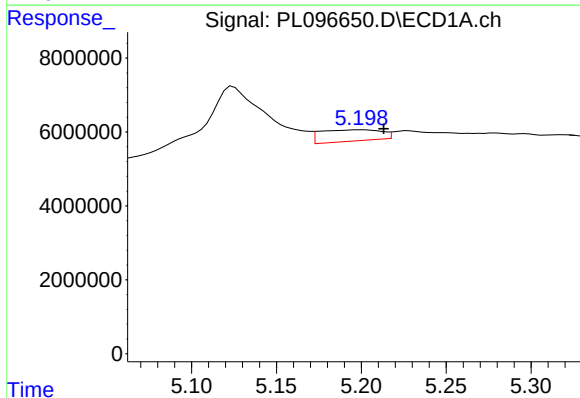


#24 Chlordane-2

R.T.: 5.200 min
Delta R.T.: -0.013 min
Response: 7621763
Conc: 43.55 ng/ml

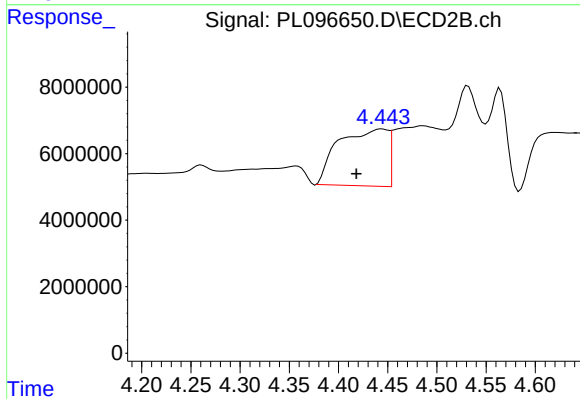

#24 Chlordane-2


R.T.: 4.444 min
Delta R.T.: 0.026 min
Response: 59416588
Conc: 244.93 ng/ml

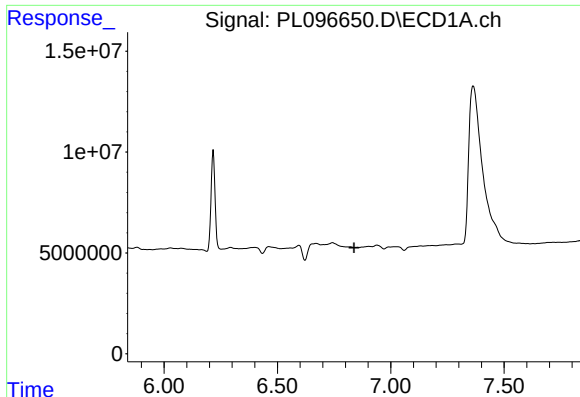

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

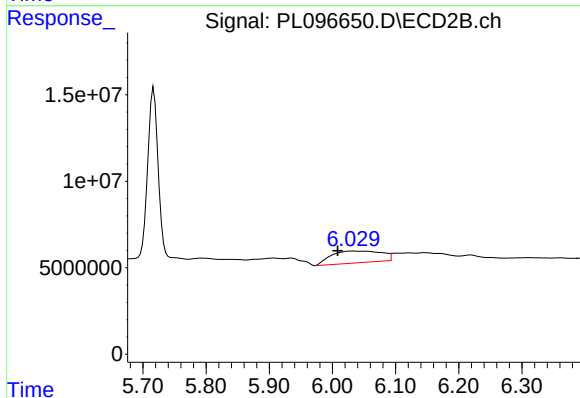


#27 Chlordane-5

R.T.: 6.032 min
Delta R.T.: 0.023 min
Response: 37918568
Conc: 148.63 ng/ml

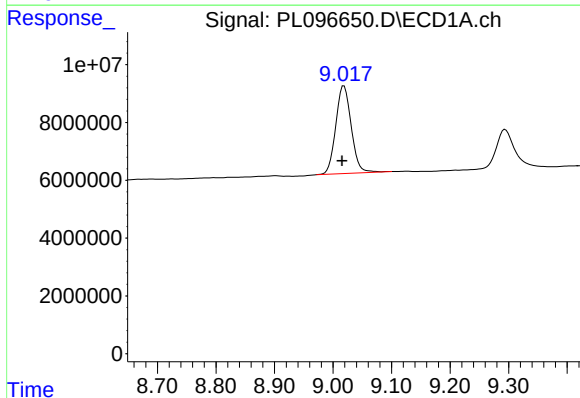

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.003 min
Response: 55983108
Conc: 23.48 ng/ml

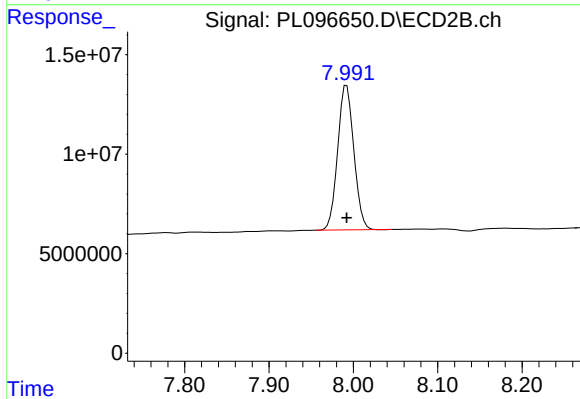

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 96778359
Conc: 22.31 ng/ml