

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073025\
 Data File : PL096646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2025 14:24
 Operator : AR\AJ
 Sample : Q2126-08
 Misc : LOQ CH 50PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LOQ-WATER-02-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 07:57:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	2.825	57062891	98222990	17.940	20.558
28)	SA Decachlor...	9.017	7.992	46501946	93625142	19.500	21.581
Target Compounds							
23)	Chlordane-1	4.688	3.836	9838127	11064969	57.833	52.781
24)	Chlordane-2	5.212	4.416	9674745	13959570	55.282	57.544
25)	Chlordane-3	5.916	5.050	33057573	35805054	49.492	51.496
26)	Chlordane-4	6.001	5.113	42317462	32056694	51.127	51.511
27)	Chlordane-5	6.838	6.008	6849664	13567290	51.835	53.182



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073025\
Data File : PL096646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2025 14:24
Operator : AR\AJ
Sample : Q2126-08
Misc : LOQ CH 50PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 07:57:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

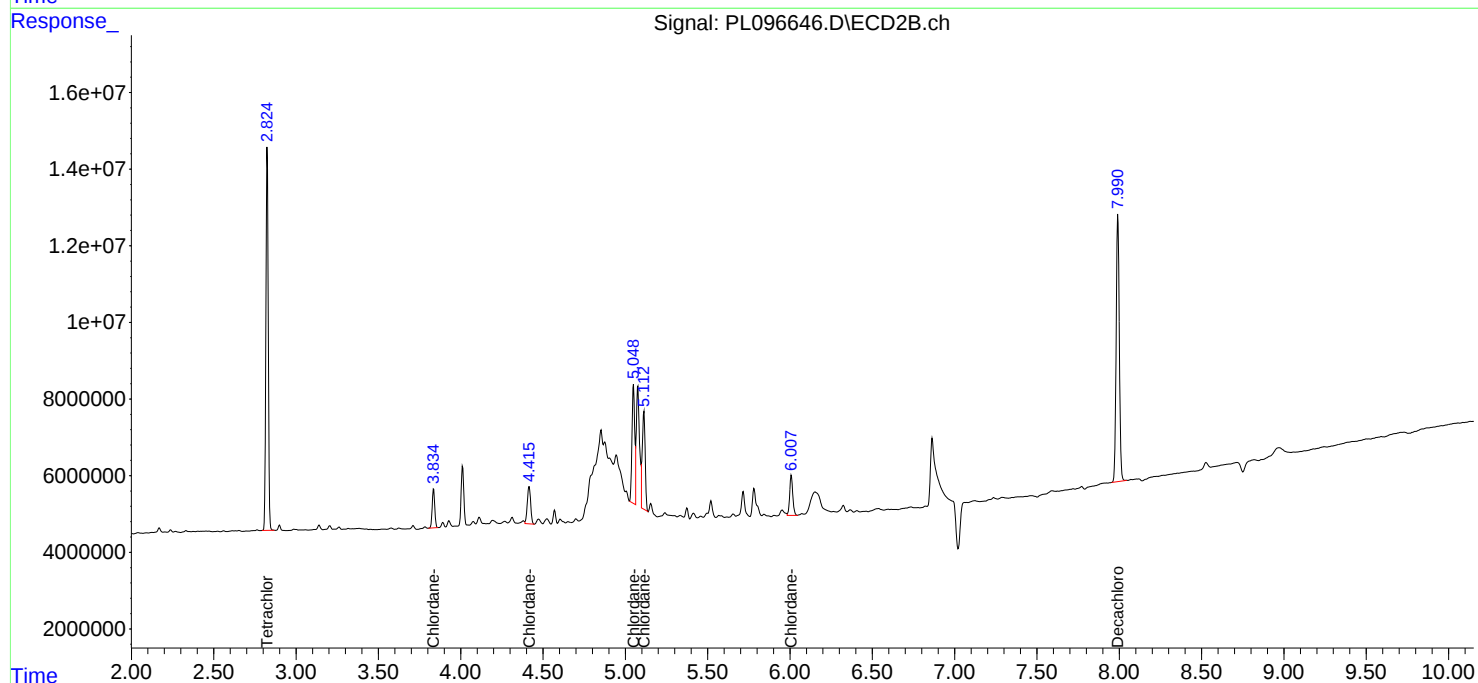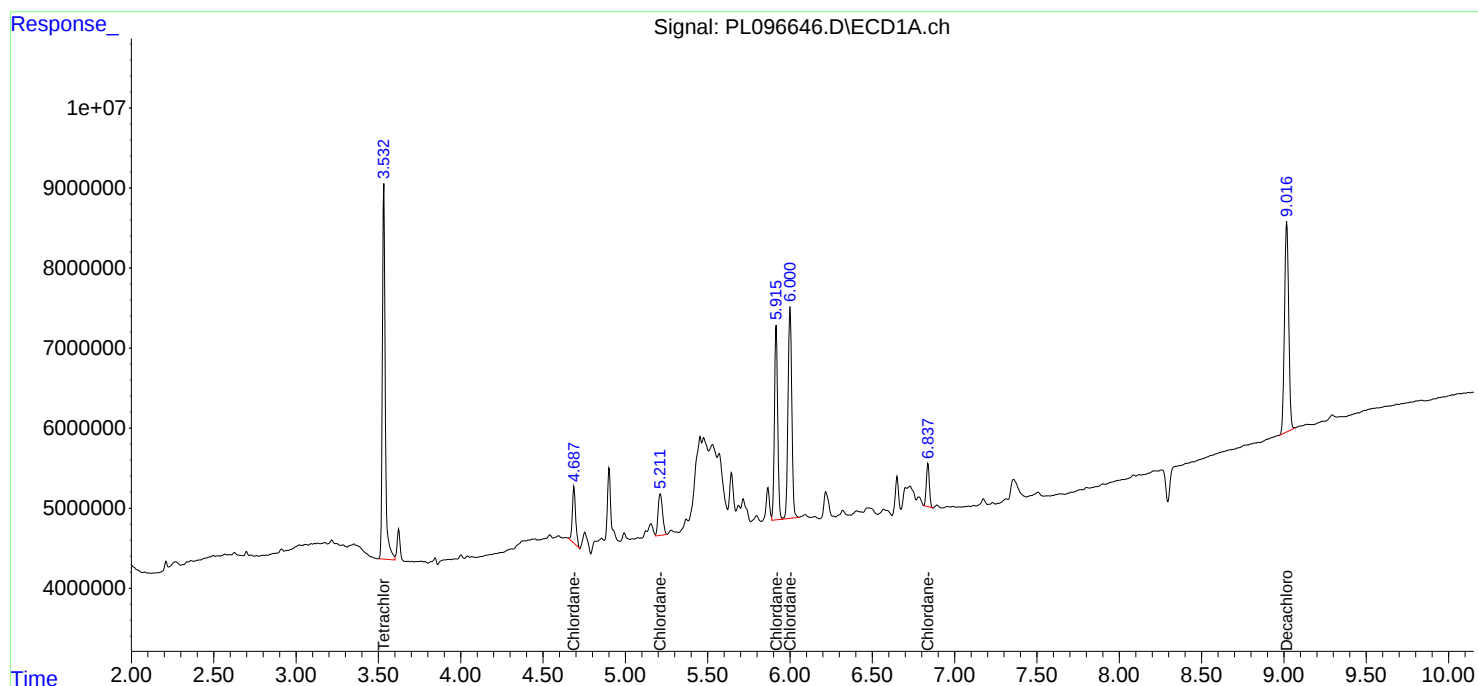


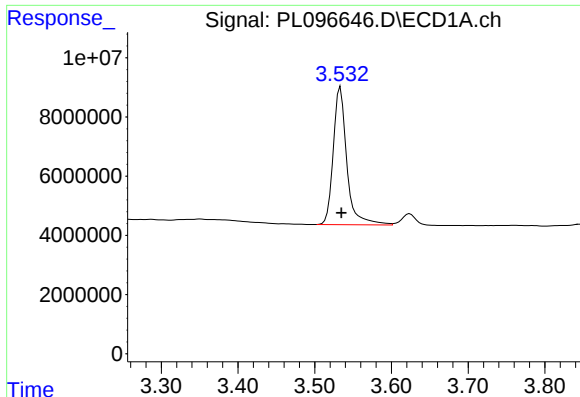

#1 Tetrachloro-m-xylene


R.T.: 3.533 min
Delta R.T.: -0.002 min
Response: 57062891
Conc: 17.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT2-2025

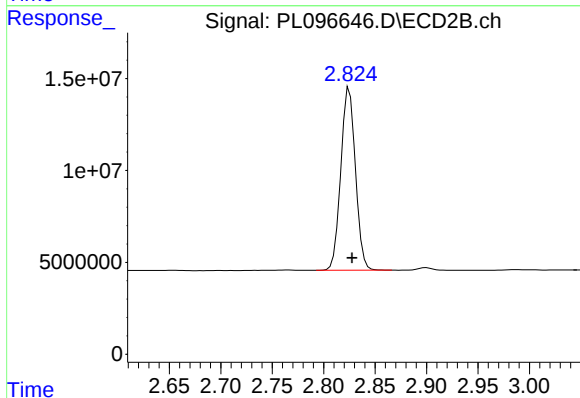


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 98222990
Conc: 20.56 ng/ml

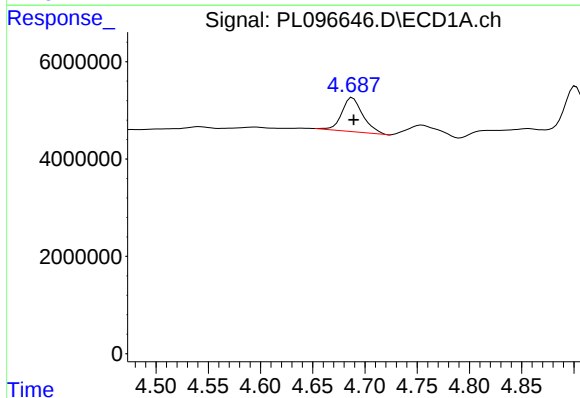


#23 Chlordane-1

R.T.: 4.688 min
Delta R.T.: -0.001 min
Response: 9838127
Conc: 57.83 ng/ml

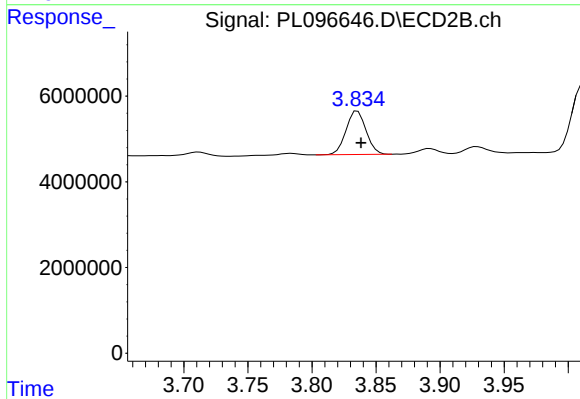

#23 Chlordane-1


R.T.: 3.836 min
Delta R.T.: -0.003 min
Response: 11064969
Conc: 52.78 ng/ml

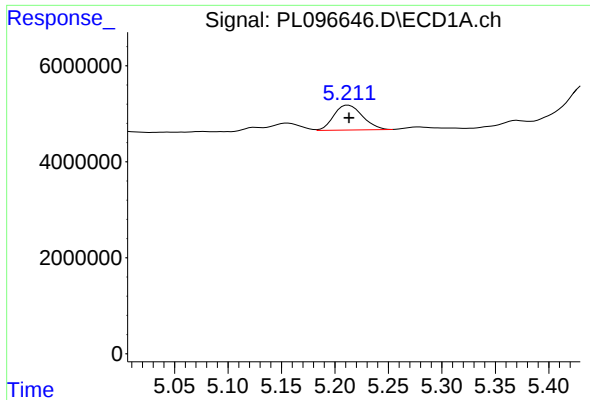

#24 Chlordane-2


R.T.: 5.212 min
Delta R.T.: 0.000 min
Response: 9674745
Conc: 55.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT2-2025

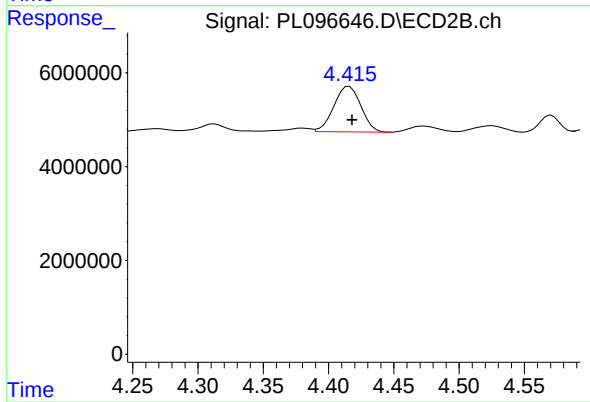


#24 Chlordane-2

R.T.: 4.416 min
Delta R.T.: -0.002 min
Response: 13959570
Conc: 57.54 ng/ml

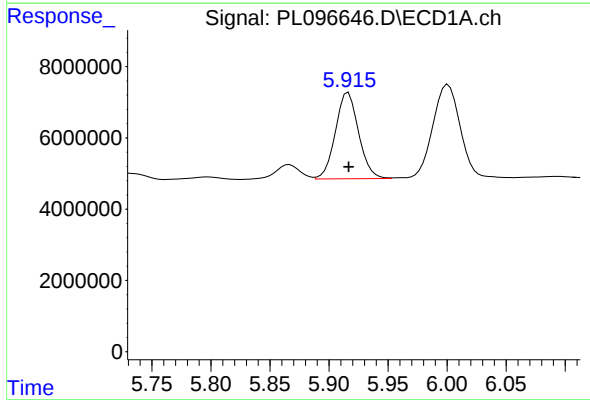


#25 Chlordane-3

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 33057573
Conc: 49.49 ng/ml

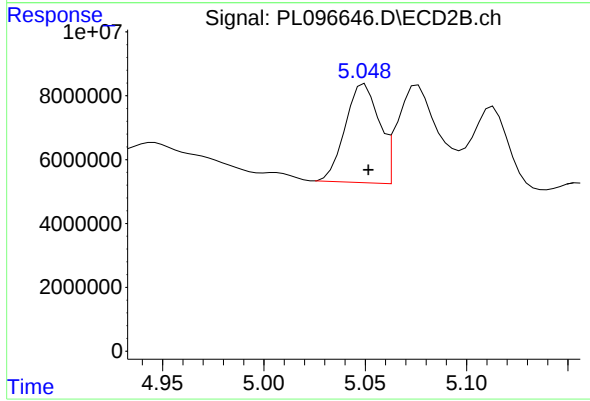

#25 Chlordane-3


R.T.: 5.050 min
Delta R.T.: -0.002 min
Response: 35805054
Conc: 51.50 ng/ml

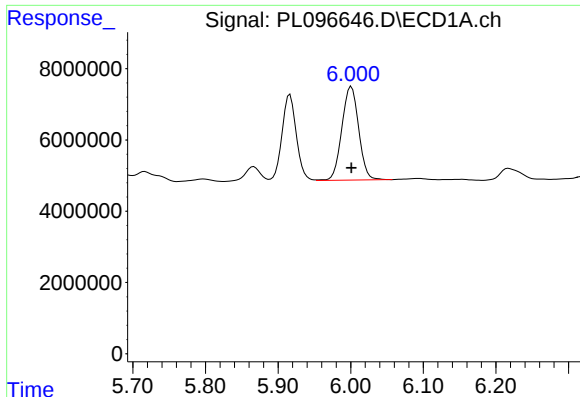

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 42317462
Conc: 51.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT2-2025

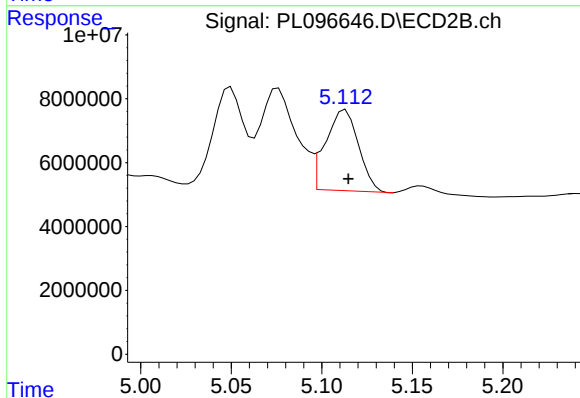


#26 Chlordane-4

R.T.: 5.113 min
Delta R.T.: -0.002 min
Response: 32056694
Conc: 51.51 ng/ml

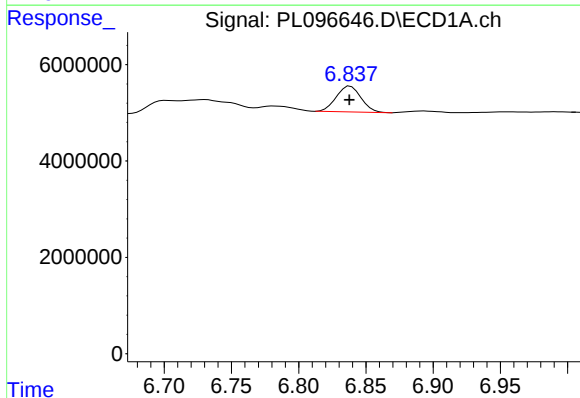


#27 Chlordane-5

R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 6849664
Conc: 51.83 ng/ml

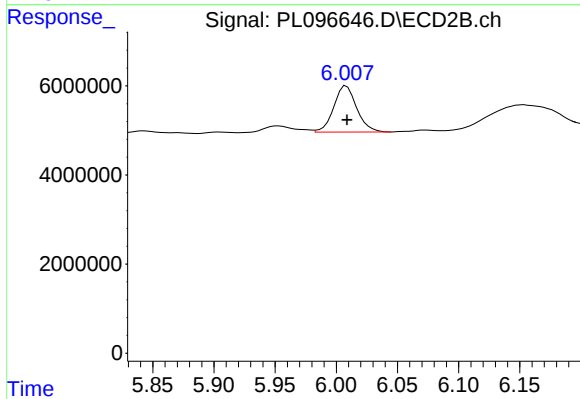

#27 Chlordane-5


R.T.: 6.008 min
Delta R.T.: 0.000 min
Response: 13567290
Conc: 53.18 ng/ml

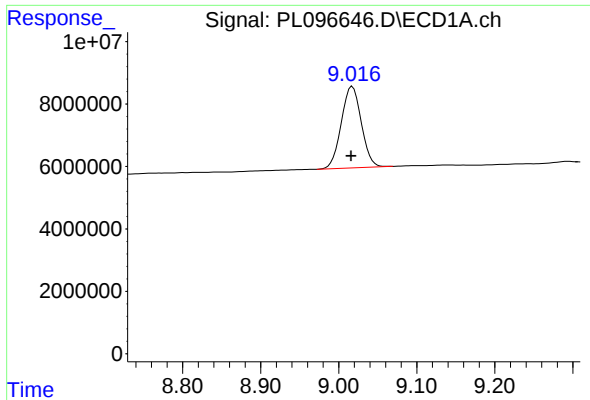

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.002 min
Response: 46501946
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
LOQ-WATER-02-QT2-2025

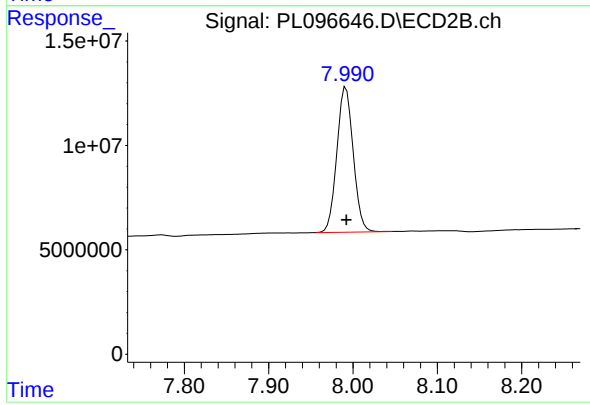

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 93625142
Conc: 21.58 ng/ml