

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073118\
 Data File : PL038722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2018 14:33
 Operator : AJ\SJ
 Sample : J4188-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HA-BASELINEWATER-N48971

Manual Integrations
 APPROVED

Sohil
 8/1/2018 9:55:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 15:05:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.926	125.4E6	48267003	16.838	18.388m
28)	SA Decachlor...	8.003	8.936	160.8E6	40690786	21.195	16.646m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073118\
Data File : PL038722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2018 14:33
Operator : AJ\SJ
Sample : J4188-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HA-BASELINEWATER-N48971


Manual Integrations
APPROVED

Sohil
8/1/2018 9:55:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 15:05:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

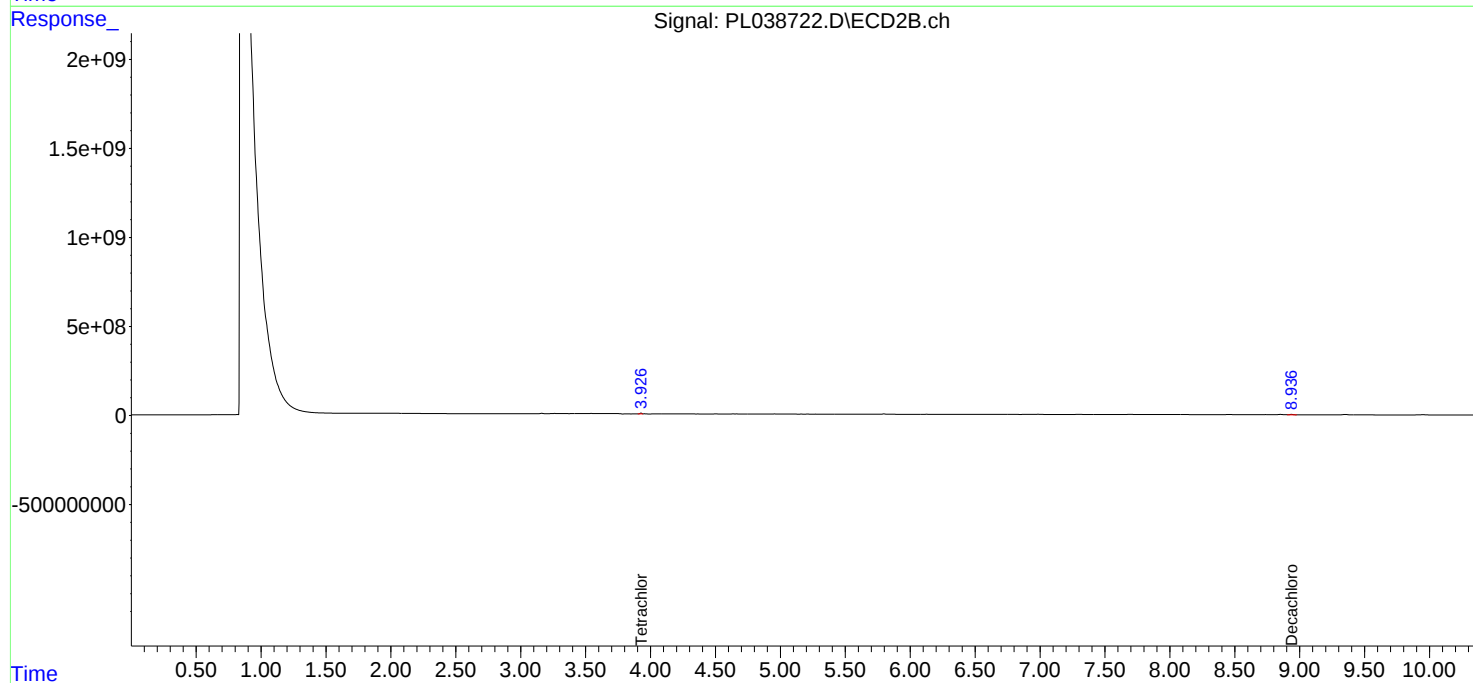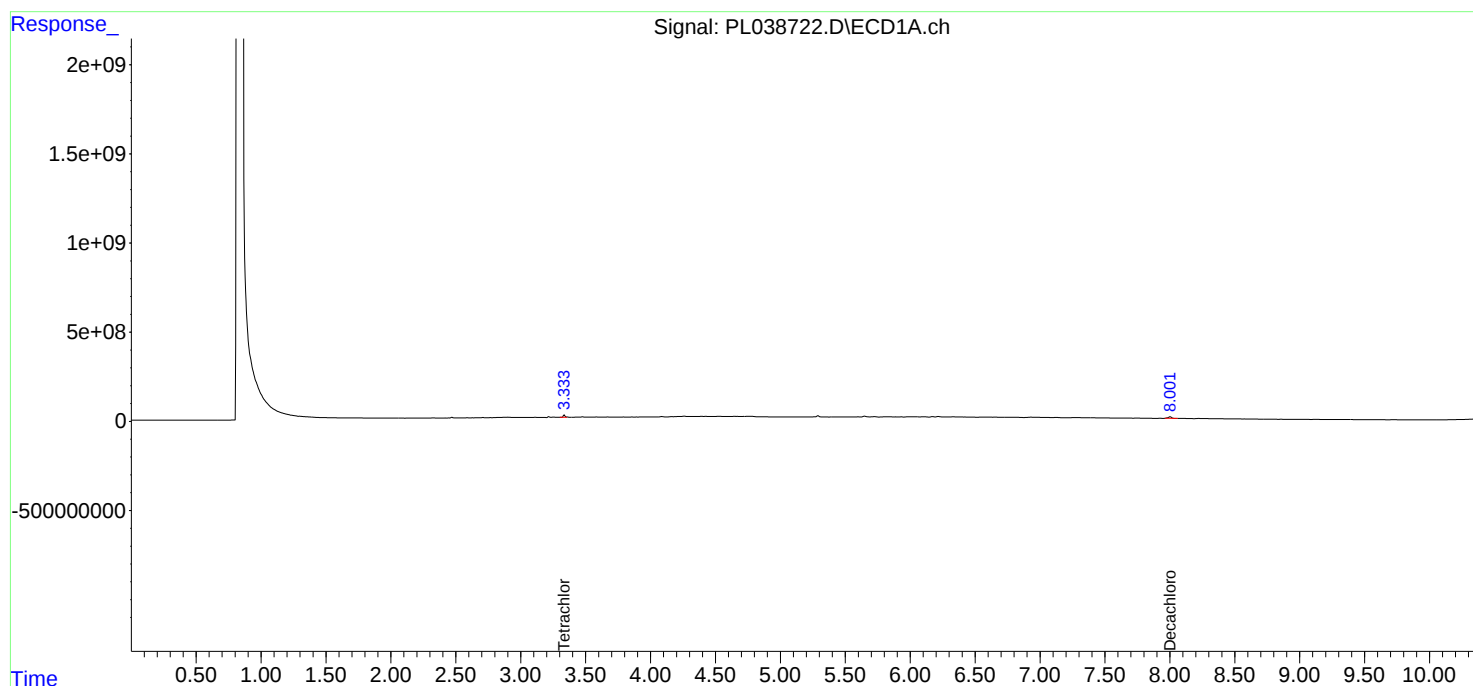

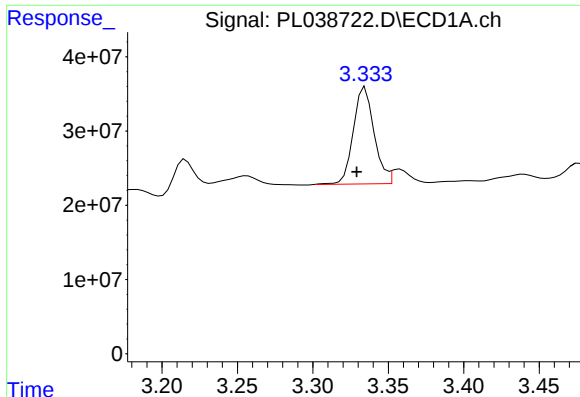


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: 0.006 min
Response: 125380571
Conc: 16.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-BASELINEWATER-N48971


Manual Integrations
APPROVED

Sohil
8/1/2018 9:55:17 AM

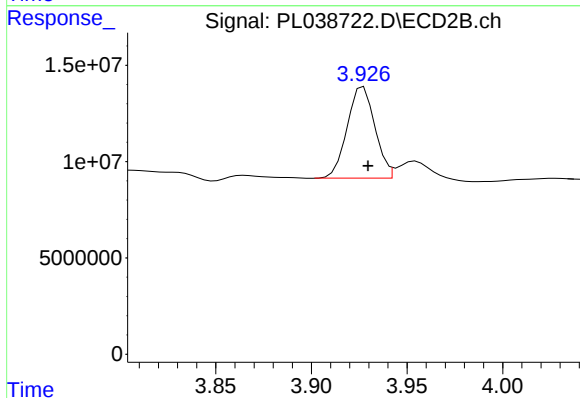


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 48267003
Conc: 18.39 ng/ml m

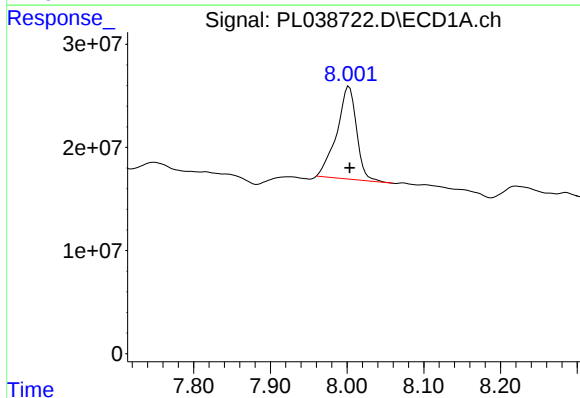

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 160781687
Conc: 21.19 ng/ml

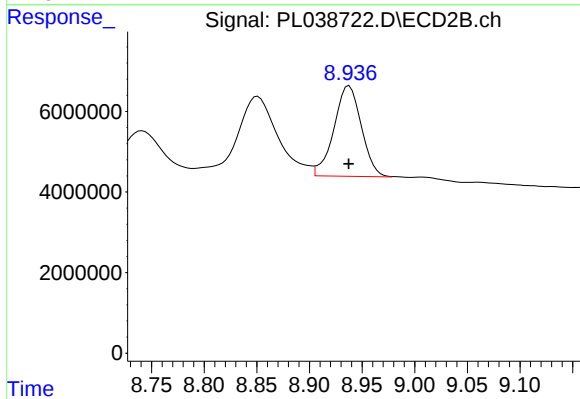

#28 Decachlorobiphenyl

R.T.: 8.936 min
Delta R.T.: 0.000 min
Response: 40690786
Conc: 16.65 ng/ml m