

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
 Data File : PL060369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 09:48
 Operator : DD\AJ
 Sample : L3183-18 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-072820

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 11:25:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

9) A	Endosulfan I	5.539f	0.000	16400495	0	9.808	N.D.	#
10) B	gamma-Chl...	0.000	6.111	0	11264033	N.D.	3.984	#
25)	Chlordane-3	0.000	6.111	0	11264033	N.D.	30.612	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
Data File : PL060369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 09:48
Operator : DD\AJ
Sample : L3183-18 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-02-072820

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 11:25:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

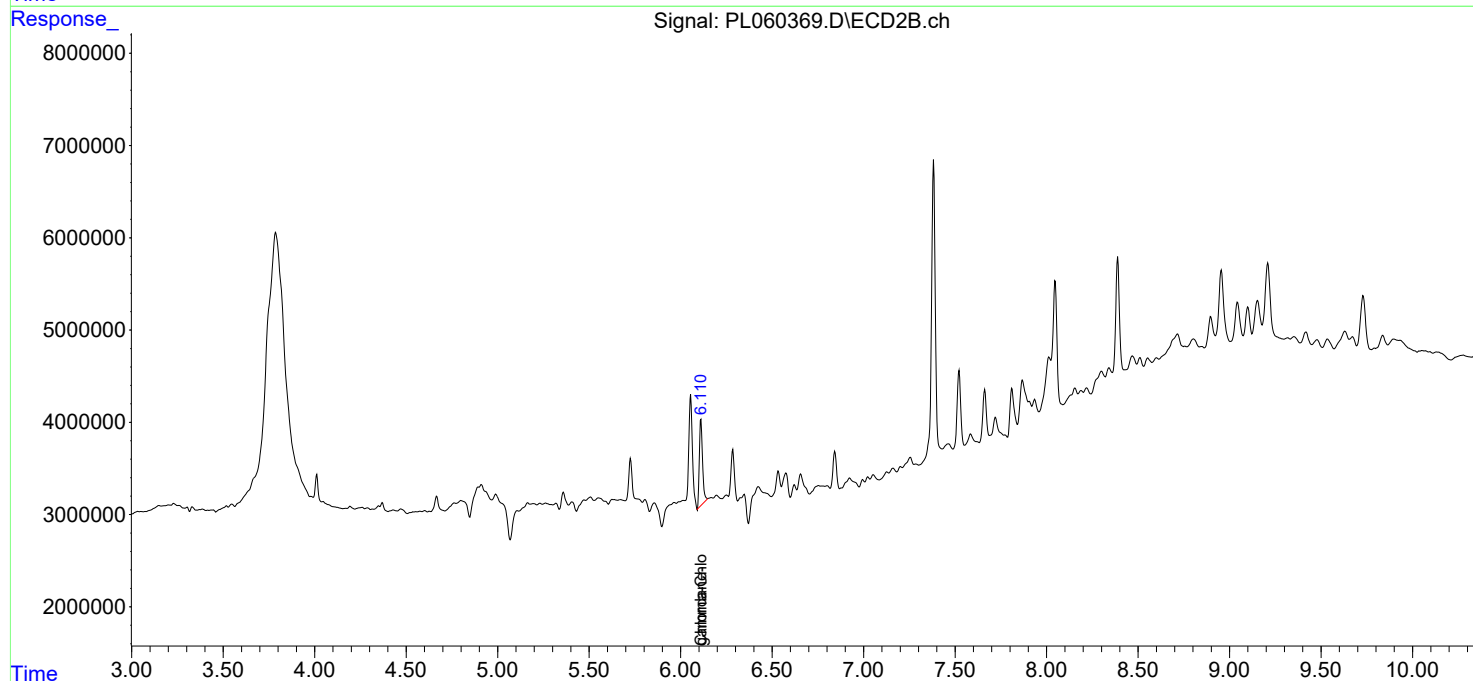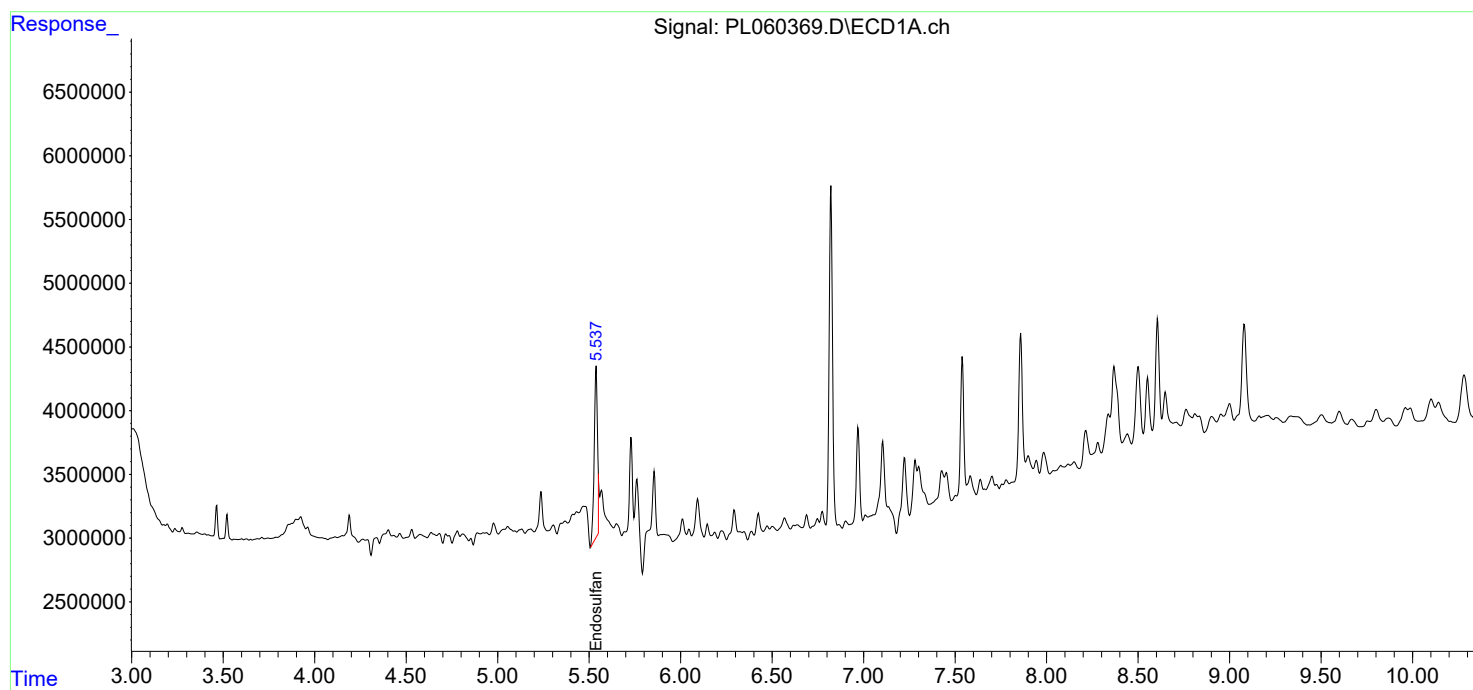


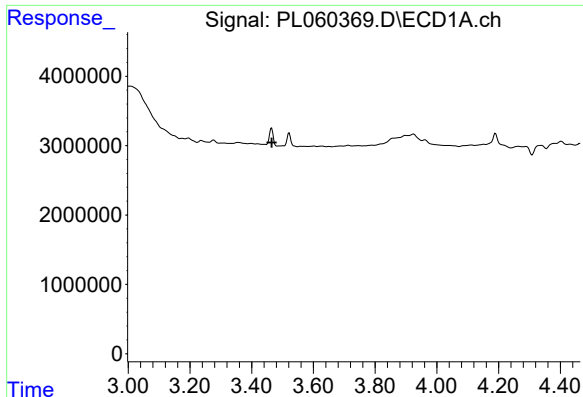

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-072820

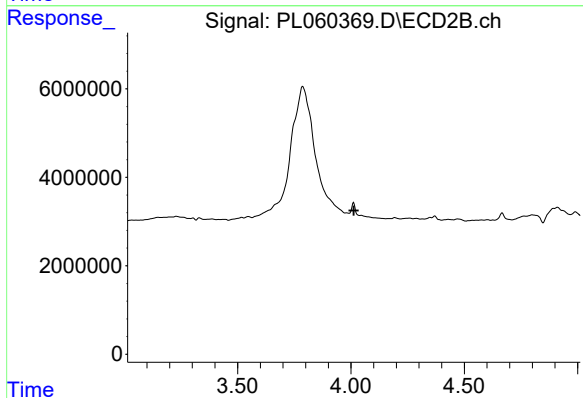


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.013 min
Response: 0
Conc: N.D.

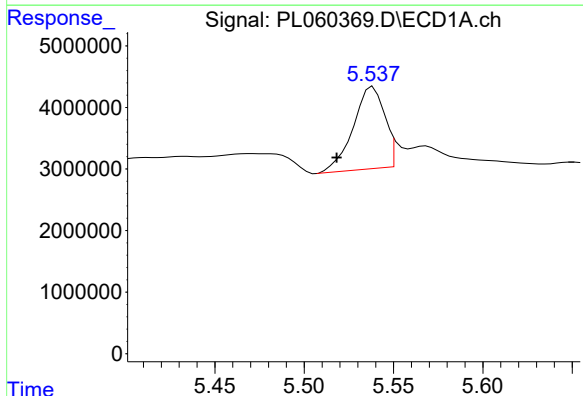


#9 Endosulfan I

R.T.: 5.539 min
Delta R.T.: 0.020 min
Response: 16400495
Conc: 9.81 ng/ml

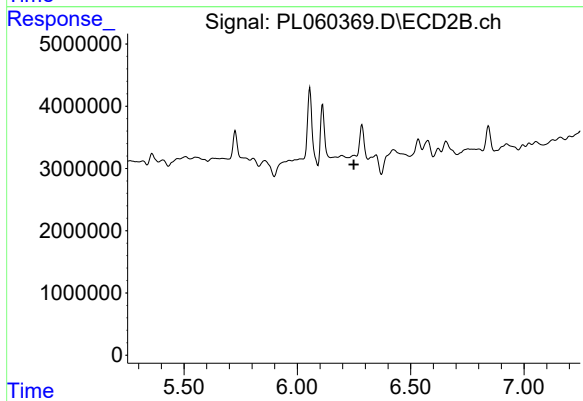

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

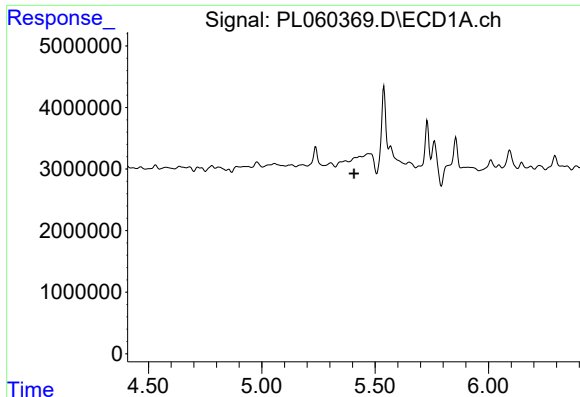

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-072820

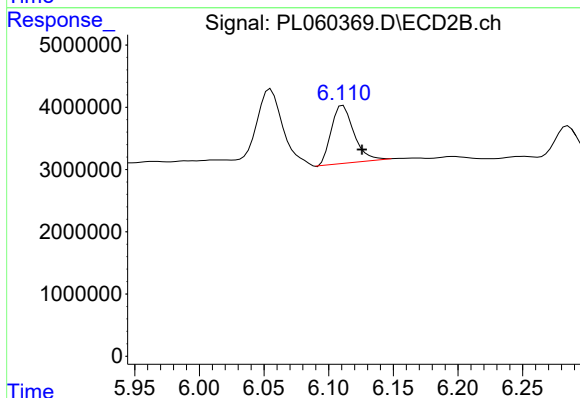


#10 gamma-Chlordane

R.T.: 6.111 min
Delta R.T.: -0.015 min
Response: 11264033
Conc: 3.98 ng/ml

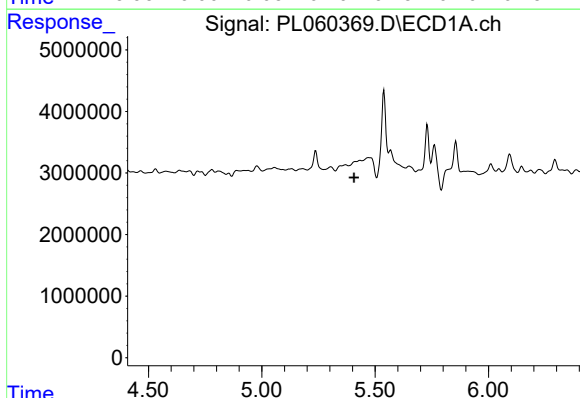


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

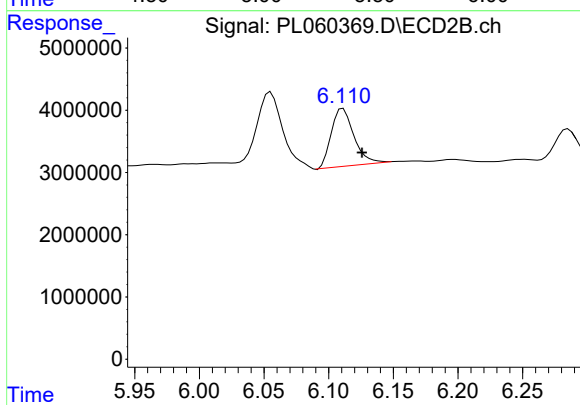

#25 Chlordane-3


R.T.: 6.111 min
Delta R.T.: -0.015 min
Response: 11264033
Conc: 30.61 ng/ml

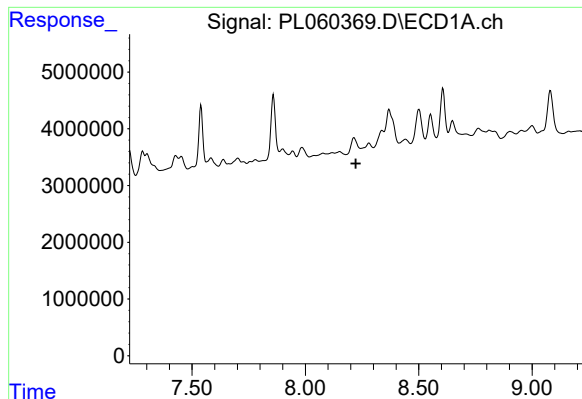

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.223 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-02-072820

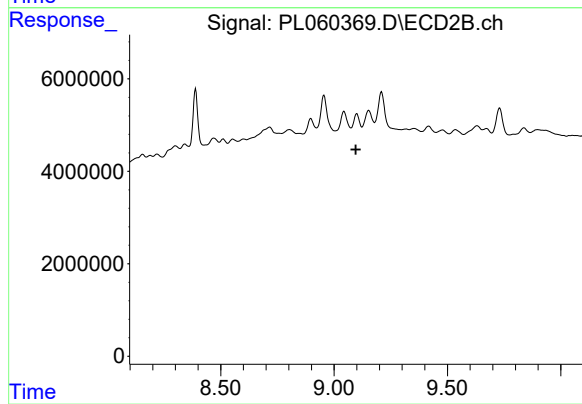

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.