

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
 Data File : PL060372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 10:46
 Operator : DD\AJ
 Sample : L3473-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 11:26:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.012	27468524	33953222	13.782	12.981
28)	SA Decachlor...	8.223	9.101	23012314	20532011	15.079	11.415
Target Compounds							
3)	MA gamma-BHC...	4.192	4.667f	12281298	13160272	4.839	3.654
9)	A Endosulfan I	5.540f	0.000	22327756	0	13.353	N.D. #
10)	B gamma-Chl...	0.000	6.111f	0	28854523	N.D.	10.205 #
13)	MA Dieldrin	5.763	0.000	8326078	0	4.704	N.D. #
25)	Chlordane-3	0.000	6.111f	0	28854523	N.D.	78.418 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
Data File : PL060372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 10:46
Operator : DD\AJ
Sample : L3473-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 11:26:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

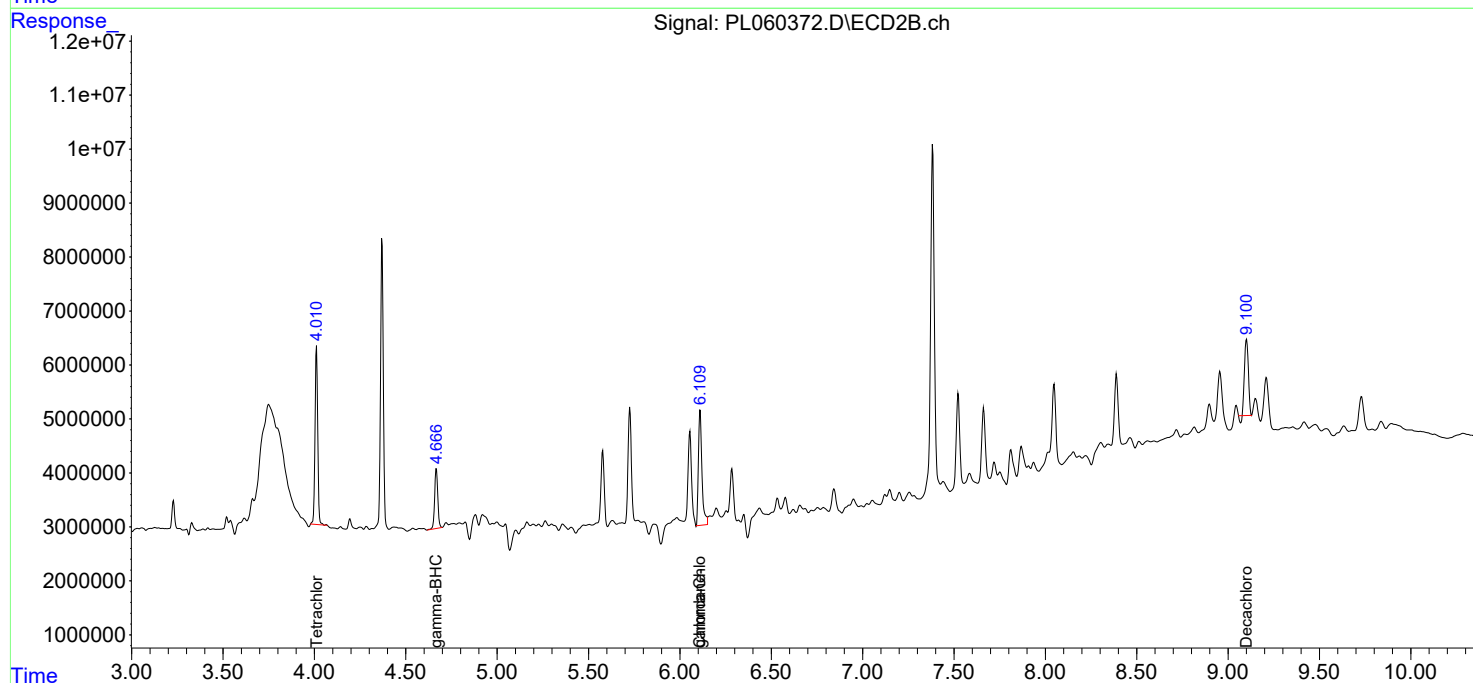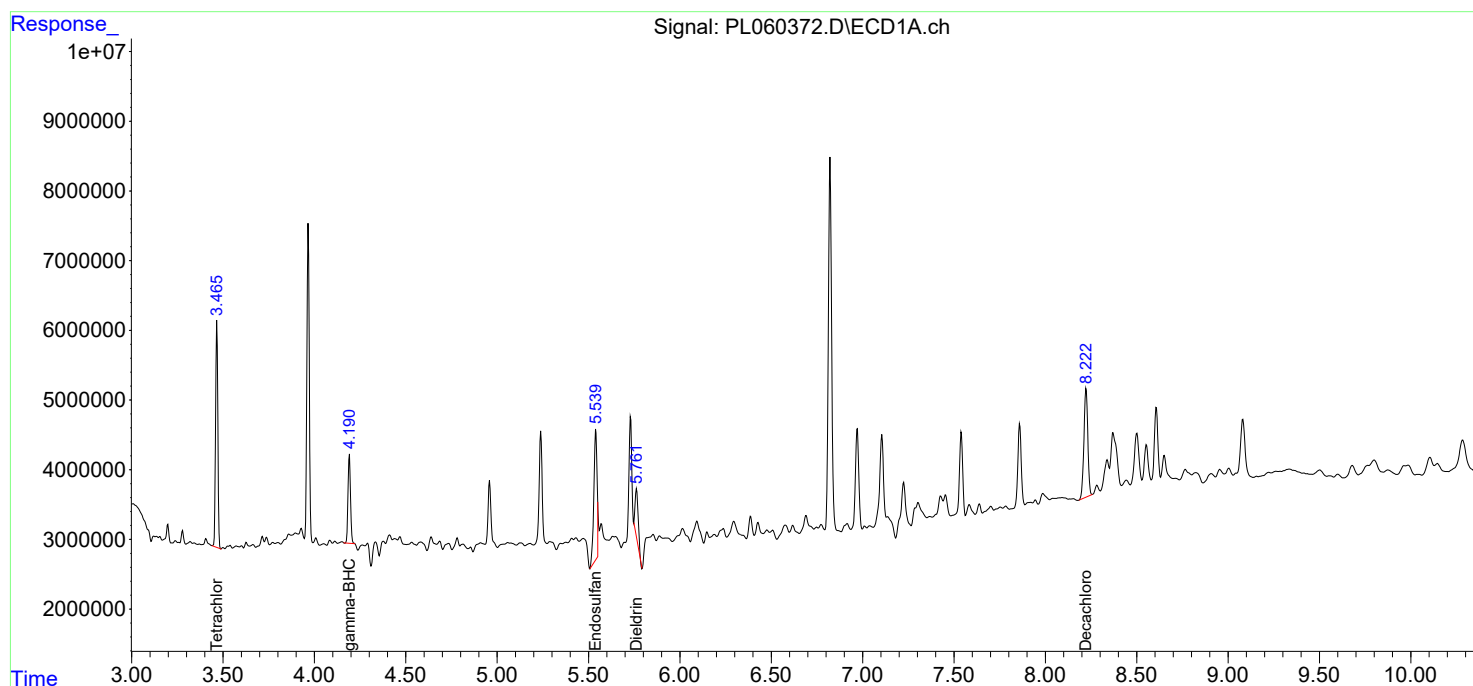


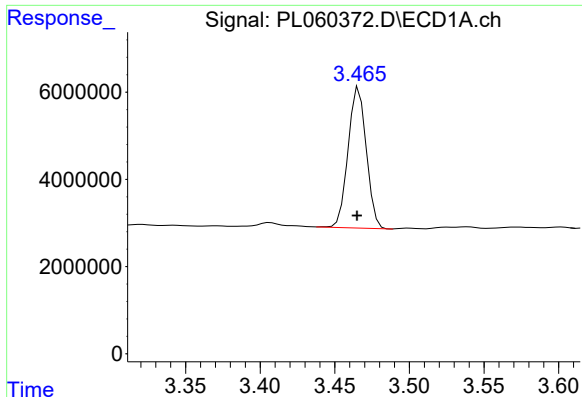

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.001 min
Response: 27468524
Conc: 13.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

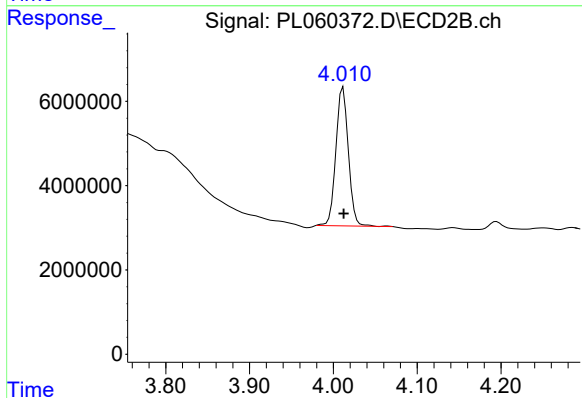


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 33953222
Conc: 12.98 ng/ml

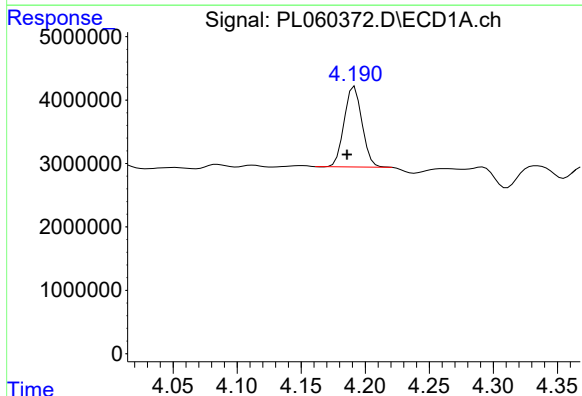


#3 gamma-BHC (Lindane)

R.T.: 4.192 min
Delta R.T.: 0.006 min
Response: 12281298
Conc: 4.84 ng/ml

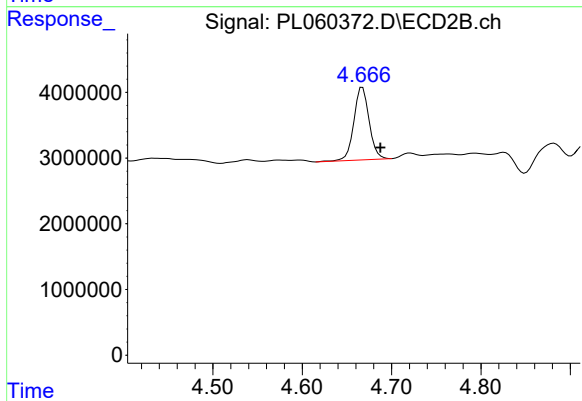

#3 gamma-BHC (Lindane)


R.T.: 4.667 min
Delta R.T.: -0.020 min
Response: 13160272
Conc: 3.65 ng/ml

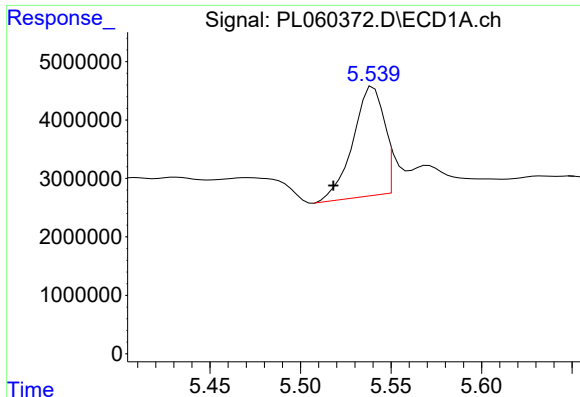

#9 Endosulfan I


R.T.: 5.540 min
Delta R.T.: 0.022 min
Response: 22327756
Conc: 13.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

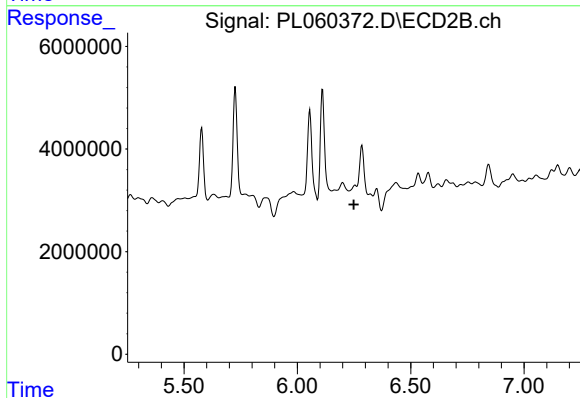


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

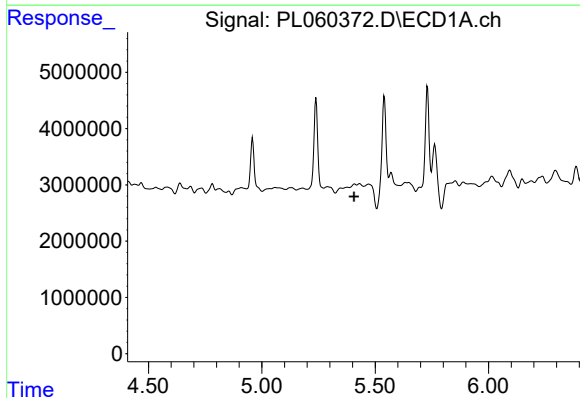


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

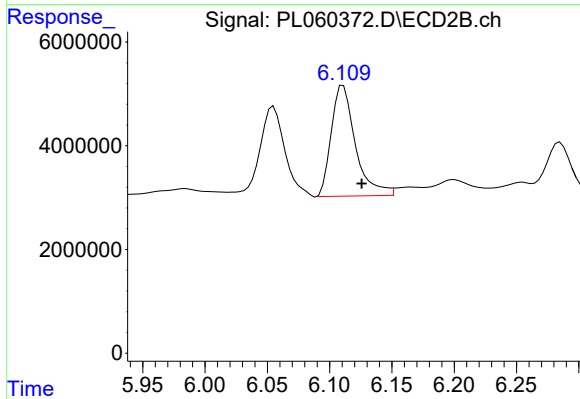

#10 gamma-Chlordane


R.T.: 6.111 min
Delta R.T.: -0.015 min
Response: 28854523
Conc: 10.20 ng/ml

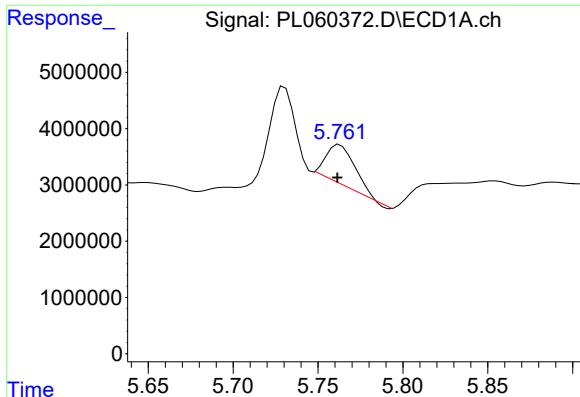

#13 Dieldrin


R.T.: 5.763 min
Delta R.T.: 0.001 min
Response: 8326078
Conc: 4.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

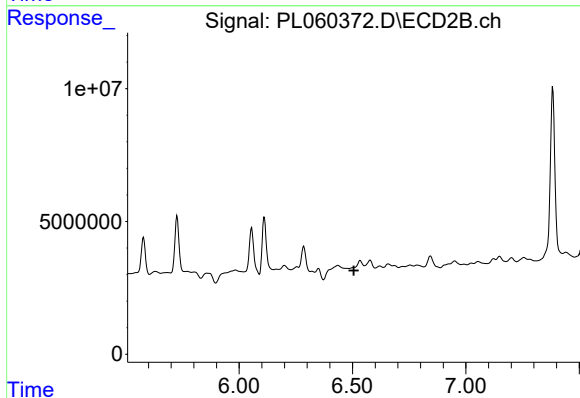


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.506 min
Response: 0
Conc: N.D.

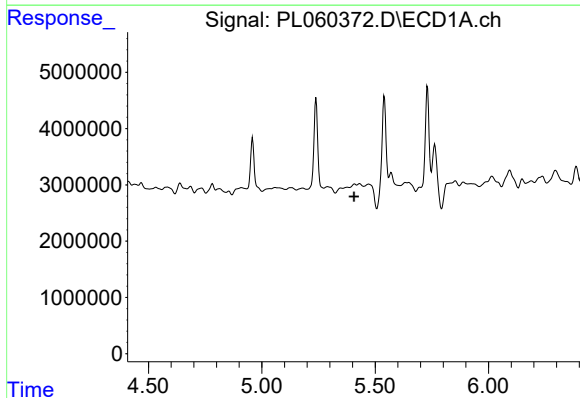


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

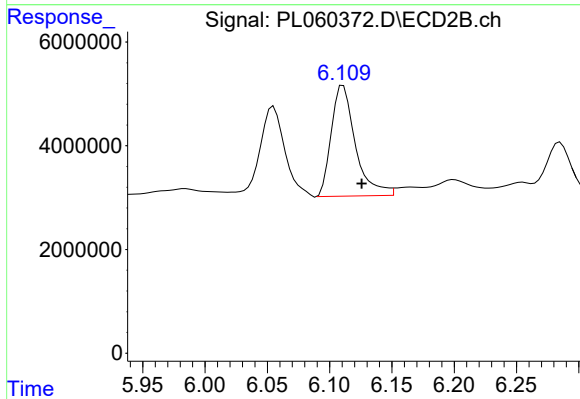

#25 Chlordane-3


R.T.: 6.111 min
Delta R.T.: -0.015 min
Response: 28854523
Conc: 78.42 ng/ml

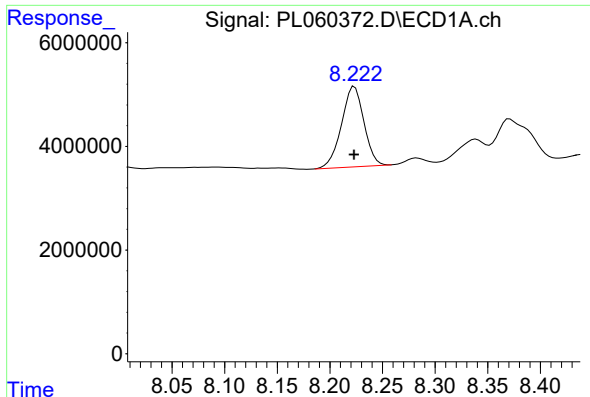

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 23012314
Conc: 15.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2-S

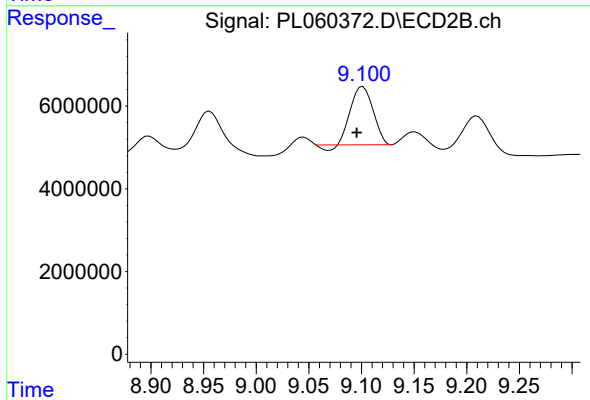

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.006 min
Response: 20532011
Conc: 11.42 ng/ml