

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
 Data File : PL060383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2020 13:21
 Operator : DD\AJ
 Sample : L3483-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-1

Manual Integrations
 APPROVED

Ankita
 7/31/2020 1:35:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:55:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.011	43814529	54381337	21.983	20.791
28)	SA Decachlor...	8.223	9.098	30029165	38004813	19.677	21.130m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073120\
Data File : PL060383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2020 13:21
Operator : DD\AJ
Sample : L3483-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
7/31/2020 1:35:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:55:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

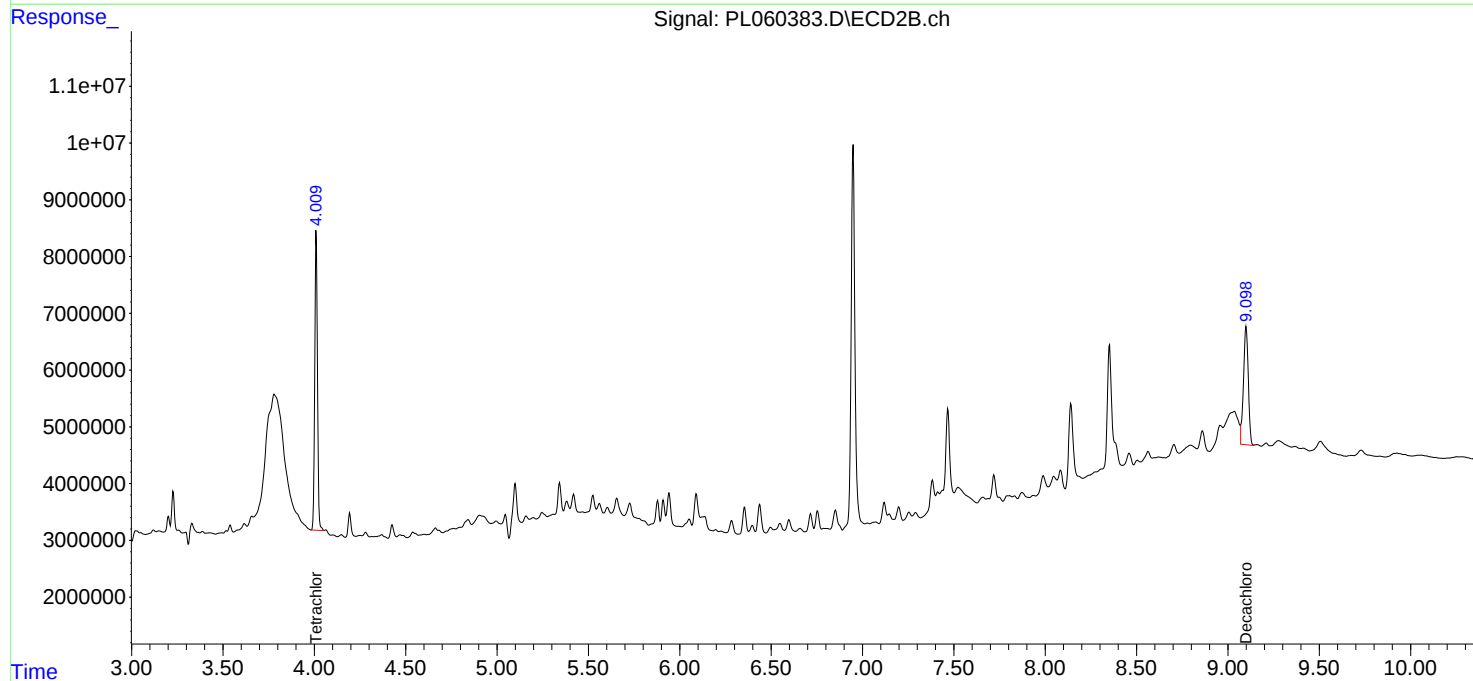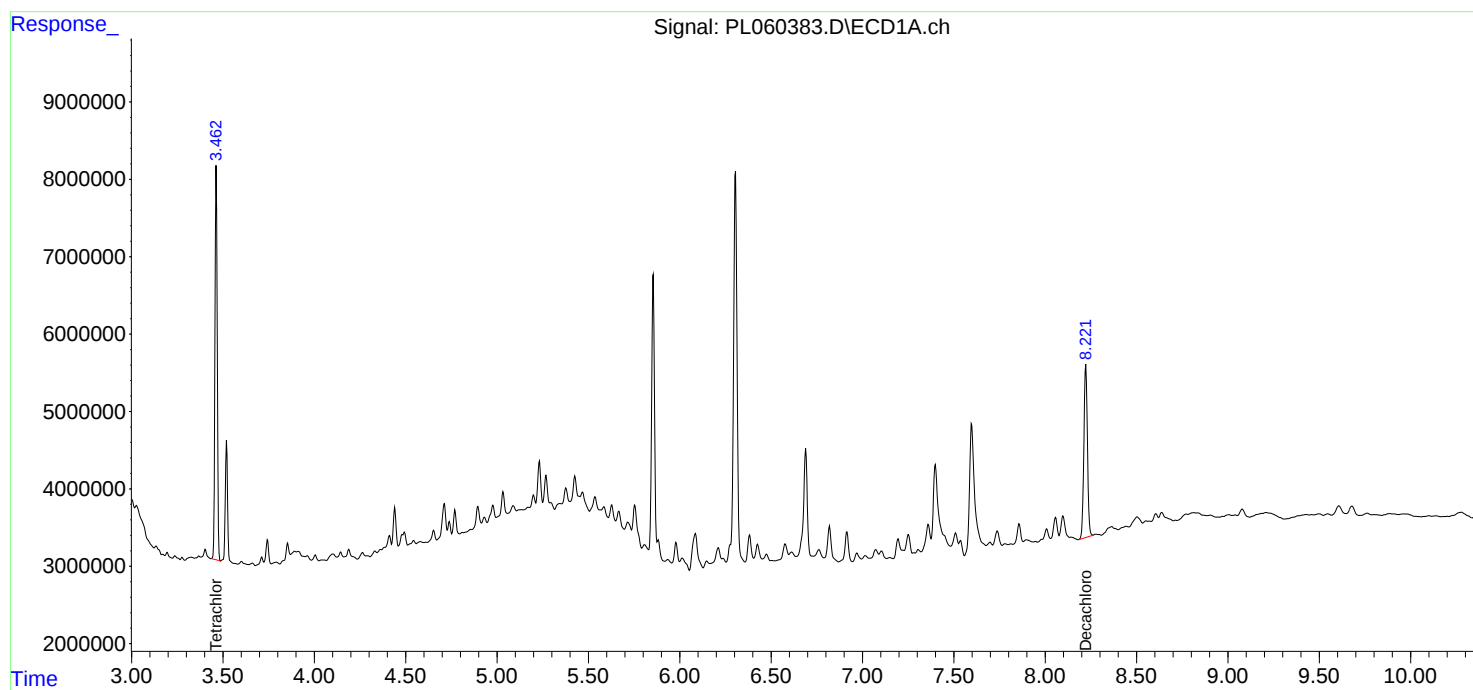

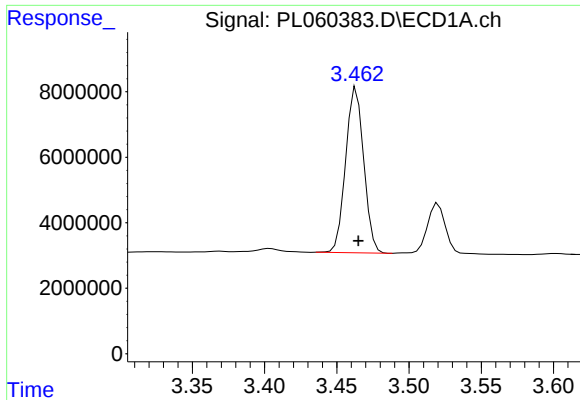


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.001 min
Response: 43814529
Conc: 21.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
7/31/2020 1:35:21 PM

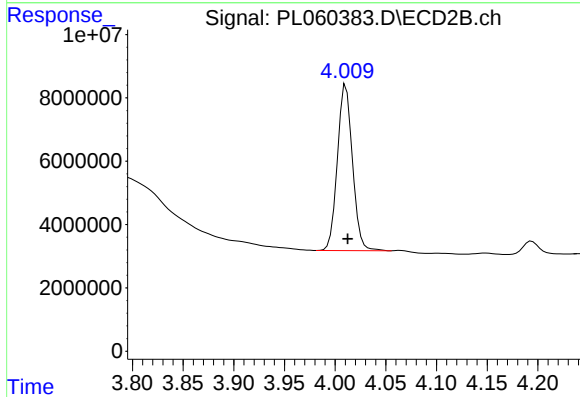


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 54381337
Conc: 20.79 ng/ml

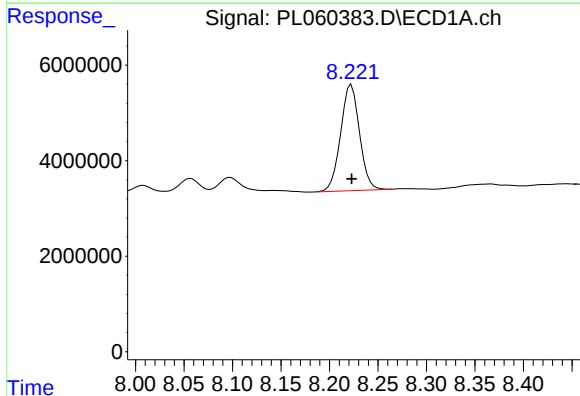

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 30029165
Conc: 19.68 ng/ml

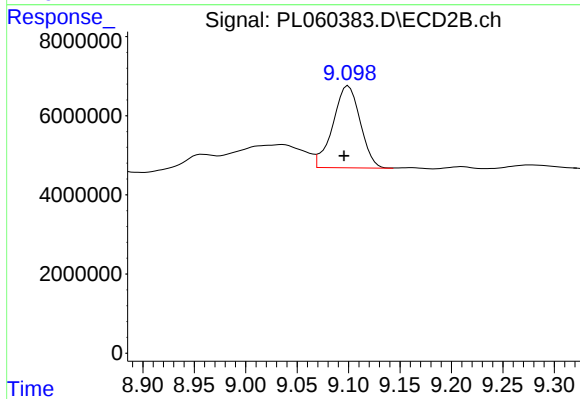

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.003 min
Response: 38004813
Conc: 21.13 ng/ml m