

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073124\
 Data File : PL090714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2024 17:34
 Operator : AR\AJ
 Sample : P3396-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-CF03-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/01/2024
 Supervised By : Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 01:37:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 15 14:16:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.787	43974978	38201185	21.119m	22.699
28) SA Decachlor...	9.057	7.930	26535765	28925026	19.969m	19.838

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073124\
Data File : PL090714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2024 17:34
Operator : AR\AJ
Sample : P3396-06
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P001-CF03-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/01/2024
Supervised By : Ankita Jodhani 08/01/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 01:37:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071524.M
Quant Title : GC Extractables
QLast Update : Mon Jul 15 14:16:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

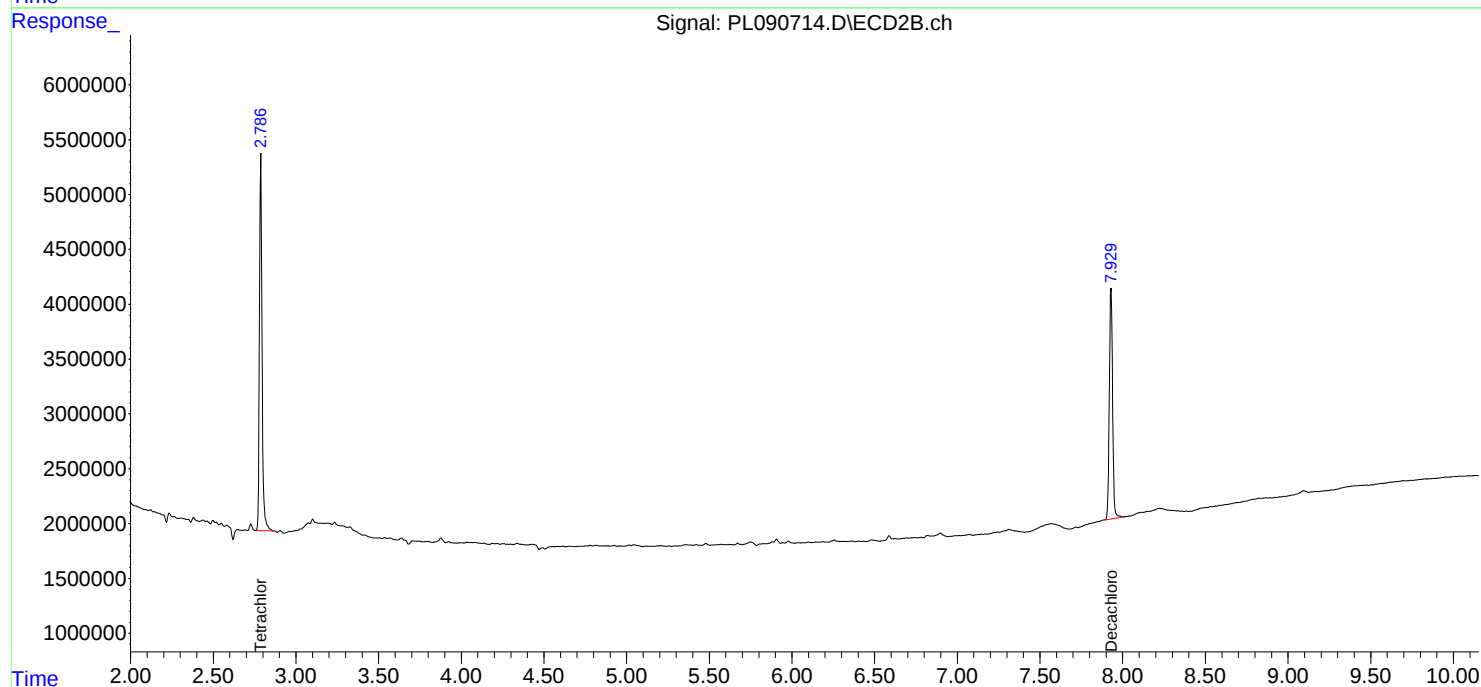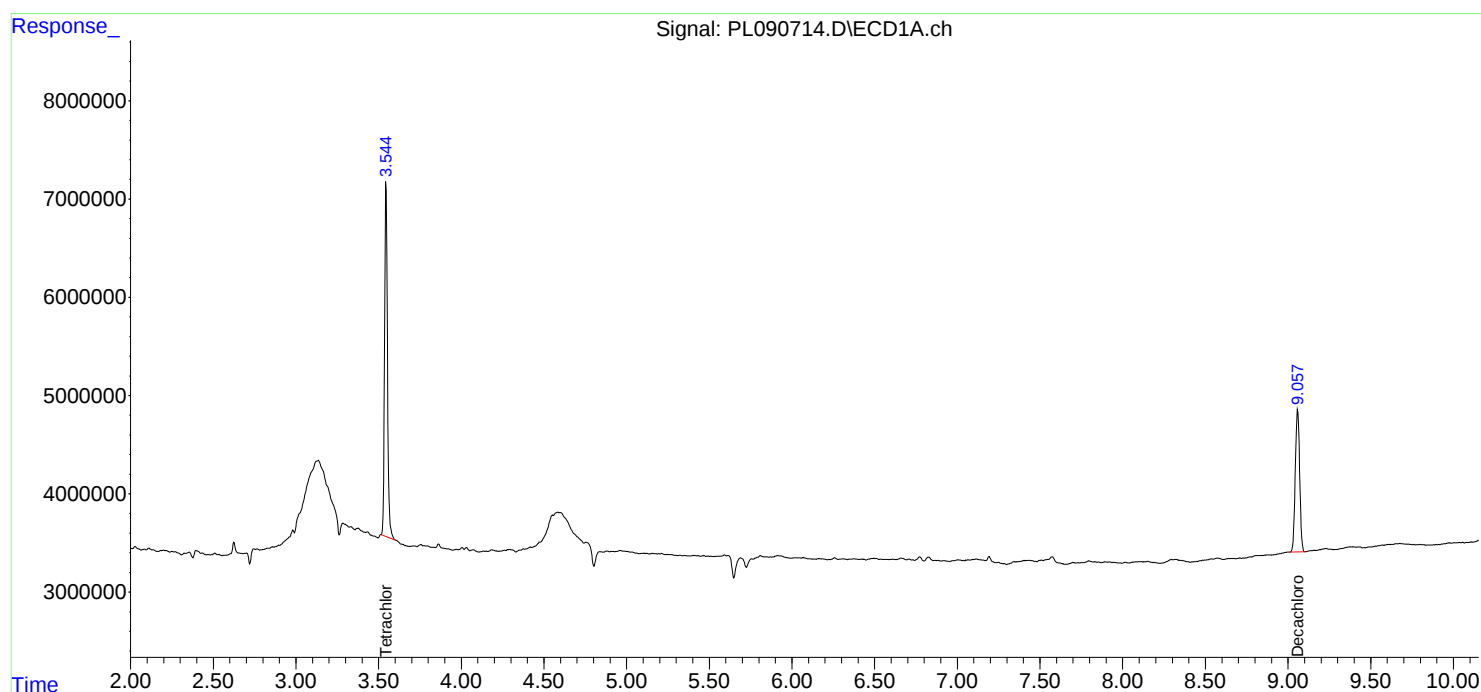

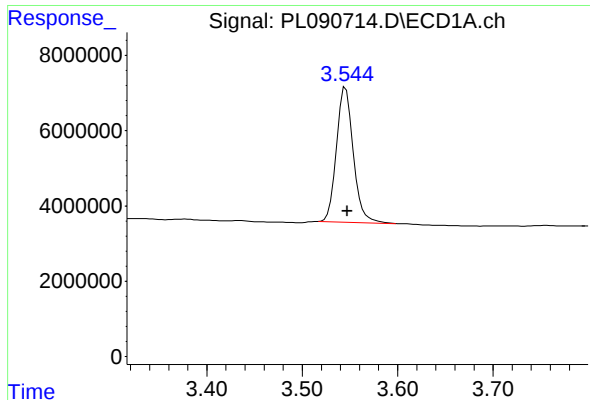


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.003 min
Response: 43974978
Conc: 21.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-CF03-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/01/2024
Supervised By :Ankita Jodhani 08/01/2024

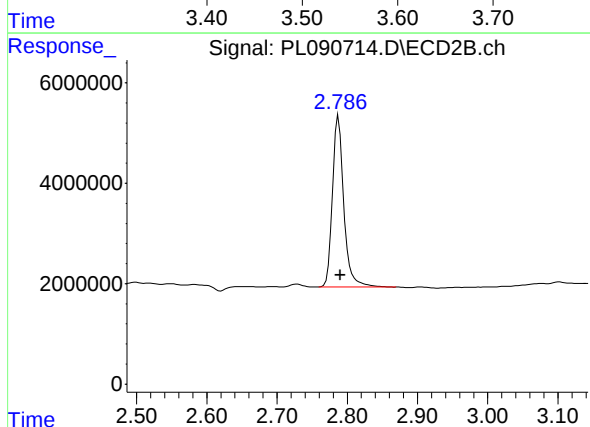


#1 Tetrachloro-m-xylene

R.T.: 2.787 min
Delta R.T.: -0.002 min
Response: 38201185
Conc: 22.70 ng/ml

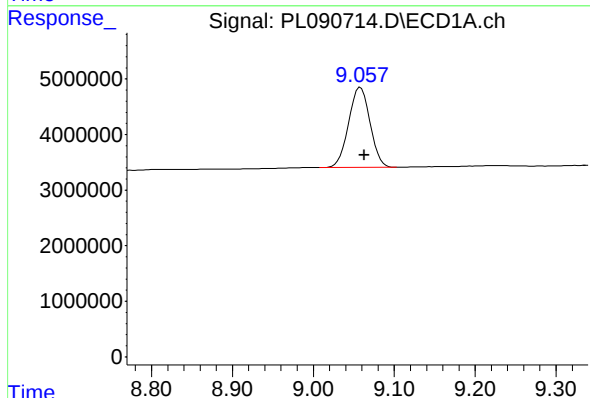

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.006 min
Response: 26535765
Conc: 19.97 ng/ml m

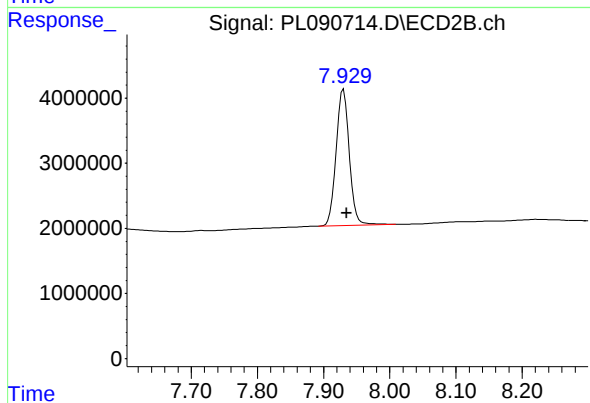

#28 Decachlorobiphenyl

R.T.: 7.930 min
Delta R.T.: -0.005 min
Response: 28925026
Conc: 19.84 ng/ml