

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073125\
 Data File : PL096654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 09:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 02:47:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.559f	0.000	4004812	0	1.259	N.D. #
Target Compounds						
8) B Heptachlo...	5.655	0.000	61734862	0	16.008	N.D. #
13) MA Dieldrin	0.000	5.429	0 87004949		N.D.	14.730 #
14) MA Endrin	0.000	5.716	0 132.0E6		N.D.	24.419 #
16) A 4,4'-DDD	6.671	0.000	19232701	0	7.607	N.D. #
24) Chlordane-2	0.000	4.409	0 12543608		N.D.	51.707 #
27) Chlordane-5	0.000	6.040f	0 33915546		N.D.	132.944 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073125\
Data File : PL096654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 09:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 02:47:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

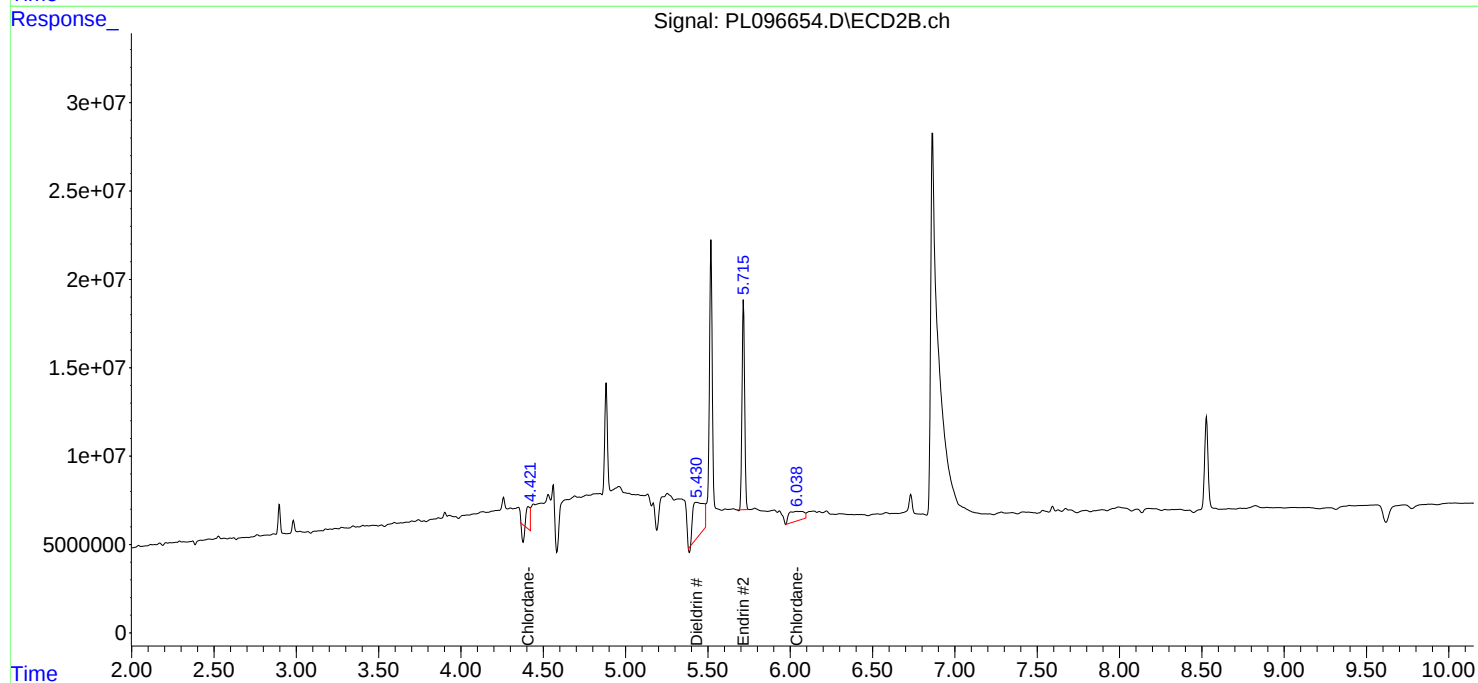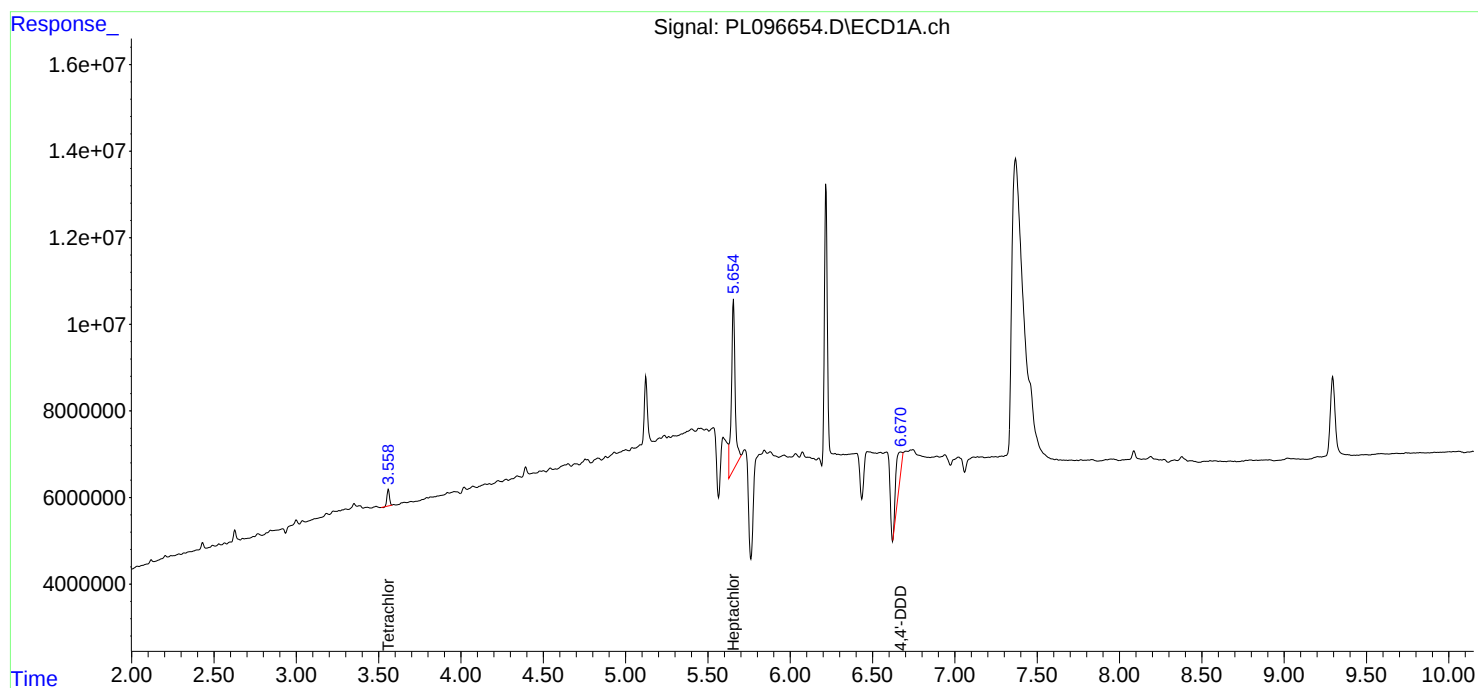


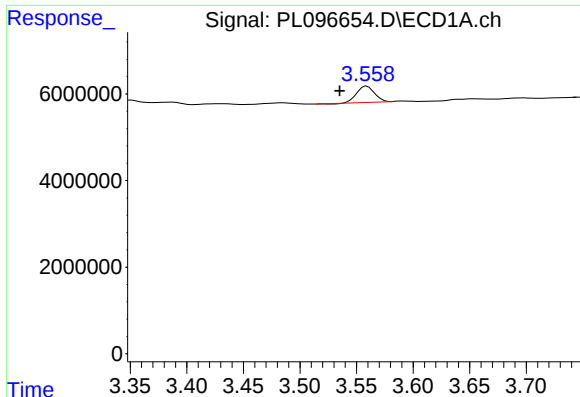

#1 Tetrachloro-m-xylene


R.T.: 3.559 min
Delta R.T.: 0.024 min
Response: 4004812
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

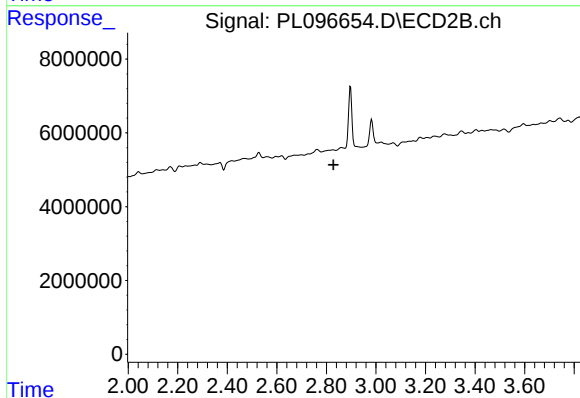


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.828 min
Response: 0
Conc: N.D.

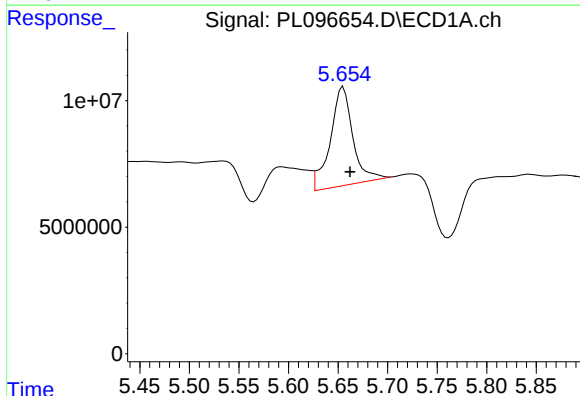


#8 Heptachlor epoxide

R.T.: 5.655 min
Delta R.T.: -0.007 min
Response: 61734862
Conc: 16.01 ng/ml

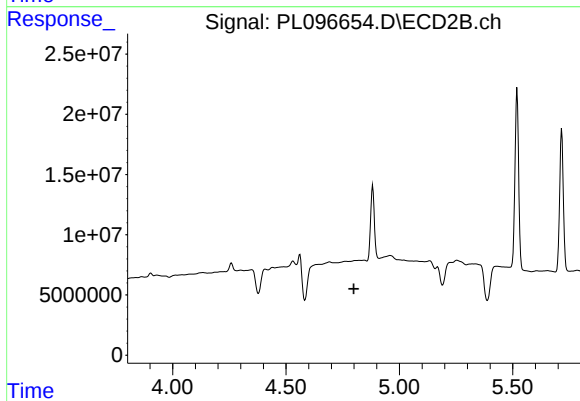

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.799 min
Response: 0
Conc: N.D.

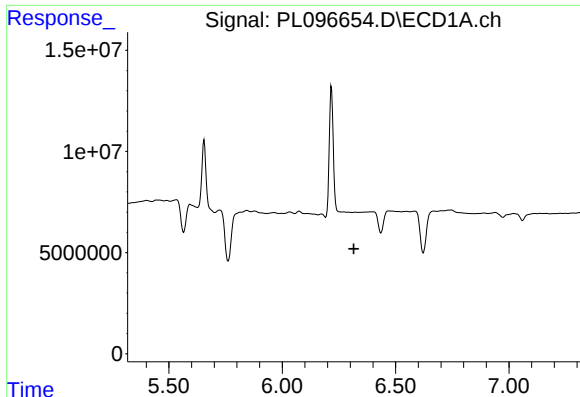

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

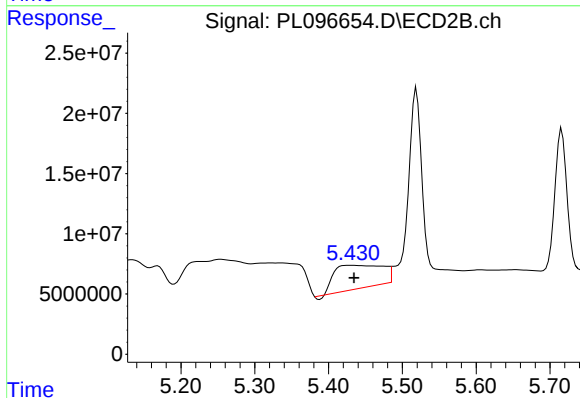


#13 Dieldrin

R.T.: 5.429 min
Delta R.T.: -0.005 min
Response: 87004949
Conc: 14.73 ng/ml

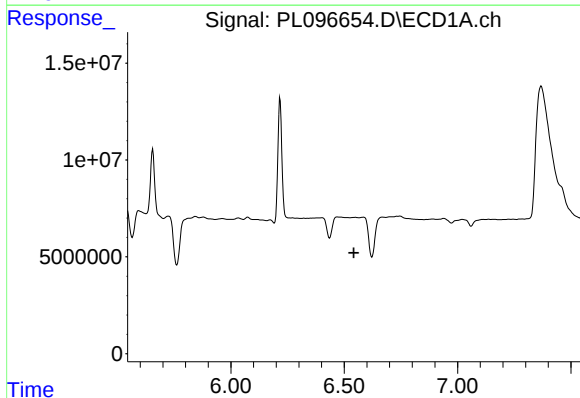


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

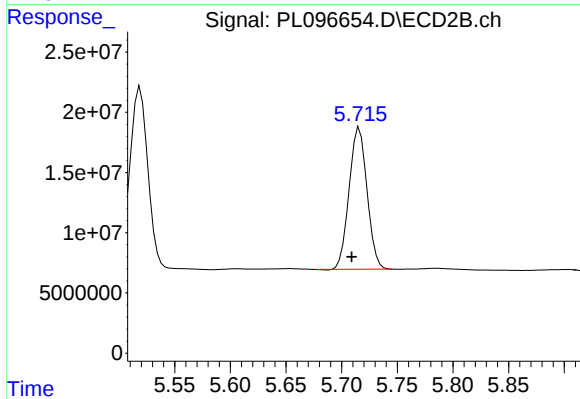

#14 Endrin


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 132010955
Conc: 24.42 ng/ml

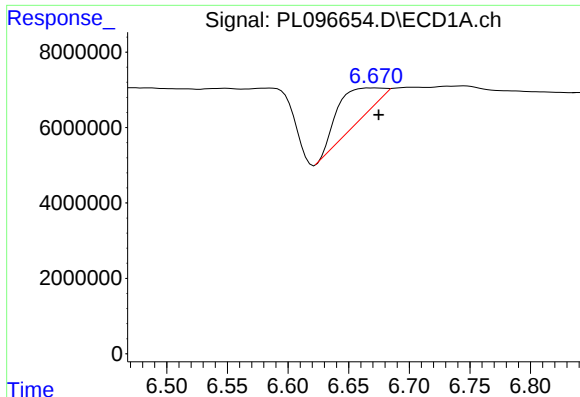

#16 4,4'-DDD


R.T.: 6.671 min
Delta R.T.: -0.004 min
Response: 19232701
Conc: 7.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

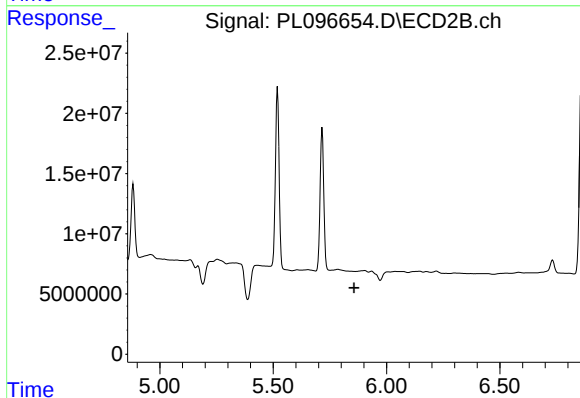


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.856 min
Response: 0
Conc: N.D.

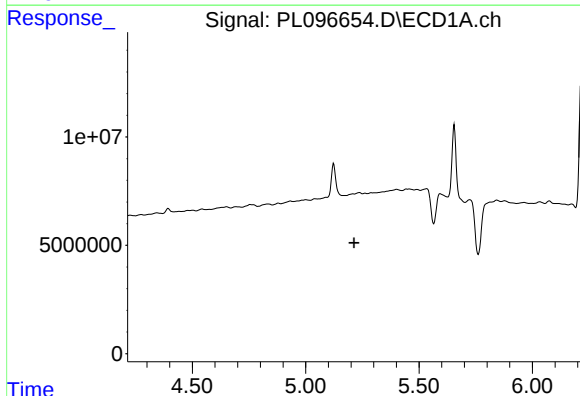

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

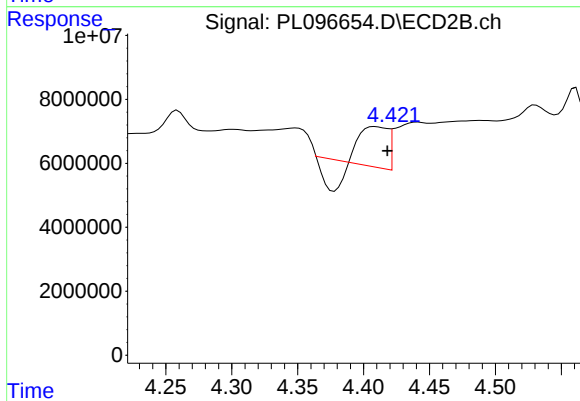

#24 Chlordane-2

R.T.: 4.409 min
Delta R.T.: -0.009 min
Response: 12543608
Conc: 51.71 ng/ml

