

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073125\
 Data File : PL096677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 17:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 02:50:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.828	67895620	101.1E6	21.346	21.165
28)	SA Decachlor...	9.013	7.991	56755646	95291248	23.800	21.965
Target Compounds							
8)	B Heptachlo...	5.653	0.000	34380141	0	8.915	N.D. #
13)	MA Dieldrin	0.000	5.429	0	28704102	N.D.	4.860 #
14)	MA Endrin	0.000	5.717	0	124.0E6	N.D.	22.936 #
22)	Mirex	8.083	0.000	5319733	0	2.146	N.D. #
24)	Chlordane-2	0.000	4.410	0	1867997	N.D.	7.700 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073125\
Data File : PL096677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 17:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 02:50:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

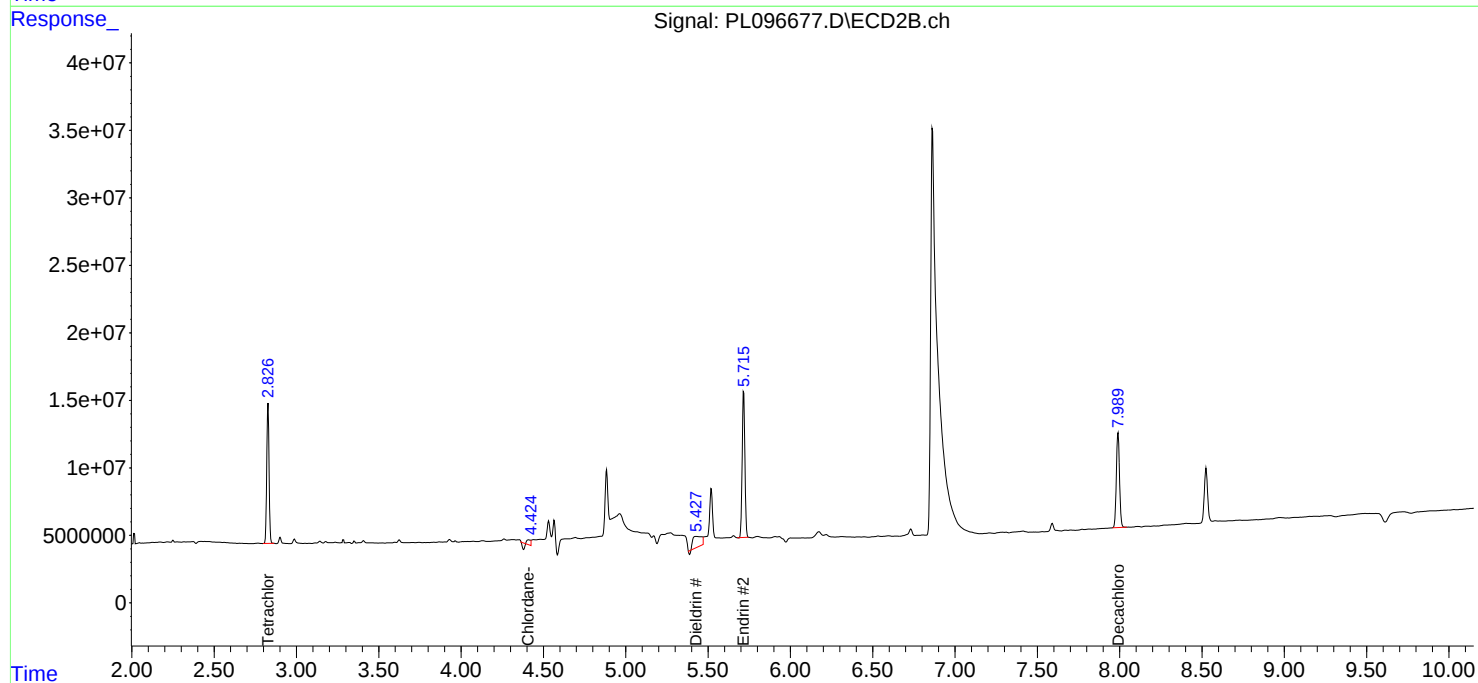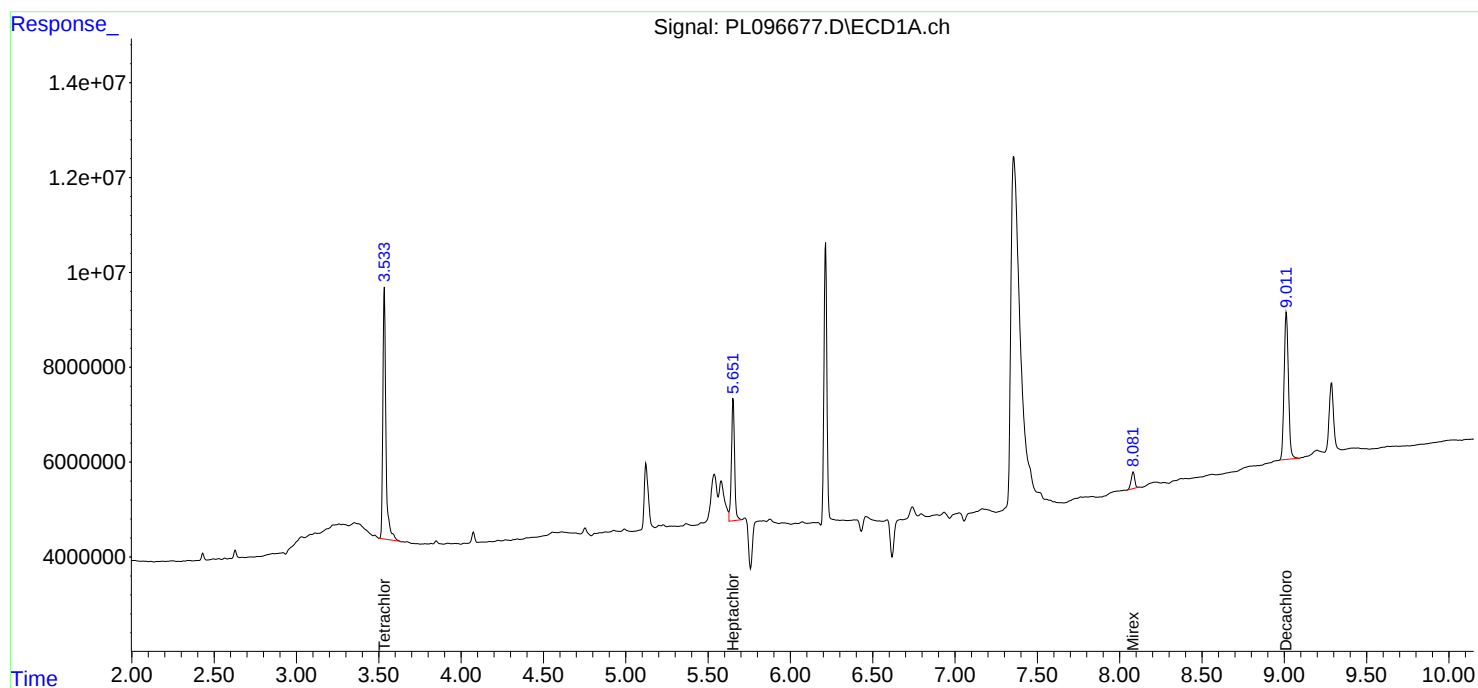


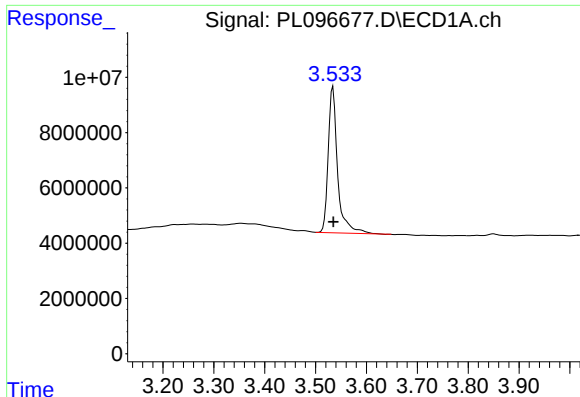

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 67895620
Conc: 21.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

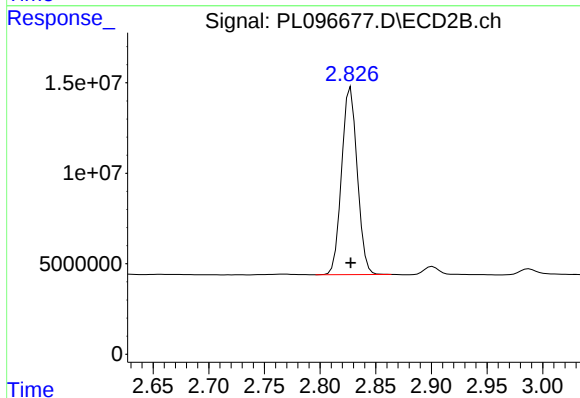


#1 Tetrachloro-m-xylene

R.T.: 2.828 min
Delta R.T.: 0.000 min
Response: 101120173
Conc: 21.16 ng/ml

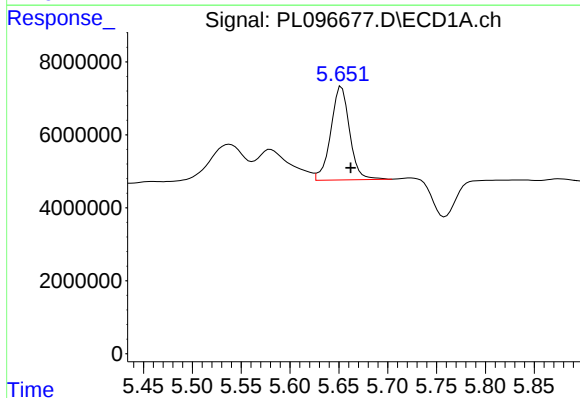


#8 Heptachlor epoxide

R.T.: 5.653 min
Delta R.T.: -0.009 min
Response: 34380141
Conc: 8.91 ng/ml

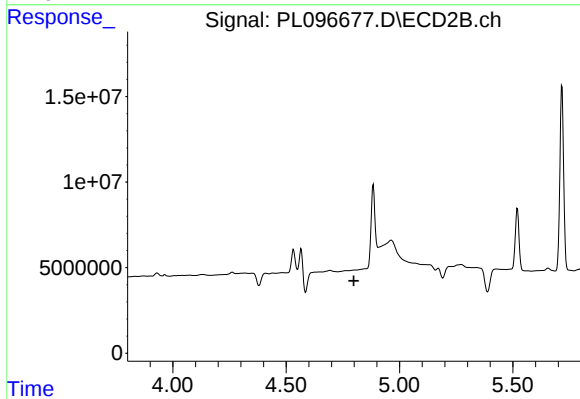

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

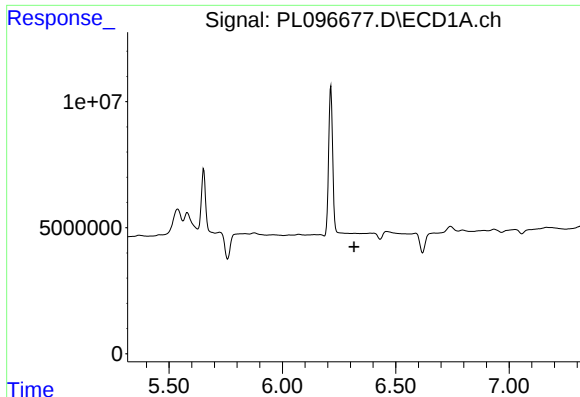

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

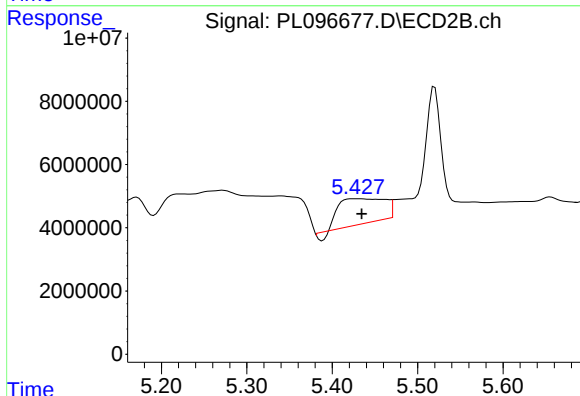


#13 Dieldrin

R.T.: 5.429 min
Delta R.T.: -0.005 min
Response: 28704102
Conc: 4.86 ng/ml

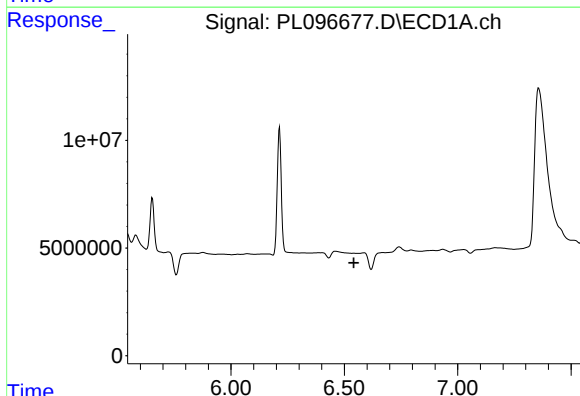


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

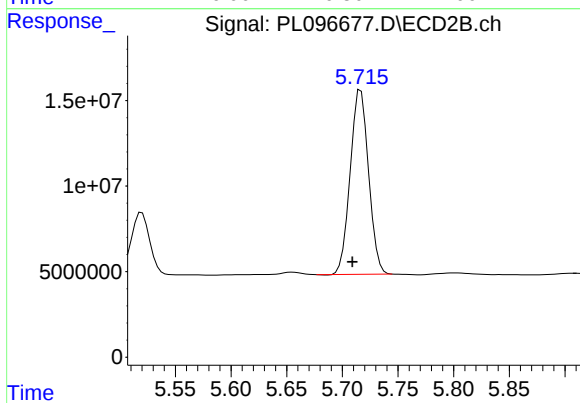

#14 Endrin


R.T.: 5.717 min
Delta R.T.: 0.008 min
Response: 123992124
Conc: 22.94 ng/ml

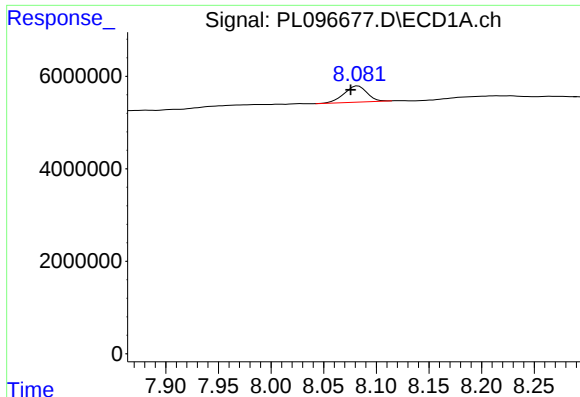

#22 Mirex


R.T.: 8.083 min
Delta R.T.: 0.007 min
Response: 5319733
Conc: 2.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

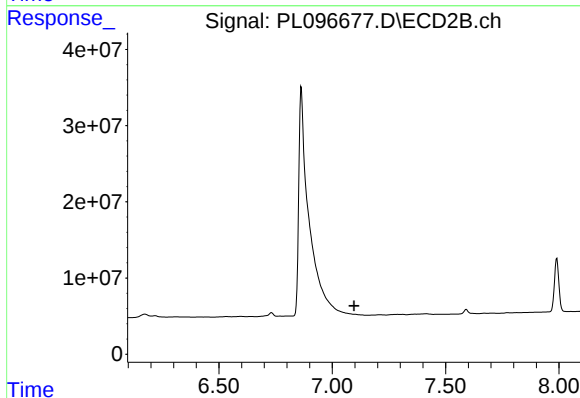


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.097 min
Response: 0
Conc: N.D.

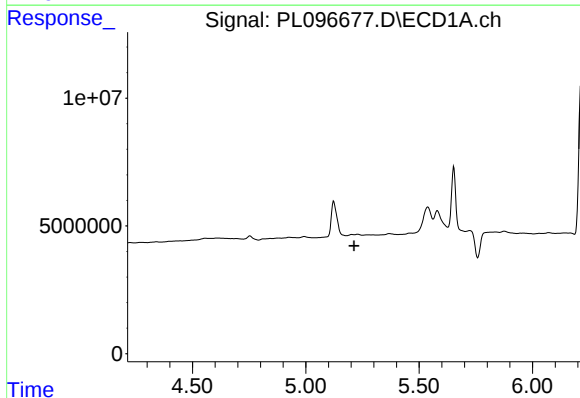


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

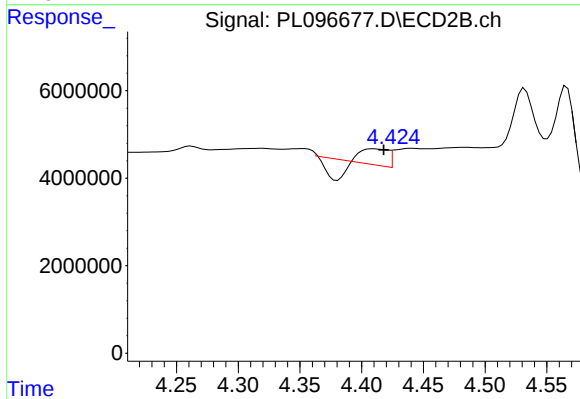

#24 Chlordane-2


R.T.: 4.410 min
Delta R.T.: -0.008 min
Response: 1867997
Conc: 7.70 ng/ml

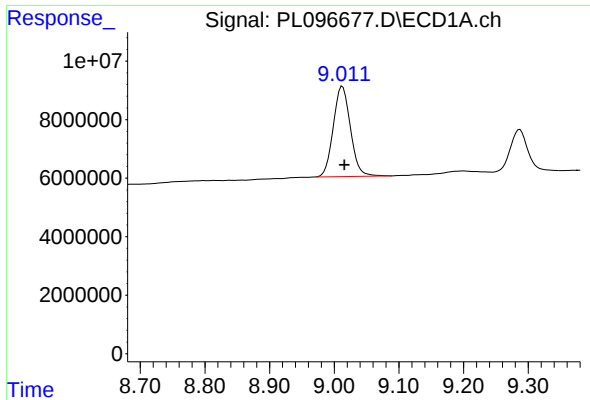

#28 Decachlorobiphenyl

R.T.: 9.013 min
Delta R.T.: -0.003 min
Response: 56755646
Conc: 23.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

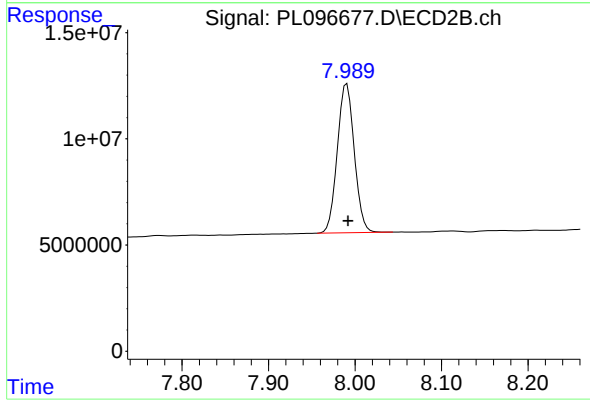

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.001 min
Response: 95291248
Conc: 21.97 ng/ml