

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
 Data File : PL038748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 06:22
 Operator : AJ\SJ
 Sample : J4200-05 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CA-DRUM-2-BASELINEWATER

Manual Integrations
 APPROVED

Sohil
 8/2/2018 5:38:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 07:52:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	3.928	28382094	10922241	3.812m	4.161m
28) SA Decachlor...	7.991	8.934	15128963	6814762	1.994m	2.788m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
Data File : PL038748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 06:22
Operator : AJ\SJ
Sample : J4200-05 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CA-DRUM-2-BASELINEWATER


Manual Integrations
APPROVED

Sohil
8/2/2018 5:38:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:52:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

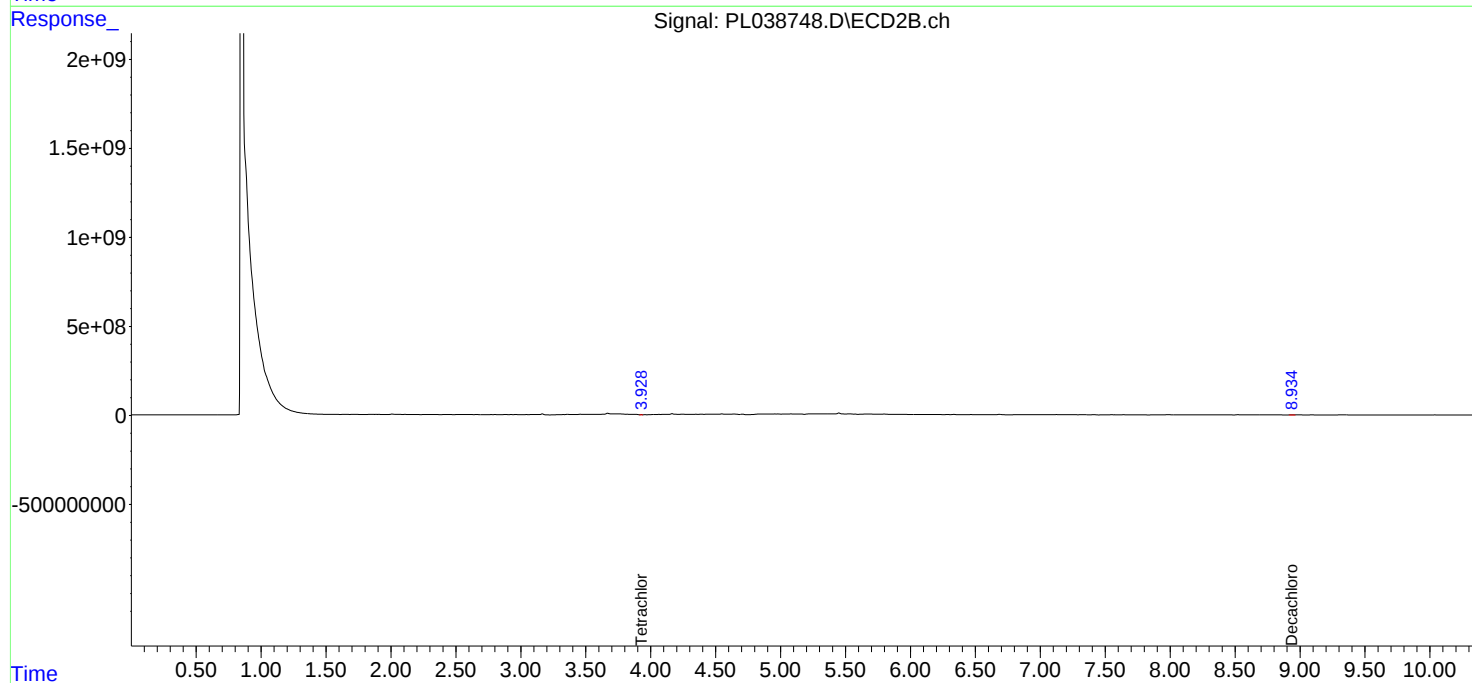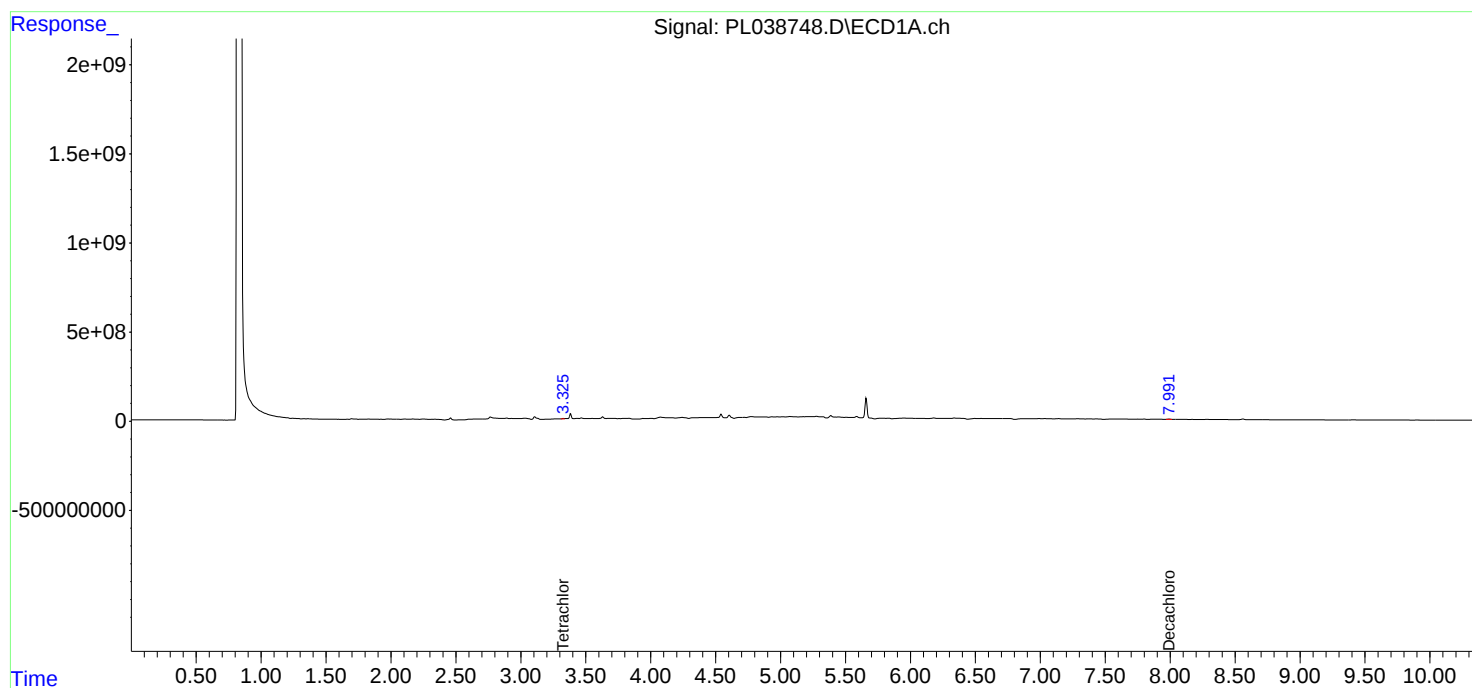

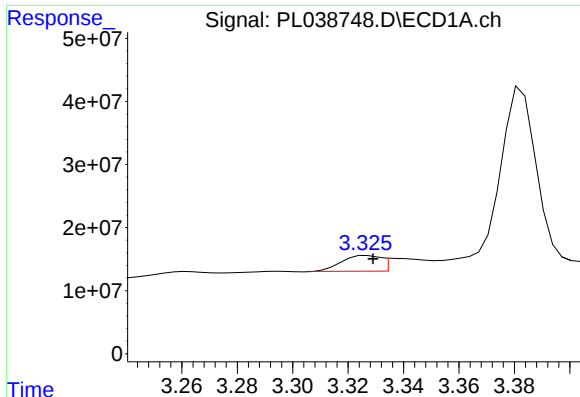


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 28382094
Conc: 3.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CA-DRUM-2-BASELINEWATER


Manual Integrations
APPROVED

Sohil
8/2/2018 5:38:46 PM

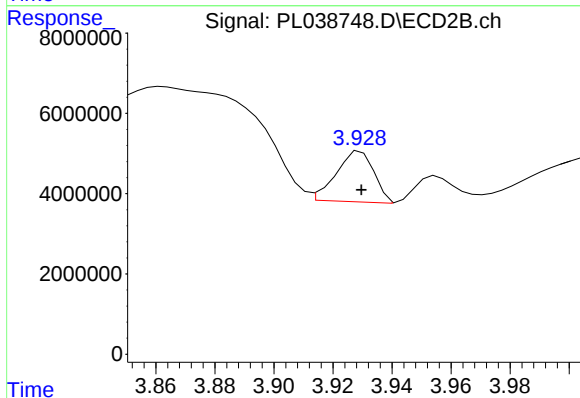


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 10922241
Conc: 4.16 ng/ml m

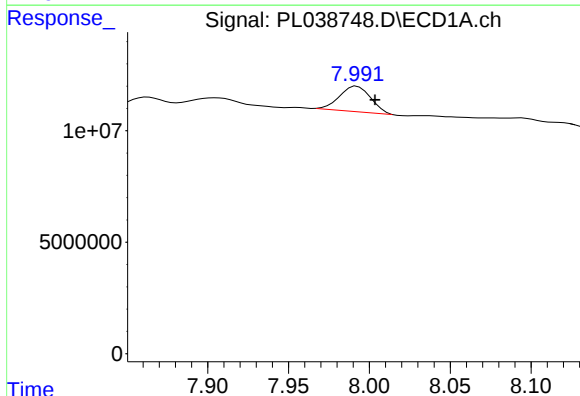

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.013 min
Response: 15128963
Conc: 1.99 ng/ml m

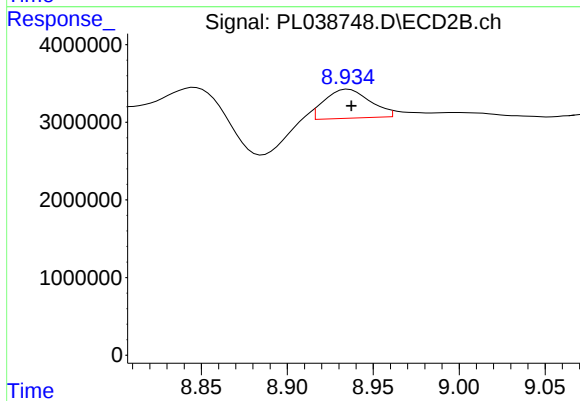

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.004 min
Response: 6814762
Conc: 2.79 ng/ml m