

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
 Data File : PL038759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 08:58
 Operator : AJ\SJ
 Sample : J4231-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2018-NYSEG-CLARK-AREA-14-4

Manual Integrations
 APPROVED

Sohil
 8/2/2018 5:38:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 11:37:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	3.928	161.2E6	62217355	21.652	23.702
28) SA Decachlor...	7.992	8.934	90924613	41844967	11.986	17.118 #
Target Compounds						
16) A 4,4'-DDD	5.945	6.721	26897529	9461636	3.667m	4.420

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
Data File : PL038759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 08:58
Operator : AJ\SJ
Sample : J4231-07
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-4


Manual Integrations
APPROVED

Sohil
8/2/2018 5:38:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 11:37:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

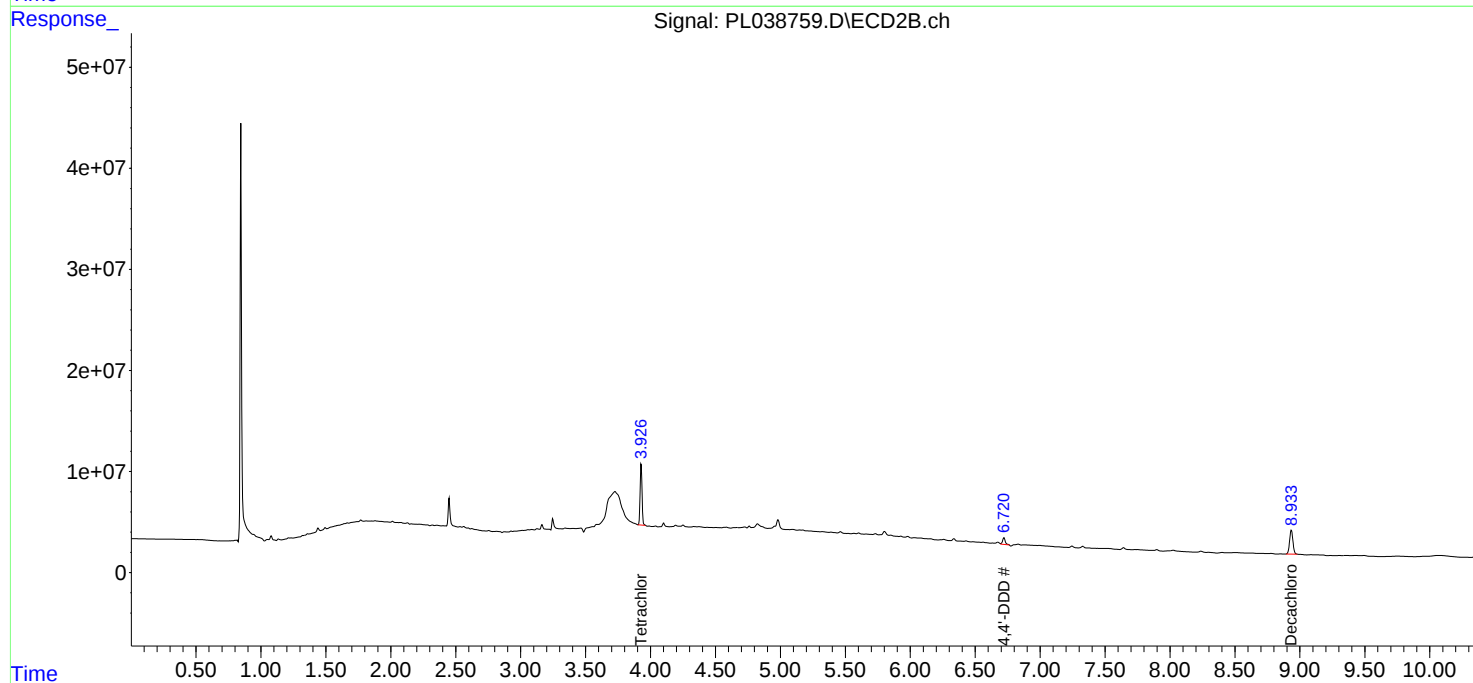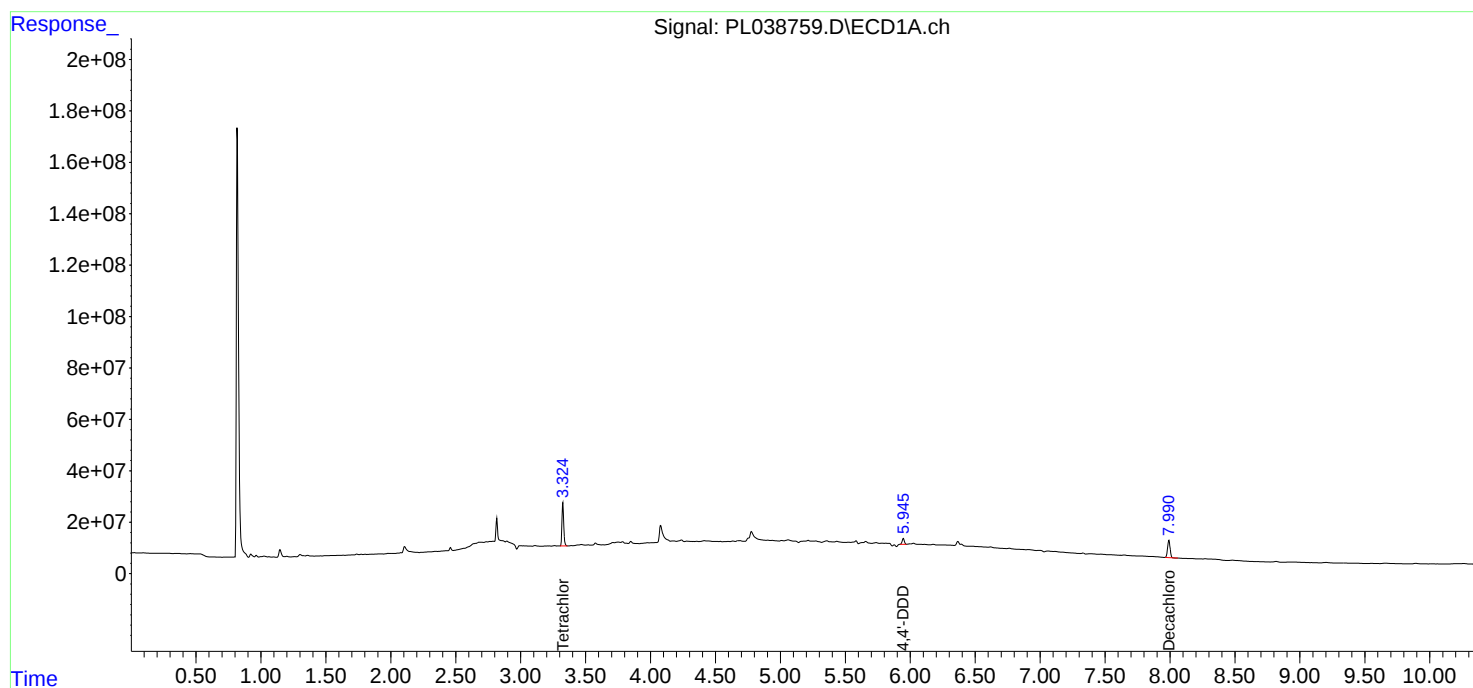

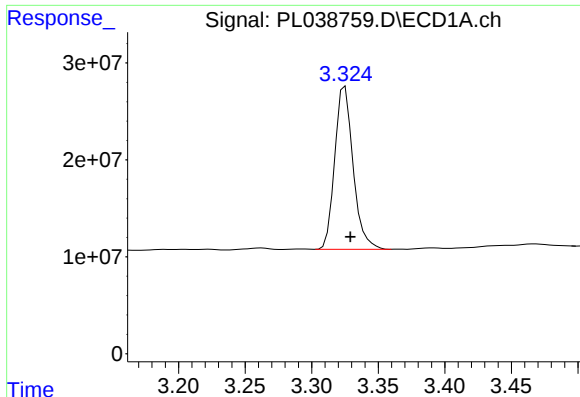


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 161226690
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-4


Manual Integrations
APPROVED

Sohil
8/2/2018 5:38:57 PM

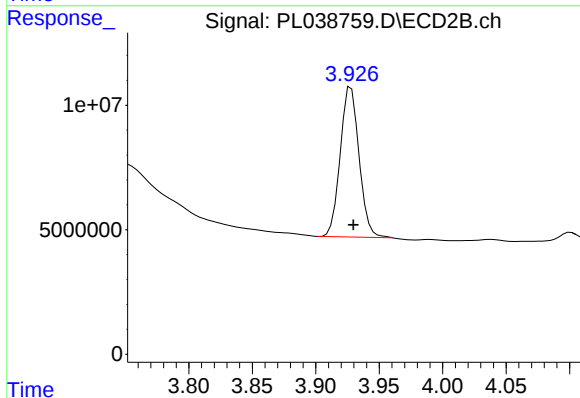


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 62217355
Conc: 23.70 ng/ml

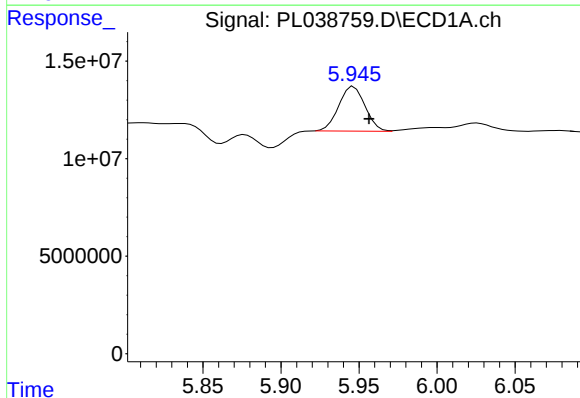


#16 4,4'-DDD

R.T.: 5.945 min
Delta R.T.: -0.011 min
Response: 26897529
Conc: 3.67 ng/ml m

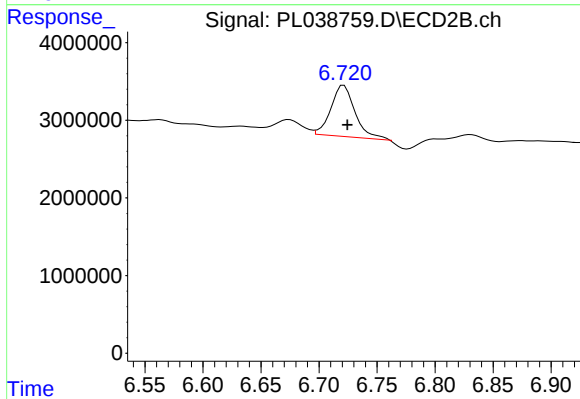

#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: -0.003 min
Response: 9461636
Conc: 4.42 ng/ml

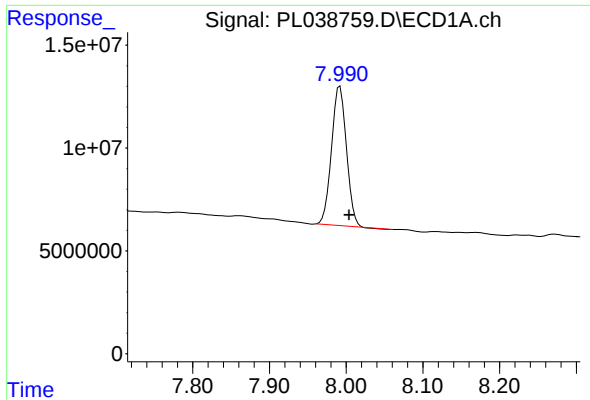


#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.012 min
Response: 90924613
Conc: 11.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
2018-NYSEG-CLARK-AREA-14-4

Manual Integrations
APPROVED

Sohil
8/2/2018 5:38:57 PM

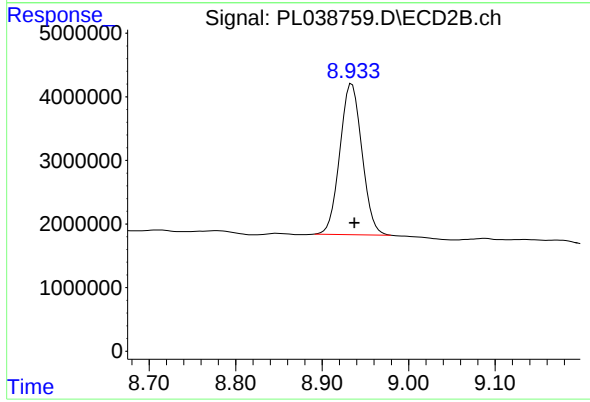

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 41844967
Conc: 17.12 ng/ml