

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
 Data File : PL038795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 18:47
 Operator : AJ\SJ
 Sample : J4257-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-001-C

Manual Integrations
 APPROVED

Sohil
 8/2/2018 5:39:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:09:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.928	162.2E6	64528136	21.788	24.583
28)	SA Decachlor...	7.992	8.936	123.7E6	48432997	16.310	19.813
Target Compounds							
17)	MA 4,4'-DDT	6.180	7.019	6269439	1470835	0.844	0.690m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
Data File : PL038795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 18:47
Operator : AJ\SJ
Sample : J4257-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-C


Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:09:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

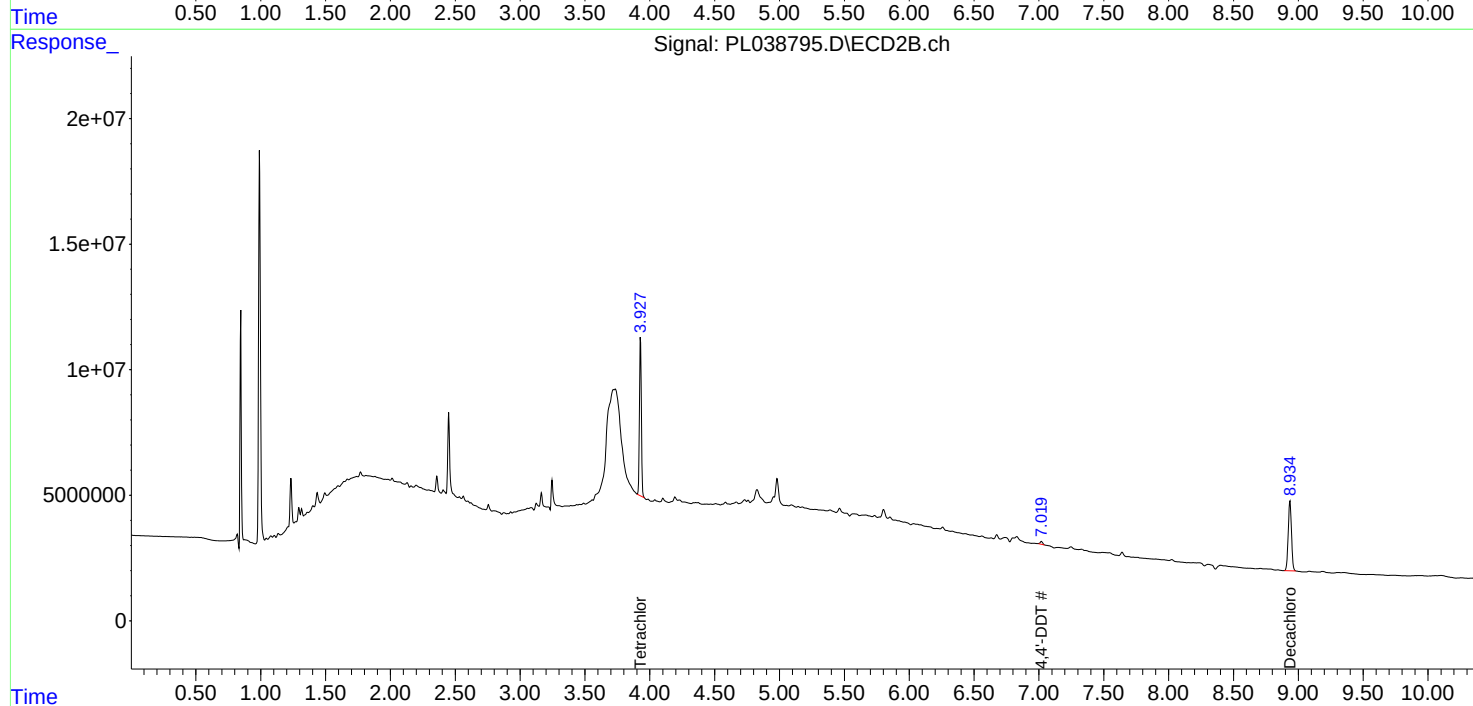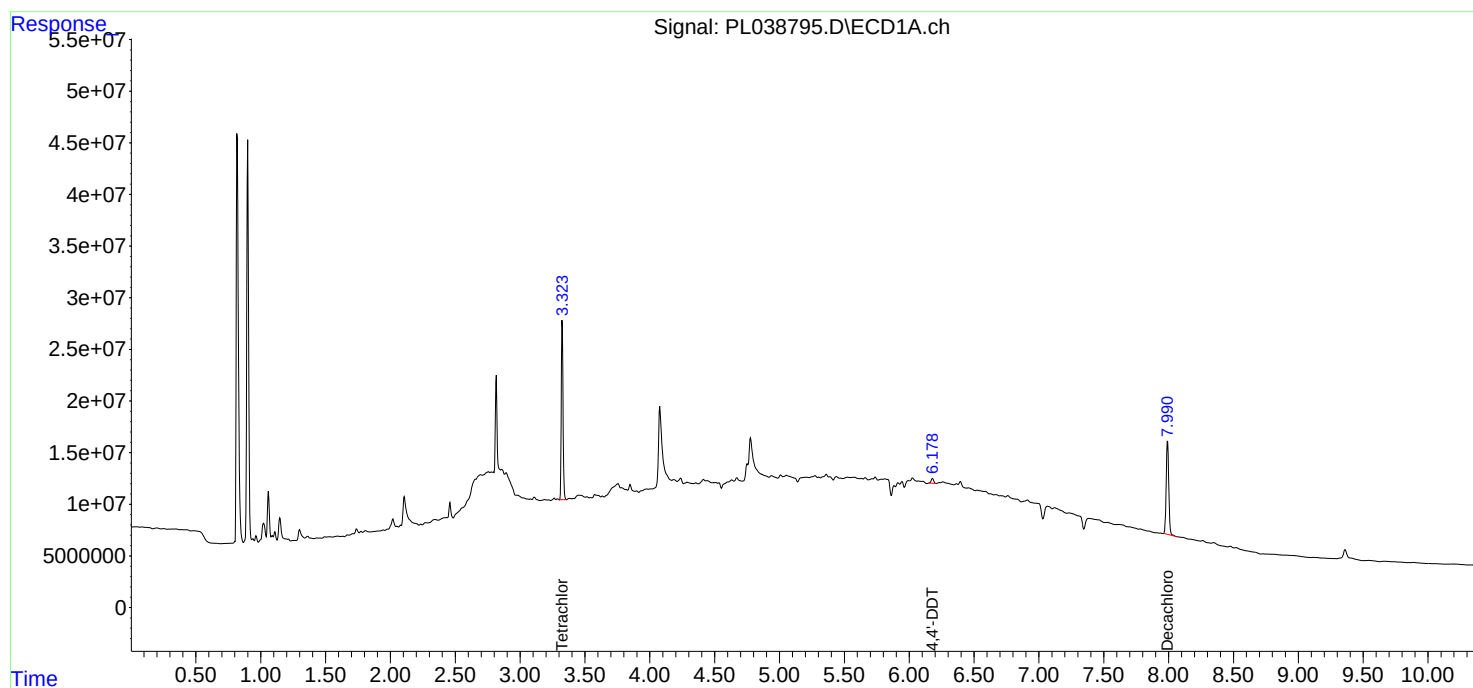

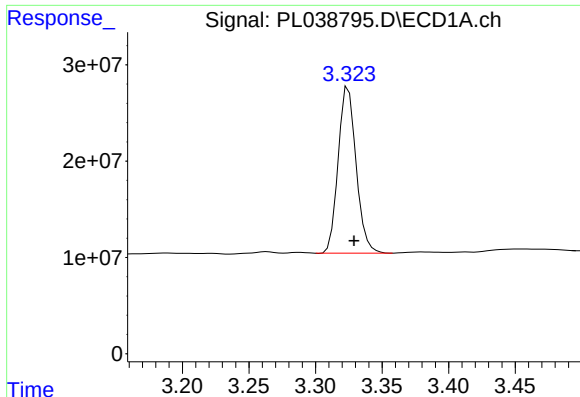


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 162243961
Conc: 21.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-C


Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:45 PM

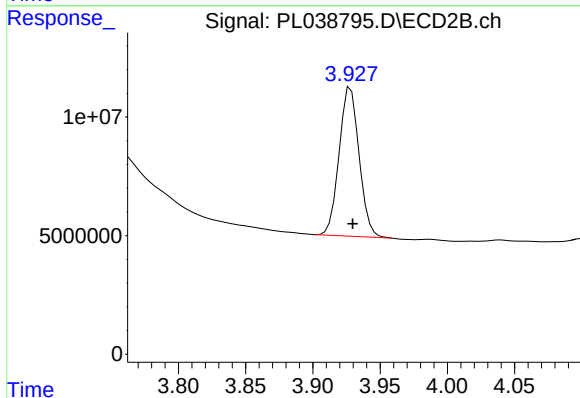


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 64528136
Conc: 24.58 ng/ml

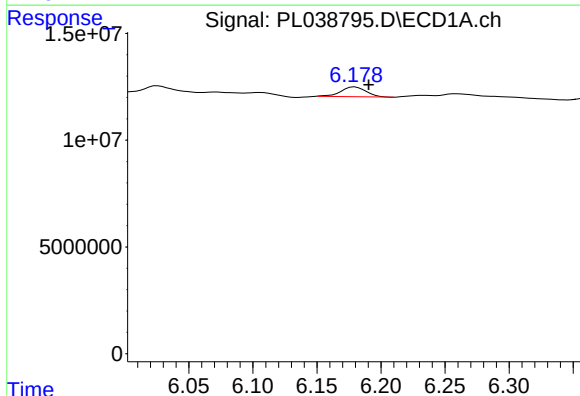


#17 4,4'-DDT

R.T.: 6.180 min
Delta R.T.: -0.011 min
Response: 6269439
Conc: 0.84 ng/ml

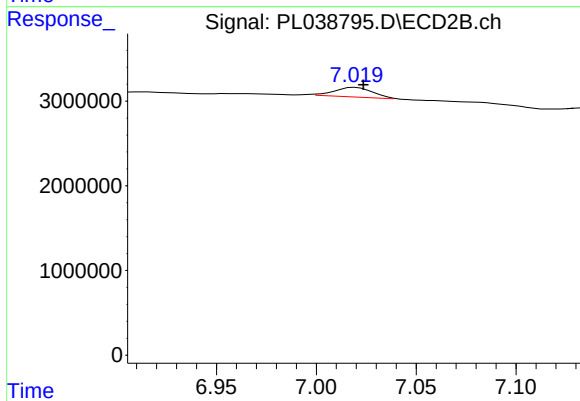

#17 4,4'-DDT

R.T.: 7.019 min
Delta R.T.: -0.005 min
Response: 1470835
Conc: 0.69 ng/ml m

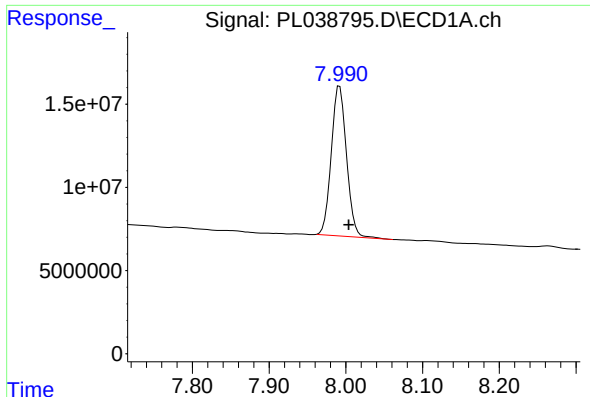

#28 Decachlorobiphenyl

R.T.: 7.992 min

Delta R.T.: -0.012 min


Response: 123726959

Conc: 16.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-C

Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:45 PM

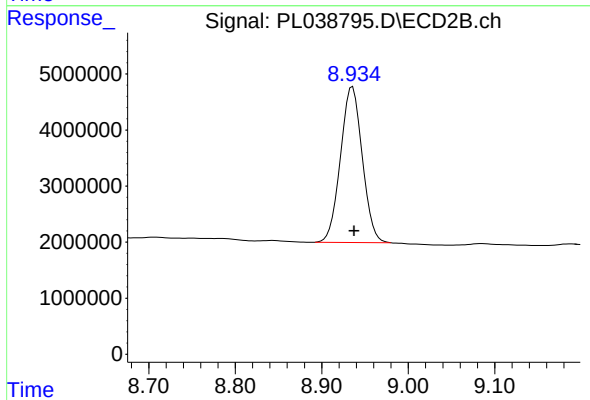

#28 Decachlorobiphenyl

R.T.: 8.936 min

Delta R.T.: -0.002 min

Response: 48432997

Conc: 19.81 ng/ml