

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
 Data File : PL038796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2018 19:01
 Operator : AJ\SJ
 Sample : J4257-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-001-D

Manual Integrations
 APPROVED

Sohil
 8/2/2018 5:39:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:10:15 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.928	159.9E6	63945173	21.476	24.361
28)	SA Decachlor...	7.993	8.935	117.2E6	46197028	15.445	18.899
Target Compounds							
17)	MA 4,4'-DDT	6.180	7.022	13696687	4357414	1.844m	2.044

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080118\
Data File : PL038796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2018 19:01
Operator : AJ\SJ
Sample : J4257-07
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-D


Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:10:15 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

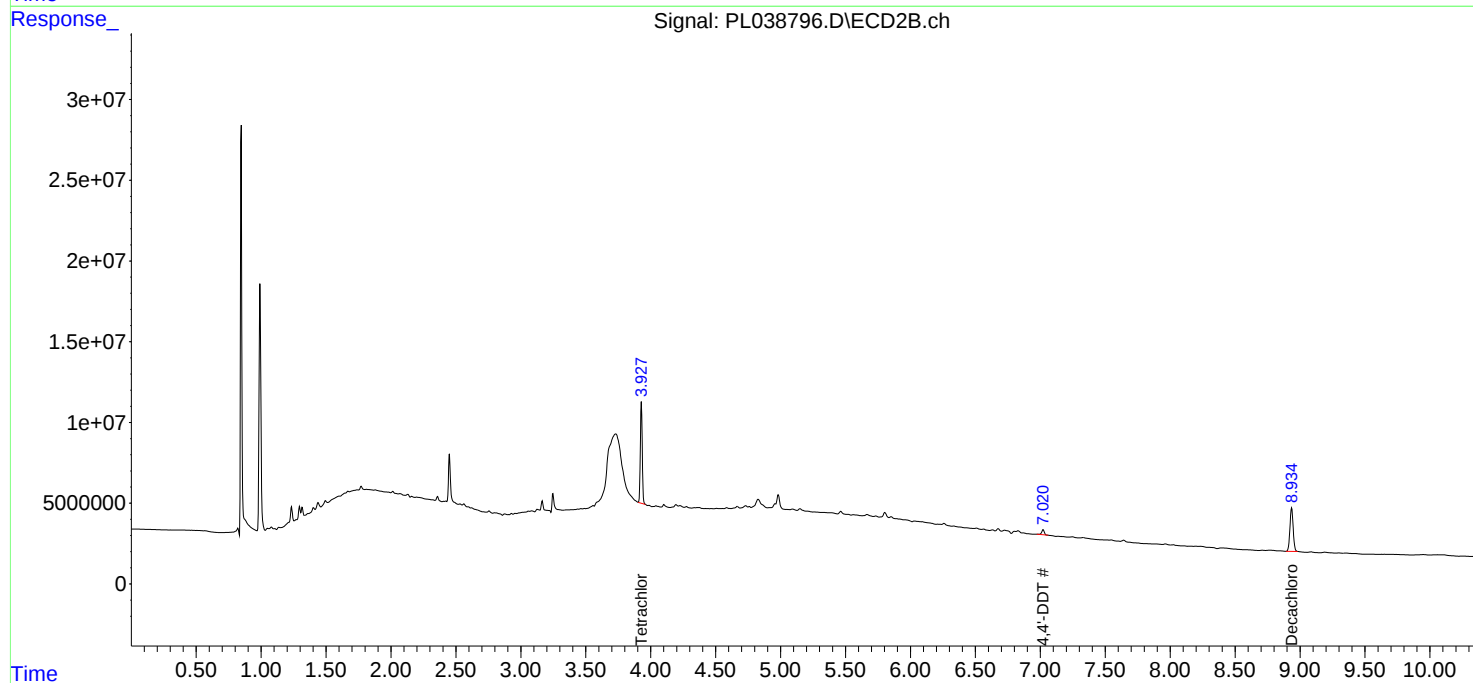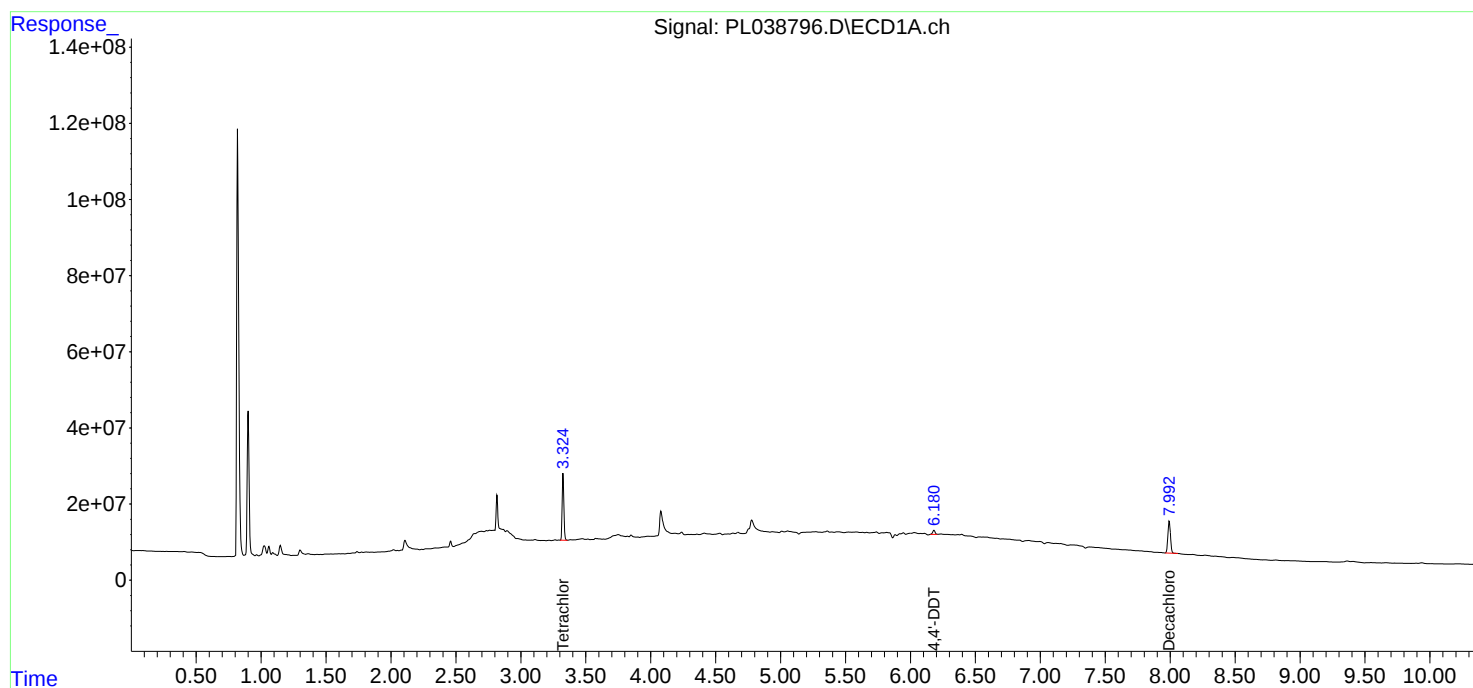

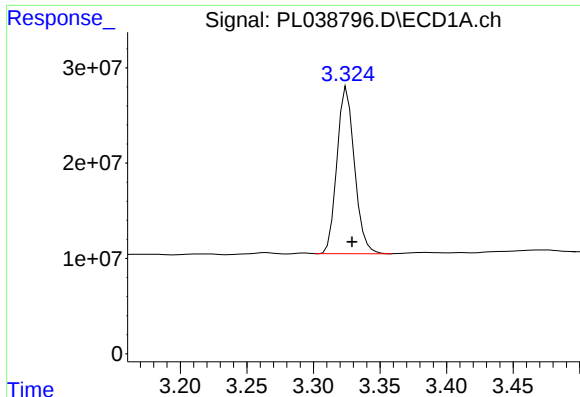


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 159922189
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-D


Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:47 PM

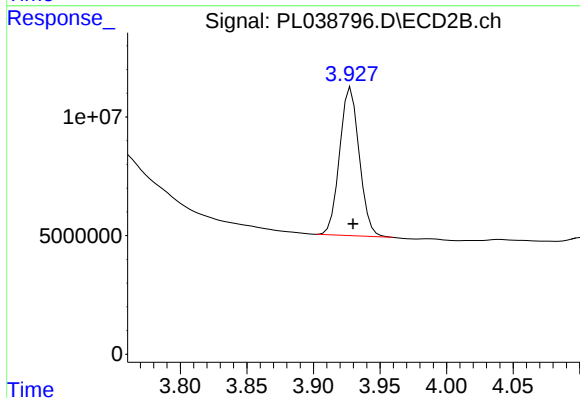


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 63945173
Conc: 24.36 ng/ml

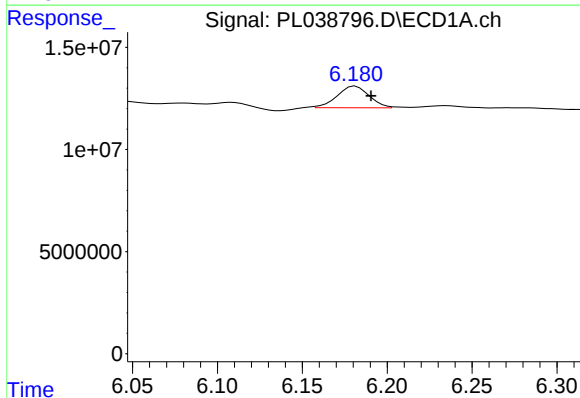


#17 4,4'-DDT

R.T.: 6.180 min
Delta R.T.: -0.010 min
Response: 13696687
Conc: 1.84 ng/ml m

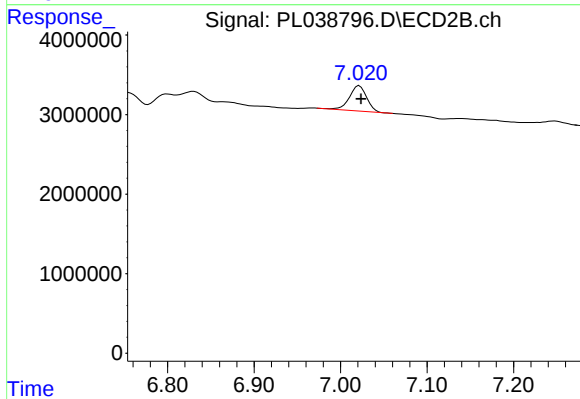

#17 4,4'-DDT

R.T.: 7.022 min
Delta R.T.: -0.002 min
Response: 4357414
Conc: 2.04 ng/ml

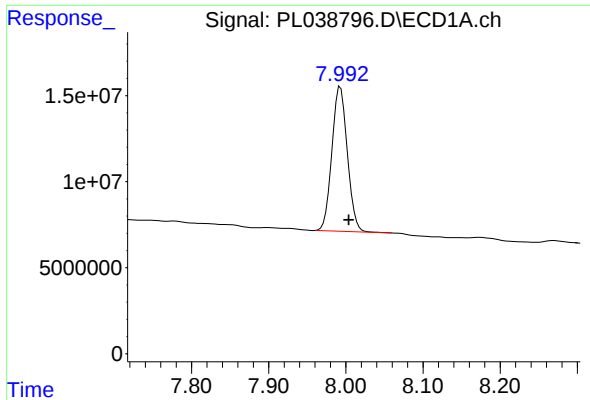


#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.011 min
Response: 117165865
Conc: 15.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-001-D

Manual Integrations
APPROVED

Sohil
8/2/2018 5:39:47 PM

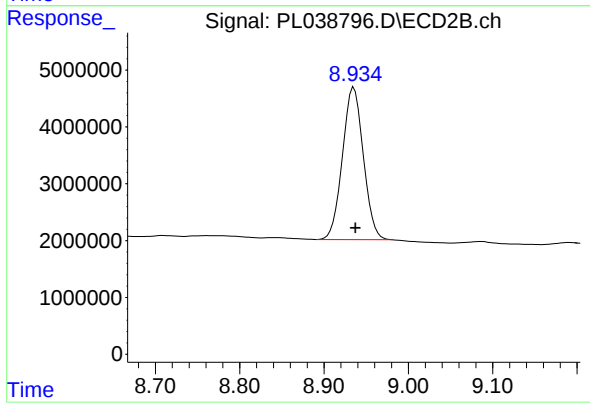

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 46197028
Conc: 18.90 ng/ml