

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080119\
 Data File : PL050964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2019 18:12
 Operator : SM\AJ
 Sample : K4066-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:02:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	238.2E6	66474117	23.706	23.298
28)	SA Decachlor...	7.979	8.957	270.5E6	72296146	26.718	25.565
Target Compounds							
6)	B beta-BHC	0.000	4.805f	0	5315549	N.D.	3.075 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080119\
Data File : PL050964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2019 18:12
Operator : SM\AJ
Sample : K4066-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:02:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

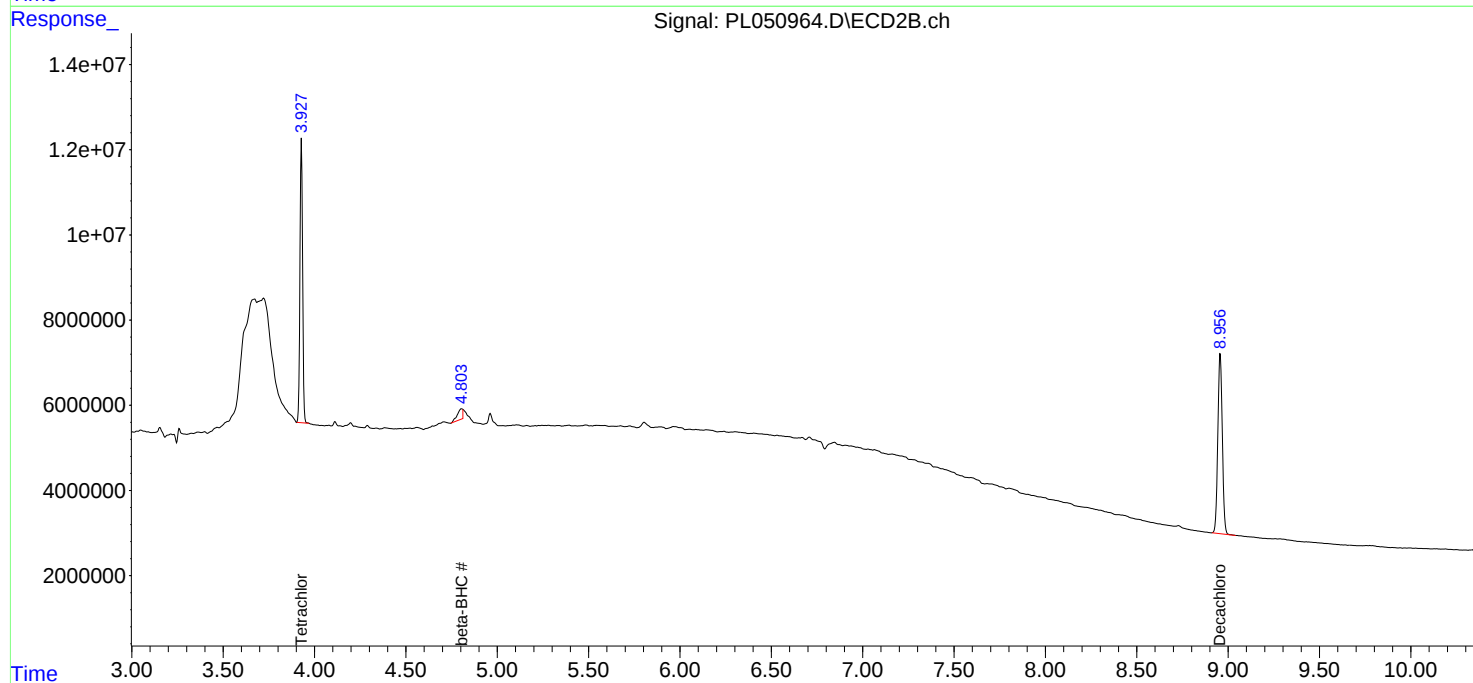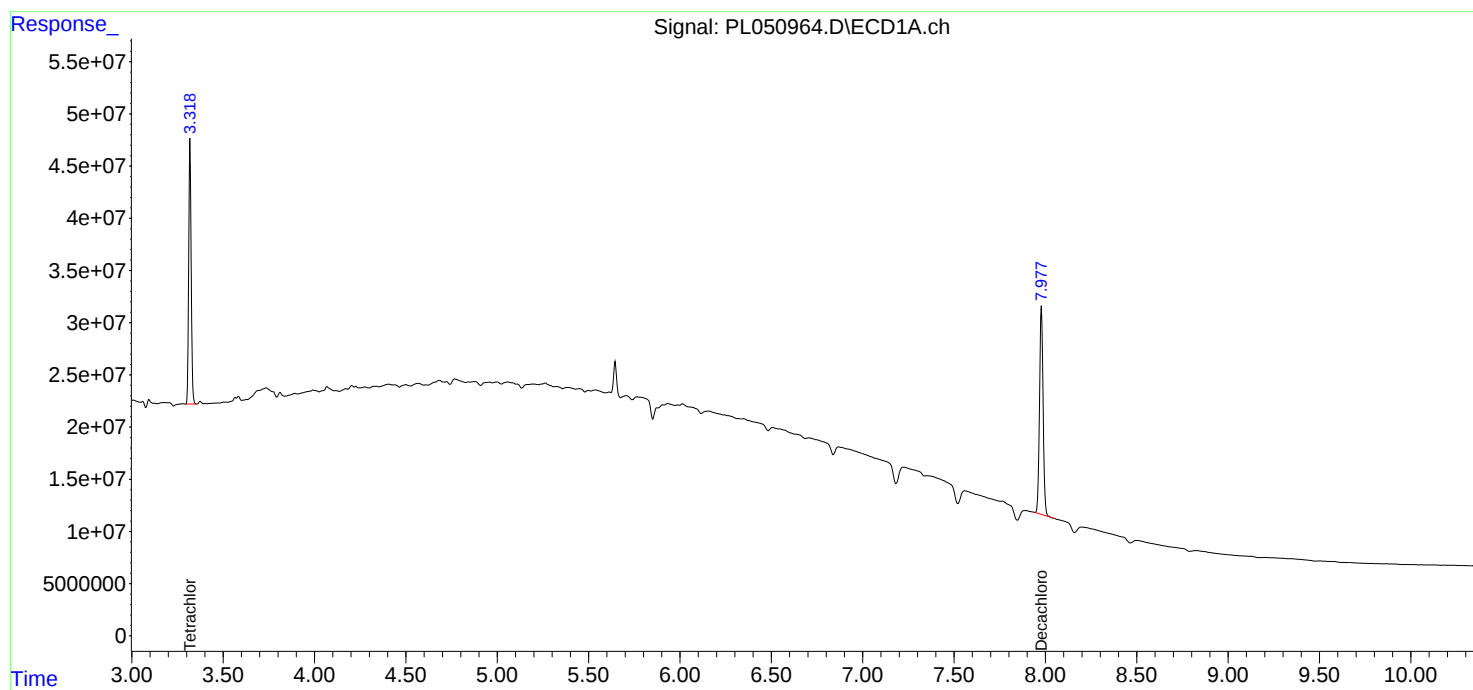


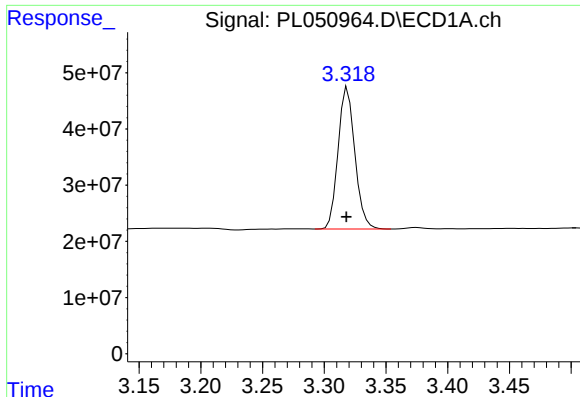

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 238197664
Conc: 23.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-A

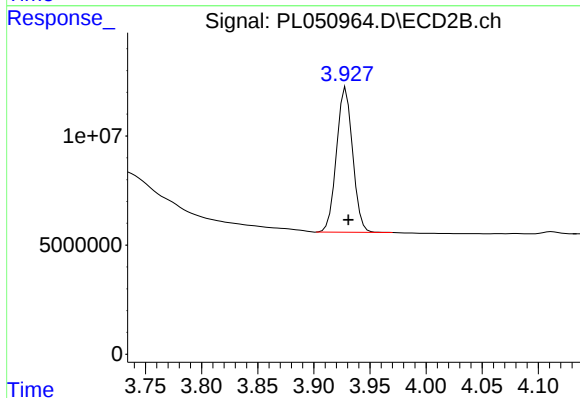


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 66474117
Conc: 23.30 ng/ml

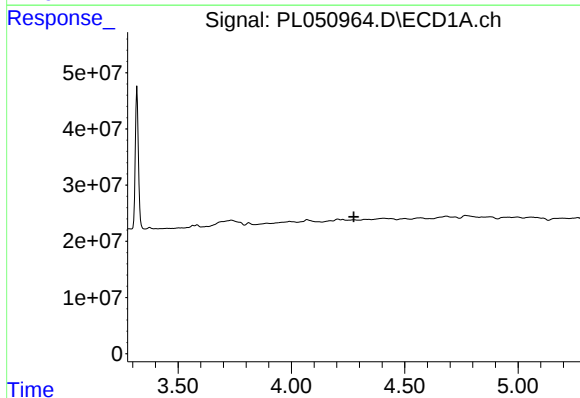


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

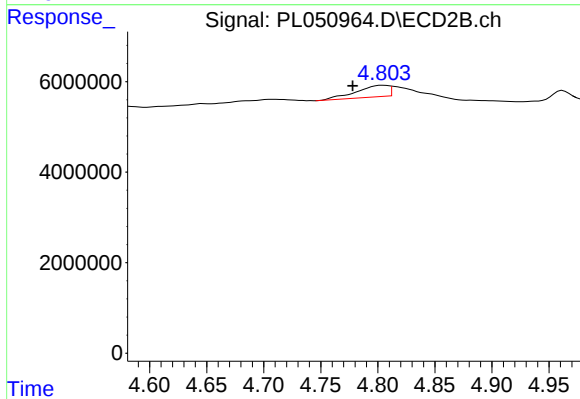

#6 beta-BHC


R.T.: 4.805 min
Delta R.T.: 0.027 min
Response: 5315549
Conc: 3.07 ng/ml

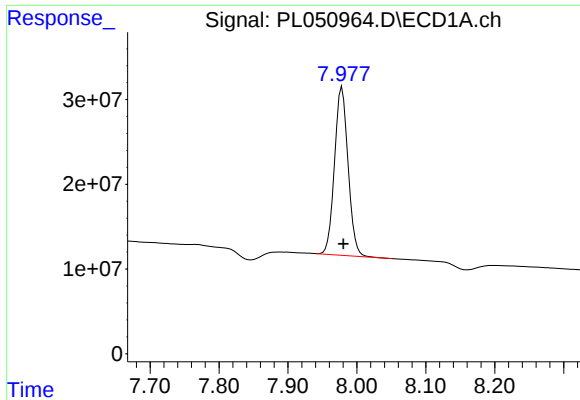

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 270533263
Conc: 26.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1-A

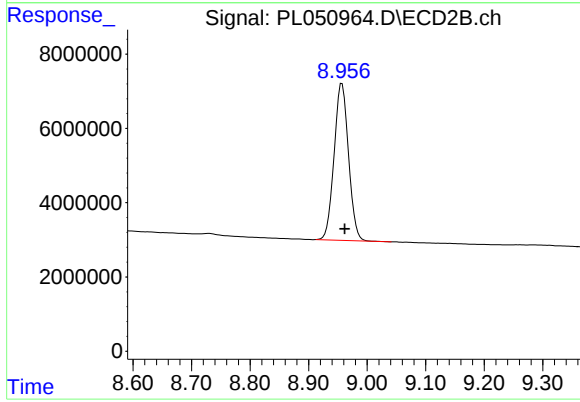

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 72296146
Conc: 25.57 ng/ml