

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080120\
 Data File : PL060429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2020 16:35
 Operator : DD\AJ
 Sample : L3518-47
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 00:02:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.012	26170517	32433499	13.131	12.400
28)	SA Decachlor...	8.223	9.102	22941483	26888718	15.033	14.950
Target Compounds							
9)	A Endosulfan I	0.000	6.244	0	5787196	N.D.	2.140 #
10)	B gamma-Chl...	0.000	6.126	0	6834758	N.D.	2.417 #
11)	B alpha-Chl...	0.000	6.200	0	19226293	N.D.	6.586 #
12)	B 4,4'-DDE	5.630	6.354	8349034	17938331	4.952	6.782 #
14)	MA Endrin	0.000	6.754f	0	2152479	N.D.	0.919 #
16)	A 4,4'-DDD	6.146	6.848	8399769	14422732	5.813	6.923
17)	MA 4,4'-DDT	6.387	7.149	25041434	48354413	18.332	23.909 #
19)	B Endosulfa...	0.000	7.276	0	3669411	N.D.	1.669 #
20)	A Methoxychlor	0.000	7.628f	0	2848529	N.D.	2.474 #
25)	Chlordane-3	0.000	6.126	0	6834758	N.D.	18.575 #
26)	Chlordane-4	0.000	6.200	0	19226293	N.D.	42.114 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080120\
Data File : PL060429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2020 16:35
Operator : DD\AJ
Sample : L3518-47
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 00:02:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

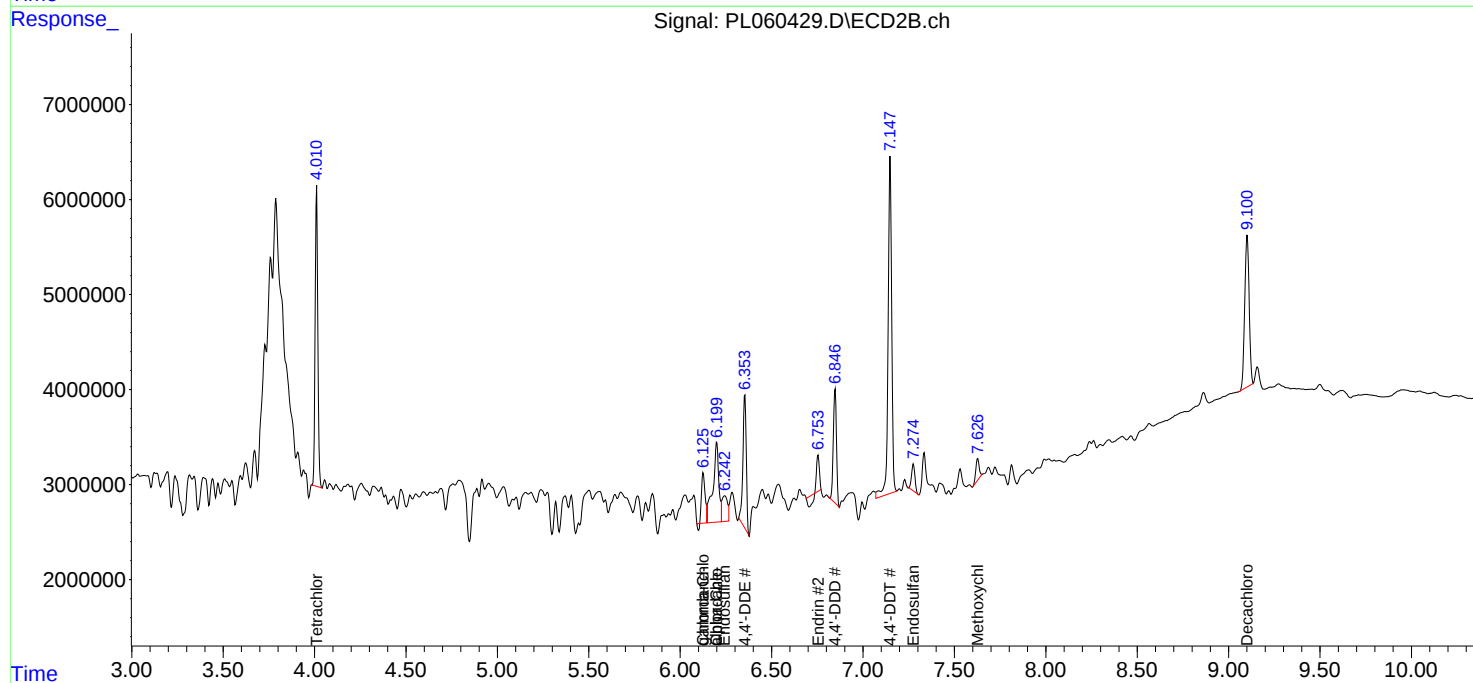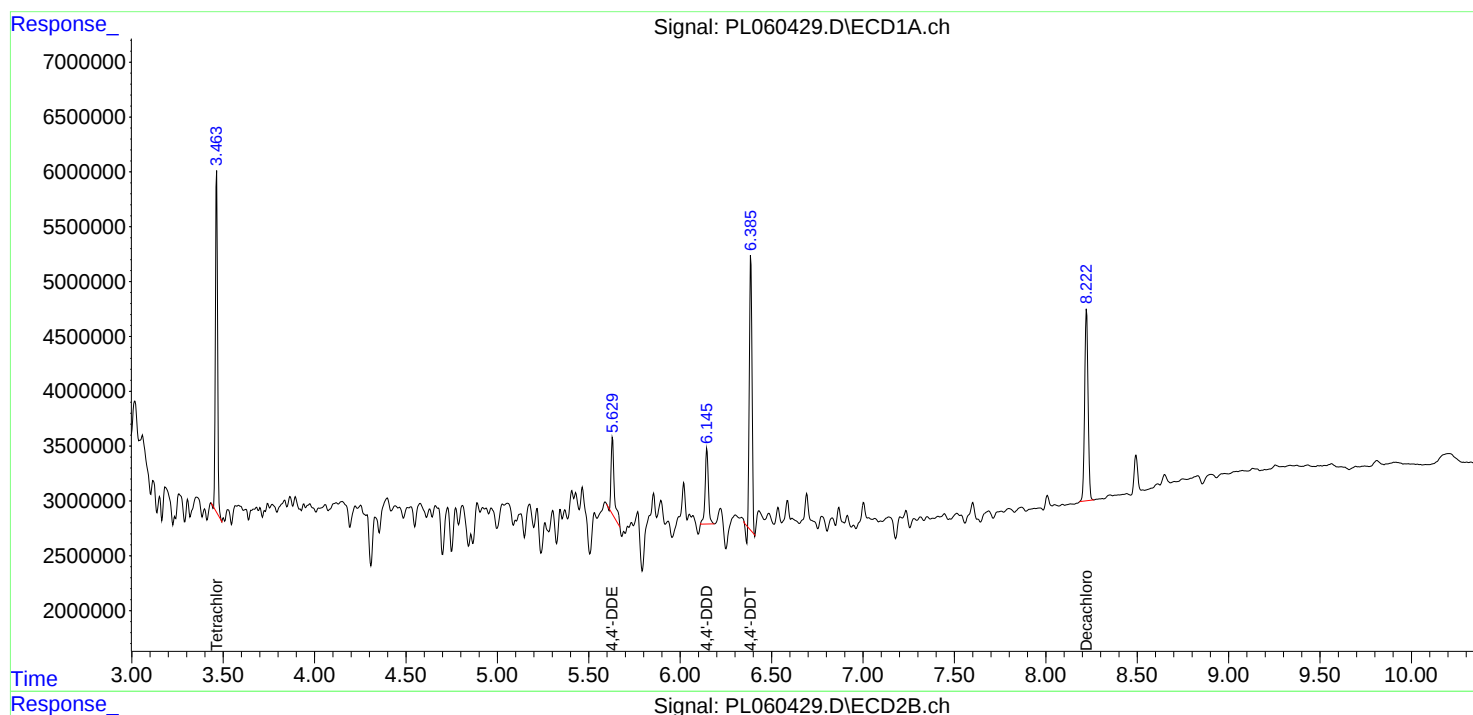


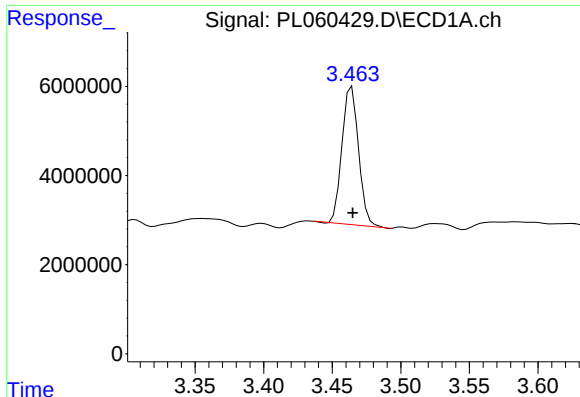

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 26170517
Conc: 13.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13

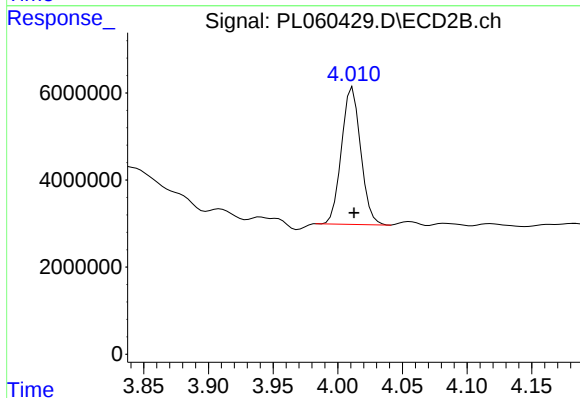


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 32433499
Conc: 12.40 ng/ml

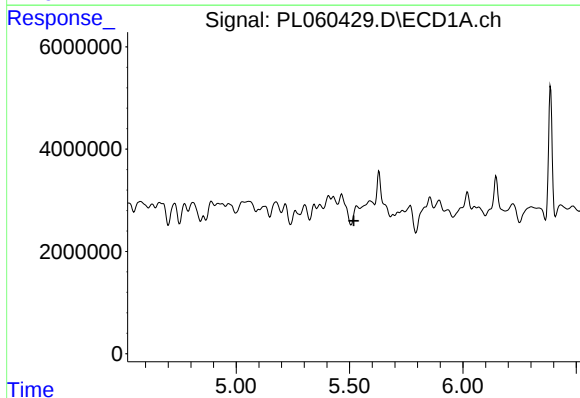


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.518 min
Response: 0
Conc: N.D.

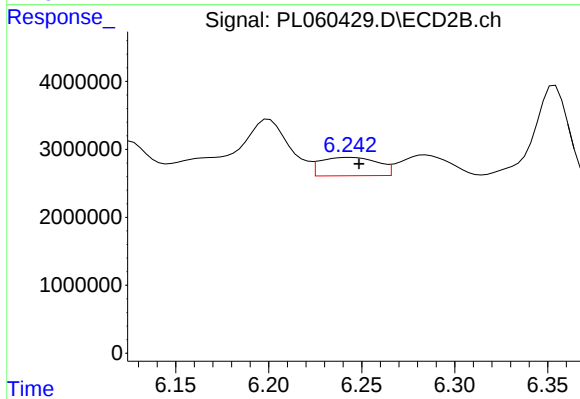

#9 Endosulfan I


R.T.: 6.244 min
Delta R.T.: -0.005 min
Response: 5787196
Conc: 2.14 ng/ml

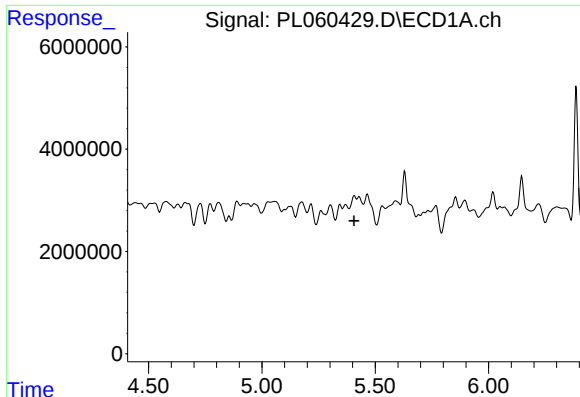

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-13

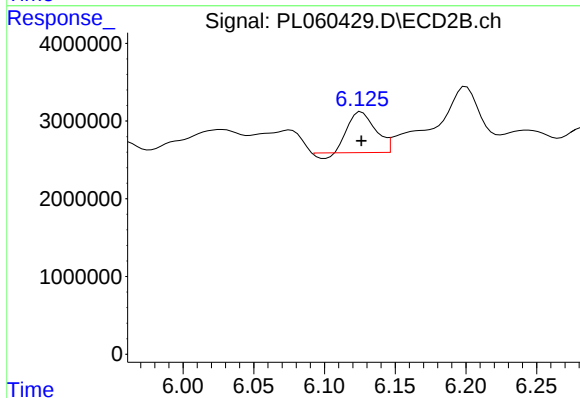


#10 gamma-Chlordane

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 6834758
Conc: 2.42 ng/ml

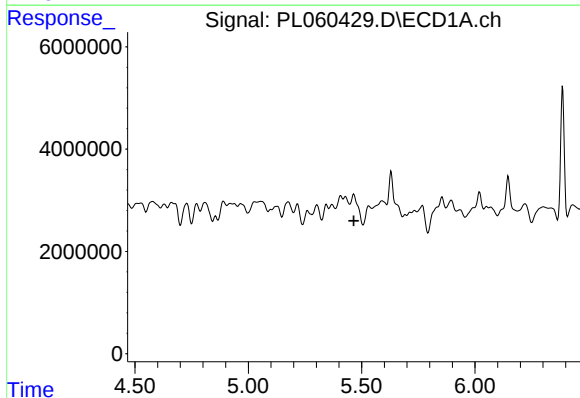


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.465 min
Response: 0
Conc: N.D.

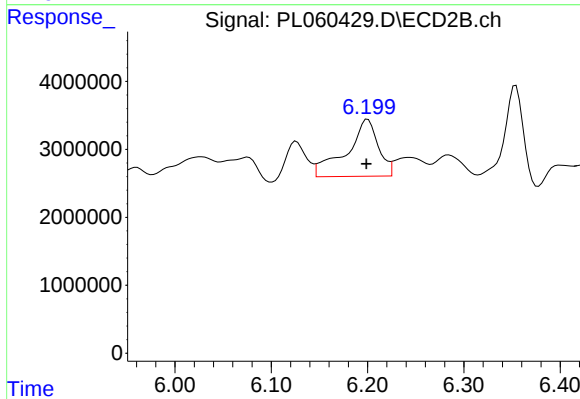

#11 alpha-Chlordane


R.T.: 6.200 min
Delta R.T.: 0.001 min
Response: 19226293
Conc: 6.59 ng/ml

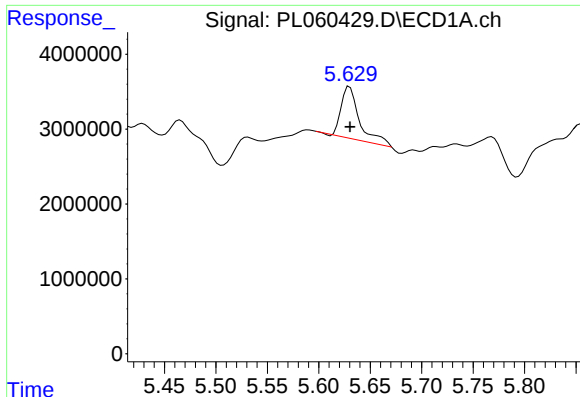

#12 4,4'-DDE


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 8349034
Conc: 4.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13

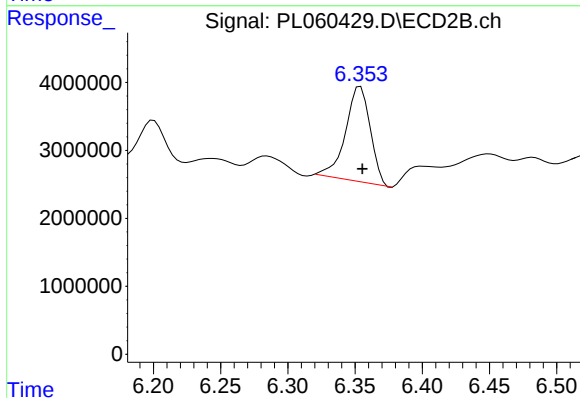


#12 4,4'-DDE

R.T.: 6.354 min
Delta R.T.: -0.002 min
Response: 17938331
Conc: 6.78 ng/ml

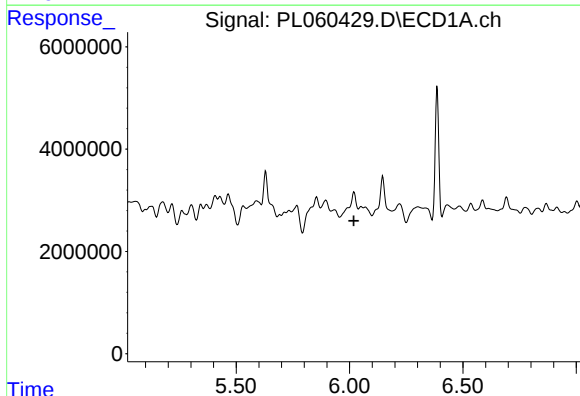


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.018 min
Response: 0
Conc: N.D.

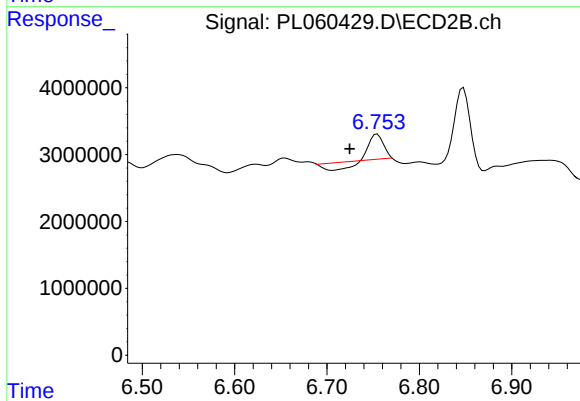

#14 Endrin


R.T.: 6.754 min
Delta R.T.: 0.030 min
Response: 2152479
Conc: 0.92 ng/ml

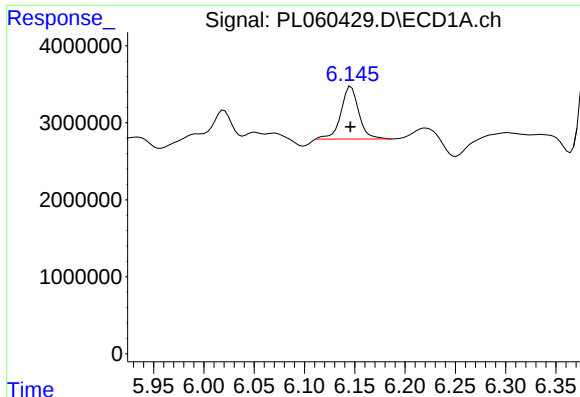

#16 4,4'-DDD


R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 8399769
Conc: 5.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13

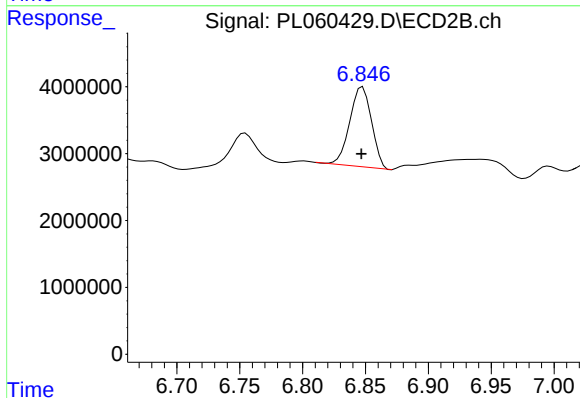


#16 4,4'-DDD

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 14422732
Conc: 6.92 ng/ml

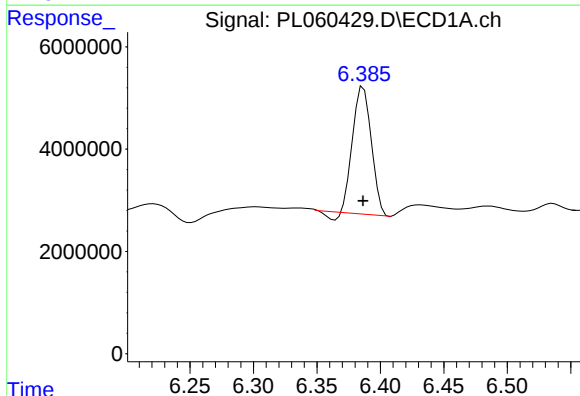


#17 4,4'-DDT

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 25041434
Conc: 18.33 ng/ml

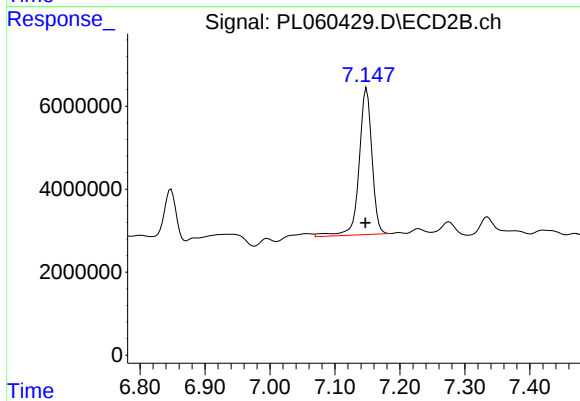

#17 4,4'-DDT


R.T.: 7.149 min
Delta R.T.: 0.002 min
Response: 48354413
Conc: 23.91 ng/ml

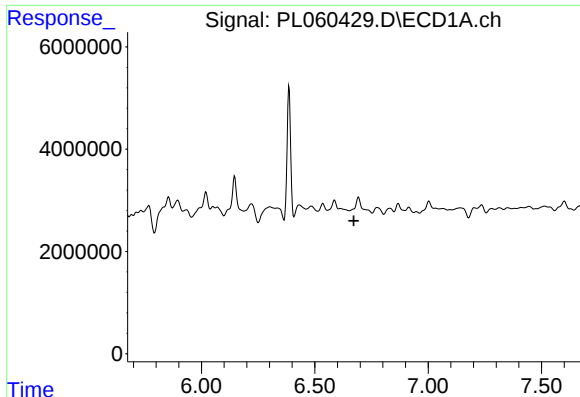

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.672 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-13

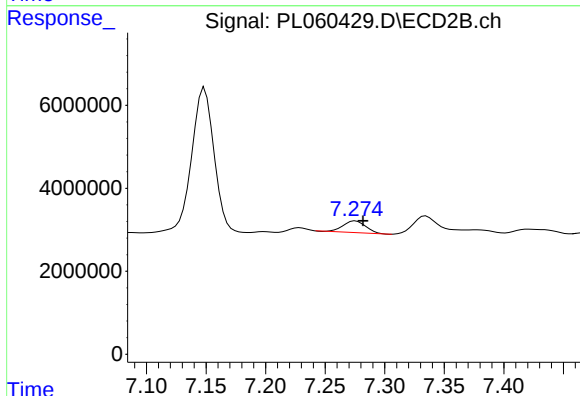


#19 Endosulfan Sulfate

R.T.: 7.276 min
Delta R.T.: -0.006 min
Response: 3669411
Conc: 1.67 ng/ml

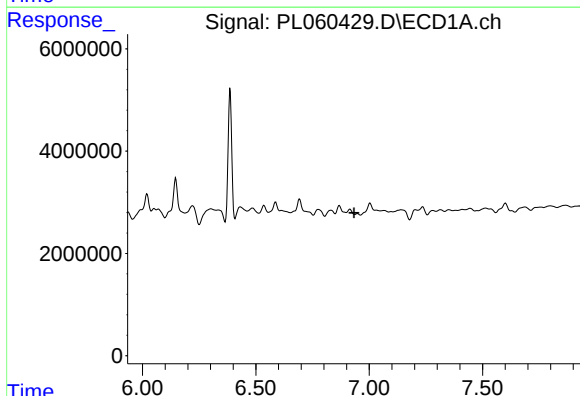


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.933 min
Response: 0
Conc: N.D.

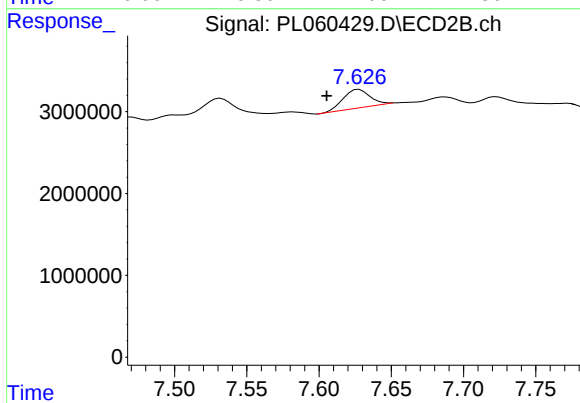

#20 Methoxychlor


R.T.: 7.628 min
Delta R.T.: 0.022 min
Response: 2848529
Conc: 2.47 ng/ml

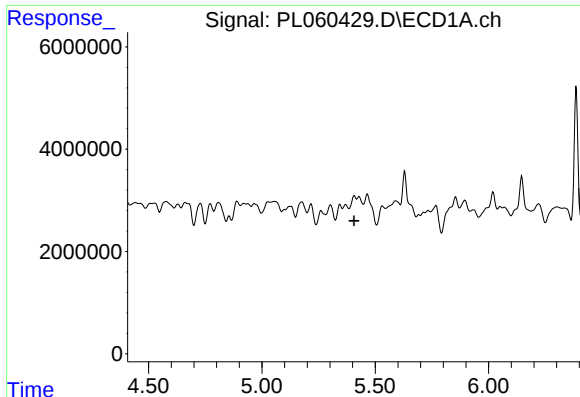

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-13

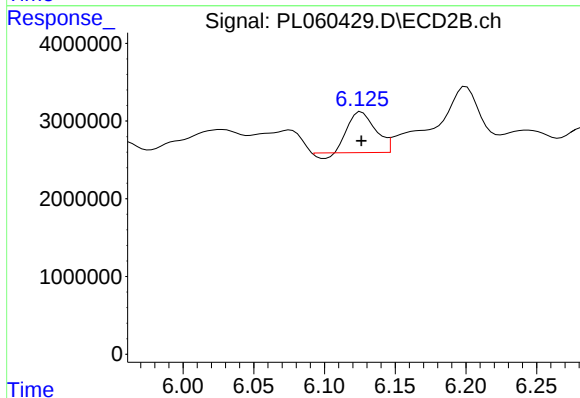


#25 Chlordane-3

R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 6834758
Conc: 18.57 ng/ml

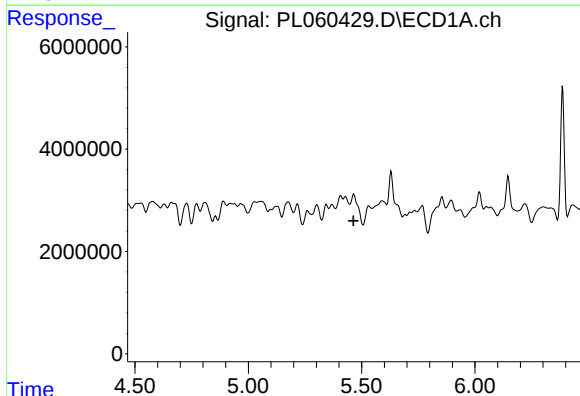


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.465 min
Response: 0
Conc: N.D.

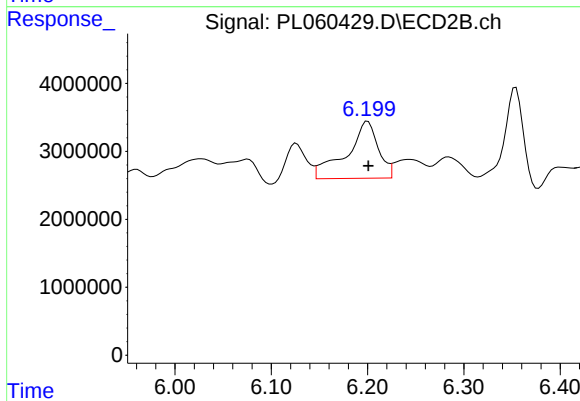

#26 Chlordane-4


R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 19226293
Conc: 42.11 ng/ml

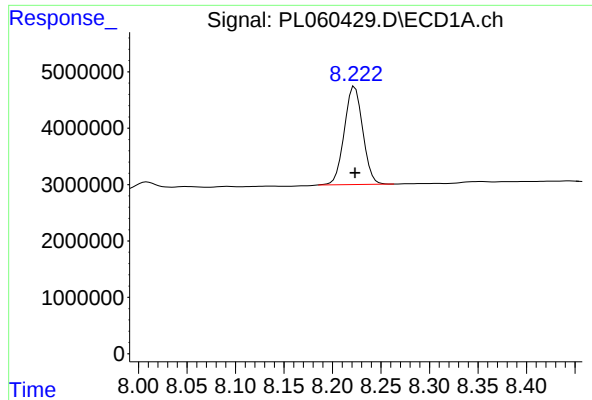

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 22941483
Conc: 15.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-13

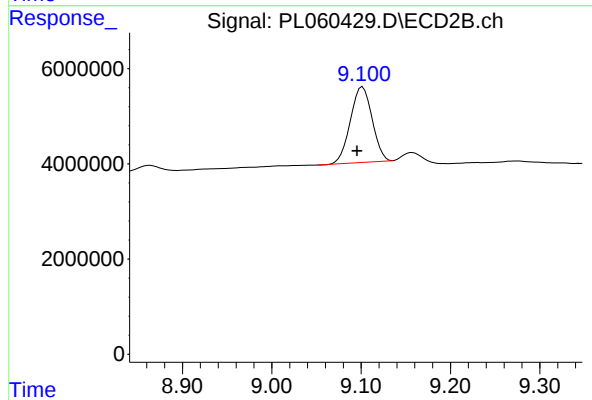

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.006 min
Response: 26888718
Conc: 14.95 ng/ml