

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080120\
 Data File : PL060415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2020 13:17
 Operator : DD\AJ
 Sample : L3518-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Ankita

8/3/2020 12:13:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 15:51:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.011	39371923	52352623	19.754	20.016
28)	SA Decachlor...	8.223	9.100	30309563	35398285	19.861	19.681
Target Compounds							
12)	B 4,4'-DDE	5.627	6.355	4085306	7285061	2.423m	2.754
16)	A 4,4'-DDD	6.147	6.851	1637074	5820864	1.133m	2.794 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080120\
Data File : PL060415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2020 13:17
Operator : DD\AJ
Sample : L3518-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-4



Manual Integrations
APPROVED


Ankita

8/3/2020 12:13:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 15:51:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

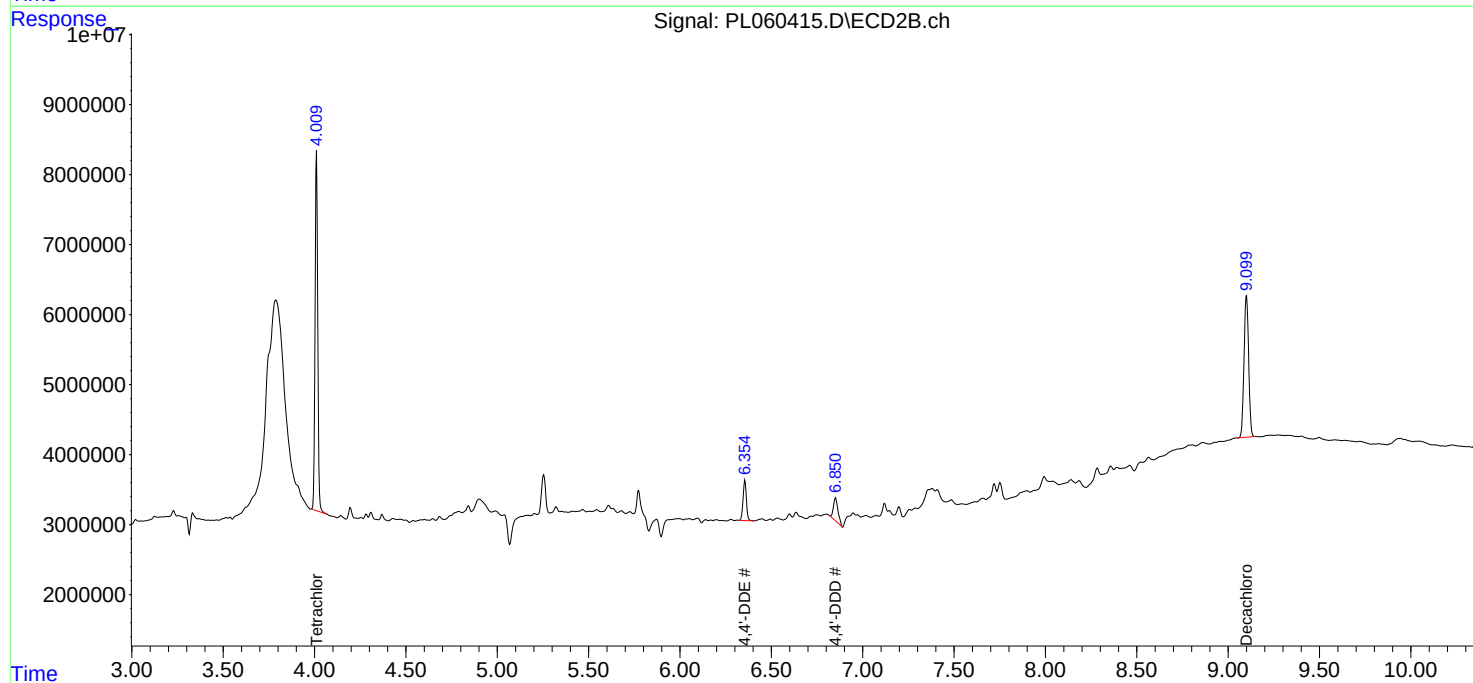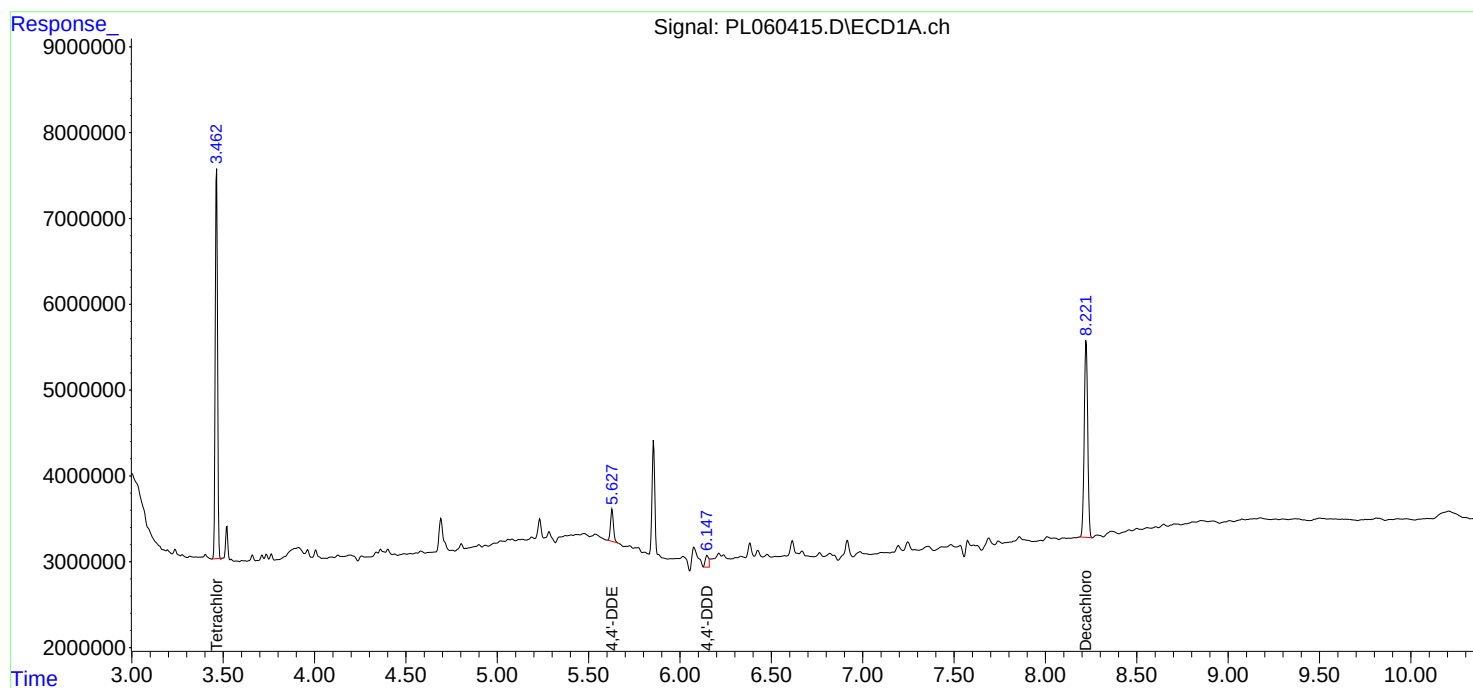

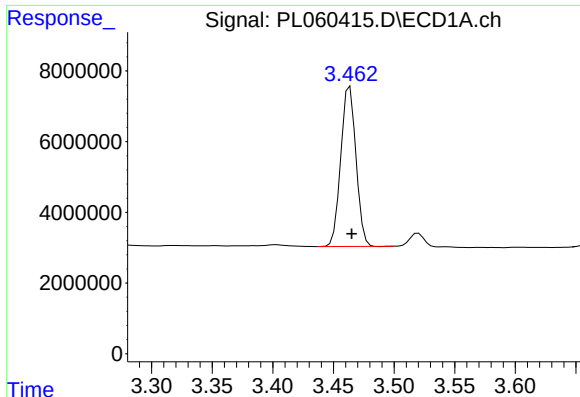

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: -0.001 min
Response: 39371923
Conc: 19.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4

Manual Integrations
APPROVED


Ankita

8/3/2020 12:13:26 PM

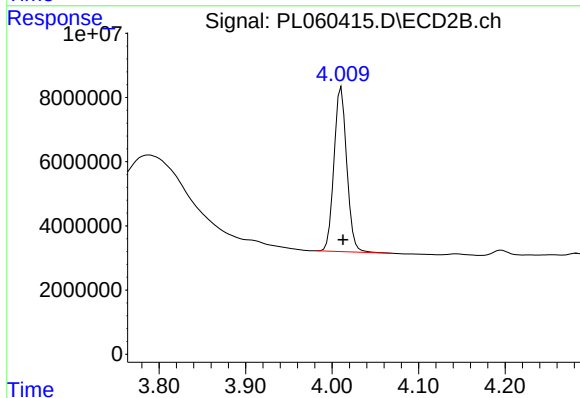


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 52352623
Conc: 20.02 ng/ml

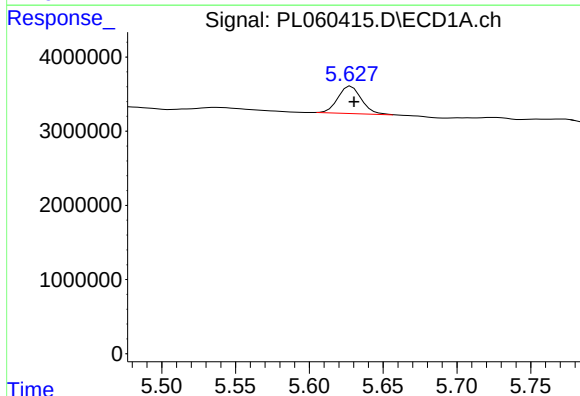


#12 4,4'-DDE

R.T.: 5.627 min
Delta R.T.: -0.003 min
Response: 4085306
Conc: 2.42 ng/ml m

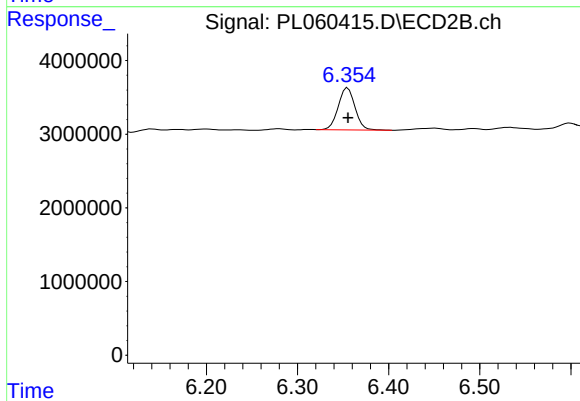

#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 7285061
Conc: 2.75 ng/ml

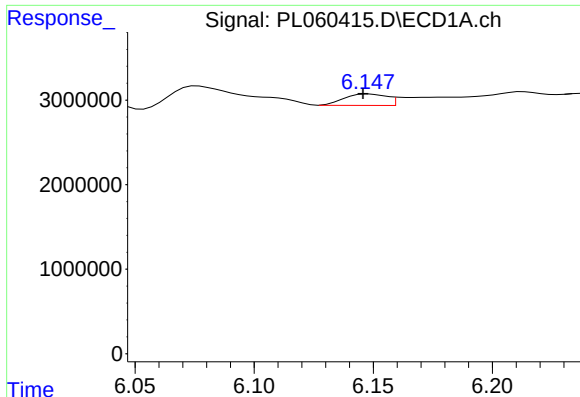

#16 4,4'-DDD


R.T.: 6.147 min
Delta R.T.: 0.000 min
Response: 1637074
Conc: 1.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-4

Manual Integrations
APPROVED


Ankita

8/3/2020 12:13:26 PM

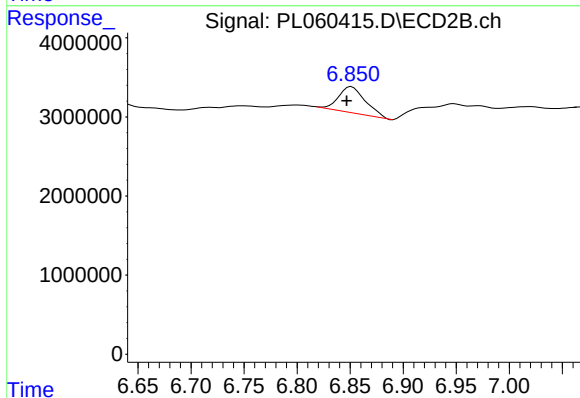


#16 4,4'-DDD

R.T.: 6.851 min
Delta R.T.: 0.005 min
Response: 5820864
Conc: 2.79 ng/ml

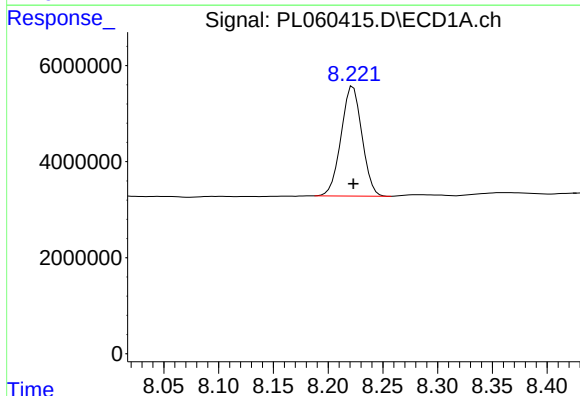

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 30309563
Conc: 19.86 ng/ml

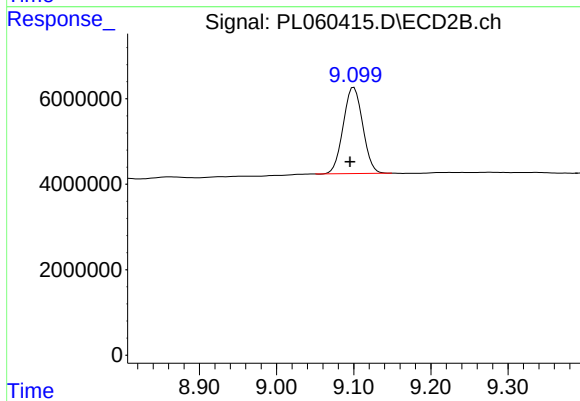

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.005 min
Response: 35398285
Conc: 19.68 ng/ml