

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 10:22
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 04:22:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) MB	Aldrin	0.000	4.042f	0	811620	N.D. 0.292 #
8) B	Heptachlo...	5.542f	0.000	1001279	0	N.D. 1.071 #
9) A	Endosulfan I	5.959	0.000	650426	0	N.D. 0.677 #
10) B	gamma-Chl...	0.000	4.835f	0	1327570	N.D. 0.542 #
13) MA	Dieldrin	0.000	5.196	0	3753505	N.D. 1.548 #
14) MA	Endrin	0.000	5.495f	0	1128441	N.D. 0.521 #
15) B	Endosulfa...	6.709	0.000	323609	0	N.D. 0.361 #
16) A	4,4'-DDD	0.000	5.603f	0	1118046	N.D. 0.599 #
24)	Chlordane-2	0.000	4.178f	0	83007	N.D. 0.843 #
25)	Chlordane-3	0.000	4.835f	0	1327570	N.D. 4.814 #
27)	Chlordane-5	0.000	5.554	0	880901	N.D. 11.541 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 10:22
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 04:22:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

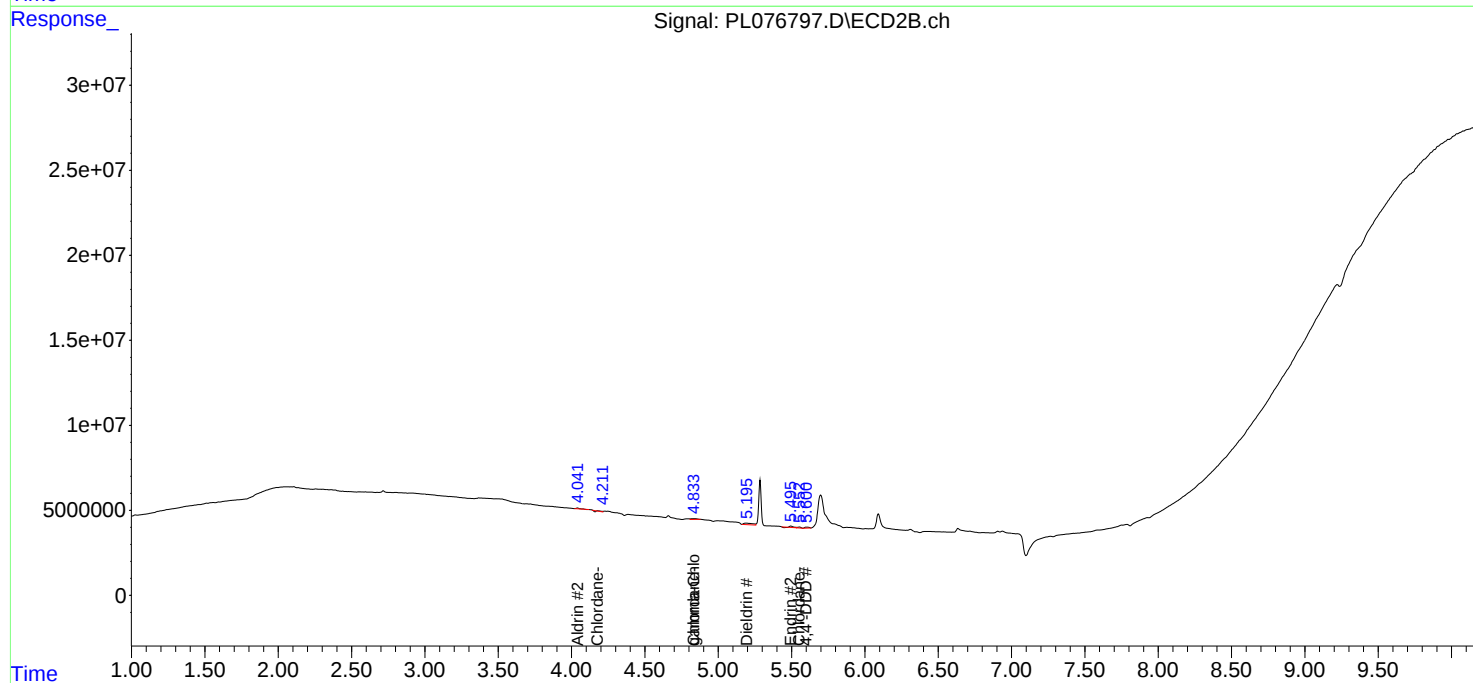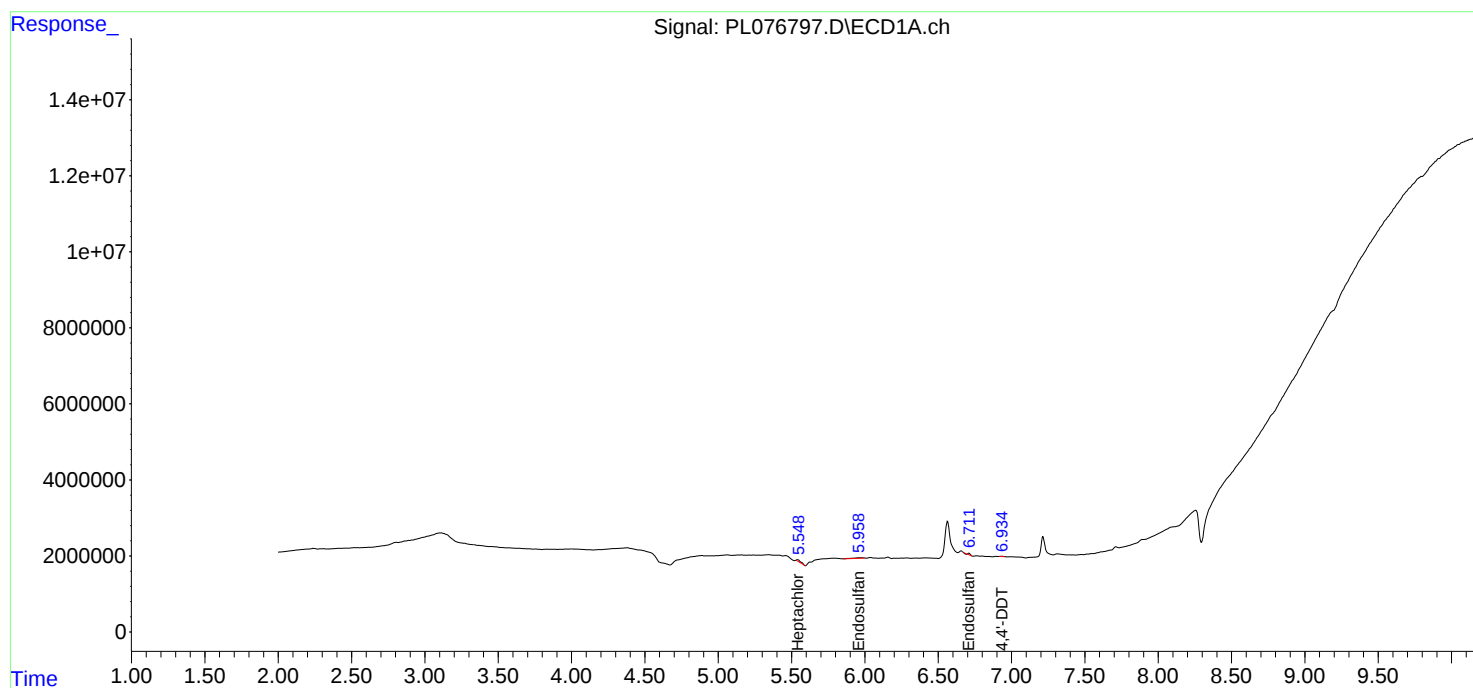

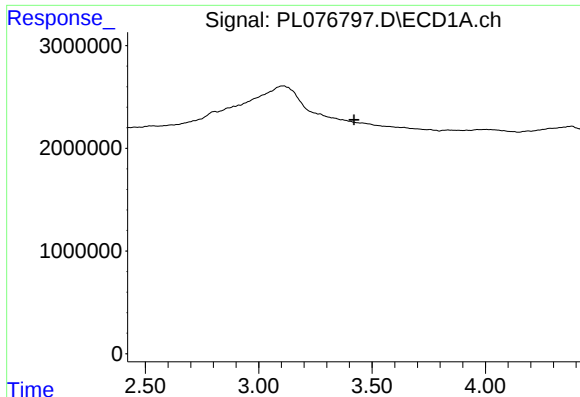

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

#1 Tetrachloro-m-xylene



R.T.: 0.000 min
Exp R.T. : 2.642 min
Response: 0
Conc: N.D.


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.139 min
Response: 0
Conc: N.D.

#5 Aldrin

R.T.: 4.042 min
Delta R.T.: -0.028 min
Response: 811620
Conc: 0.29 ng/ml

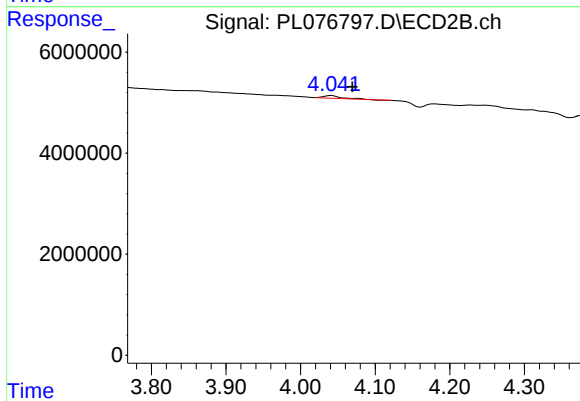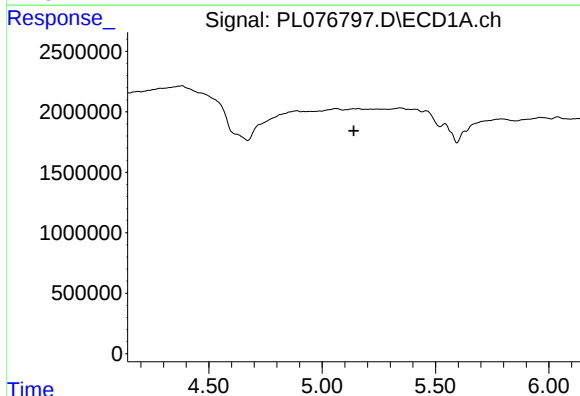


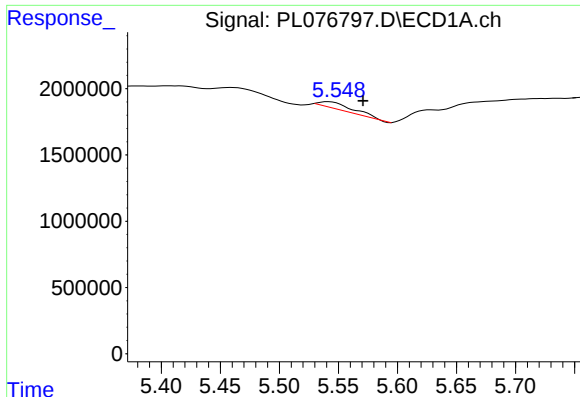

#8 Heptachlor epoxide


R.T.: 5.542 min
Delta R.T.: -0.029 min
Response: 1001279
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

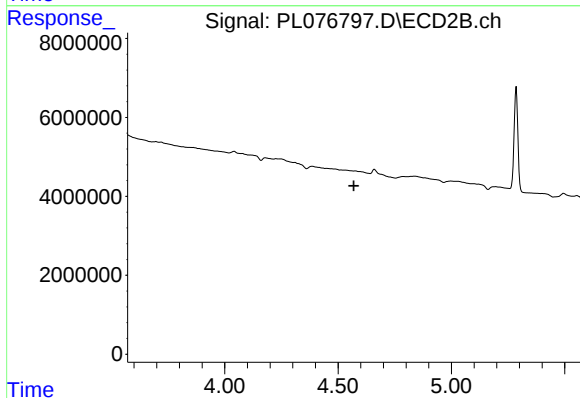


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.569 min
Response: 0
Conc: N.D.

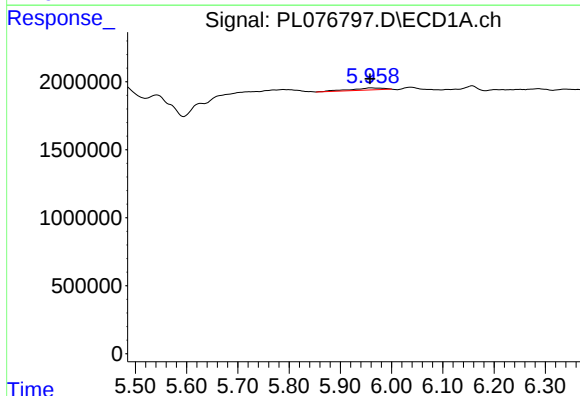


#9 Endosulfan I

R.T.: 5.959 min
Delta R.T.: 0.001 min
Response: 650426
Conc: 0.68 ng/ml

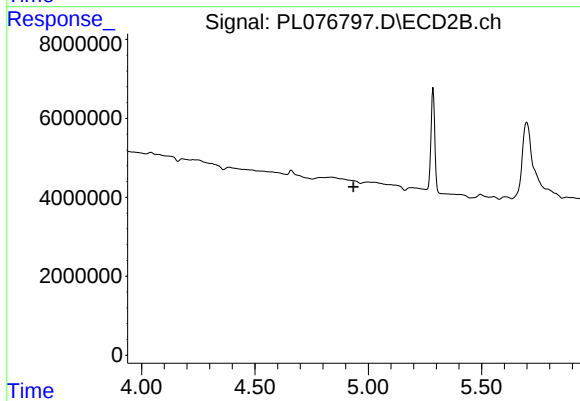

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 4.935 min
Response: 0
Conc: N.D.

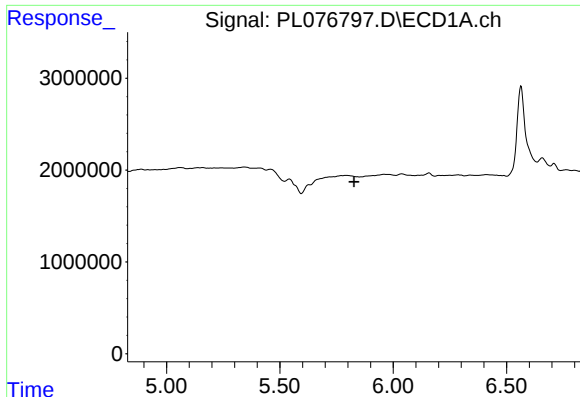

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

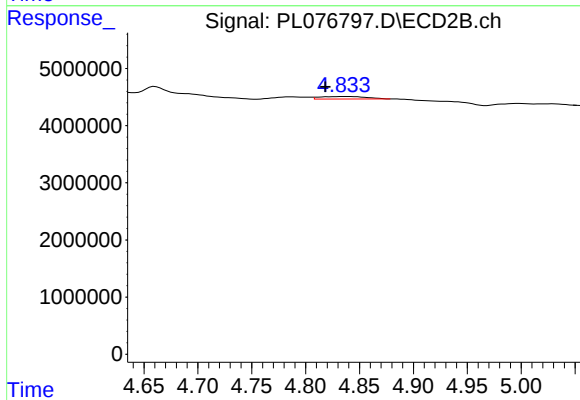


#10 gamma-Chlordane

R.T.: 4.835 min
Delta R.T.: 0.016 min
Response: 1327570
Conc: 0.54 ng/ml

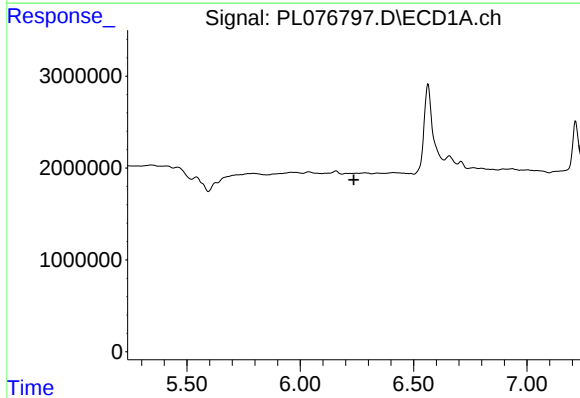


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

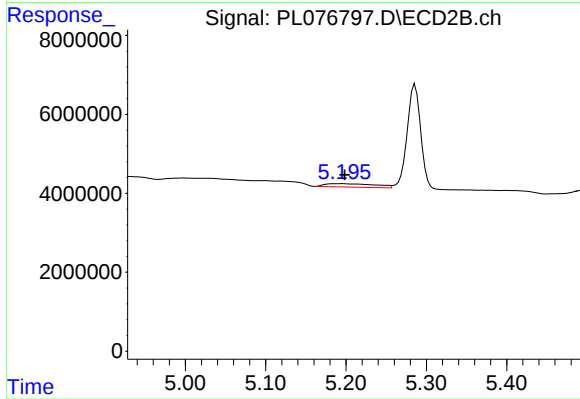

#13 Dieldrin


R.T.: 5.196 min
Delta R.T.: -0.002 min
Response: 3753505
Conc: 1.55 ng/ml

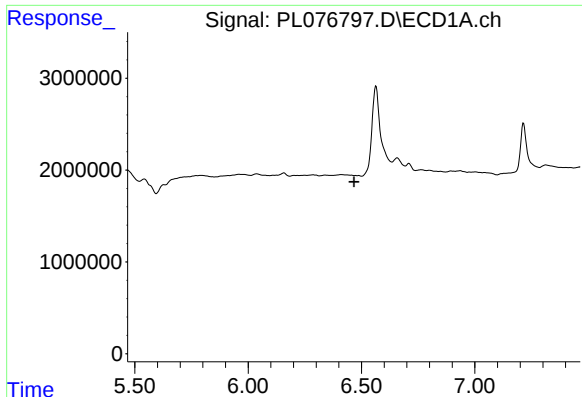

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

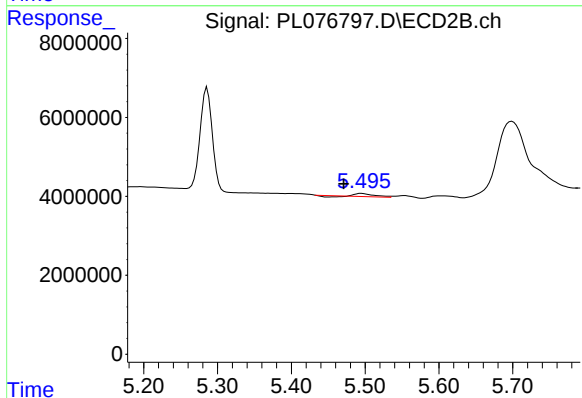


#14 Endrin

R.T.: 5.495 min
Delta R.T.: 0.024 min
Response: 1128441
Conc: 0.52 ng/ml

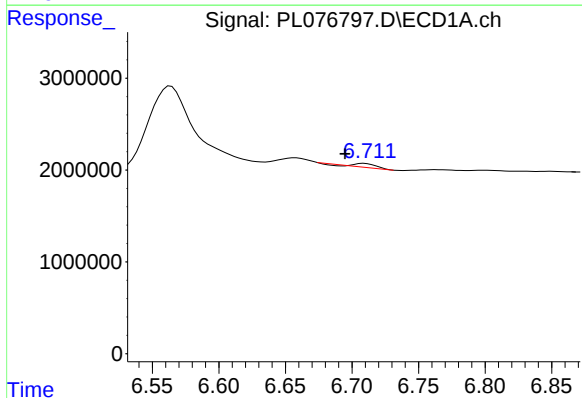


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.015 min
Response: 323609
Conc: 0.36 ng/ml

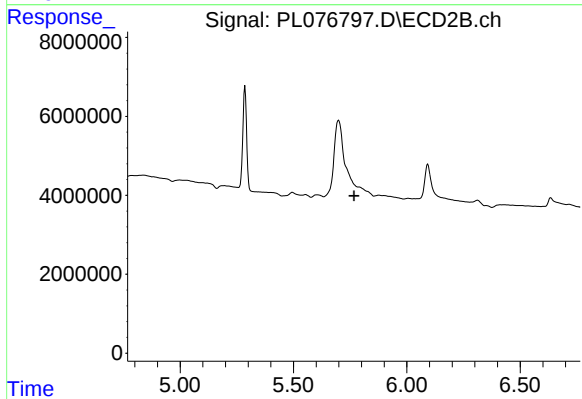

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.767 min
Response: 0
Conc: N.D.

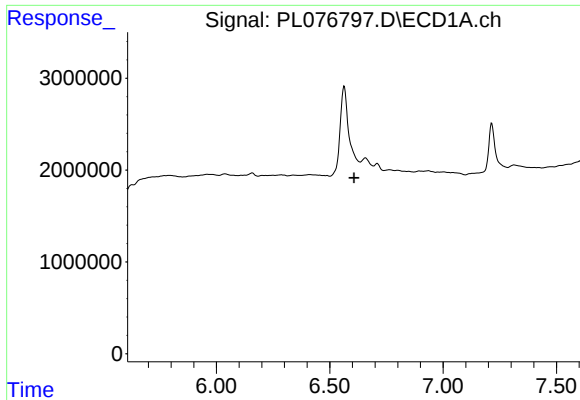

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

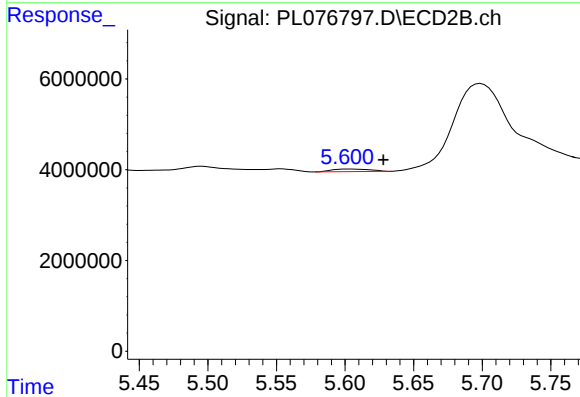


#16 4,4'-DDD

R.T.: 5.603 min
Delta R.T.: -0.025 min
Response: 1118046
Conc: 0.60 ng/ml

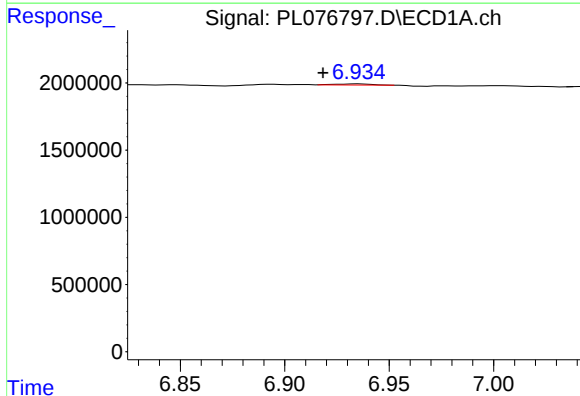


#17 4,4'-DDT

R.T.: 6.935 min
Delta R.T.: 0.017 min
Response: 79821
Conc: 0.09 ng/ml

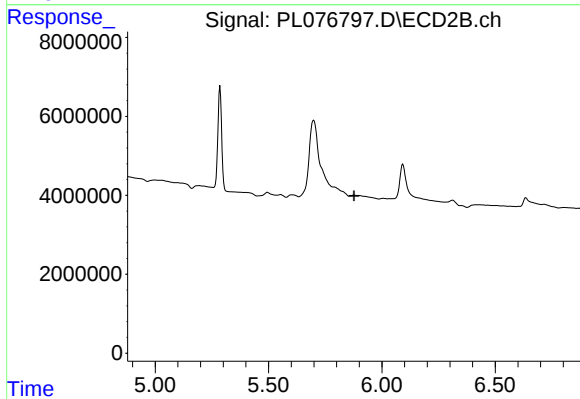

#17 4,4'-DDT


R.T.: 5.877 min
Delta R.T.: 0.000 min
Response: -676957
Conc: N.D.

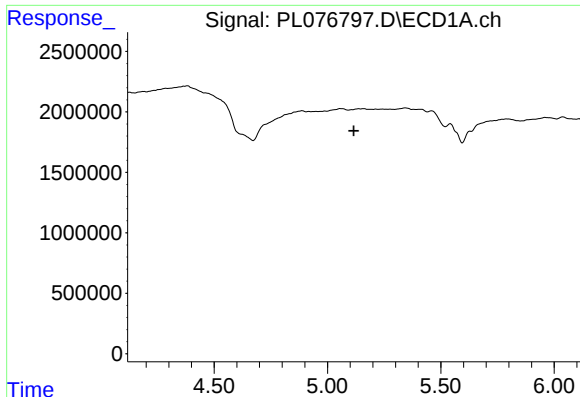

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

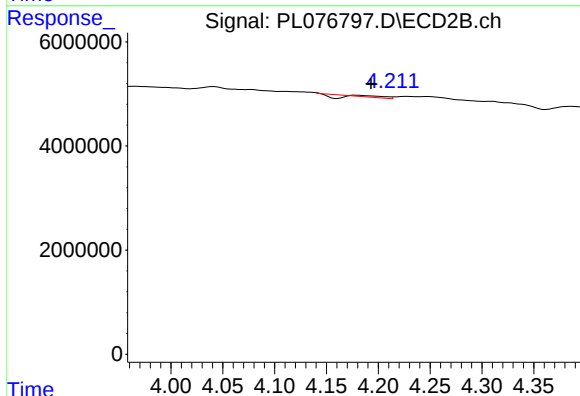


#24 Chlordane-2

R.T.: 4.178 min
Delta R.T.: -0.015 min
Response: 83007
Conc: 0.84 ng/ml

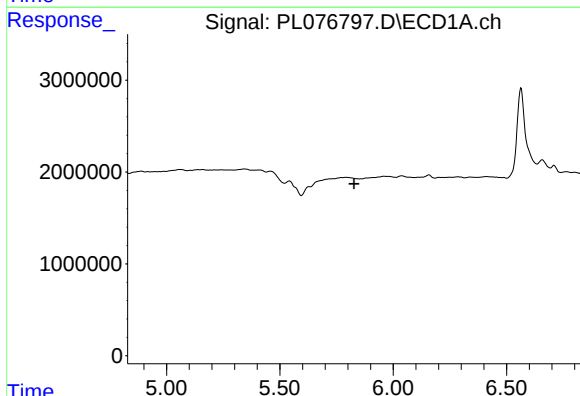


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

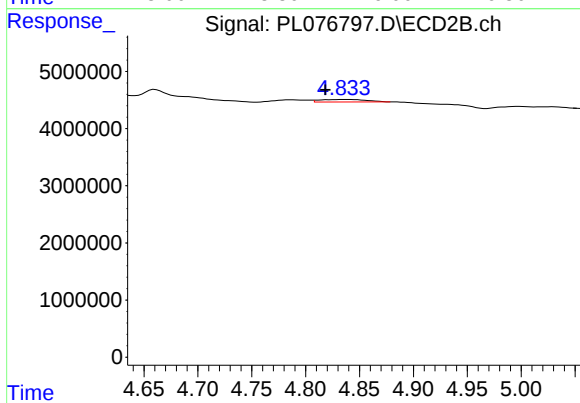

#25 Chlordane-3


R.T.: 4.835 min
Delta R.T.: 0.016 min
Response: 1327570
Conc: 4.81 ng/ml

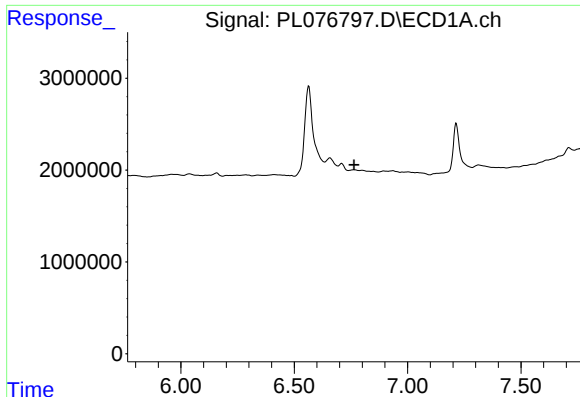

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

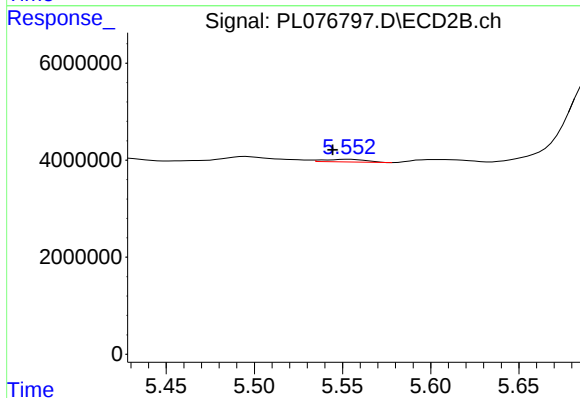


#27 Chlordane-5

R.T.: 5.554 min
Delta R.T.: 0.009 min
Response: 880901
Conc: 11.54 ng/ml

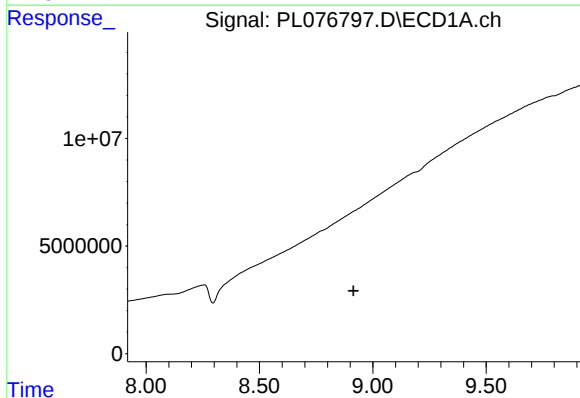

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.915 min
Response: 0
Conc: N.D.

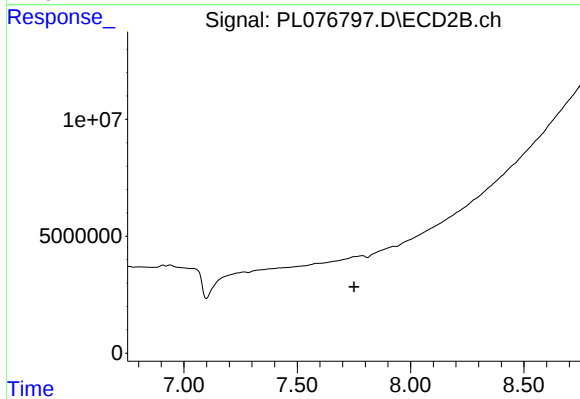

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.