

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 14:00
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:27:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 14:27:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	55337653	162.8E6	50.000	50.000
28)	SA Decachlor...	8.914	7.750	44260061	112.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.581	3.621	19339172	41377402	500.000	500.000
24)	Chlordane-2	5.116	4.193	21135860	50021073	500.000	500.000
25)	Chlordane-3	5.827	4.818	82411866	140.7E6	500.000	500.000
26)	Chlordane-4	5.906	4.879	100.1E6	146.2E6	500.000	500.000
27)	Chlordane-5	6.764	5.544	17919854	39238078	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 14:00
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:27:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 14:27:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

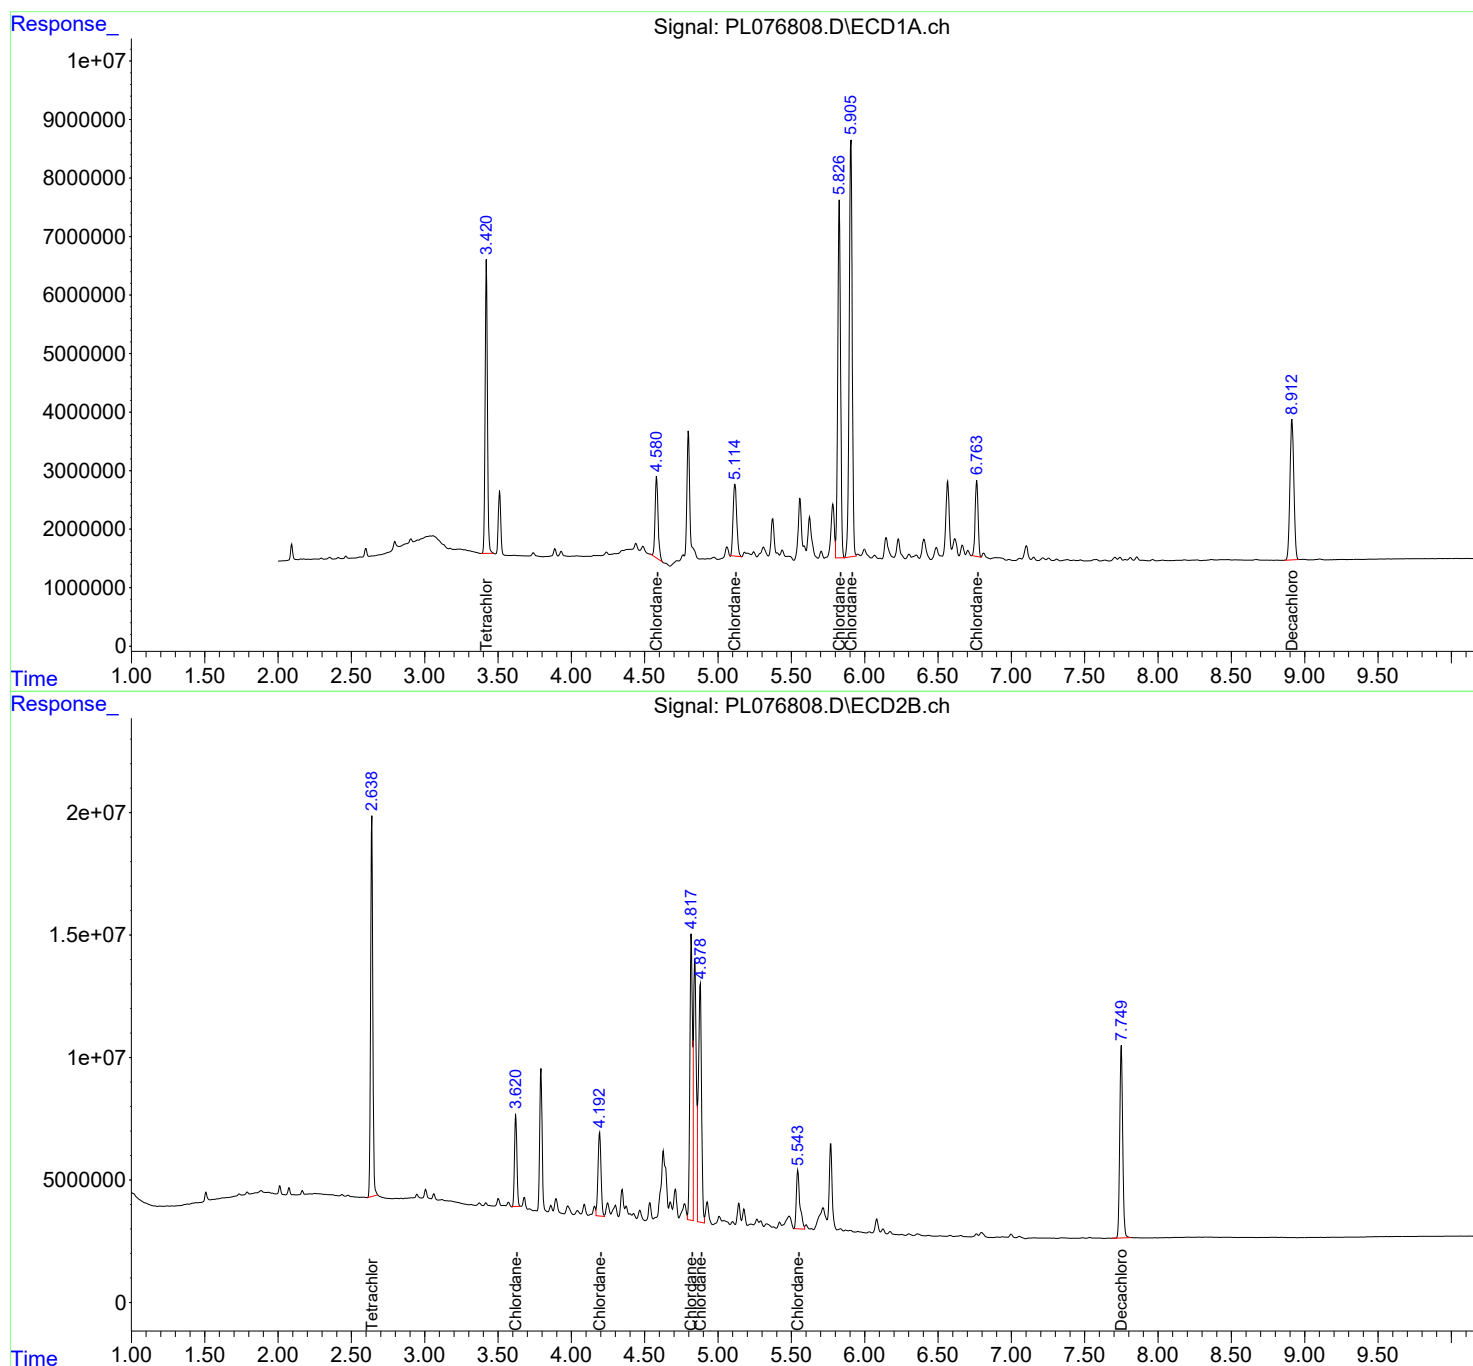


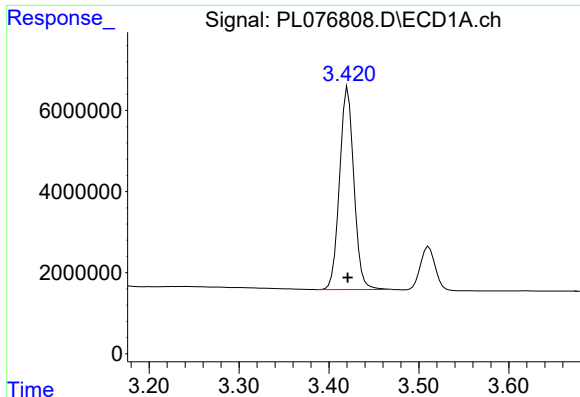

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 55337653
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

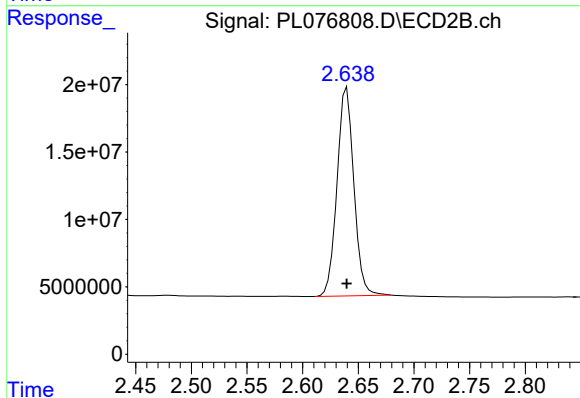


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 162829993
Conc: 50.00 ng/ml

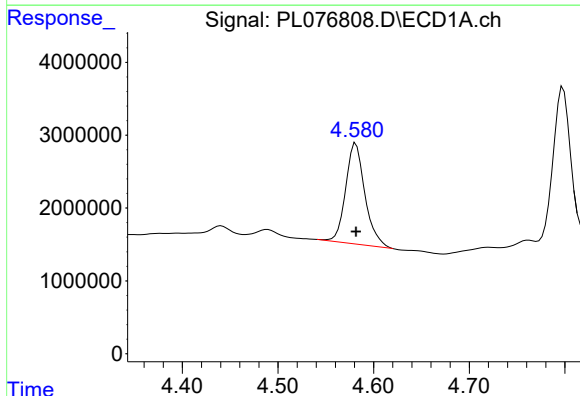


#23 Chlordane-1

R.T.: 4.581 min
Delta R.T.: 0.000 min
Response: 19339172
Conc: 500.00 ng/ml

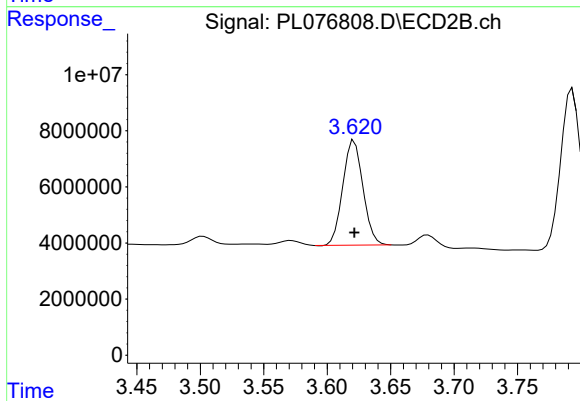

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 41377402
Conc: 500.00 ng/ml

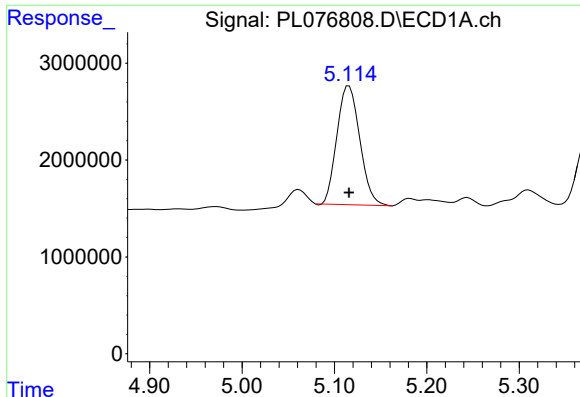

#24 Chlordane-2


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 21135860
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

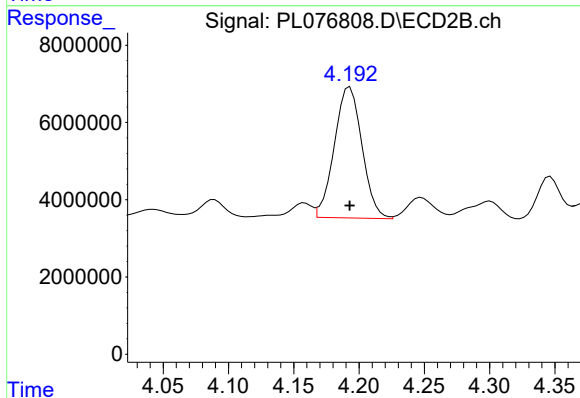


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 50021073
Conc: 500.00 ng/ml

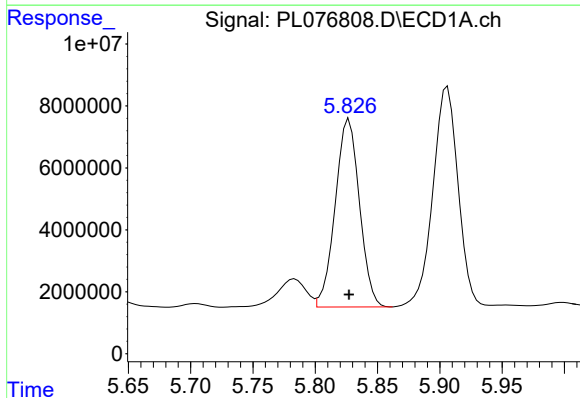


#25 Chlordane-3

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 82411866
Conc: 500.00 ng/ml

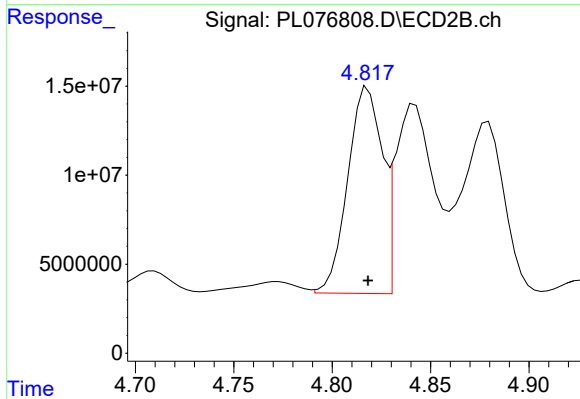

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 140723017
Conc: 500.00 ng/ml

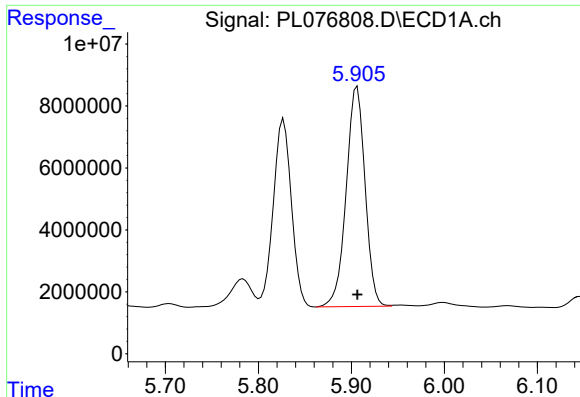

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 100089946
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

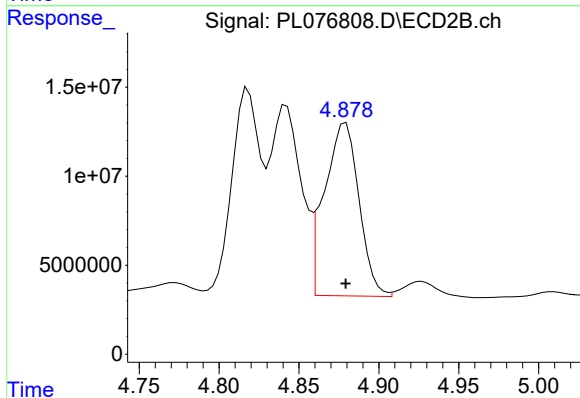


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 146197046
Conc: 500.00 ng/ml

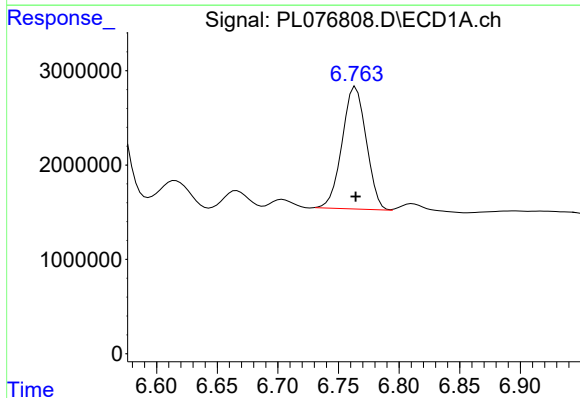


#27 Chlordane-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 17919854
Conc: 500.00 ng/ml

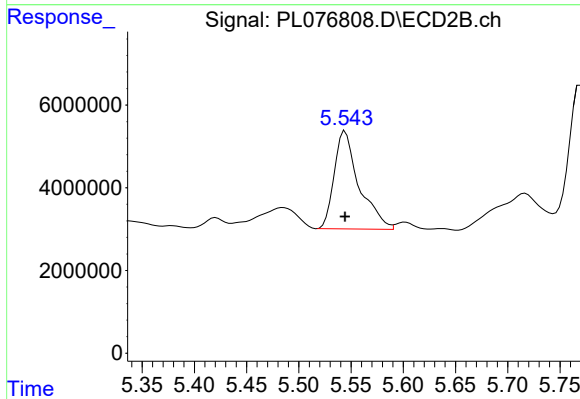

#27 Chlordane-5


R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 39238078
Conc: 500.00 ng/ml

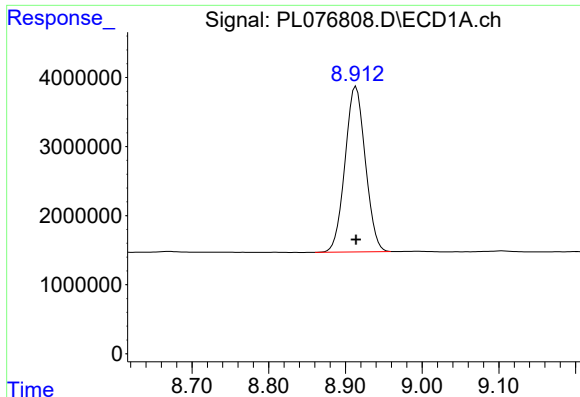

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 44260061
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

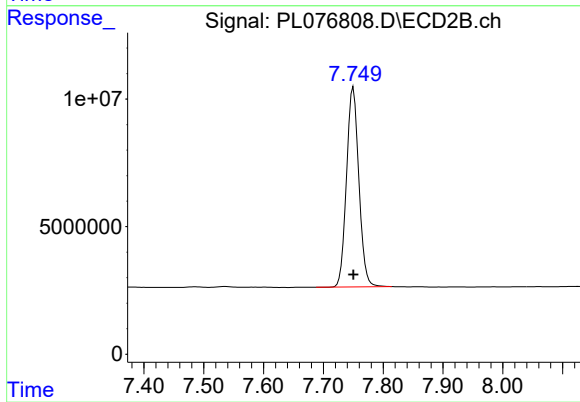

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 112261831
Conc: 50.00 ng/ml