

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 14:14
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:32:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 14:27:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	27037109	81124989	24.429	24.911
28)	SA Decachlor...	8.914	7.750	23092206	58456533	26.087	26.036
Target Compounds							
23)	Chlordane-1	4.582	3.622	9428220	20494459	243.760	247.653
24)	Chlordane-2	5.115	4.193	10967701	25451322	259.457	254.406
25)	Chlordane-3	5.827	4.818	40097717	69518350	243.276	247.004
26)	Chlordane-4	5.906	4.880	49292150	71780823	246.239	245.493
27)	Chlordane-5	6.764	5.544	8944810	19746420	249.578	251.623



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 14:14
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:32:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 14:27:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

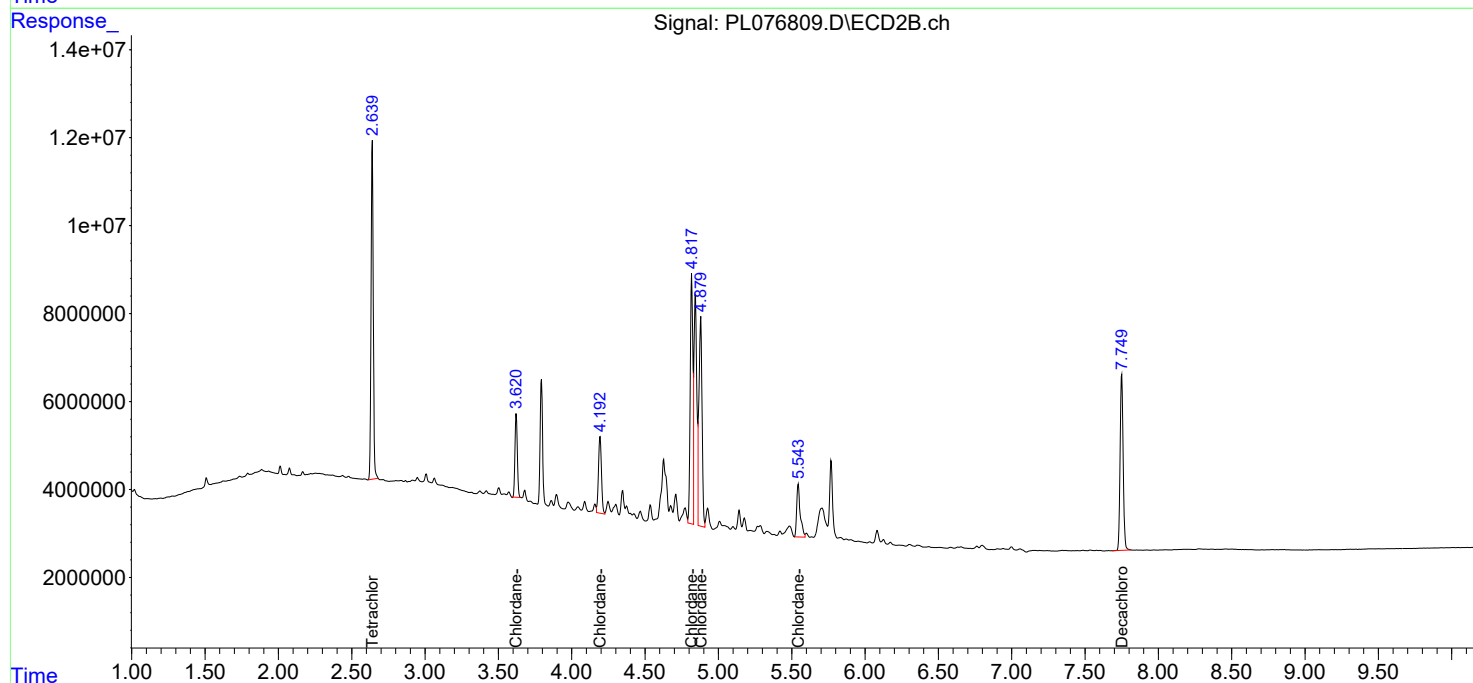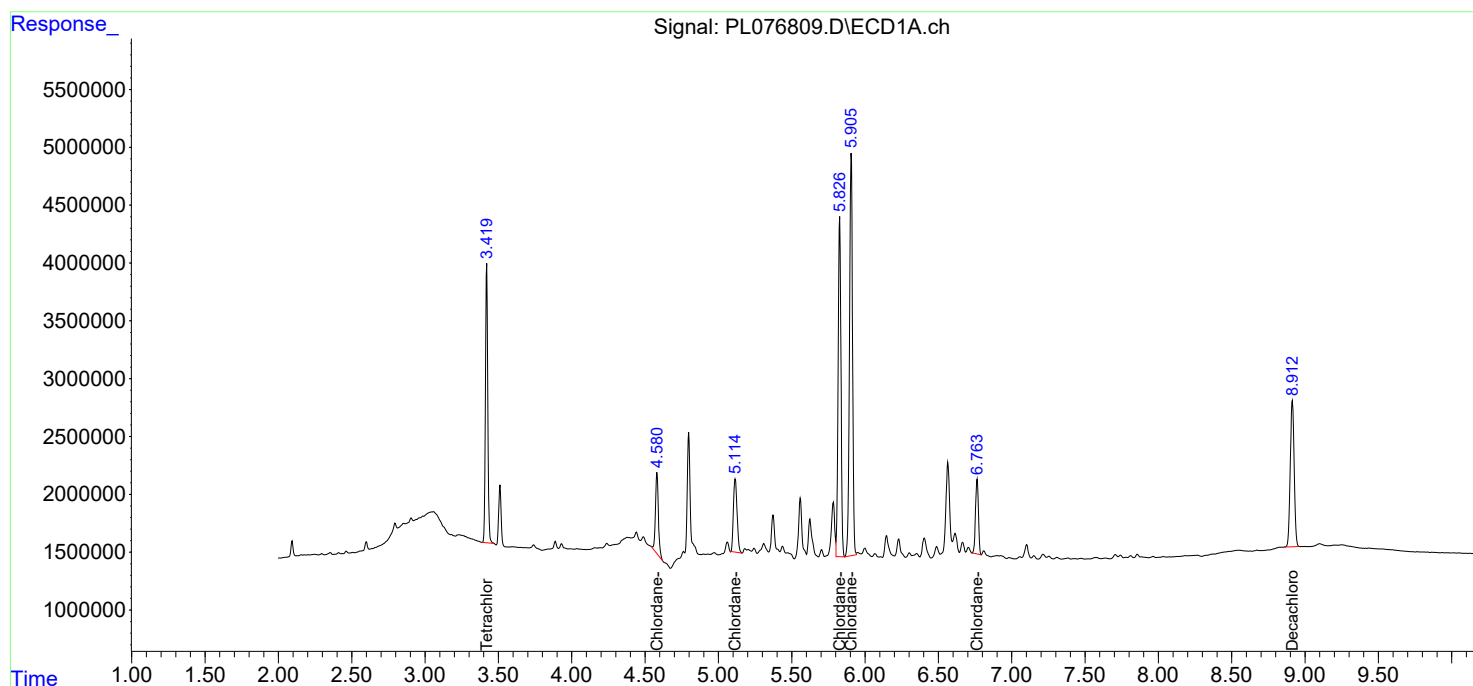


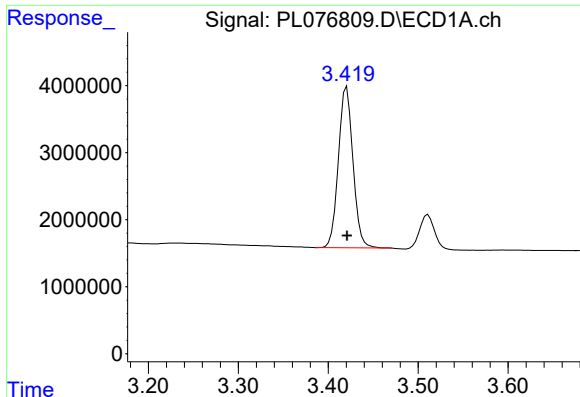

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 27037109
Conc: 24.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

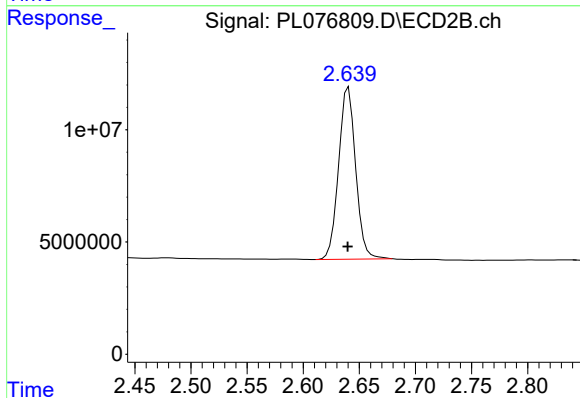


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 81124989
Conc: 24.91 ng/ml

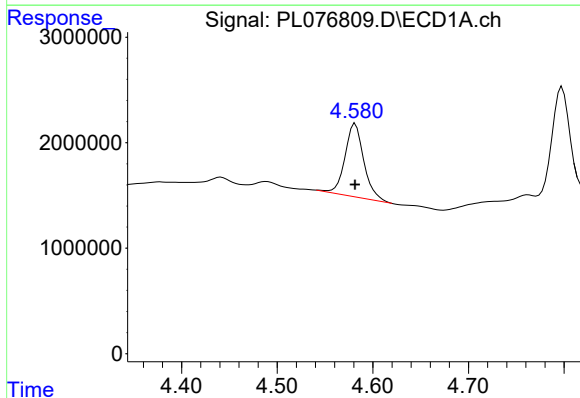


#23 Chlordane-1

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 9428220
Conc: 243.76 ng/ml

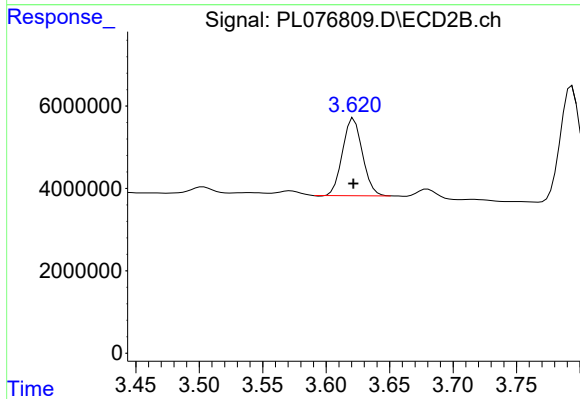

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 20494459
Conc: 247.65 ng/ml

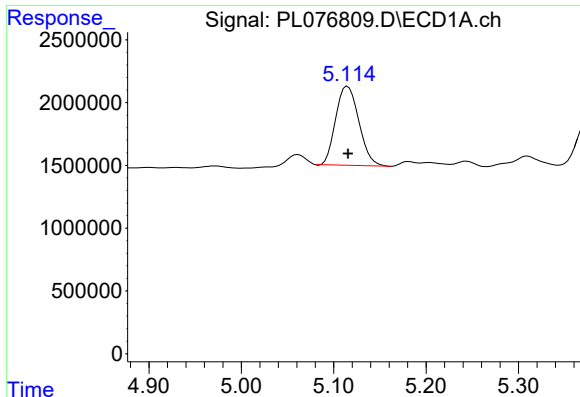

#24 Chlordane-2


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 10967701
Conc: 259.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

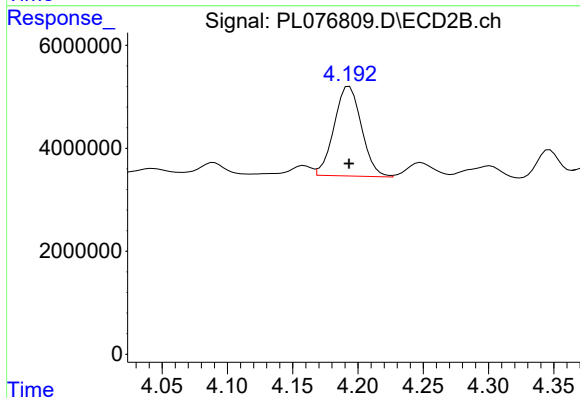


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 25451322
Conc: 254.41 ng/ml

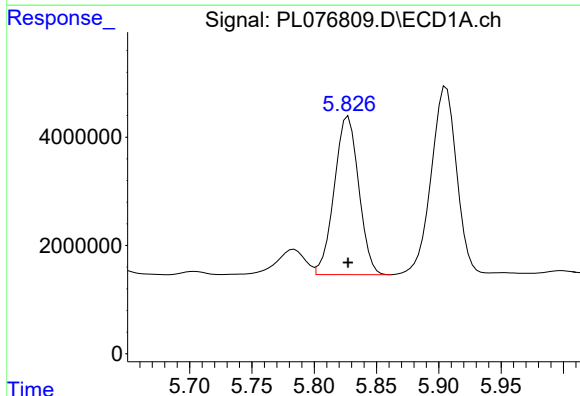


#25 Chlordane-3

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 40097717
Conc: 243.28 ng/ml

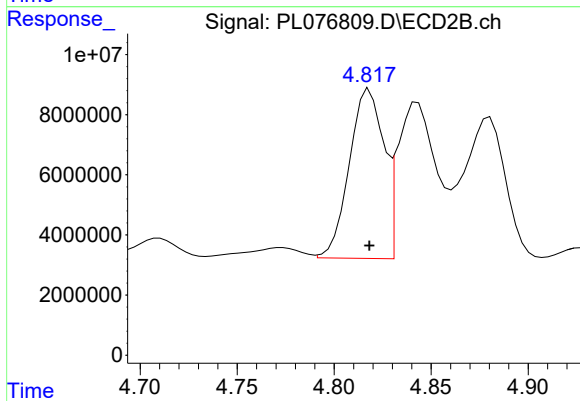

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 69518350
Conc: 247.00 ng/ml

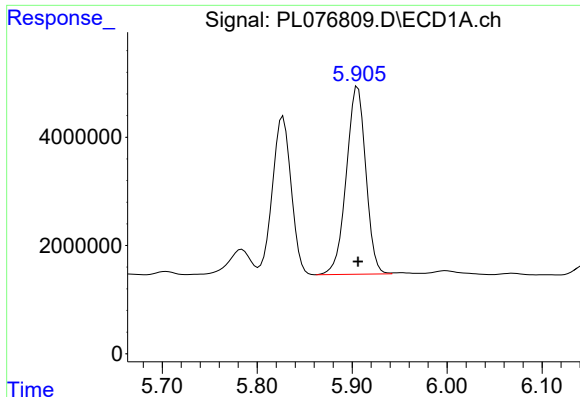

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 49292150
Conc: 246.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

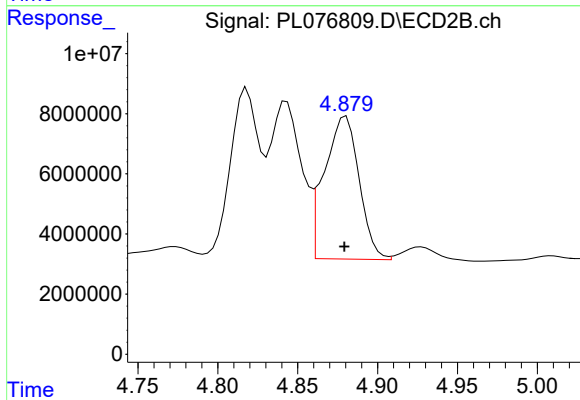


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 71780823
Conc: 245.49 ng/ml

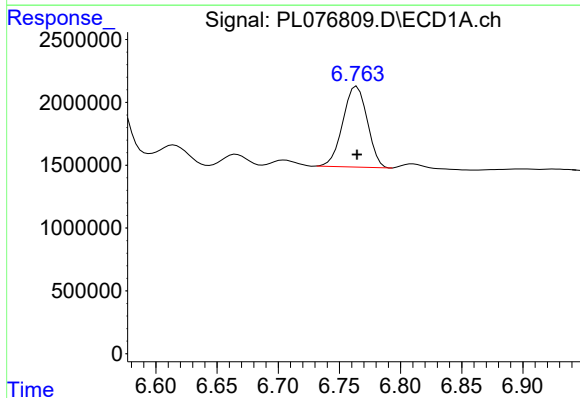


#27 Chlordane-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 8944810
Conc: 249.58 ng/ml

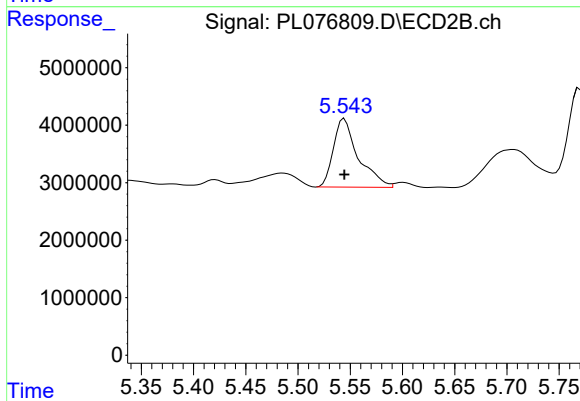

#27 Chlordane-5


R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 19746420
Conc: 251.62 ng/ml

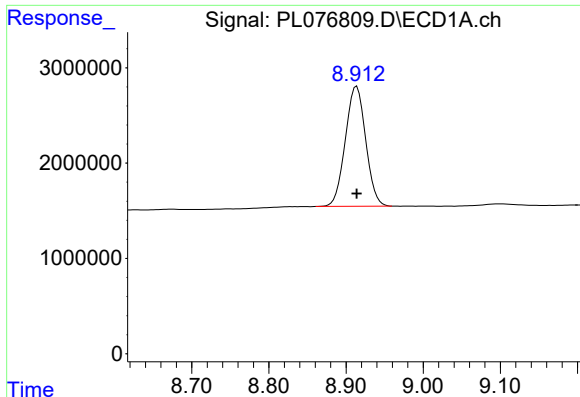

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 23092206
Conc: 26.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

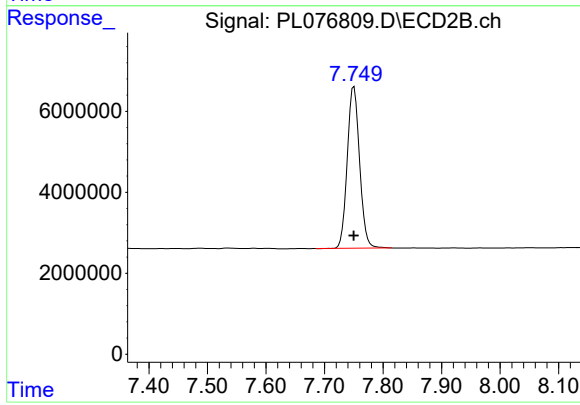

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 58456533
Conc: 26.04 ng/ml