

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 14:28
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:49:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 14:27:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.641	4908799	14707022	4.459	4.561
28)	SA Decachlor...	8.913	7.749	4870070	11594421	5.730	5.337
Target Compounds							
23)	Chlordane-1	4.580	3.621	1778587	3660579	46.612	45.055
24)	Chlordane-2	5.115	4.193	2094723	5010435	51.335	51.753
25)	Chlordane-3	5.826	4.817	7608382	13131729	46.141	47.003
26)	Chlordane-4	5.905	4.879	9365185	14291132	47.088	49.316
27)	Chlordane-5	6.763	5.544	1639095	3702648	46.454	48.589



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 14:28
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:49:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 14:27:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

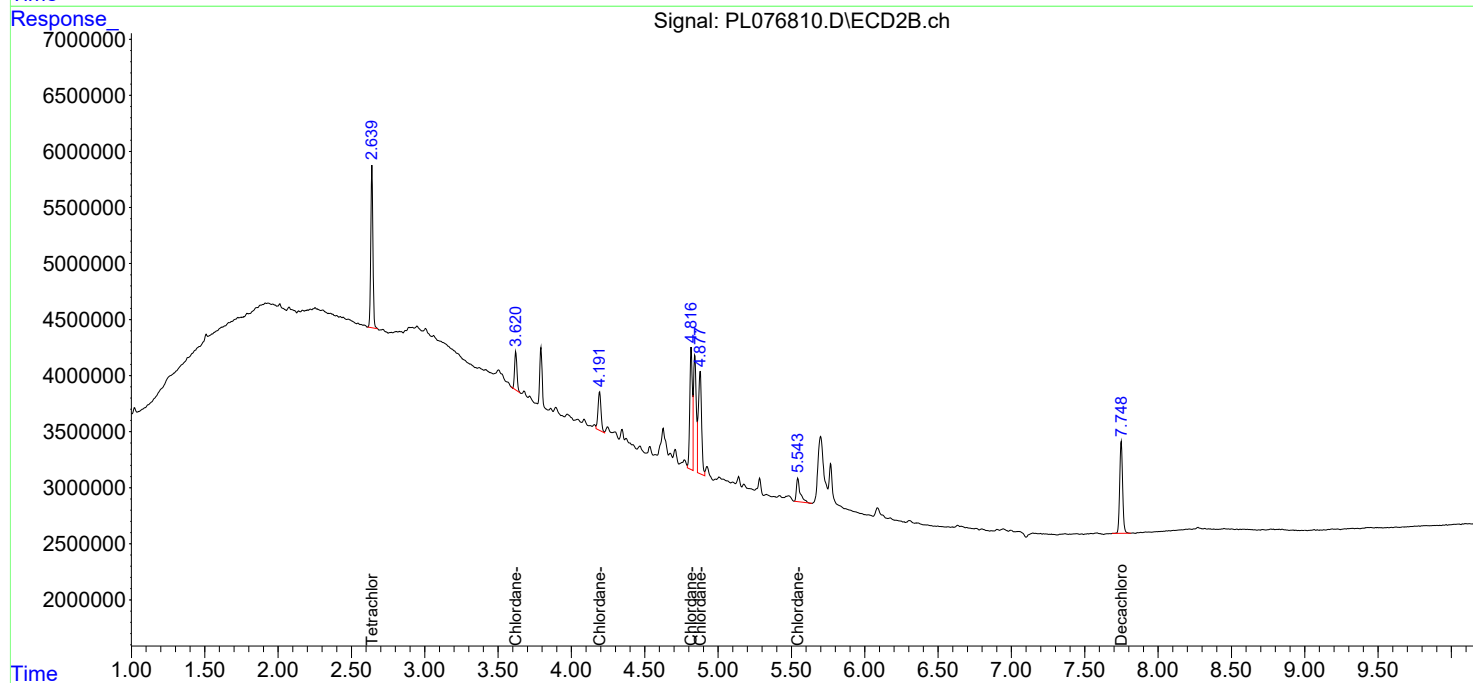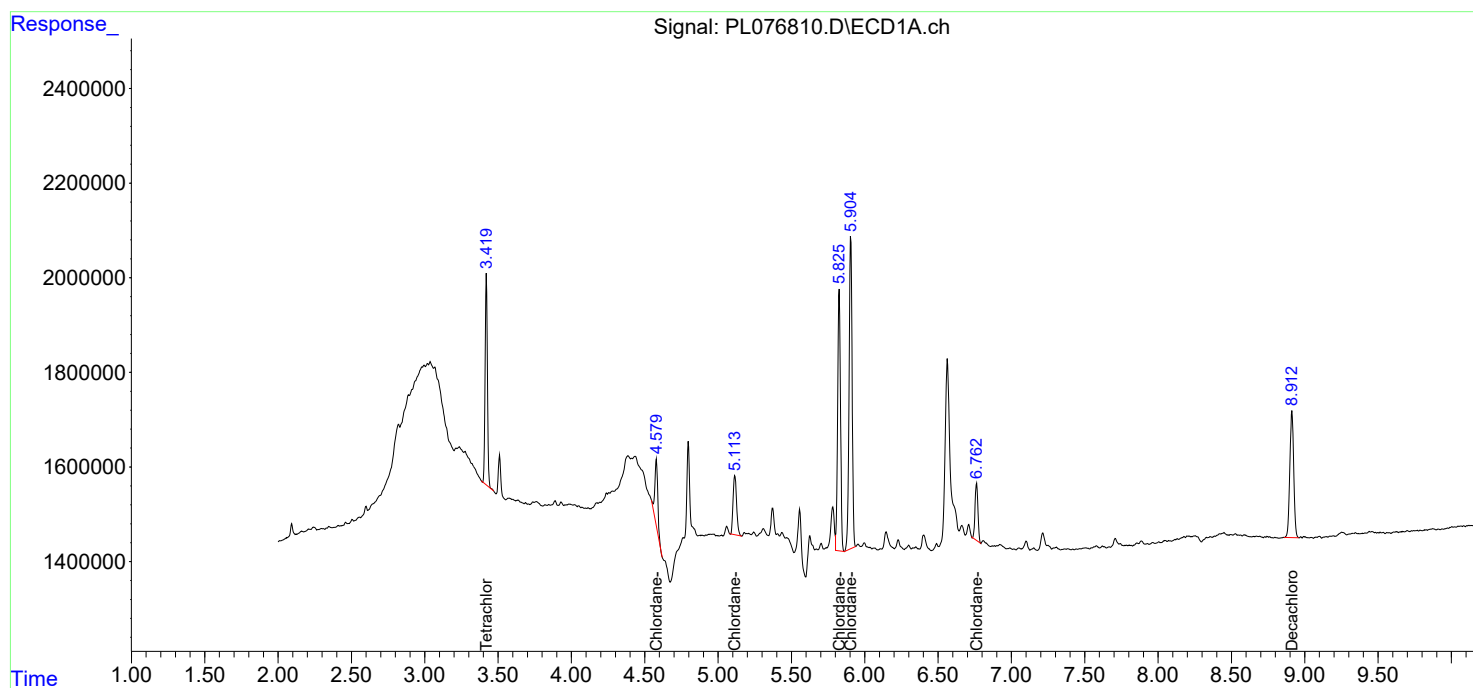


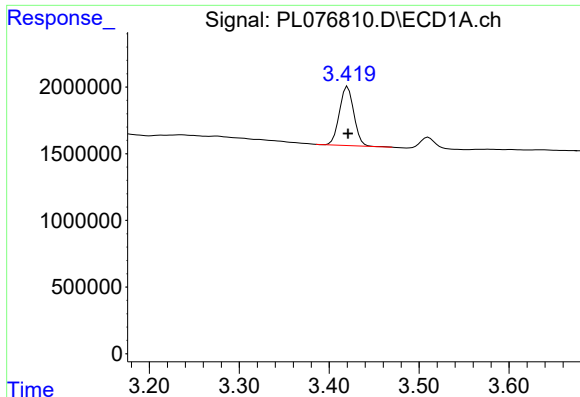

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 4908799
Conc: 4.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

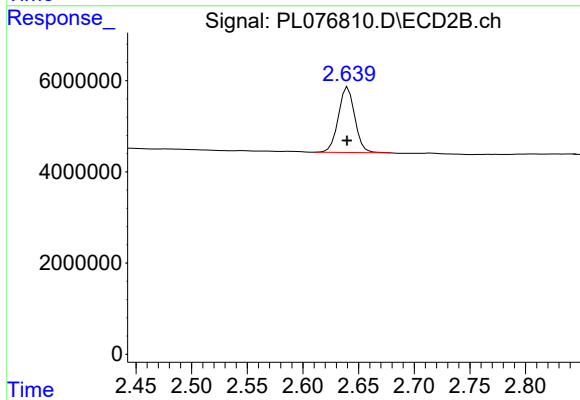


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 14707022
Conc: 4.56 ng/ml

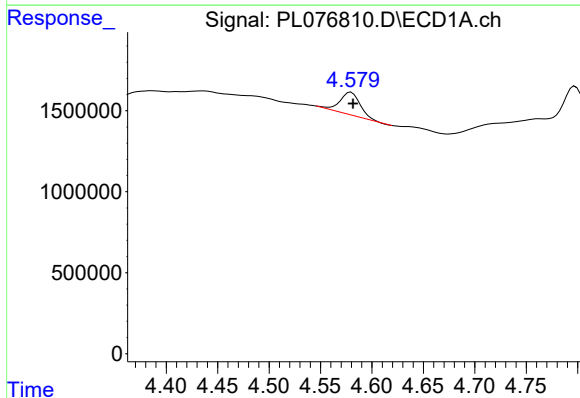


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: -0.002 min
Response: 1778587
Conc: 46.61 ng/ml

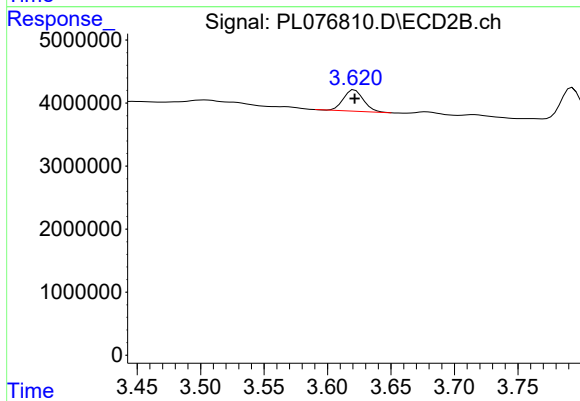

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 3660579
Conc: 45.05 ng/ml

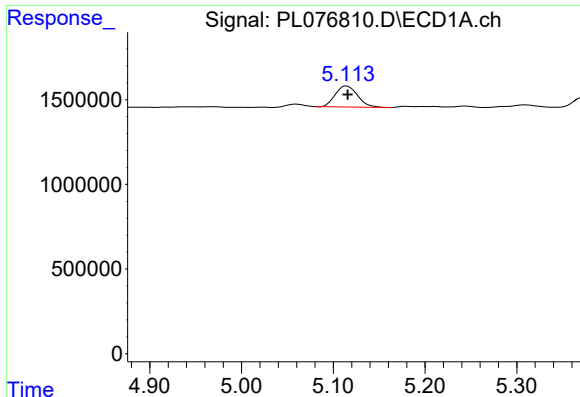

#24 Chlordane-2


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 2094723
Conc: 51.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

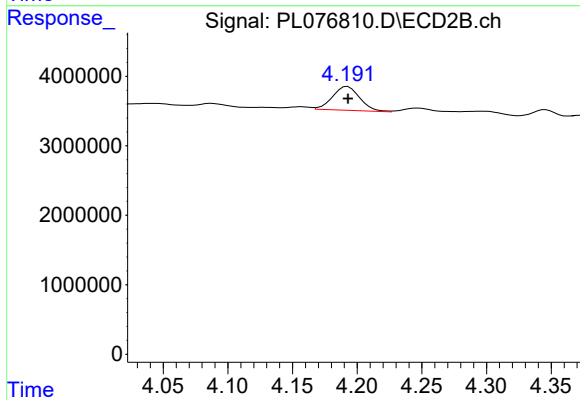


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 5010435
Conc: 51.75 ng/ml

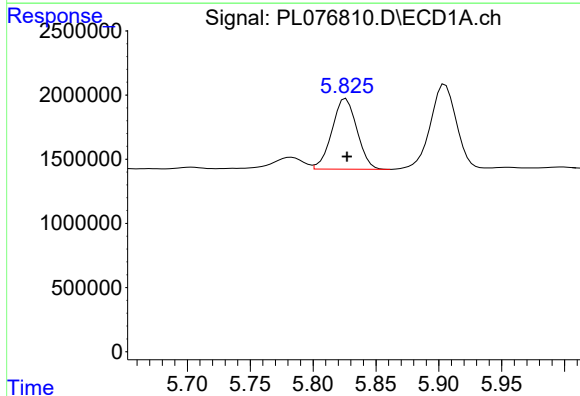


#25 Chlordane-3

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 7608382
Conc: 46.14 ng/ml

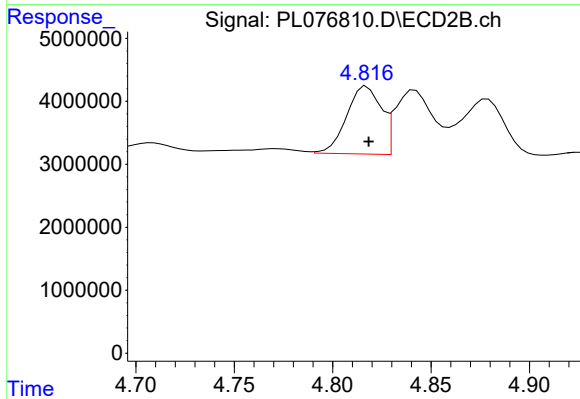

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 13131729
Conc: 47.00 ng/ml

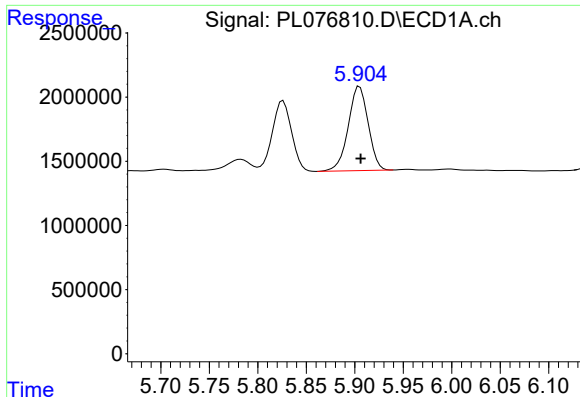

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: -0.001 min
Response: 9365185
Conc: 47.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

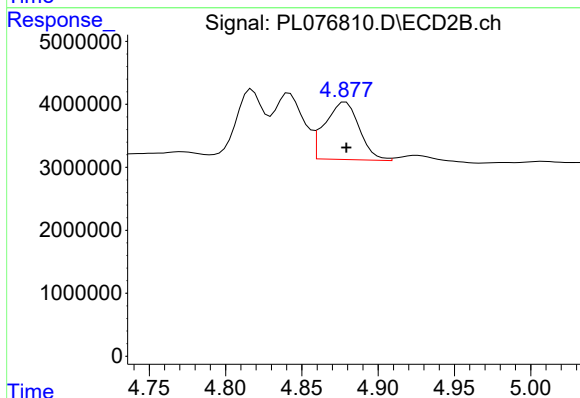


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 14291132
Conc: 49.32 ng/ml

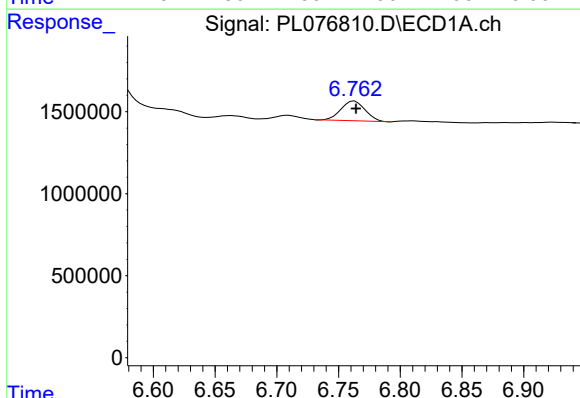


#27 Chlordane-5

R.T.: 6.763 min
Delta R.T.: -0.001 min
Response: 1639095
Conc: 46.45 ng/ml

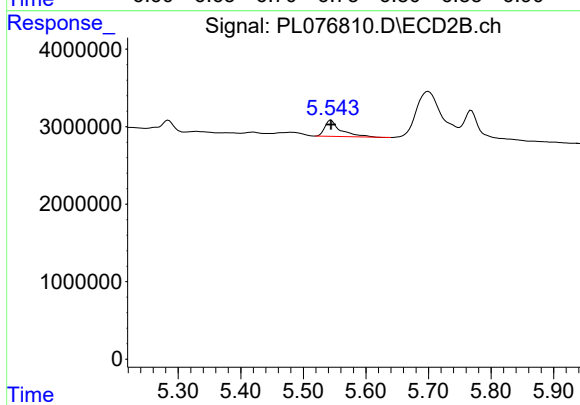

#27 Chlordane-5


R.T.: 5.544 min
Delta R.T.: 0.000 min
Response: 3702648
Conc: 48.59 ng/ml

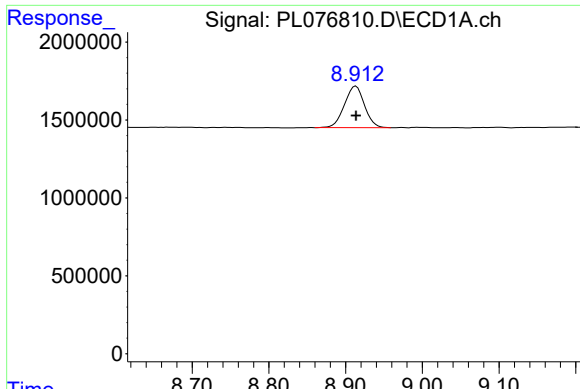

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.000 min
Response: 4870070
Conc: 5.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

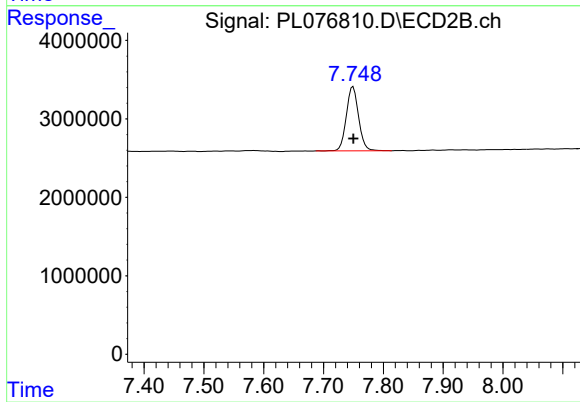

#28 Decachlorobiphenyl

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 11594421
Conc: 5.34 ng/ml