

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 16:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 04:23:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.640	20697668	52913052	21.741	22.925
28)	SA Decachlor...	8.910	7.747	19694688	49480091	24.784	25.736
Target Compounds							
4)	MA Heptachlor	4.792	0.000	938562	0	0.767	N.D. #
5)	MB Aldrin	0.000	4.084	0	507776	N.D.	0.183 #
6)	B beta-BHC	0.000	3.761	0	345232	N.D.	0.283 #
10)	B gamma-Chl...	0.000	4.816	0	917309	N.D.	0.375 #
12)	B 4,4'-DDE	0.000	5.074	0	186831	N.D.	0.080 #
13)	MA Dieldrin	0.000	5.197	0	580331	N.D.	0.239 #
15)	B Endosulfa...	6.711f	0.000	631375	0	0.704	N.D. #
16)	A 4,4'-DDD	0.000	5.624	0	3922798	N.D.	2.101 #
21)	B Endrin ke...	7.572f	0.000	252821	0	0.271	N.D. #
25)	Chlordane-3	0.000	4.816	0	917309	N.D.	3.326 #
27)	Chlordane-5	0.000	5.566f	0	1128301	N.D.	14.782 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 16:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 04:23:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

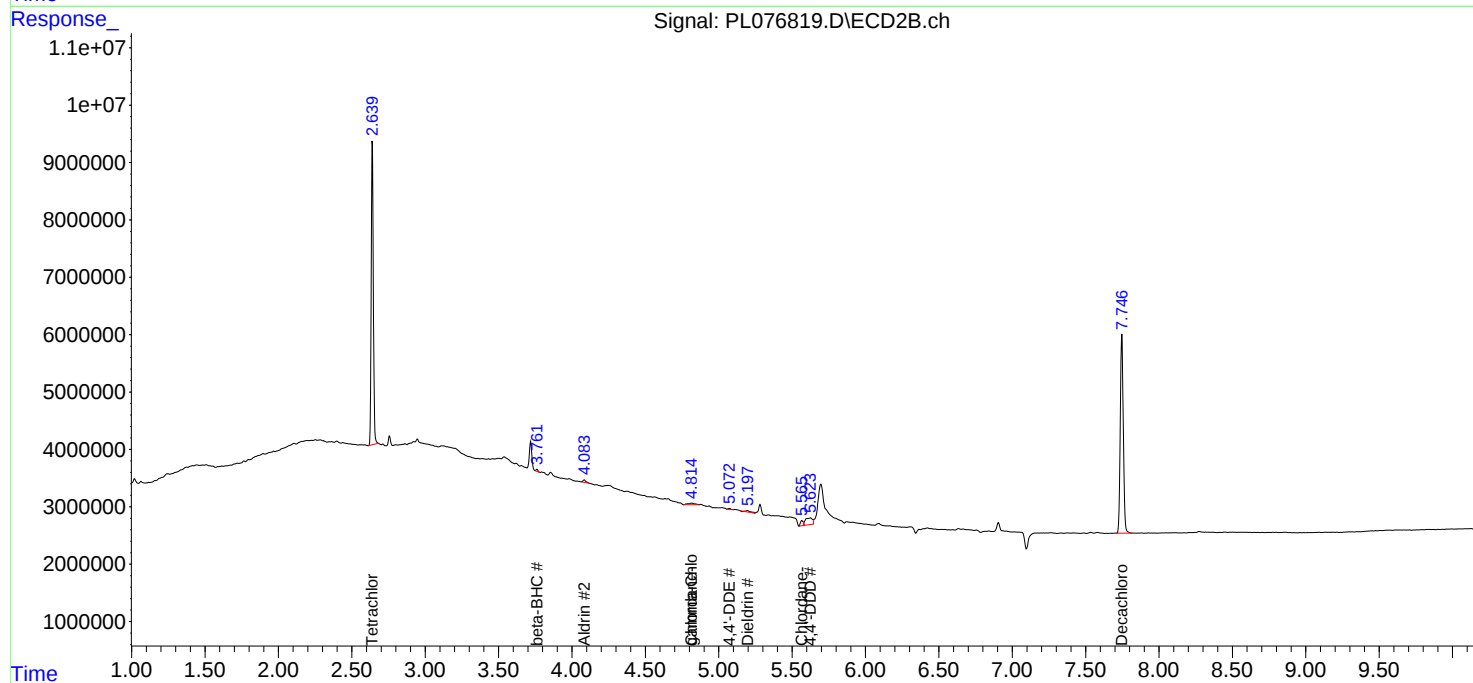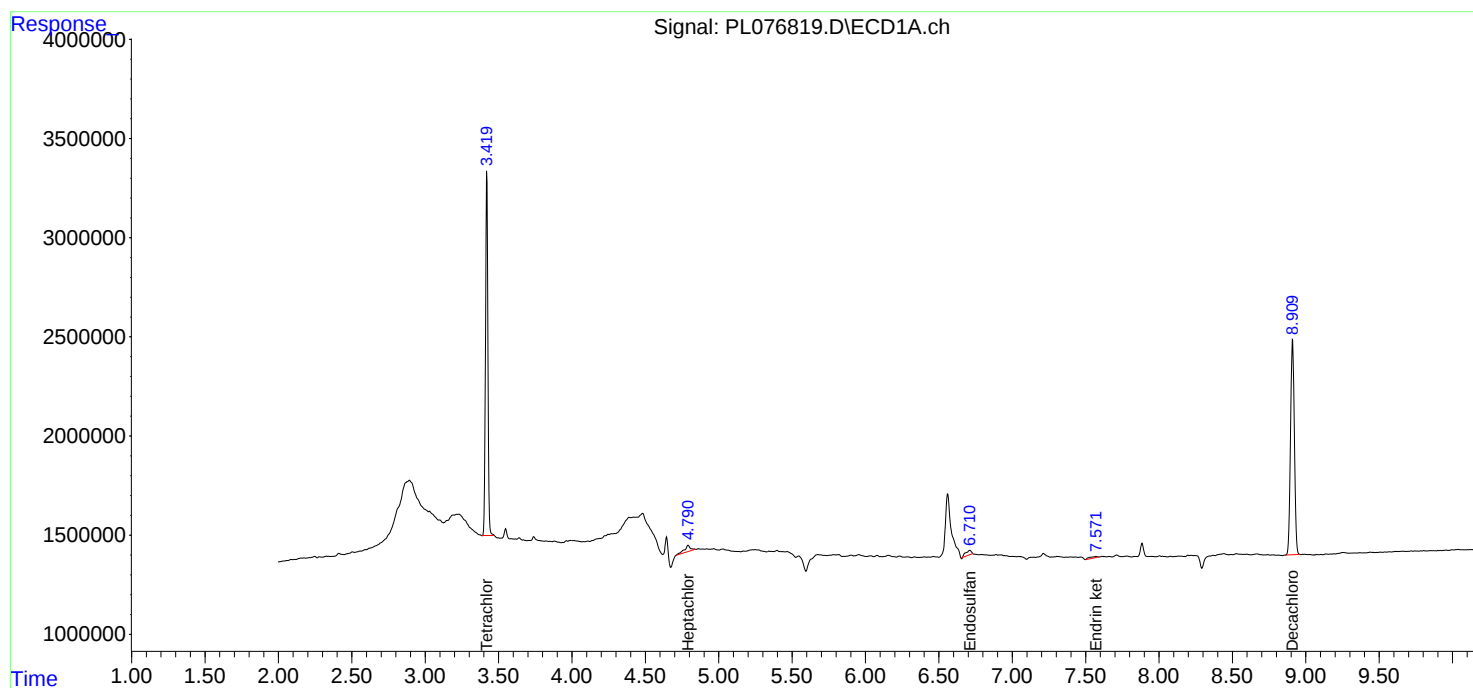


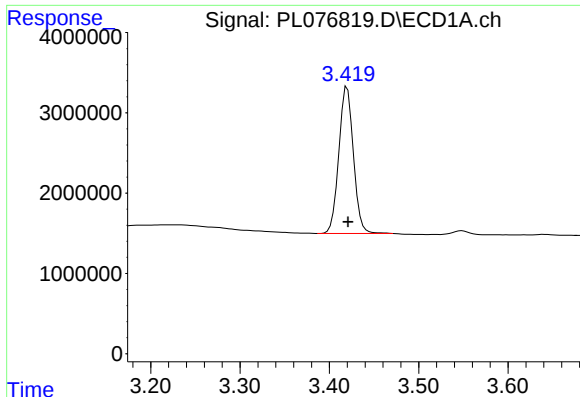

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 20697668
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

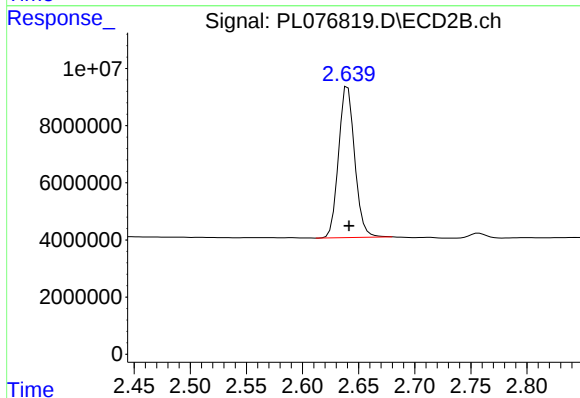


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.001 min
Response: 52913052
Conc: 22.92 ng/ml

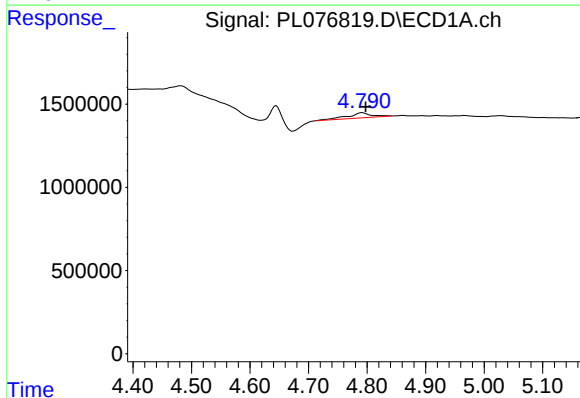


#4 Heptachlor

R.T.: 4.792 min
Delta R.T.: -0.006 min
Response: 938562
Conc: 0.77 ng/ml

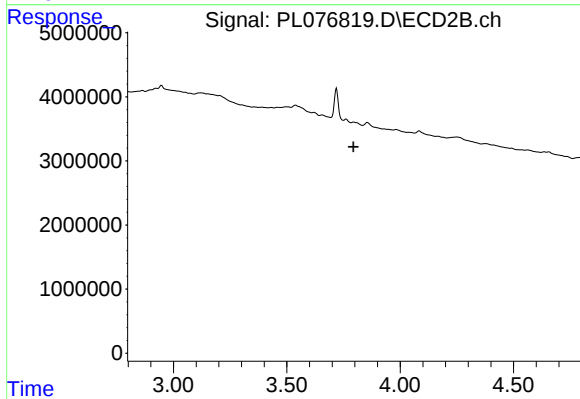

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.794 min
Response: 0
Conc: N.D.

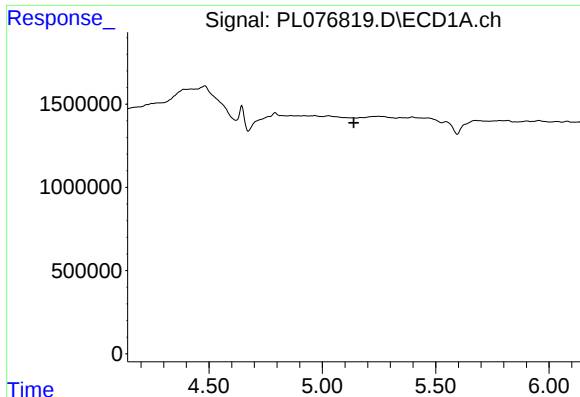

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

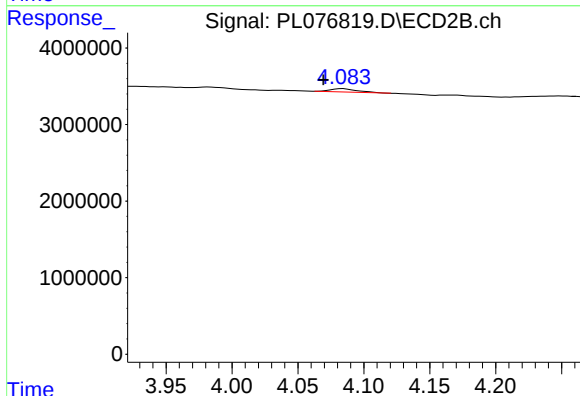


#5 Aldrin

R.T.: 4.084 min
Delta R.T.: 0.015 min
Response: 507776
Conc: 0.18 ng/ml

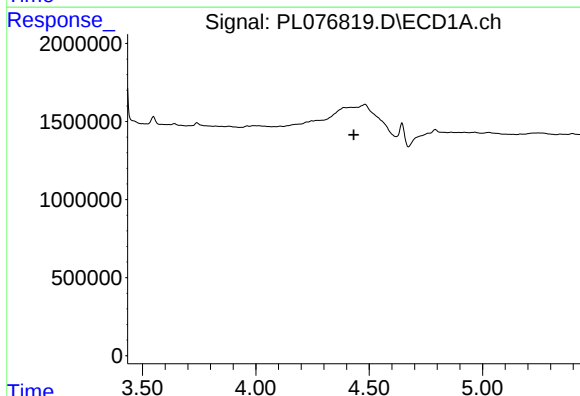


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.433 min
Response: 0
Conc: N.D.

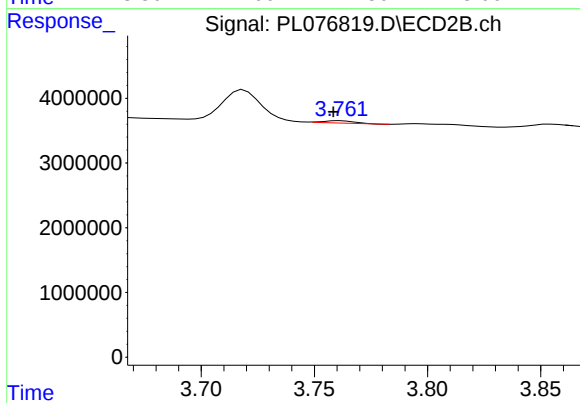

#6 beta-BHC


R.T.: 3.761 min
Delta R.T.: 0.003 min
Response: 345232
Conc: 0.28 ng/ml

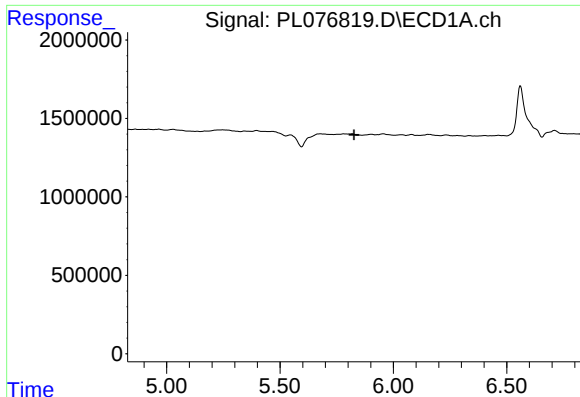

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

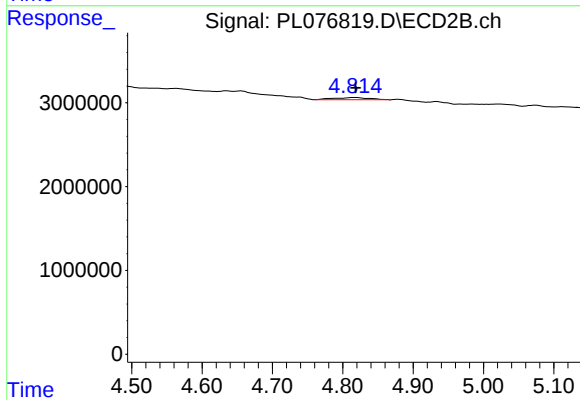


#10 gamma-Chlordane

R.T.: 4.816 min
Delta R.T.: -0.003 min
Response: 917309
Conc: 0.37 ng/ml

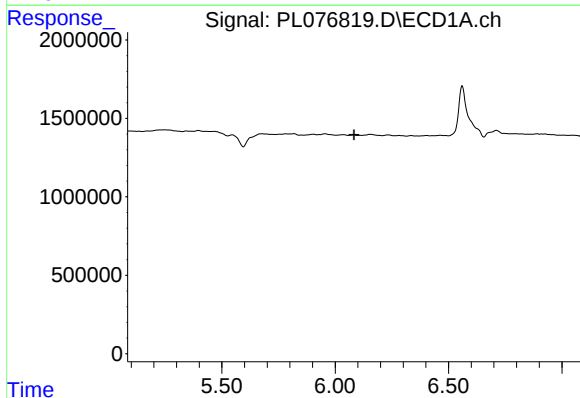


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.083 min
Response: 0
Conc: N.D.

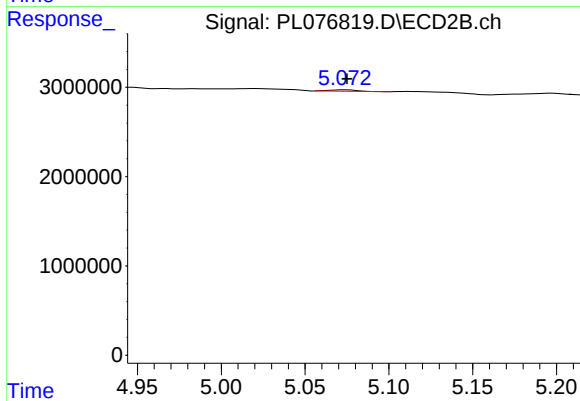

#12 4,4'-DDE


R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 186831
Conc: 0.08 ng/ml

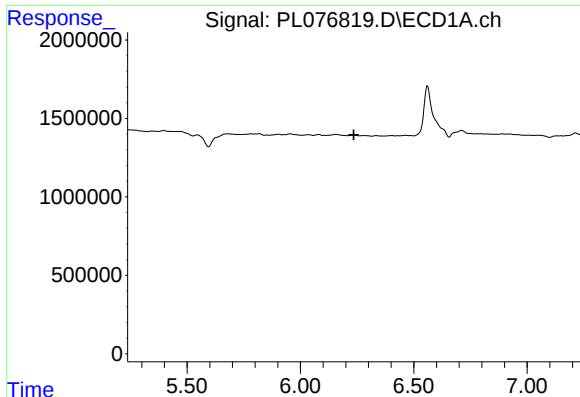

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

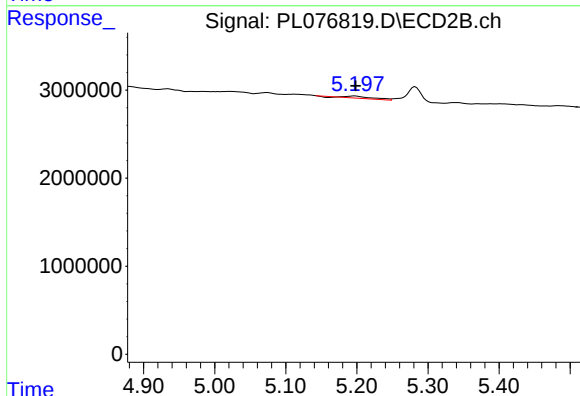


#13 Dieldrin

R.T.: 5.197 min
Delta R.T.: -0.001 min
Response: 580331
Conc: 0.24 ng/ml

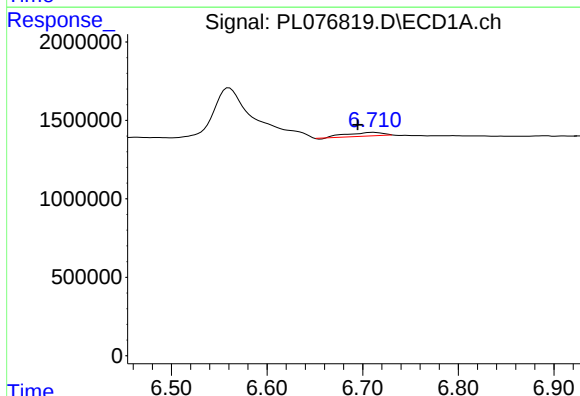


#15 Endosulfan II

R.T.: 6.711 min
Delta R.T.: 0.016 min
Response: 631375
Conc: 0.70 ng/ml

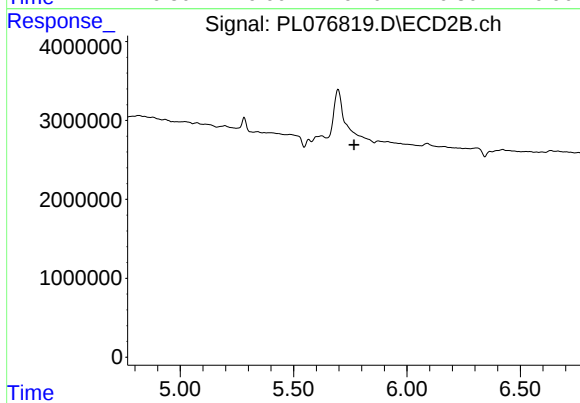

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.767 min
Response: 0
Conc: N.D.

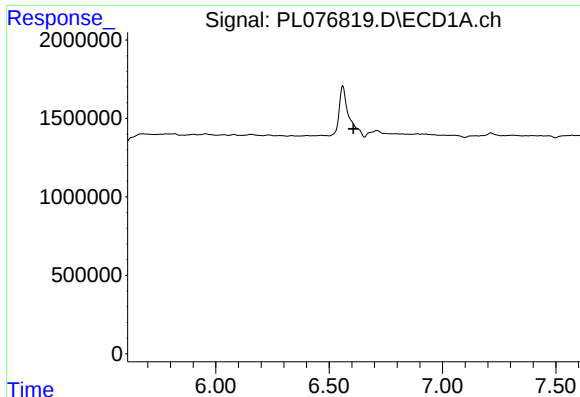

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.608 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

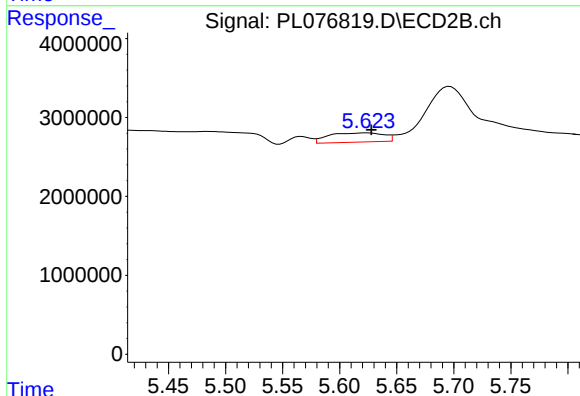


#16 4,4'-DDD

R.T.: 5.624 min
Delta R.T.: -0.004 min
Response: 3922798
Conc: 2.10 ng/ml

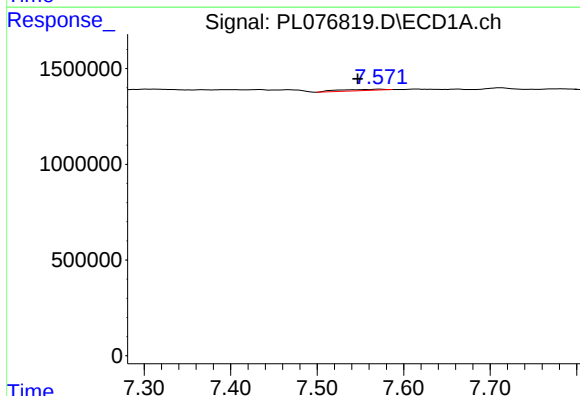


#21 Endrin ketone

R.T.: 7.572 min
Delta R.T.: 0.025 min
Response: 252821
Conc: 0.27 ng/ml

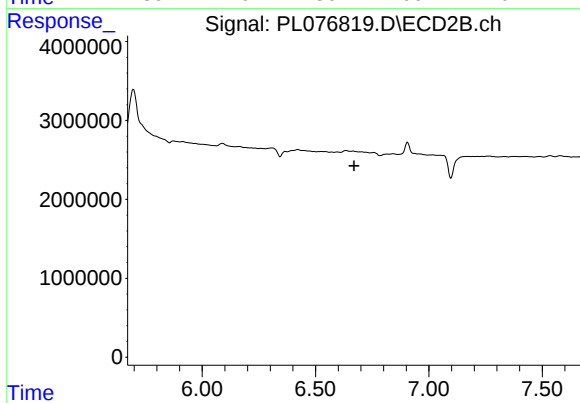

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.670 min
Response: 0
Conc: N.D.

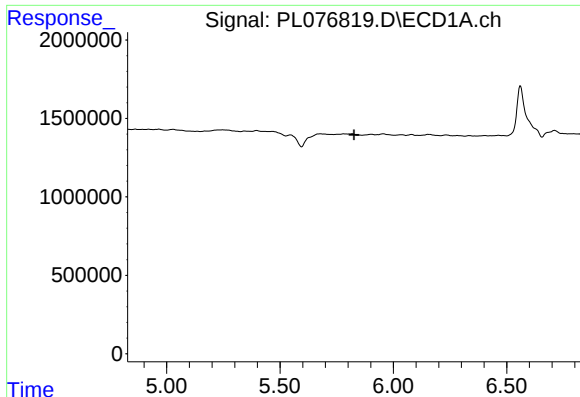

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

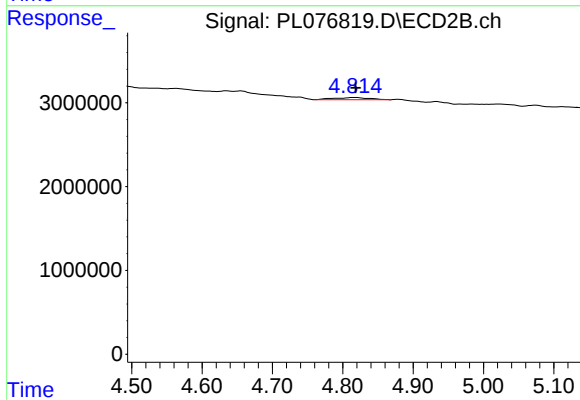


#25 Chlordane-3

R.T.: 4.816 min
Delta R.T.: -0.002 min
Response: 917309
Conc: 3.33 ng/ml

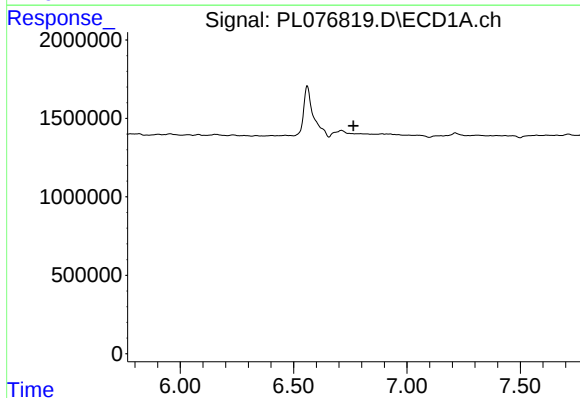


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

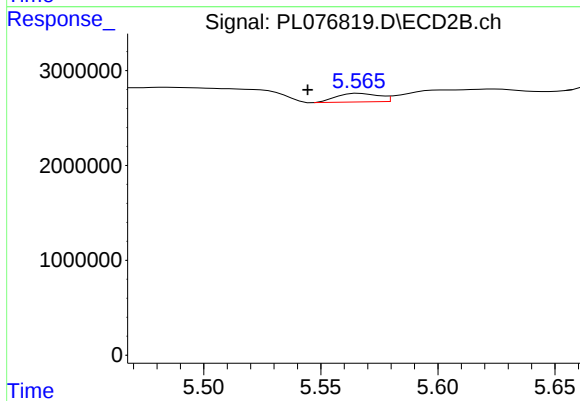

#27 Chlordane-5


R.T.: 5.566 min
Delta R.T.: 0.022 min
Response: 1128301
Conc: 14.78 ng/ml

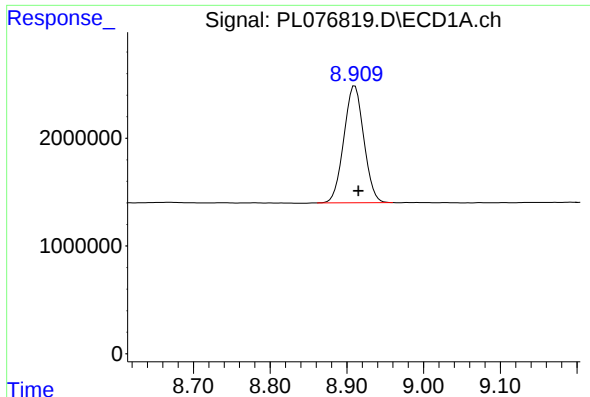

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: -0.005 min
Response: 19694688
Conc: 24.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

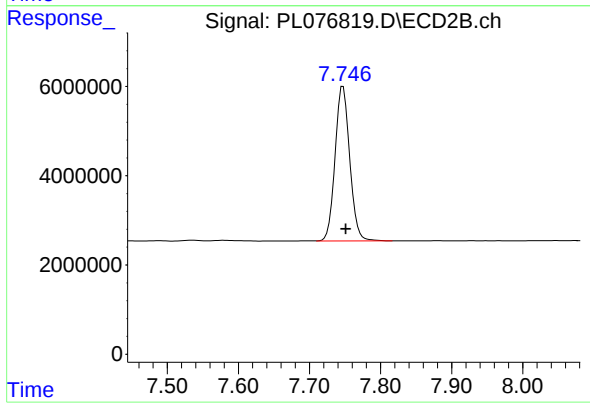

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: -0.004 min
Response: 49480091
Conc: 25.74 ng/ml