

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 13:33
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:31:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 14:27:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.641	109.5E6	317.9E6	98.965	97.604
28)	SA Decachlor...	8.914	7.750	81851368	210.7E6	92.466	93.860
Target Compounds							
23)	Chlordane-1	4.582	3.622	37599573	79773759	972.109	963.977
24)	Chlordane-2	5.115	4.194	39564185	93614799	935.949	935.754
25)	Chlordane-3	5.828	4.819	164.9E6	275.6E6	1000.670	979.392
26)	Chlordane-4	5.906	4.881	197.9E6	286.7E6	988.570	980.485
27)	Chlordane-5	6.765	5.545	34827233	74271320	971.750	946.419



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 13:33
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:31:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 14:27:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

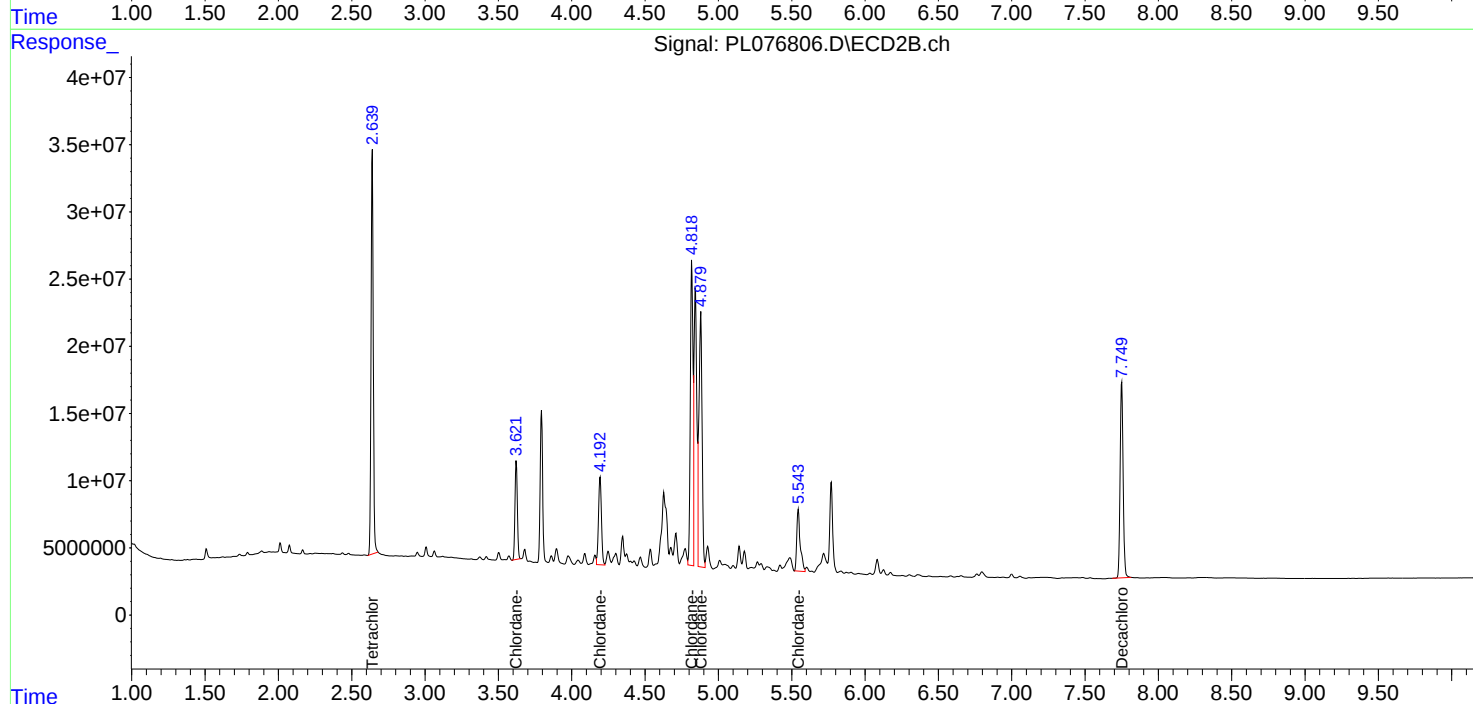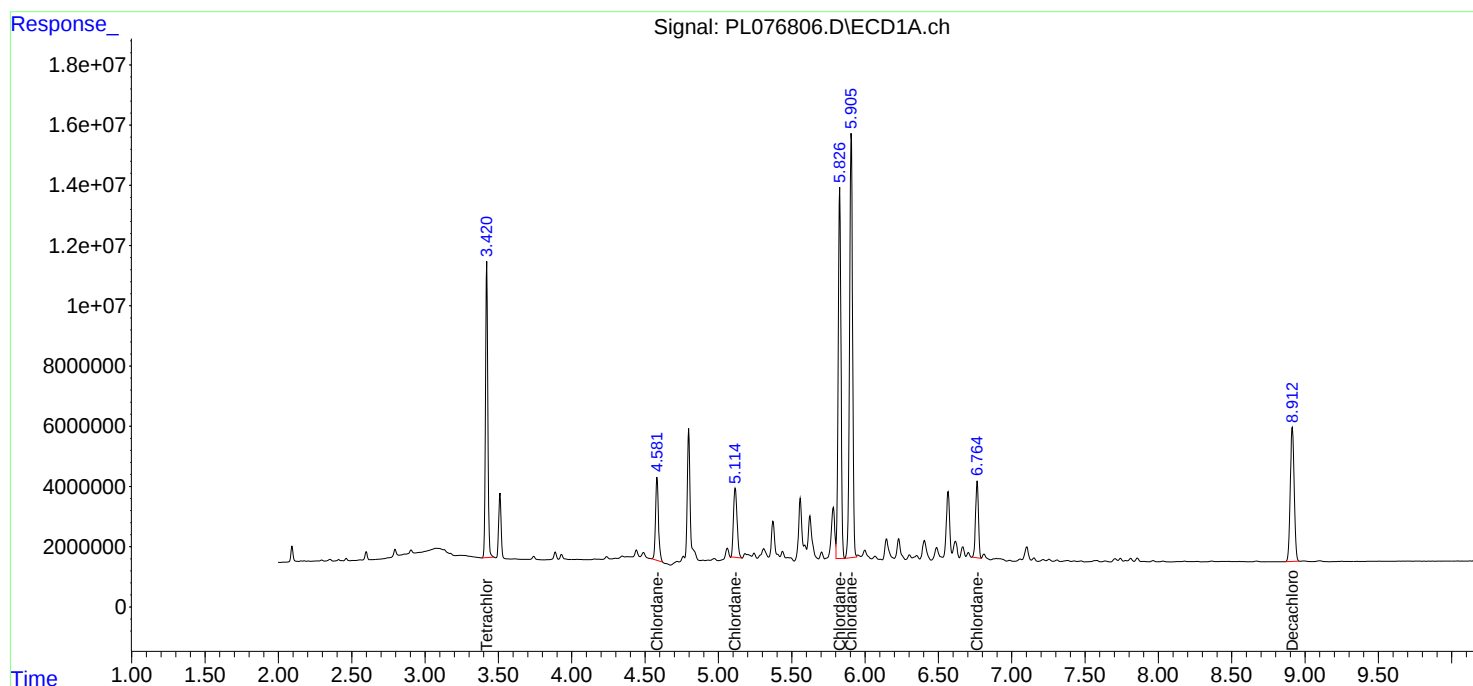


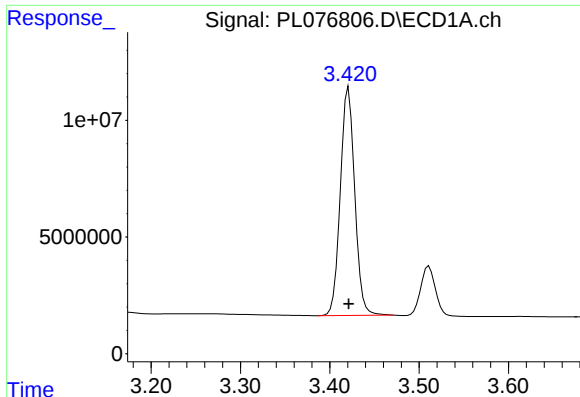

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 109529400
Conc: 98.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

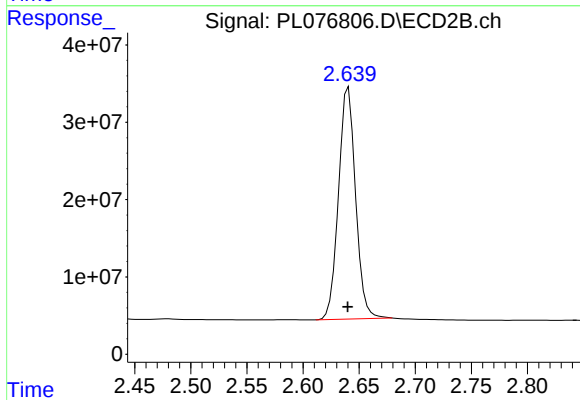


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 317857645
Conc: 97.60 ng/ml

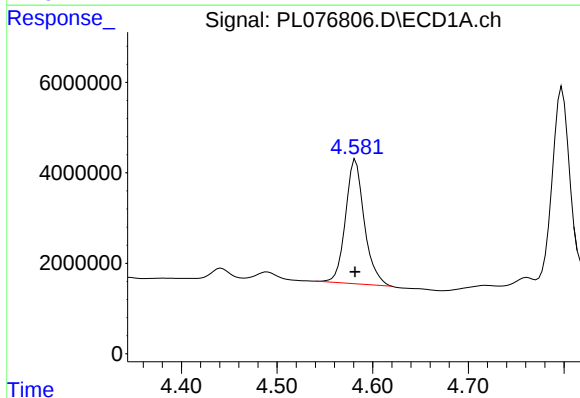


#23 Chlordane-1

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 37599573
Conc: 972.11 ng/ml

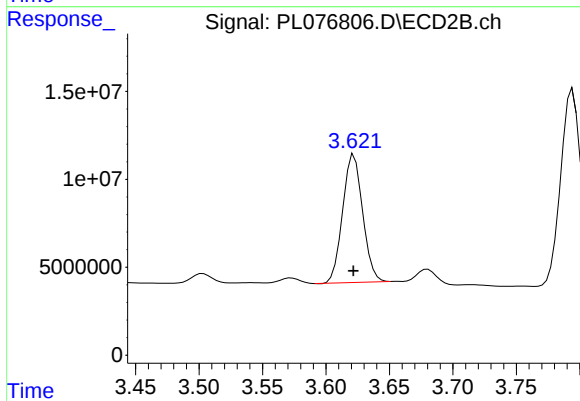

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 79773759
Conc: 963.98 ng/ml

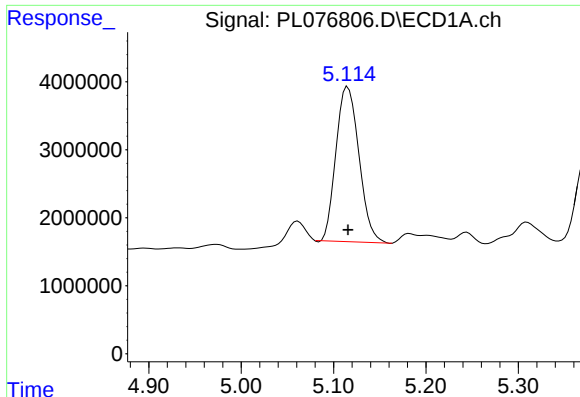

#24 Chlordane-2


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 39564185
Conc: 935.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

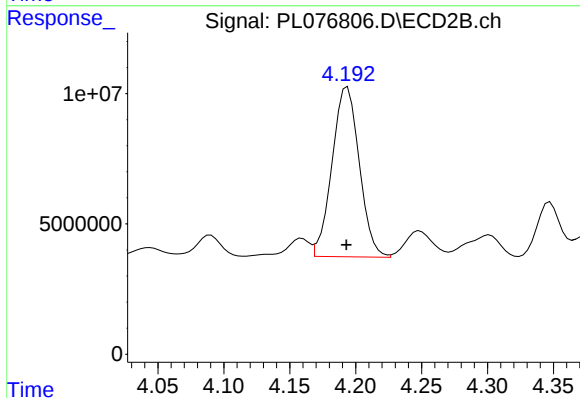


#24 Chlordane-2

R.T.: 4.194 min
Delta R.T.: 0.000 min
Response: 93614799
Conc: 935.75 ng/ml

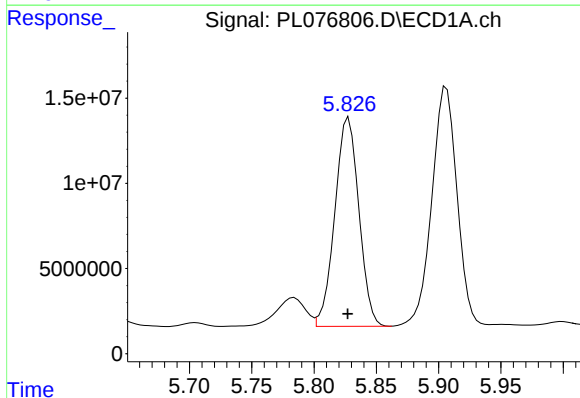


#25 Chlordane-3

R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 164934245
Conc: 1000.67 ng/ml

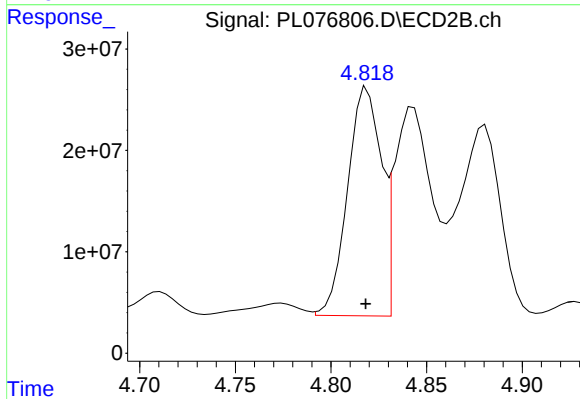

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 275646048
Conc: 979.39 ng/ml

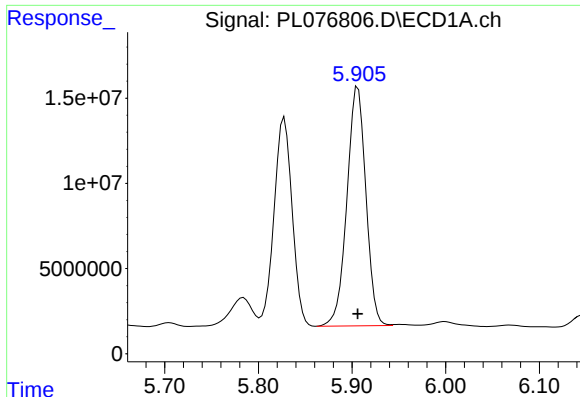

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 197891771
Conc: 988.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

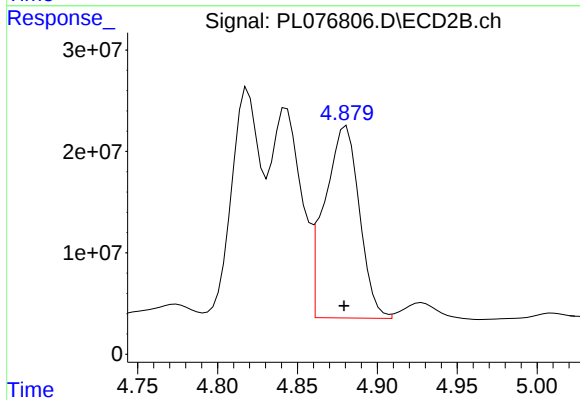


#26 Chlordane-4

R.T.: 4.881 min
Delta R.T.: 0.001 min
Response: 286688012
Conc: 980.48 ng/ml

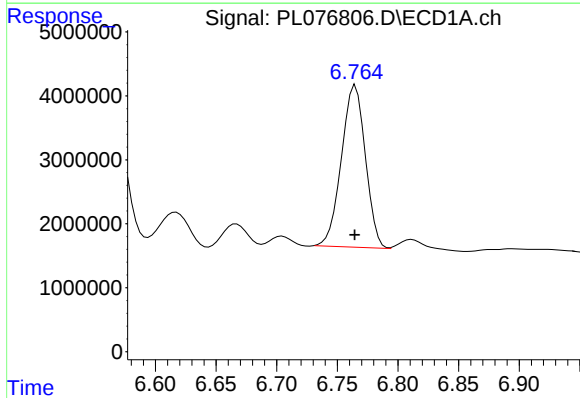


#27 Chlordane-5

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 34827233
Conc: 971.75 ng/ml

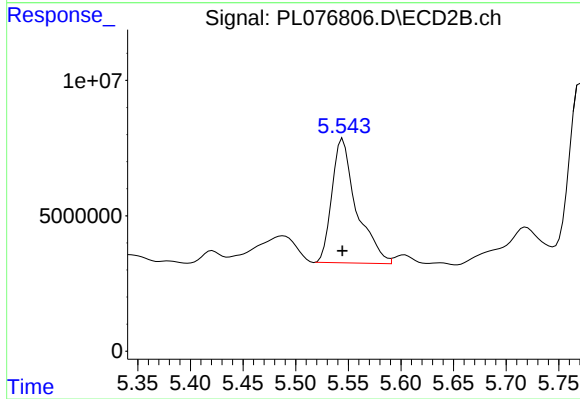

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 74271320
Conc: 946.42 ng/ml

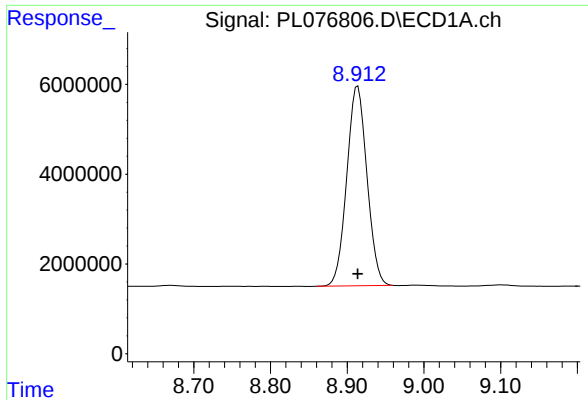

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 81851368
Conc: 92.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

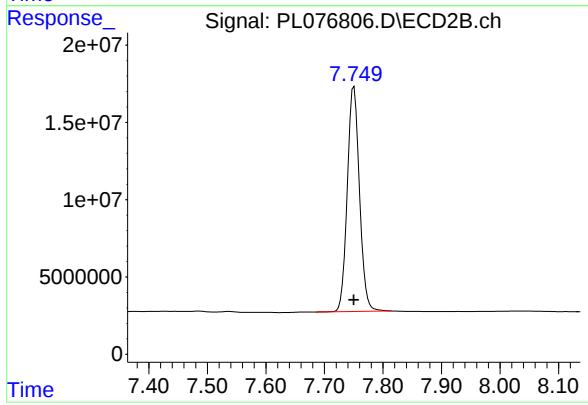

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 210736906
Conc: 93.86 ng/ml