

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 13:46
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 14:32:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 14:27:09 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	82538778	242.9E6	74.577	74.586
28)	SA Decachlor...	8.914	7.751	63464786	162.3E6	71.695	72.297
Target Compounds							
23)	Chlordane-1	4.581	3.622	28646081	60910487	740.623	736.036
24)	Chlordane-2	5.116	4.193	30434040	72588090	719.962	725.575
25)	Chlordane-3	5.827	4.819	123.7E6	210.8E6	750.464	748.932
26)	Chlordane-4	5.906	4.880	148.9E6	217.7E6	744.043	744.588
27)	Chlordane-5	6.764	5.545	26390209	56896410	736.340	725.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 13:46
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 14:32:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 14:27:09 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

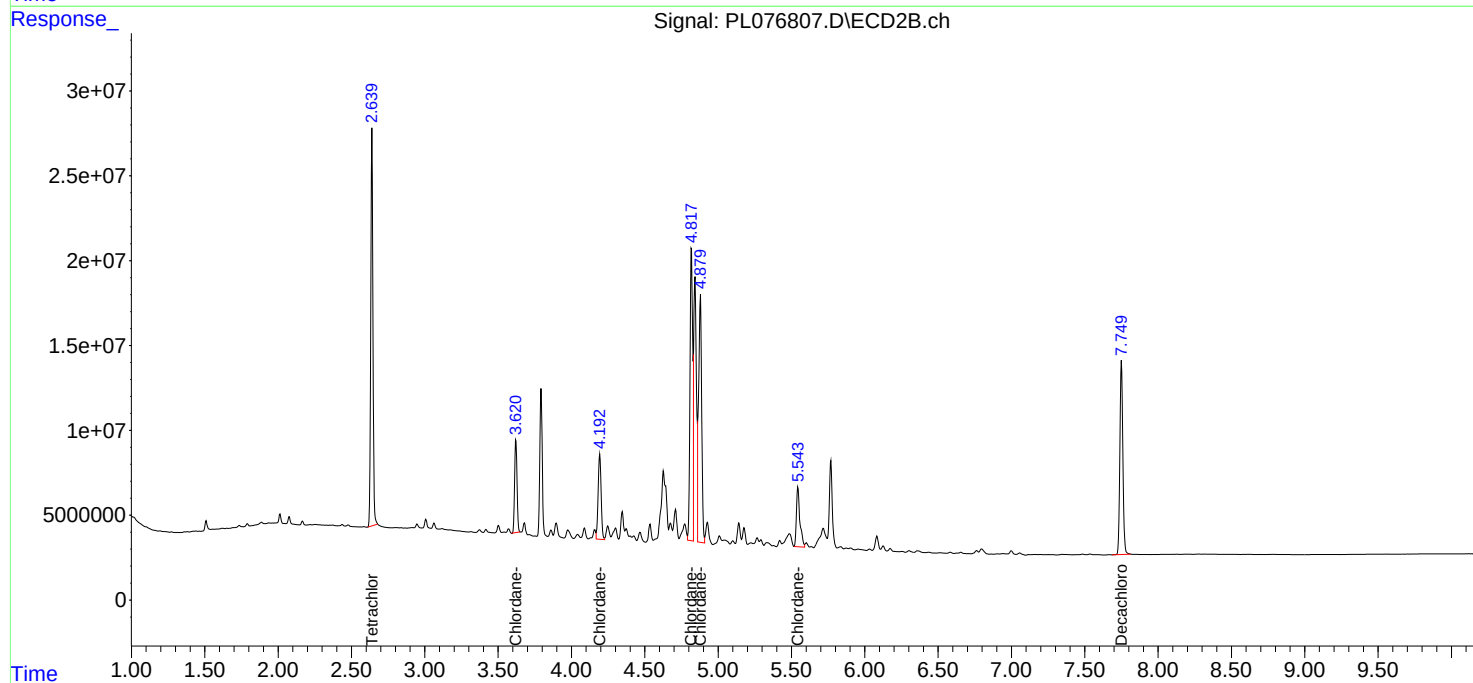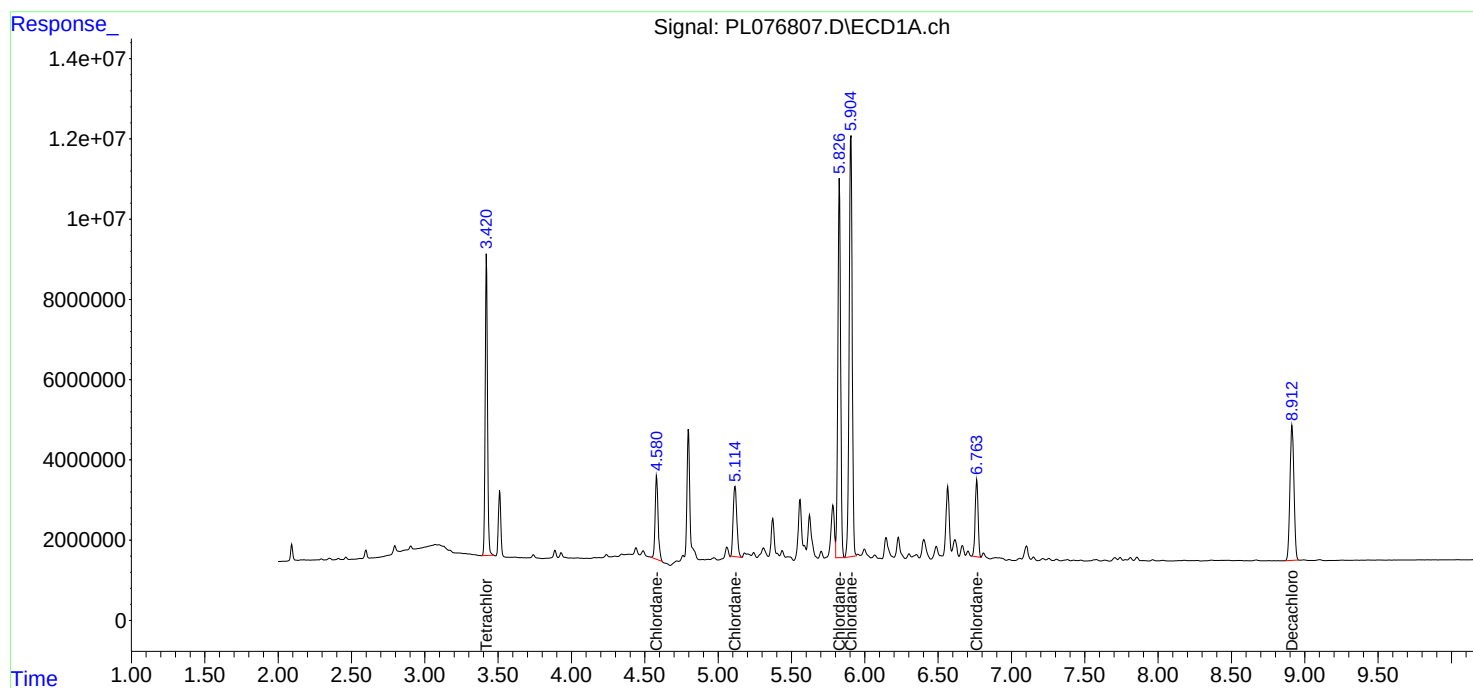


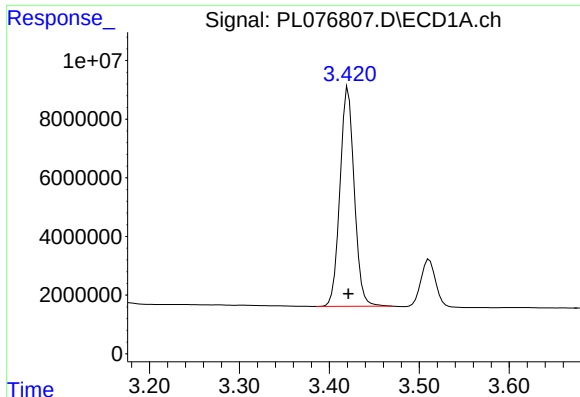

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 82538778
Conc: 74.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

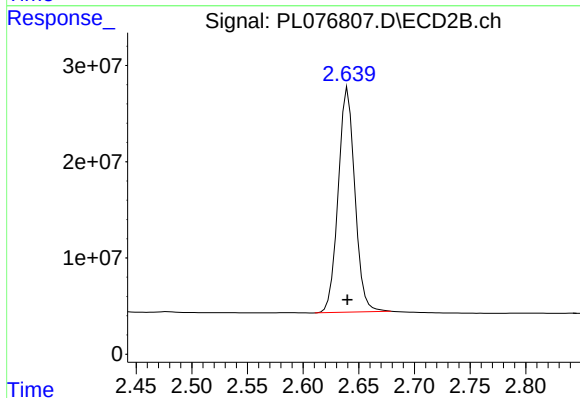


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 242895661
Conc: 74.59 ng/ml

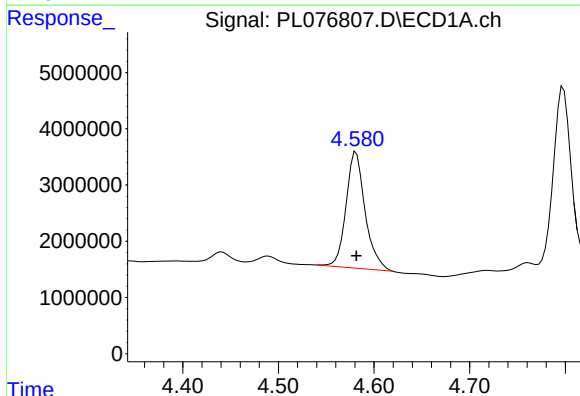


#23 Chlordane-1

R.T.: 4.581 min
Delta R.T.: 0.000 min
Response: 28646081
Conc: 740.62 ng/ml

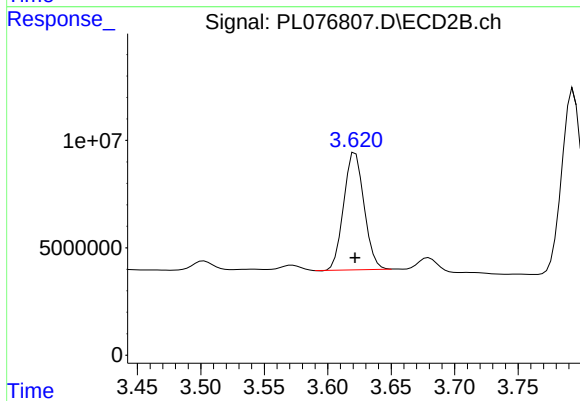

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 60910487
Conc: 736.04 ng/ml

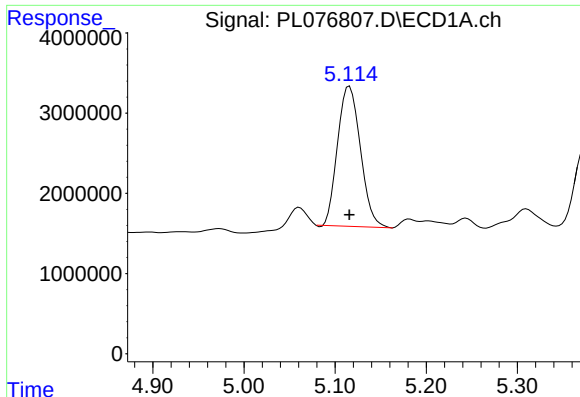

#24 Chlordane-2


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 30434040
Conc: 719.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

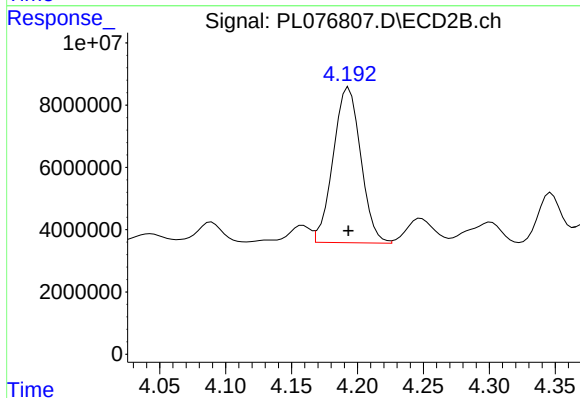


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 72588090
Conc: 725.58 ng/ml

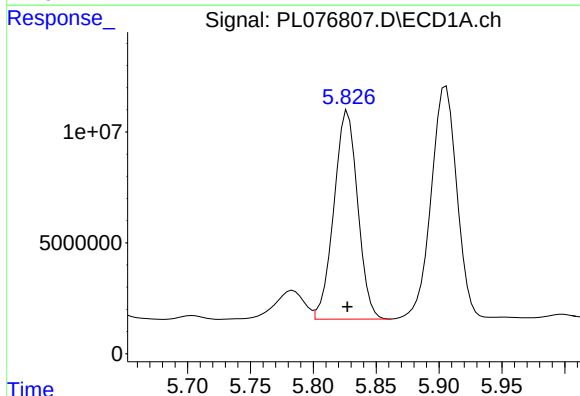


#25 Chlordane-3

R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 123694352
Conc: 750.46 ng/ml

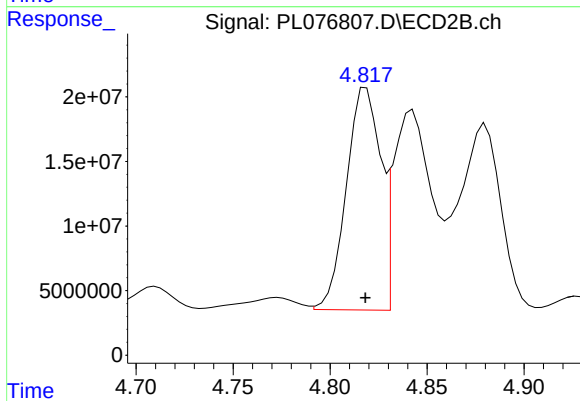

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 210783962
Conc: 748.93 ng/ml

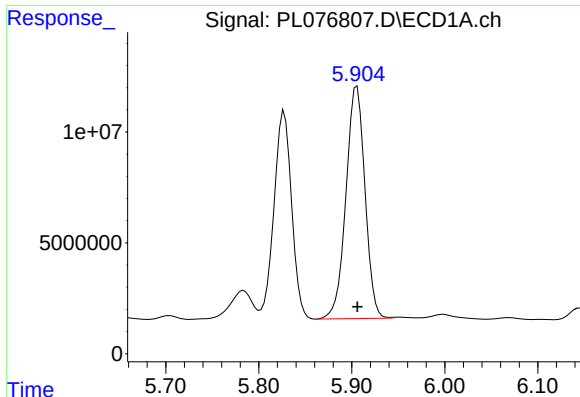

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 148942381
Conc: 744.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

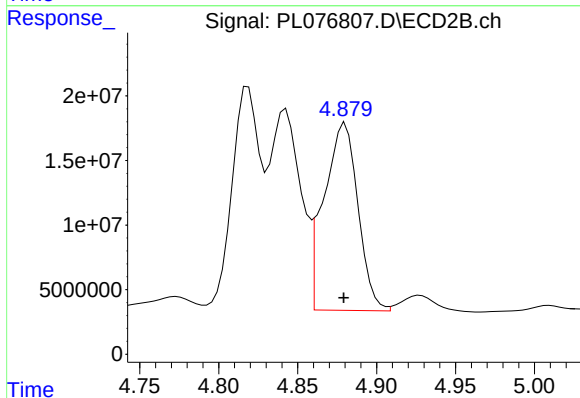


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 217713193
Conc: 744.59 ng/ml

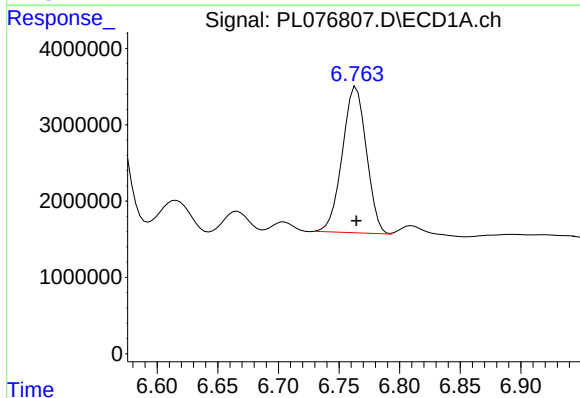


#27 Chlordane-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 26390209
Conc: 736.34 ng/ml

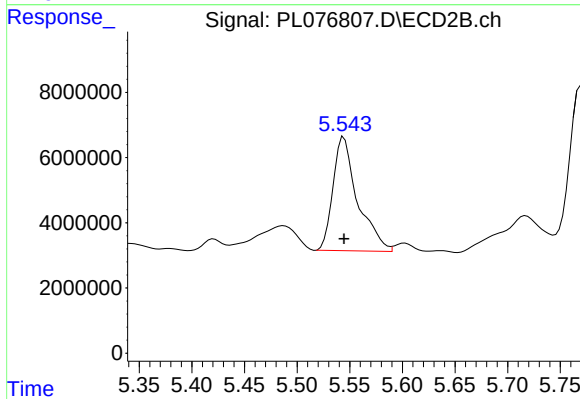

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 56896410
Conc: 725.02 ng/ml

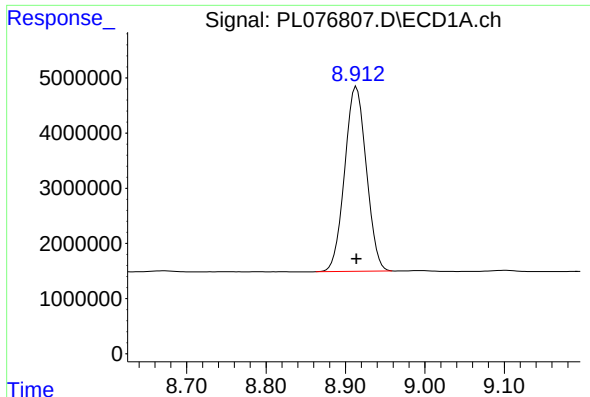

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 63464786
Conc: 71.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

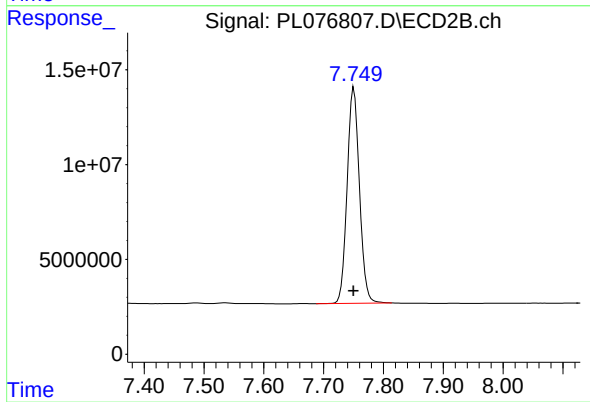

#28 Decachlorobiphenyl

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 162323606
Conc: 72.30 ng/ml