

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
 Data File : PL076817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2022 16:20
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL080122CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 16:34:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.640	55288837	165.3E6	51.520	52.123
28)	SA Decachlor...	8.915	7.750	45315973	116.7E6	50.944	52.236
Target Compounds							
23)	Chlordane-1	4.582	3.622	19784433	42580986	526.862	533.687
24)	Chlordane-2	5.116	4.194	21435735	51220395	514.837	520.051
25)	Chlordane-3	5.828	4.819	83984848	145.0E6	520.196	525.907
26)	Chlordane-4	5.906	4.880	101.8E6	149.9E6	518.827	519.484
27)	Chlordane-5	6.765	5.545	18278376	40094735	523.991	525.284



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080122\
Data File : PL076817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2022 16:20
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL080122CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 16:34:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

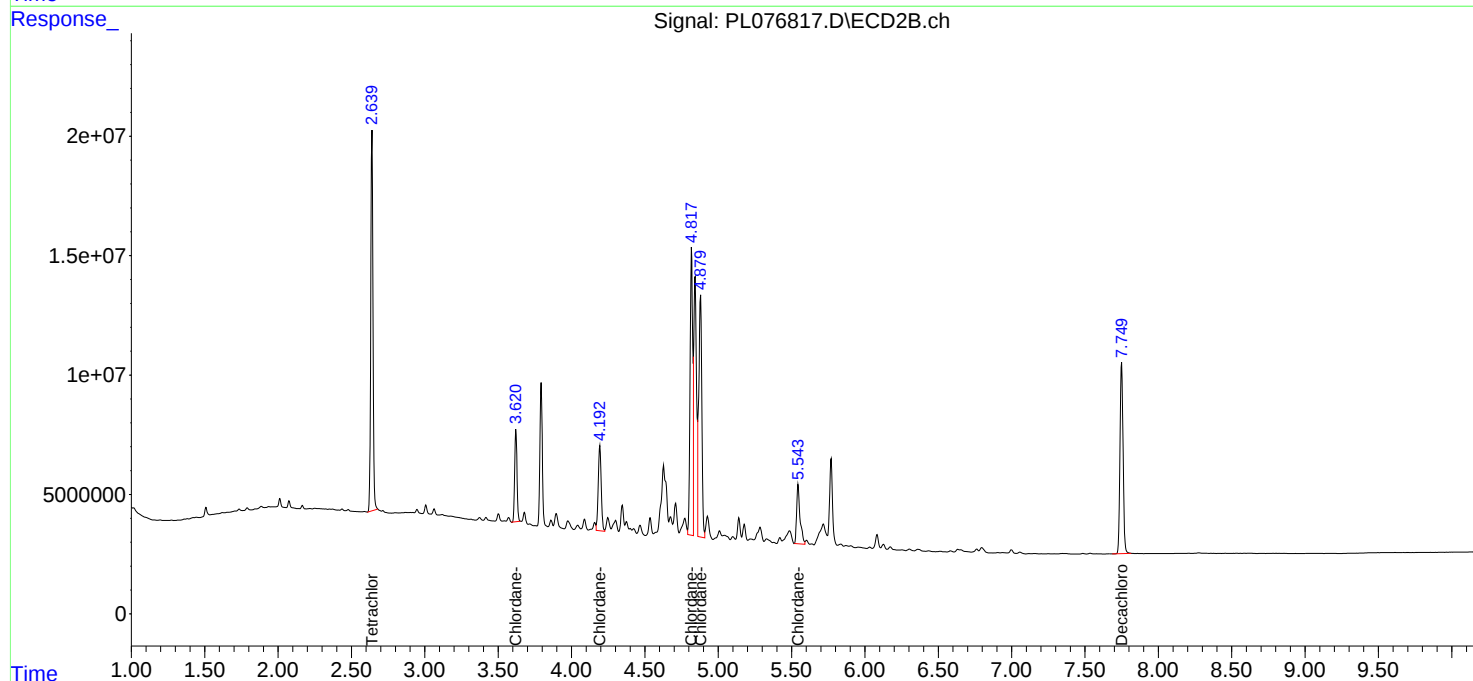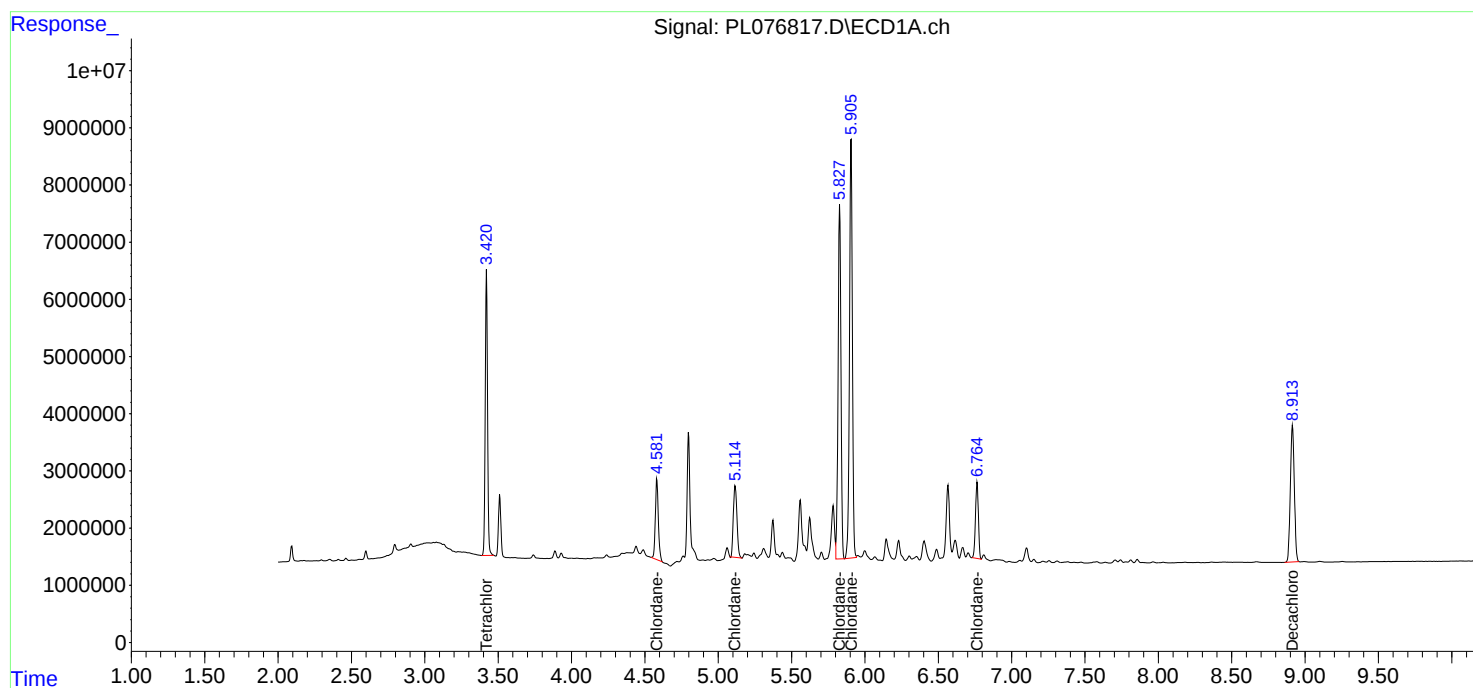


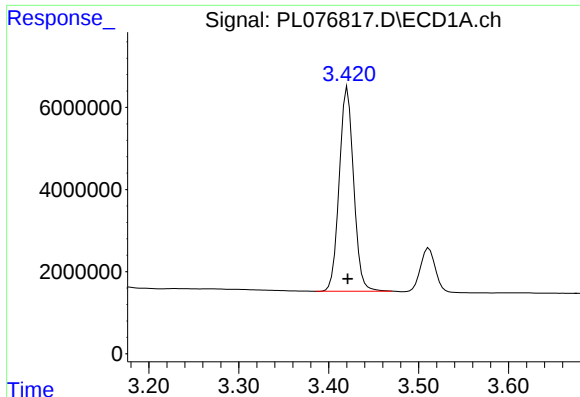

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 55288837
Conc: 51.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080122CHLOR

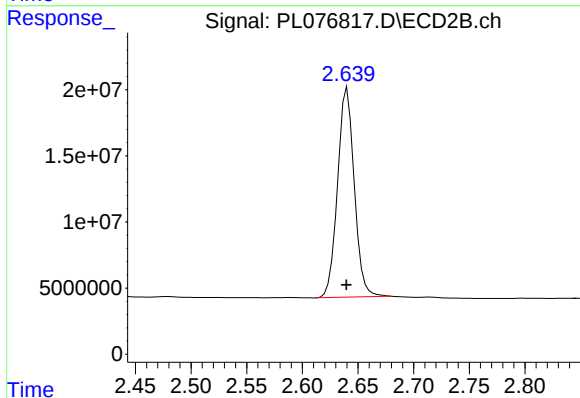


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 165334618
Conc: 52.12 ng/ml

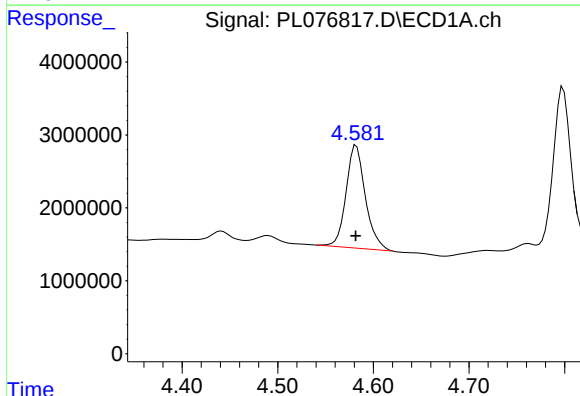


#23 Chlordane-1

R.T.: 4.582 min
Delta R.T.: 0.000 min
Response: 19784433
Conc: 526.86 ng/ml

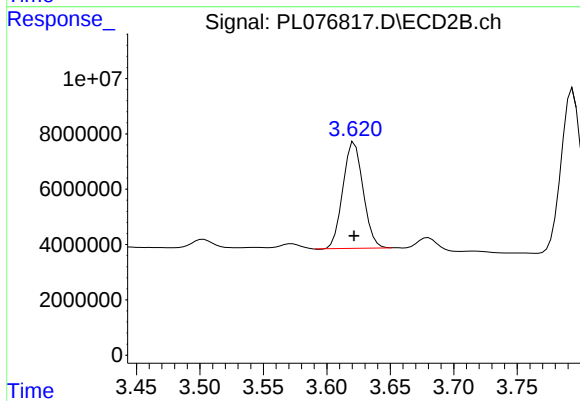

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 42580986
Conc: 533.69 ng/ml

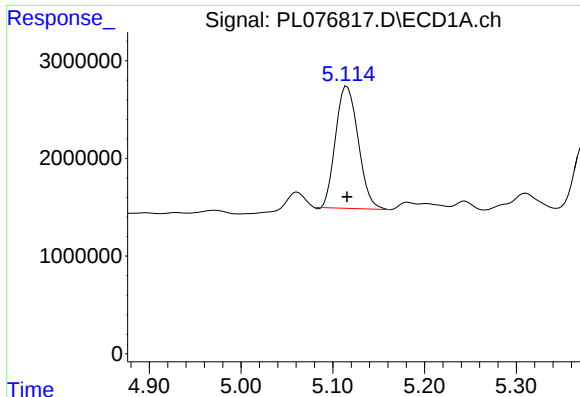

#24 Chlordane-2


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 21435735
Conc: 514.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080122CHLOR

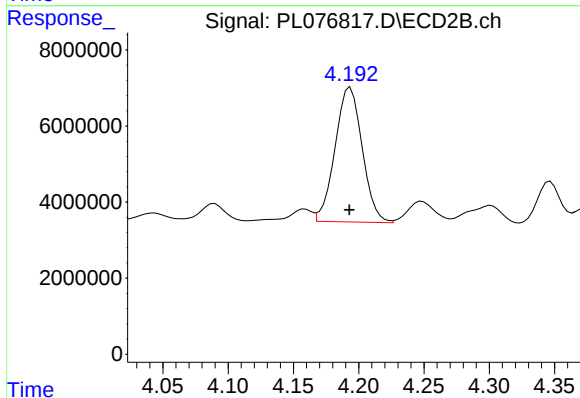


#24 Chlordane-2

R.T.: 4.194 min
Delta R.T.: 0.000 min
Response: 51220395
Conc: 520.05 ng/ml

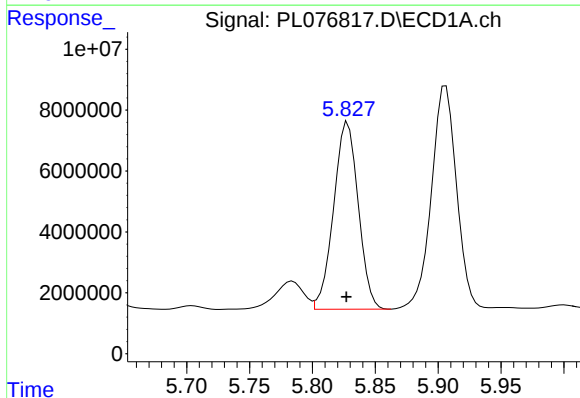


#25 Chlordane-3

R.T.: 5.828 min
Delta R.T.: 0.001 min
Response: 83984848
Conc: 520.20 ng/ml

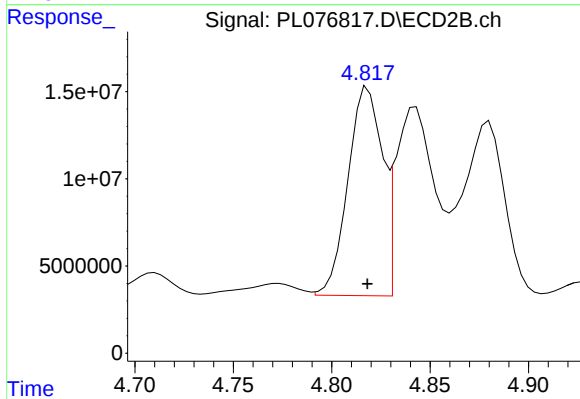

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 145028761
Conc: 525.91 ng/ml

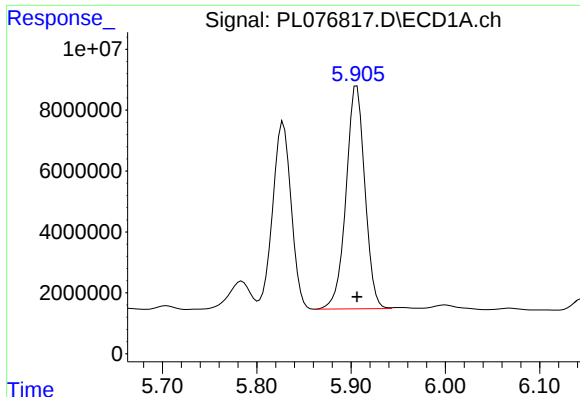

#26 Chlordane-4


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 101807662
Conc: 518.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080122CHLOR

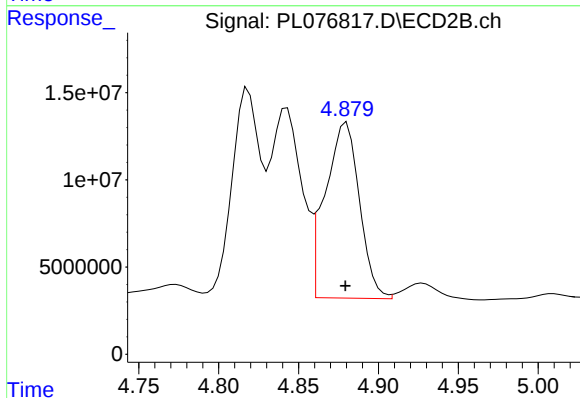


#26 Chlordane-4

R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 149851645
Conc: 519.48 ng/ml

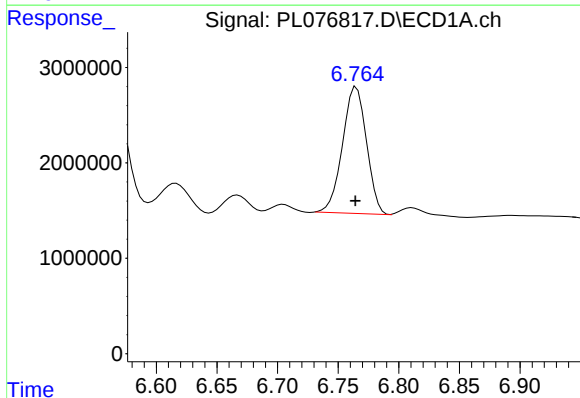


#27 Chlordane-5

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 18278376
Conc: 523.99 ng/ml

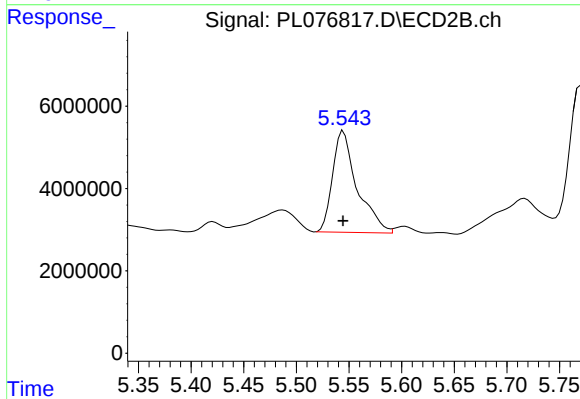

#27 Chlordane-5


R.T.: 5.545 min
Delta R.T.: 0.000 min
Response: 40094735
Conc: 525.28 ng/ml

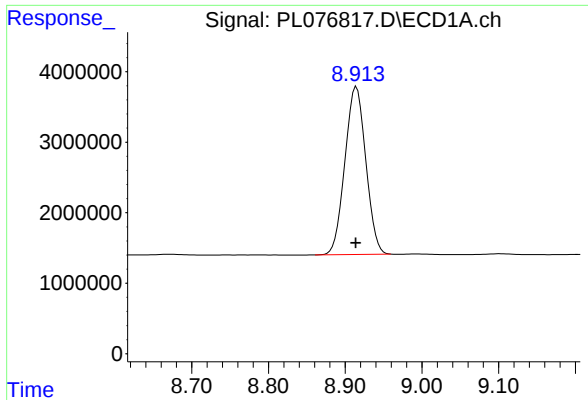

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.000 min
Response: 45315973
Conc: 50.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080122CHLOR

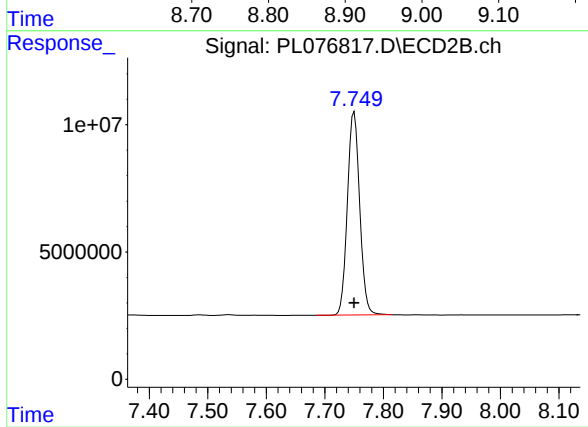

#28 Decachlorobiphenyl

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 116737655
Conc: 52.24 ng/ml