

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 17:09
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:22:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:17:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.682	11971750	18753526	5.516	4.998
28)	SA Decachlor...	9.024	7.869	8711844	7508536	6.350	5.937
Target Compounds							
23)	Chlordane-1	4.644	3.689	49577320	18509757	51.270	47.739
24)	Chlordane-2	5.177	4.270	52241298	23536969	59.574	57.439
25)	Chlordane-3	5.891	4.903	191.0E6	67813043	48.825	50.084
26)	Chlordane-4	5.974	4.966	228.1E6	69996271	50.648	49.430
27)	Chlordane-5	6.824	5.865	35625096	24476744	52.680	49.365


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 17:09
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:22:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:17:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

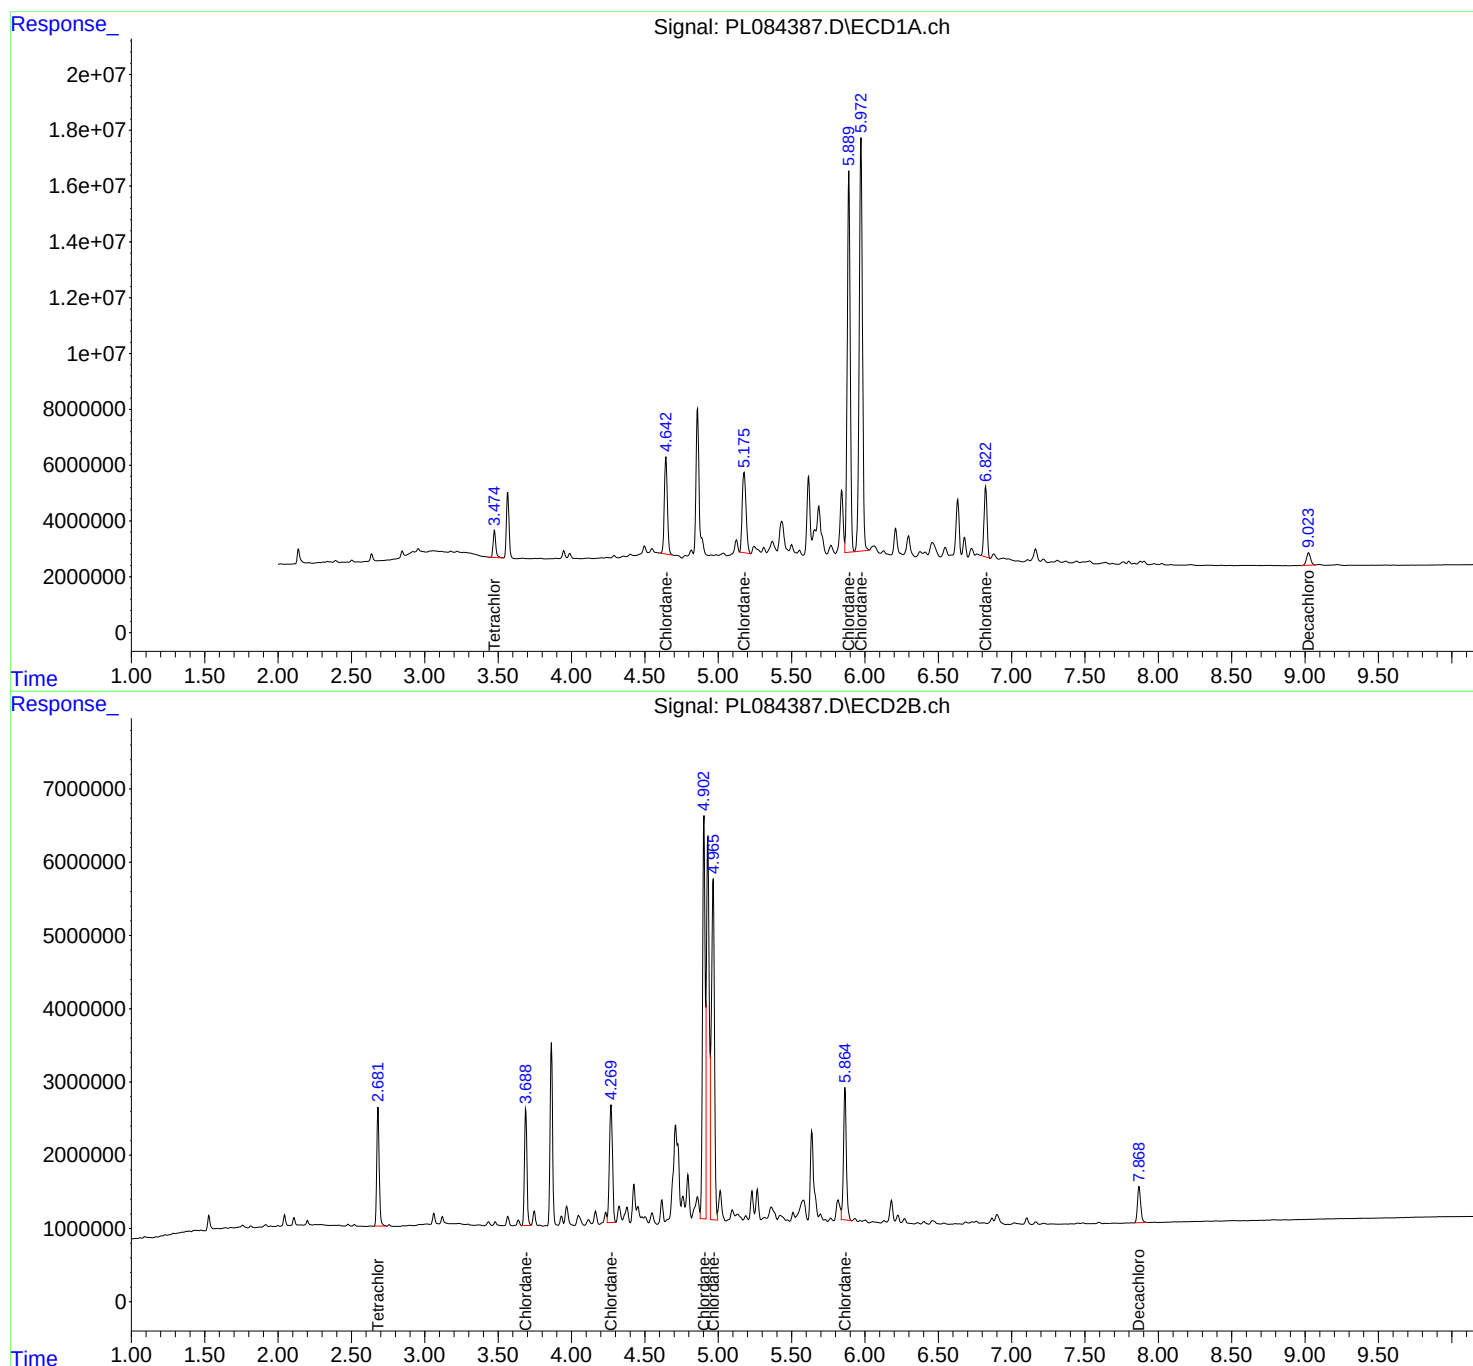


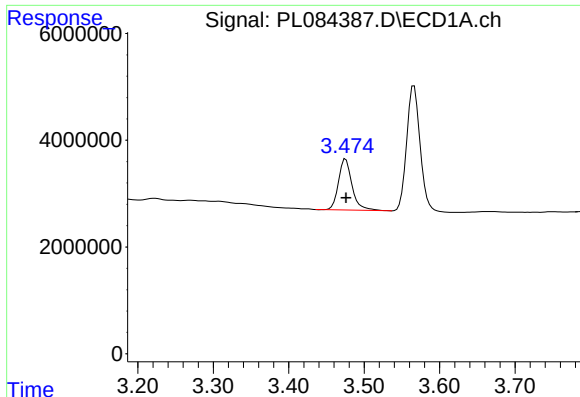

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 11971750
Conc: 5.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

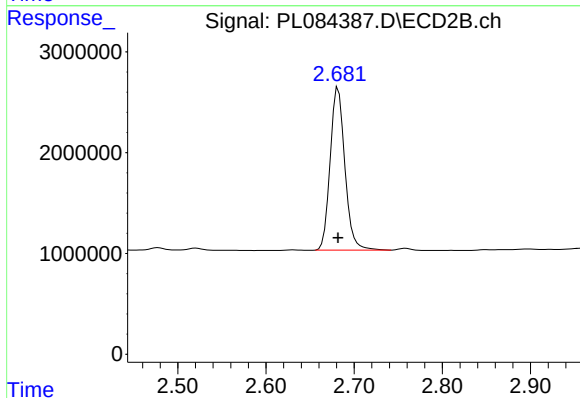


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 18753526
Conc: 5.00 ng/ml

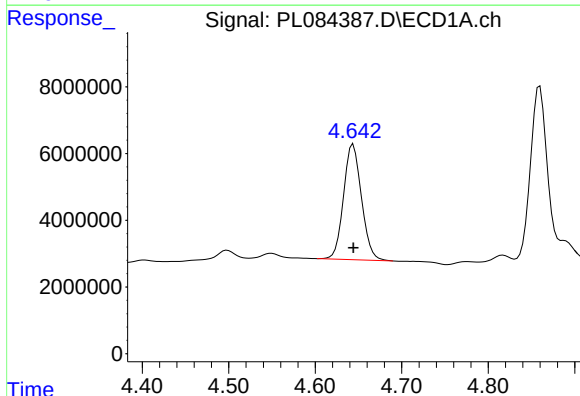


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 49577320
Conc: 51.27 ng/ml

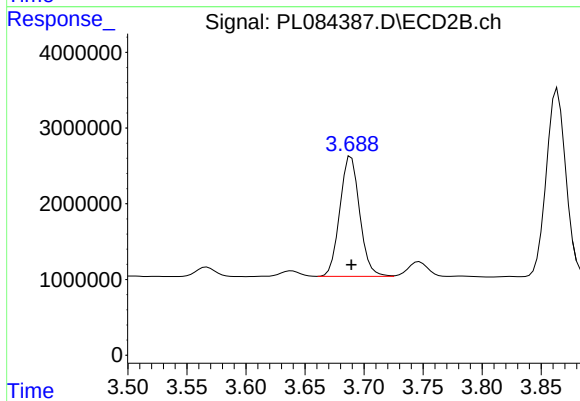

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 18509757
Conc: 47.74 ng/ml

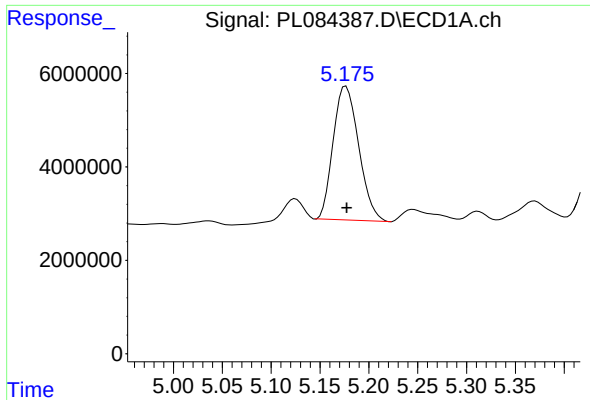

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 52241298
Conc: 59.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

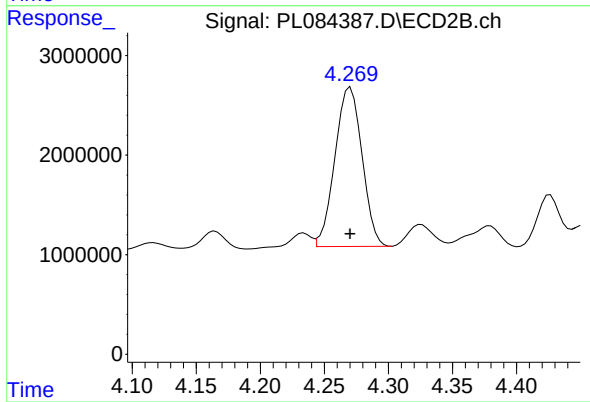


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 23536969
Conc: 57.44 ng/ml

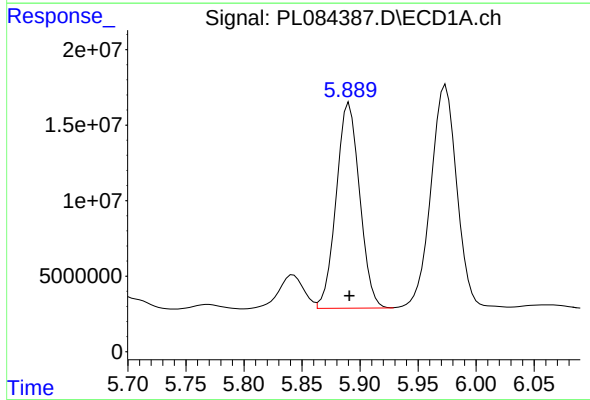


#25 Chlordane-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 191044447
Conc: 48.83 ng/ml

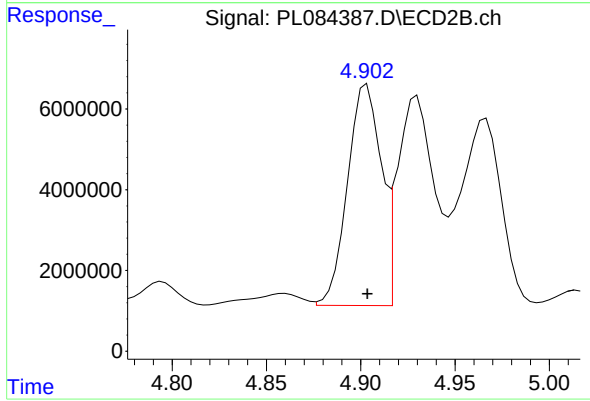

#25 Chlordane-3


R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 67813043
Conc: 50.08 ng/ml

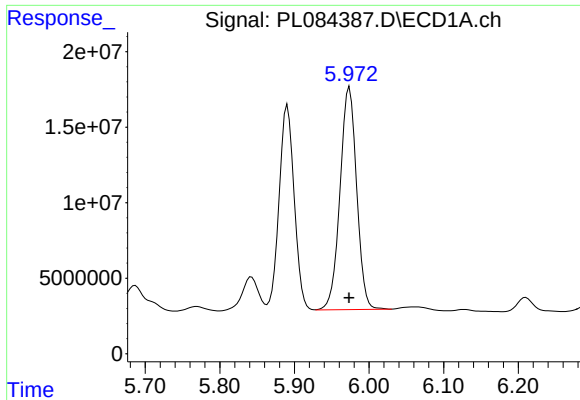

#26 Chlordane-4


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 228149190
Conc: 50.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

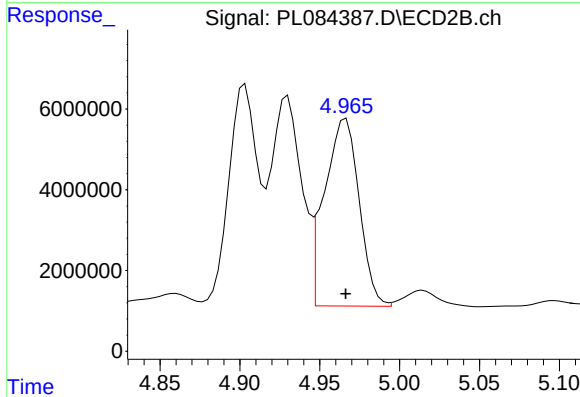


#26 Chlordane-4

R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 69996271
Conc: 49.43 ng/ml

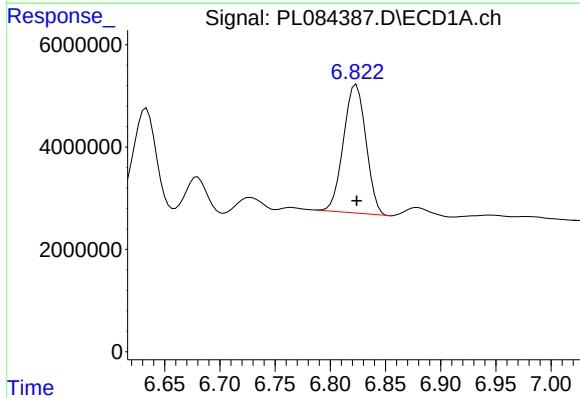


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.000 min
Response: 35625096
Conc: 52.68 ng/ml

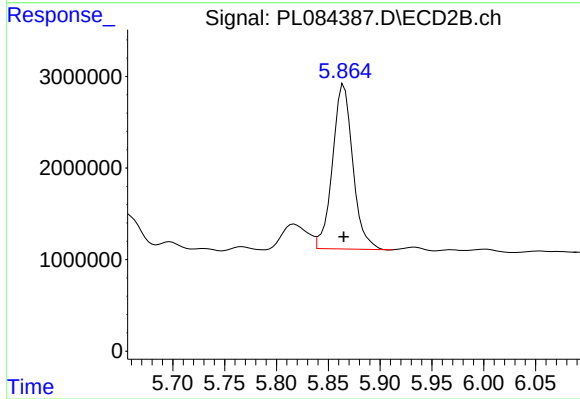

#27 Chlordane-5

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 24476744
Conc: 49.37 ng/ml

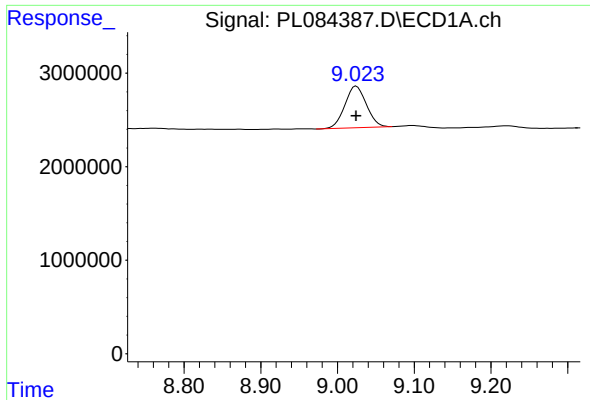

#28 Decachlorobiphenyl


R.T.: 9.024 min

Delta R.T.: 0.000 min

Response: 8711844

Conc: 6.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

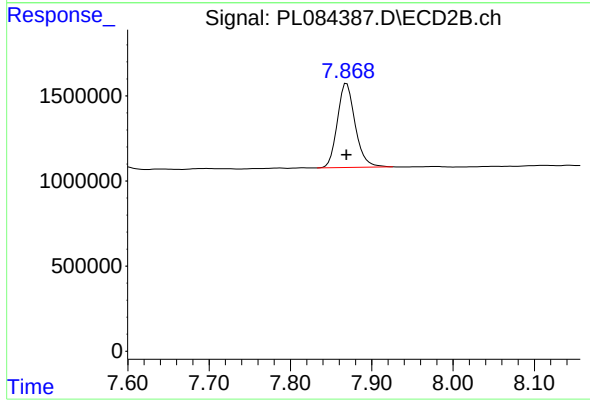

#28 Decachlorobiphenyl

R.T.: 7.869 min

Delta R.T.: 0.000 min

Response: 7508536

Conc: 5.94 ng/ml