

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 16:14
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:17:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:17:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.682	225.6E6	390.1E6	103.929	103.947
28)	SA Decachlor...	9.025	7.870	133.6E6	127.7E6	97.376	100.986
Target Compounds							
23)	Chlordane-1	4.645	3.690	1028.9E6	410.5E6	1064.031	1058.786
24)	Chlordane-2	5.178	4.270	900.2E6	412.3E6	1026.601	1006.217
25)	Chlordane-3	5.891	4.904	4119.9E6	1346.9E6	1052.907	994.743
26)	Chlordane-4	5.975	4.967	4726.2E6	1430.0E6	1049.201	1009.816
27)	Chlordane-5	6.824	5.865	728.7E6	521.2E6	1077.493	1051.088



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 16:14
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:17:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:17:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

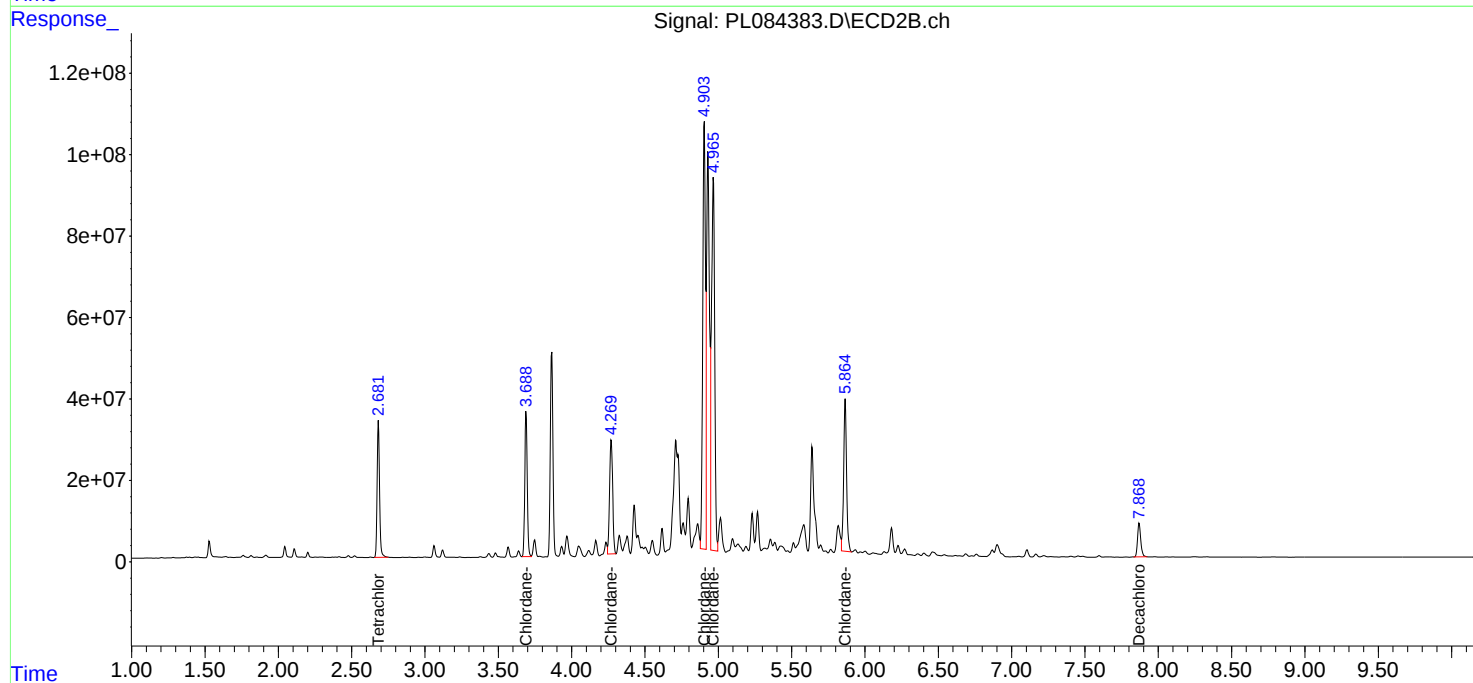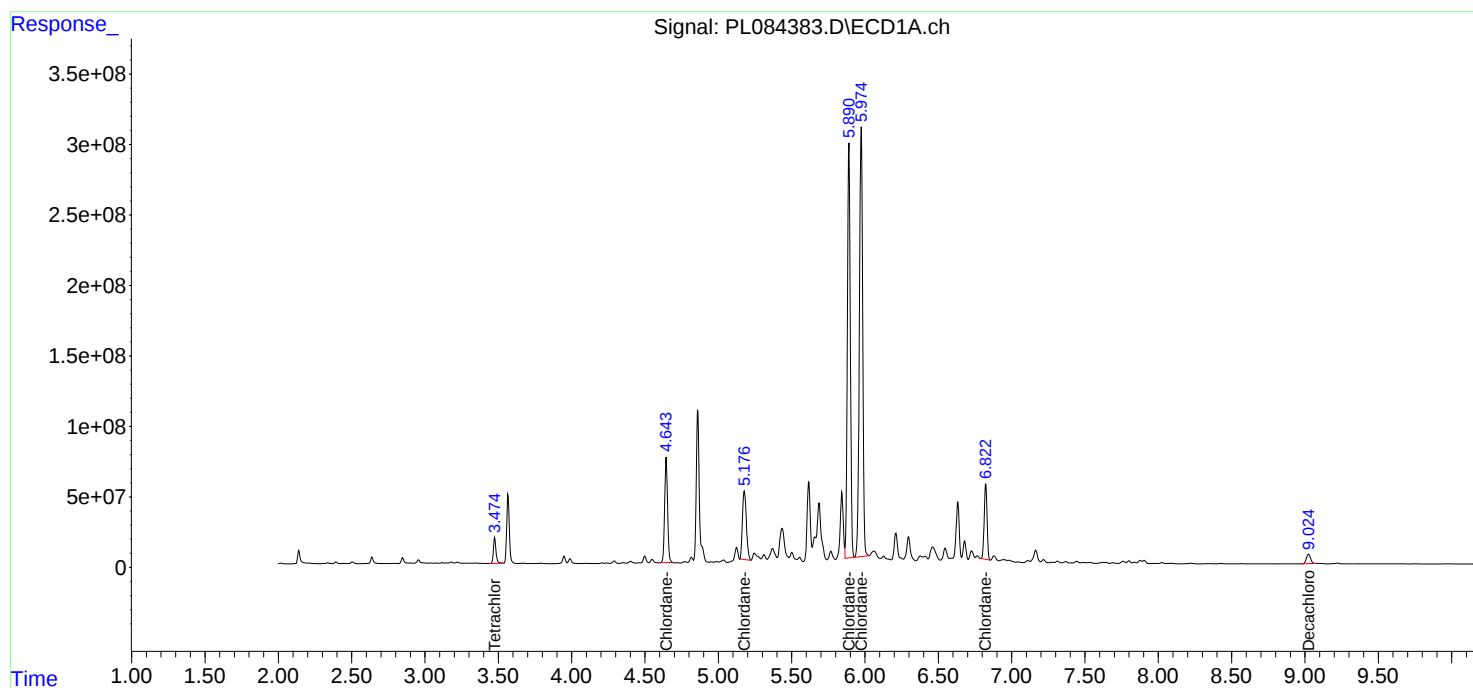


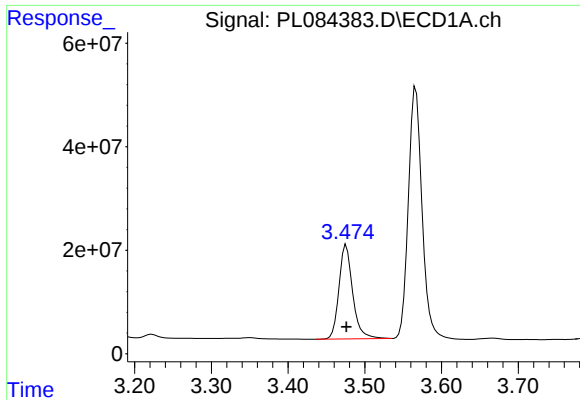

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 225575085
Conc: 103.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

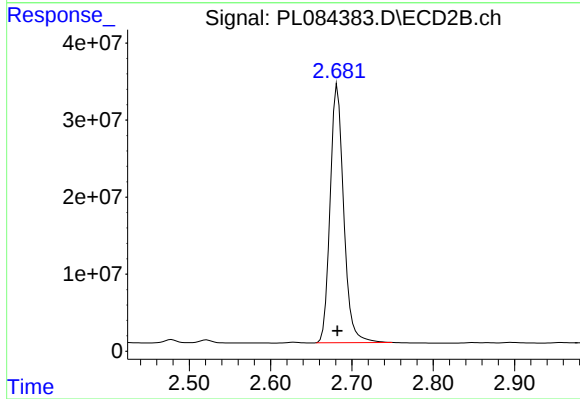


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 390064117
Conc: 103.95 ng/ml

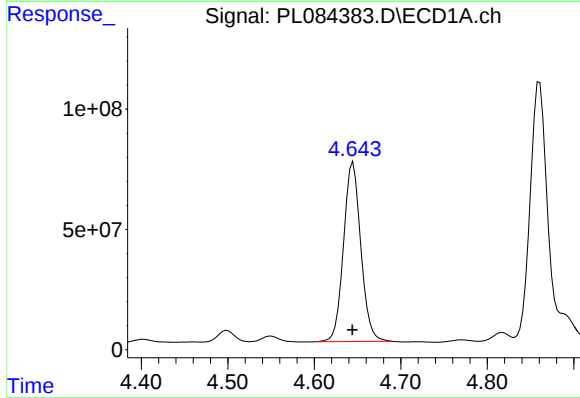


#23 Chlordane-1

R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 1028907163
Conc: 1064.03 ng/ml

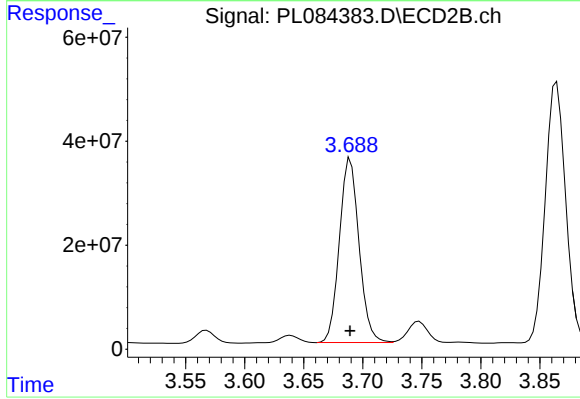

#23 Chlordane-1


R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 410519389
Conc: 1058.79 ng/ml

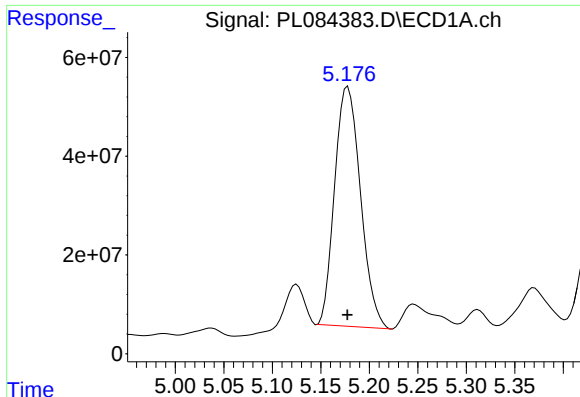

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 900241561
Conc: 1026.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

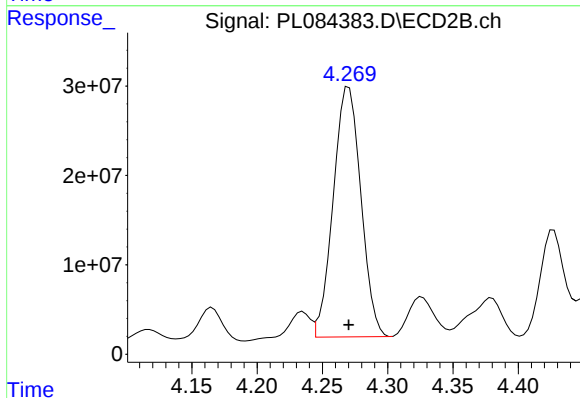


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 412320500
Conc: 1006.22 ng/ml

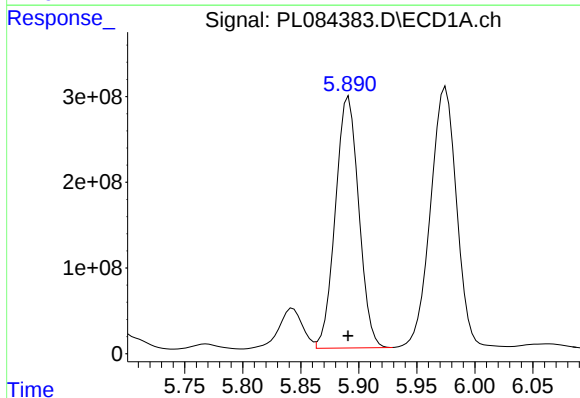


#25 Chlordane-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 4119850808
Conc: 1052.91 ng/ml

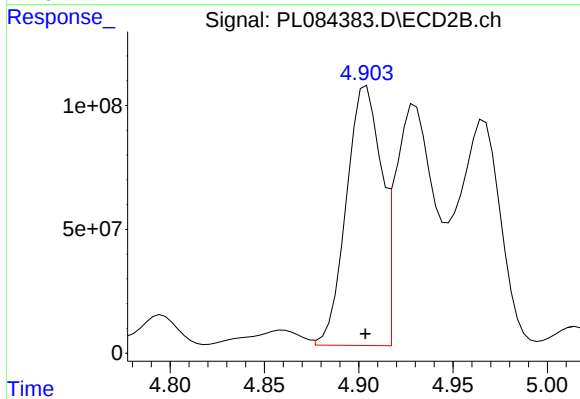

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 1346855336
Conc: 994.74 ng/ml

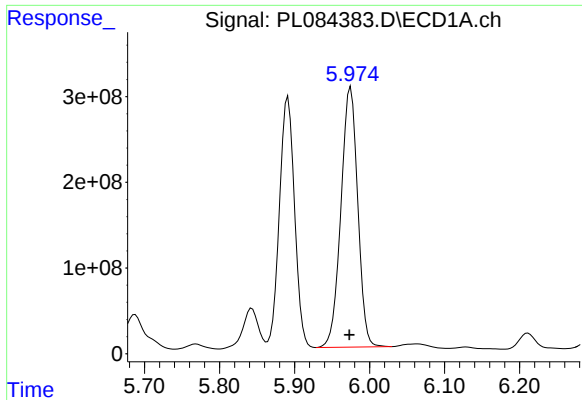

#26 Chlordane-4


R.T.: 5.975 min
Delta R.T.: 0.002 min
Response: 4726232174
Conc: 1049.20 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

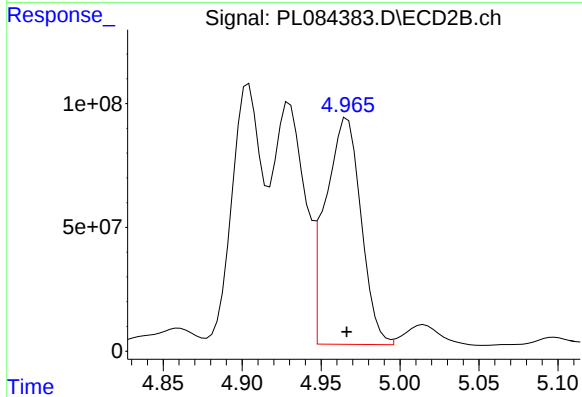


#26 Chlordane-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 1429971395
Conc: 1009.82 ng/ml

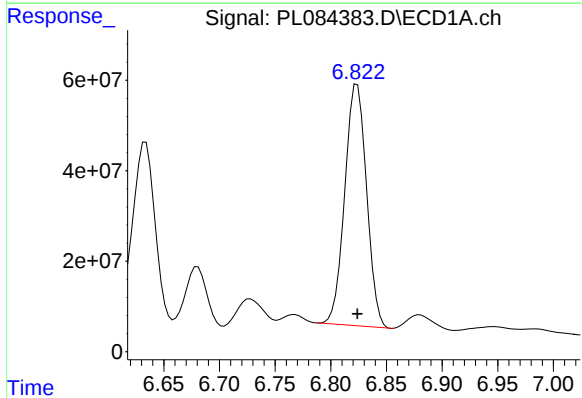


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.000 min
Response: 728654276
Conc: 1077.49 ng/ml

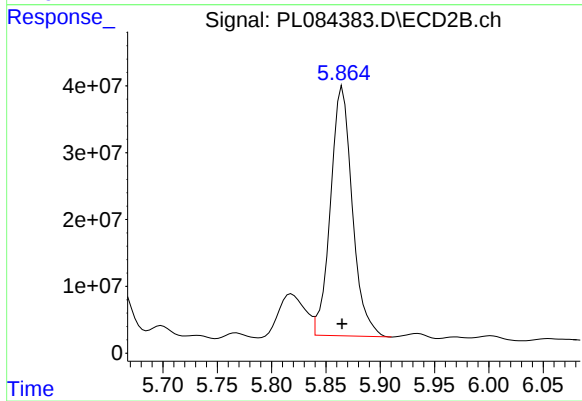

#27 Chlordane-5


R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 521161057
Conc: 1051.09 ng/ml

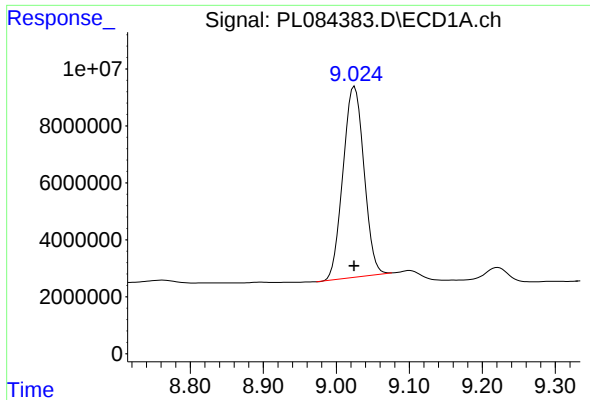

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 133598209
Conc: 97.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

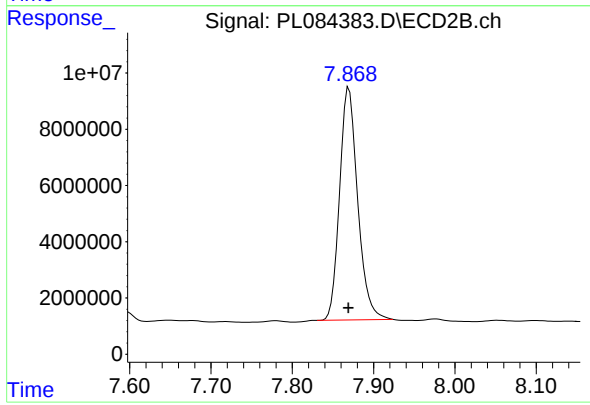

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.000 min
Response: 127723512
Conc: 100.99 ng/ml