

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 16:28
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:18:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:17:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.682	164.6E6	286.1E6	75.838	76.243
28)	SA Decachlor...	9.025	7.870	100.5E6	94663686	73.236	74.847
Target Compounds							
23)	Chlordane-1	4.644	3.690	743.9E6	298.6E6	769.304	770.188
24)	Chlordane-2	5.177	4.270	662.3E6	305.7E6	755.306	746.066
25)	Chlordane-3	5.890	4.904	3005.8E6	1013.2E6	768.199	748.329
26)	Chlordane-4	5.974	4.967	3436.0E6	1064.1E6	762.777	751.480
27)	Chlordane-5	6.823	5.865	523.4E6	379.3E6	773.946	764.970



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 16:28
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:18:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:17:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

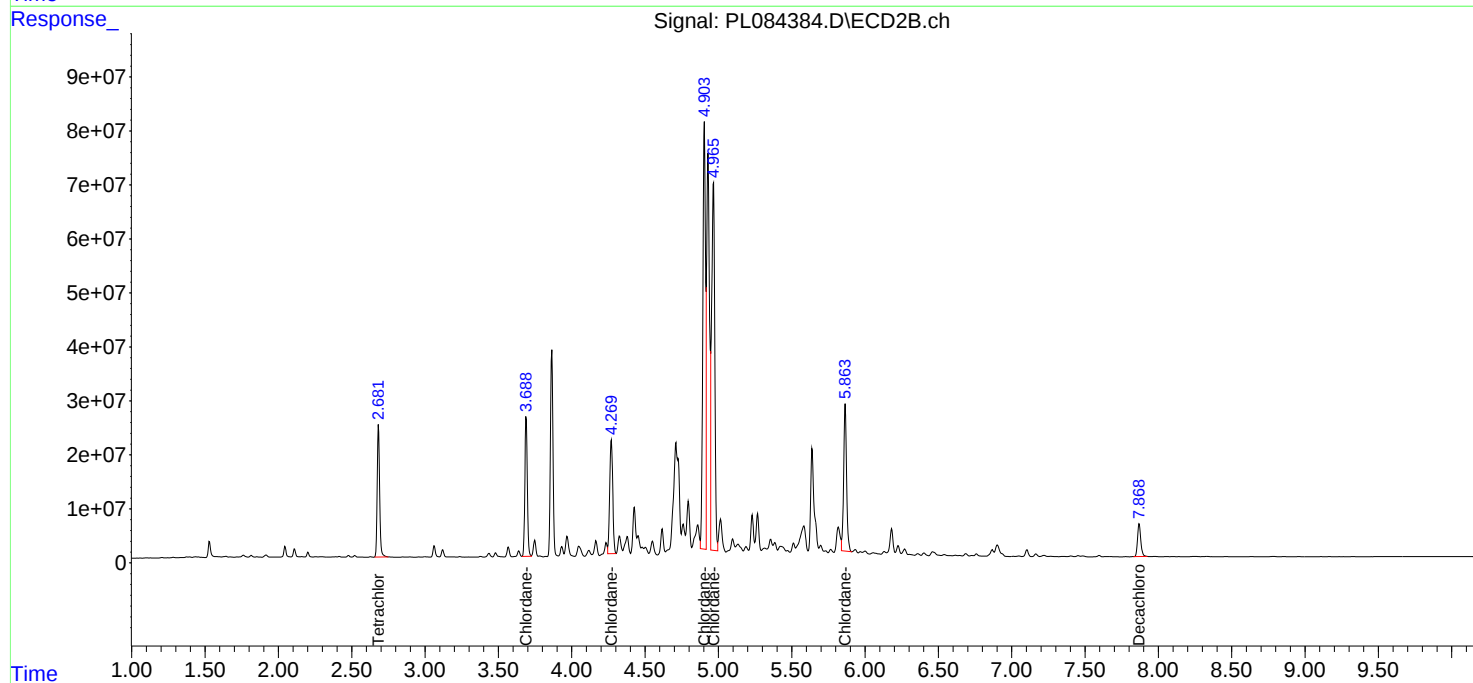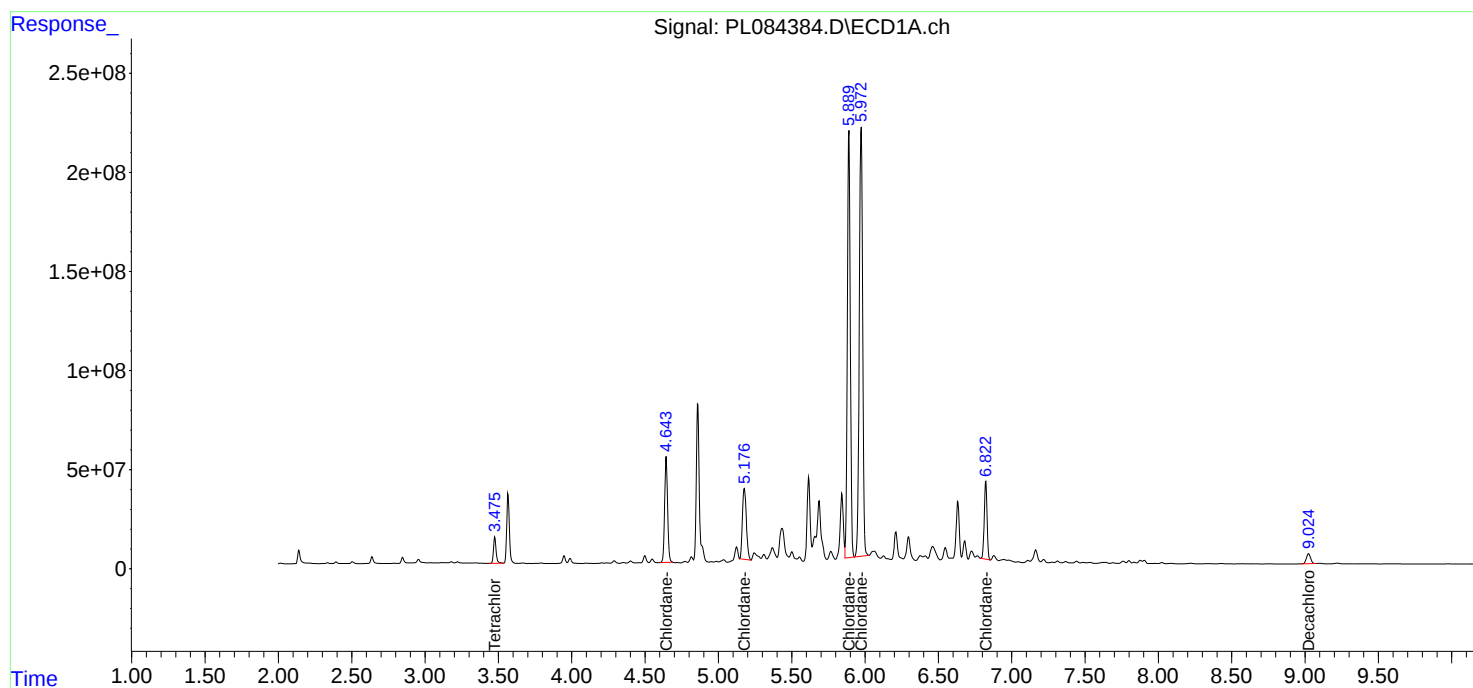


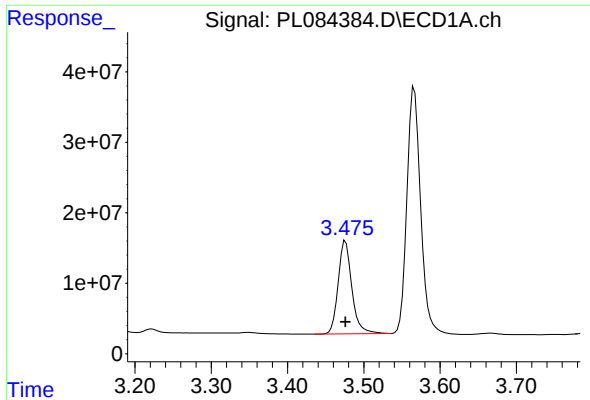

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 164604843
Conc: 75.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

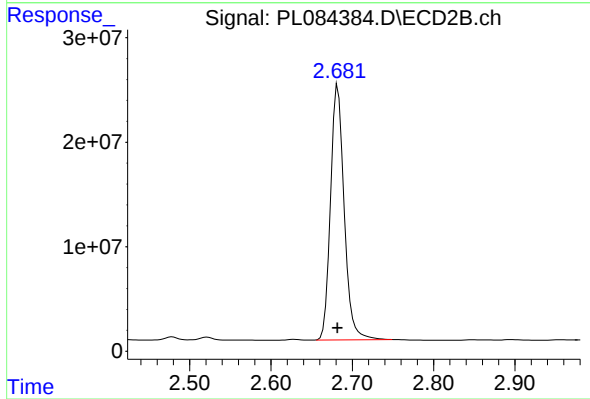


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 286105191
Conc: 76.24 ng/ml

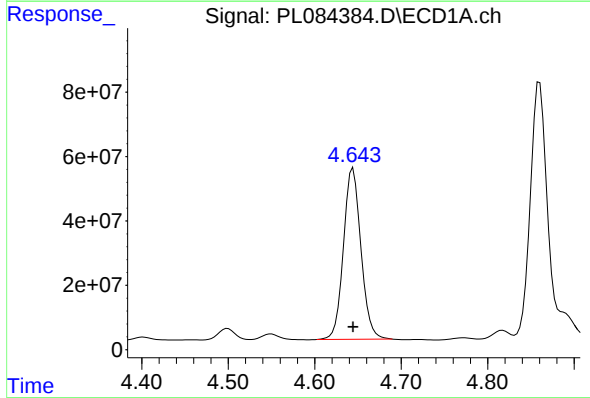


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 743908758
Conc: 769.30 ng/ml

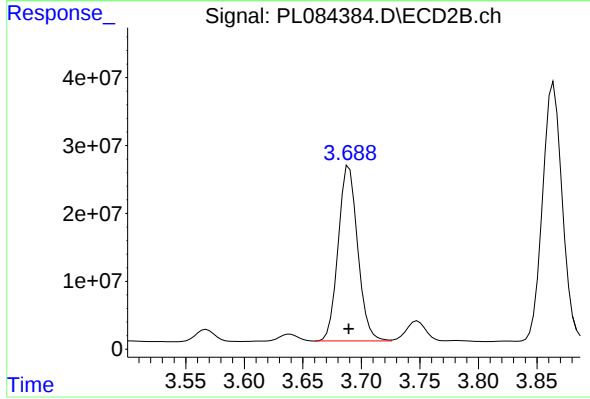

#23 Chlordane-1


R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 298622336
Conc: 770.19 ng/ml

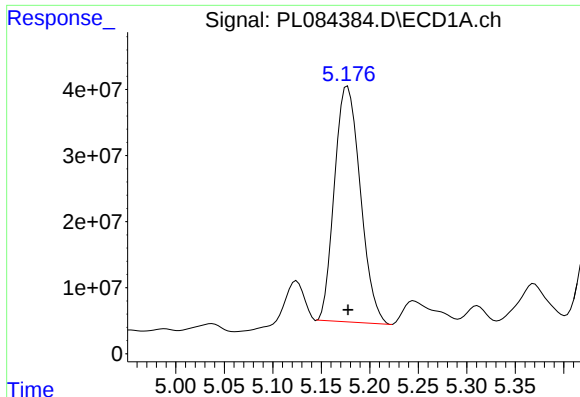

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 662339159
Conc: 755.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

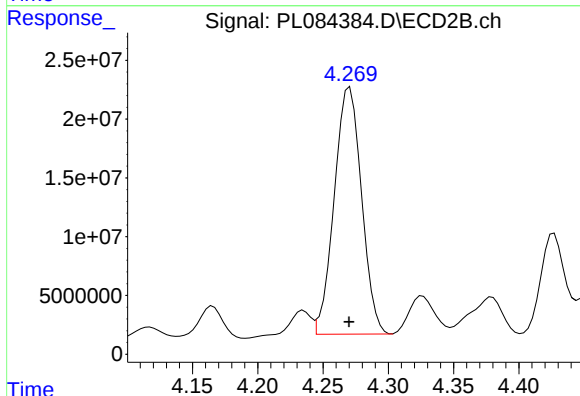


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 305717580
Conc: 746.07 ng/ml

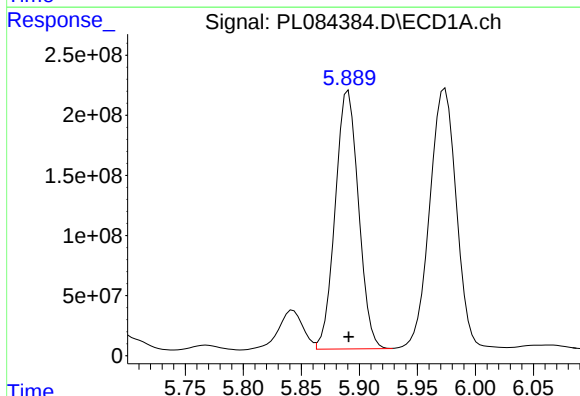


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 3005835929
Conc: 768.20 ng/ml

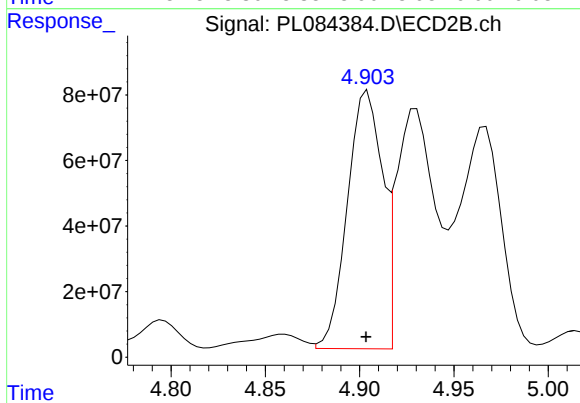

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 1013217421
Conc: 748.33 ng/ml

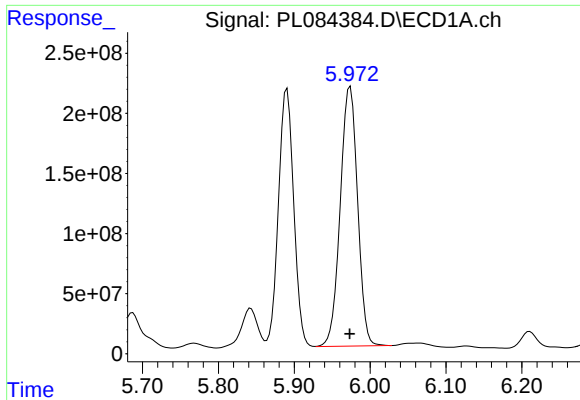

#26 Chlordane-4


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 3436003927
Conc: 762.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

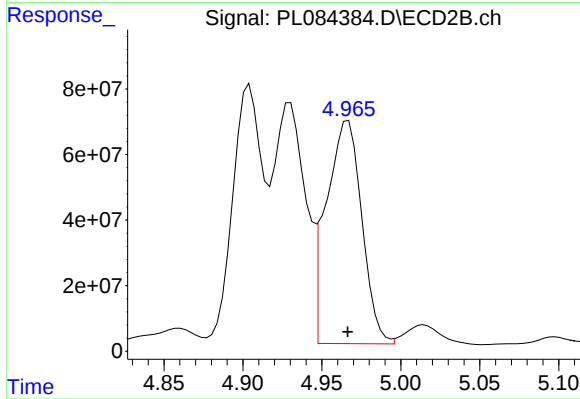


#26 Chlordane-4

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 1064149108
Conc: 751.48 ng/ml

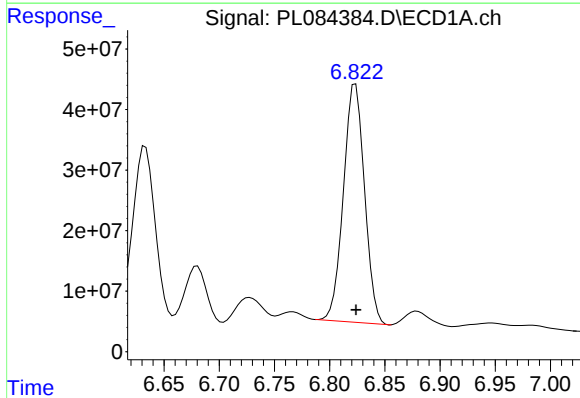


#27 Chlordane-5

R.T.: 6.823 min
Delta R.T.: 0.000 min
Response: 523380382
Conc: 773.95 ng/ml

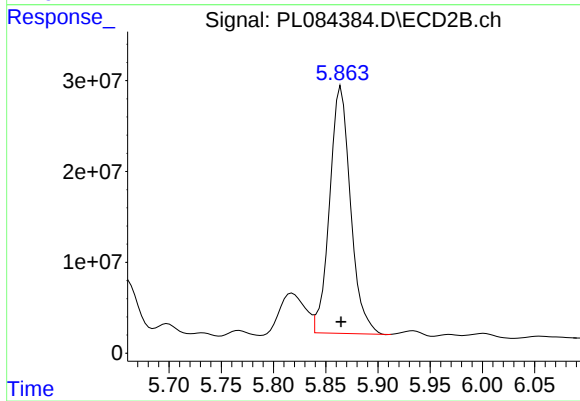

#27 Chlordane-5


R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 379294929
Conc: 764.97 ng/ml

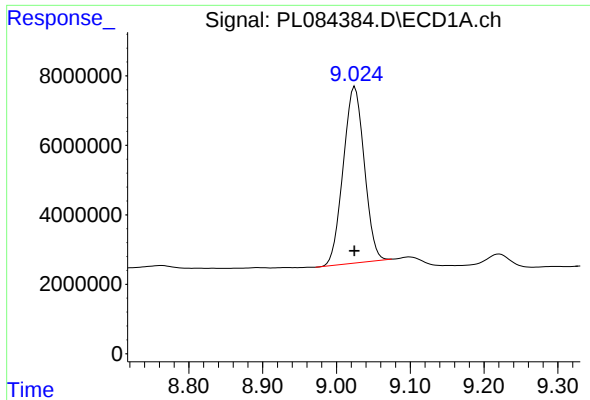

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 100478172
Conc: 73.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

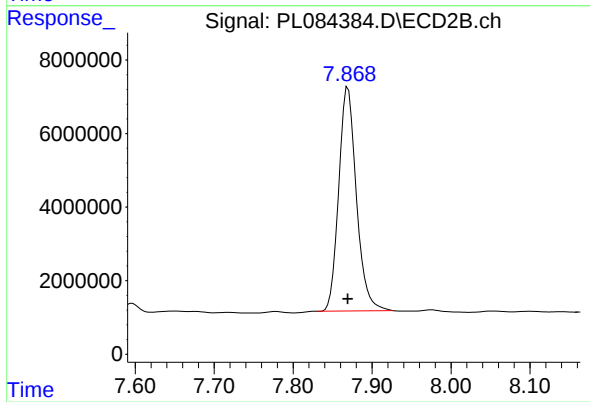

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.000 min
Response: 94663686
Conc: 74.85 ng/ml