

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 16:41
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:18:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:17:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.682	108.5E6	187.6E6	50.000	50.000
28)	SA Decachlor...	9.024	7.869	68598979	63238050	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.644	3.689	483.5E6	193.9E6	500.000	500.000
24)	Chlordane-2	5.178	4.270	438.5E6	204.9E6	500.000	500.000
25)	Chlordane-3	5.891	4.904	1956.4E6	677.0E6	500.000	500.000
26)	Chlordane-4	5.973	4.966	2252.3E6	708.0E6	500.000	500.000
27)	Chlordane-5	6.824	5.865	338.1E6	247.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 16:41
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:18:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:17:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

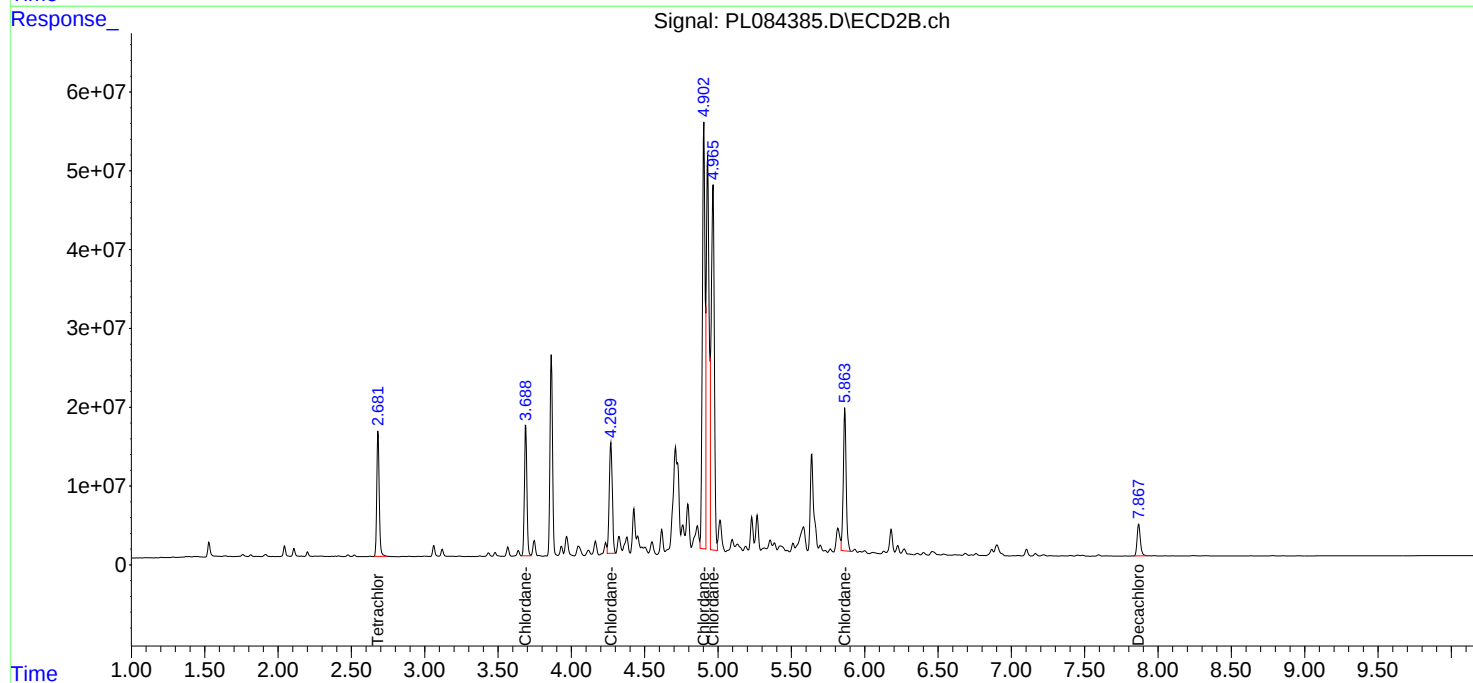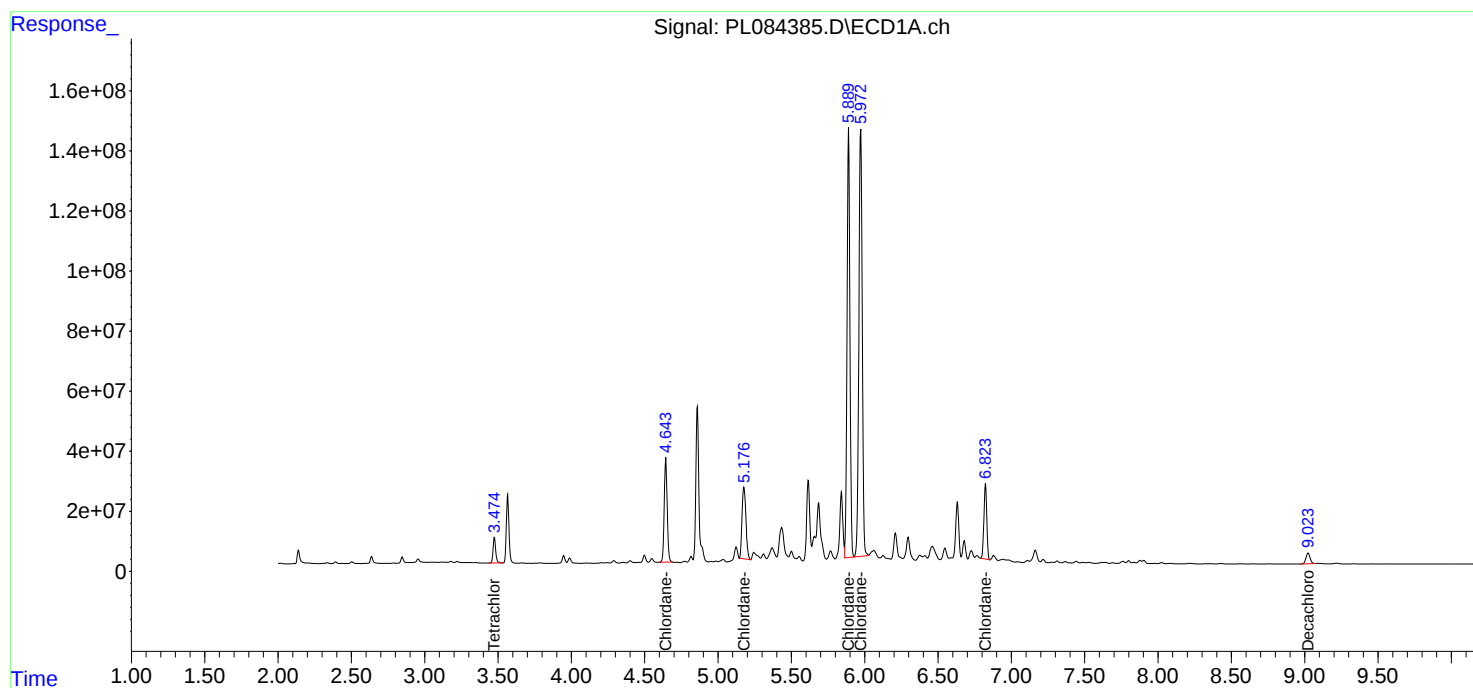


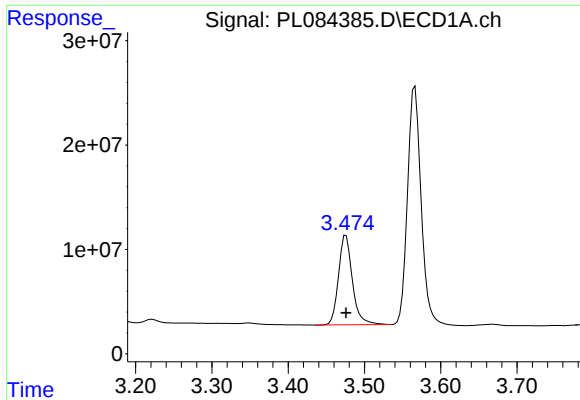

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 108523367
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

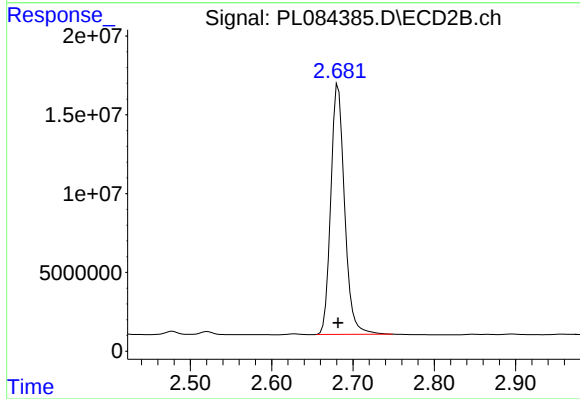


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 187626792
Conc: 50.00 ng/ml

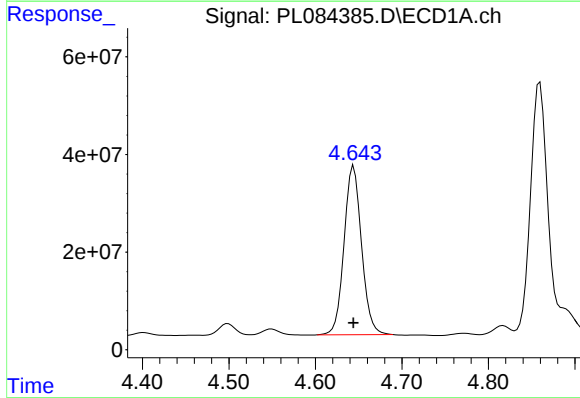


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 483494873
Conc: 500.00 ng/ml

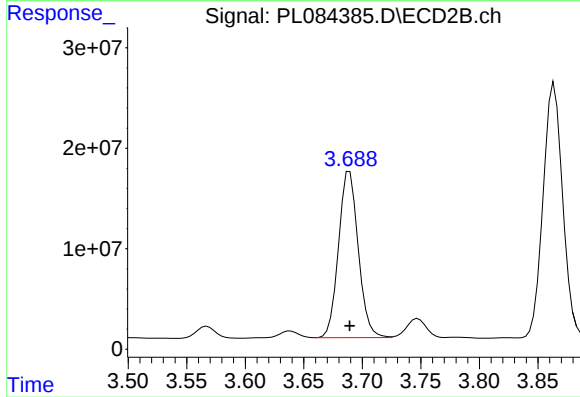

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 193863297
Conc: 500.00 ng/ml

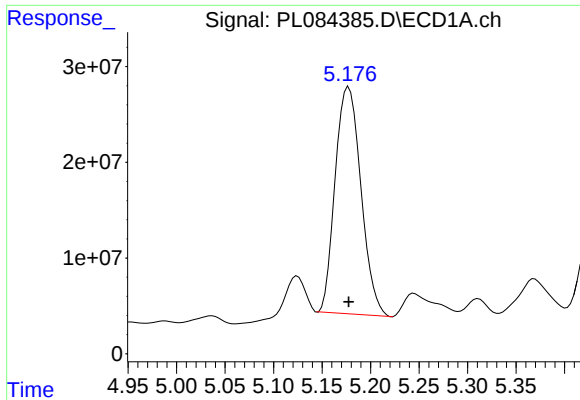

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 438457568
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

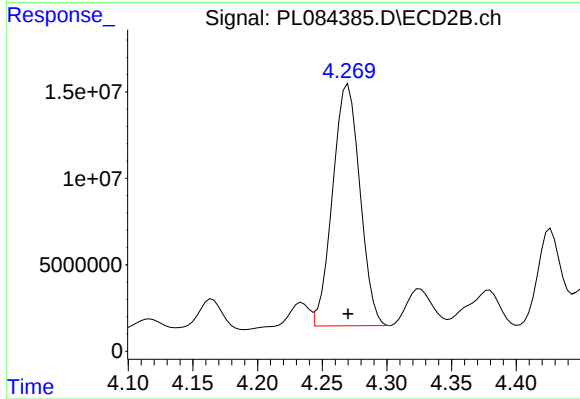


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 204886383
Conc: 500.00 ng/ml

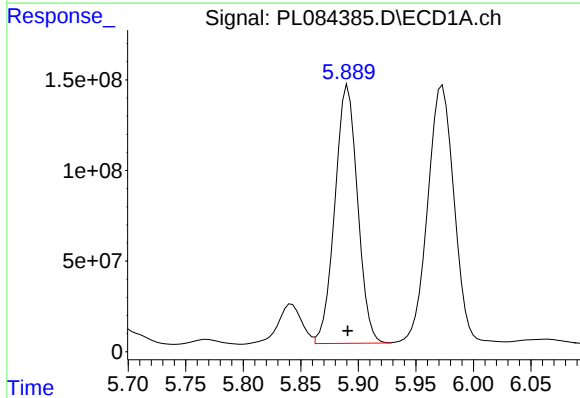


#25 Chlordane-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 1956417337
Conc: 500.00 ng/ml

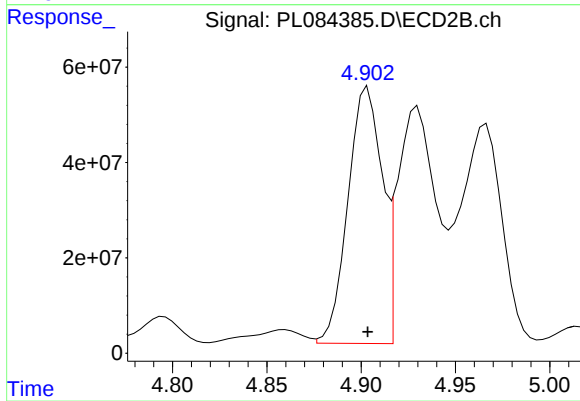

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 676986521
Conc: 500.00 ng/ml

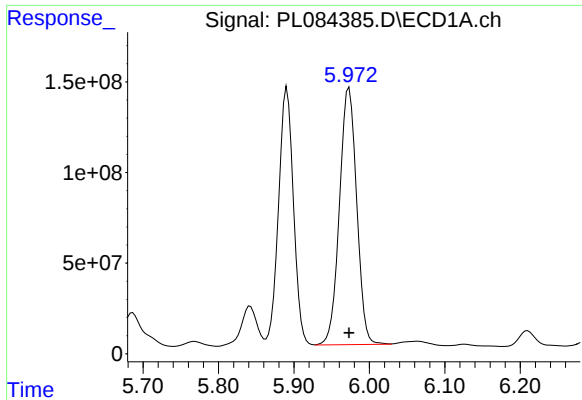

#26 Chlordane-4


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 2252300376
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

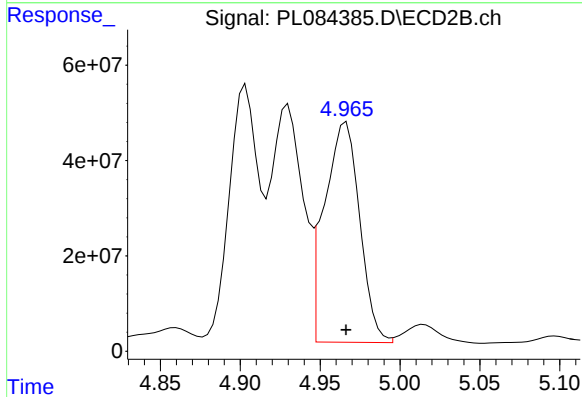


#26 Chlordane-4

R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 708035899
Conc: 500.00 ng/ml

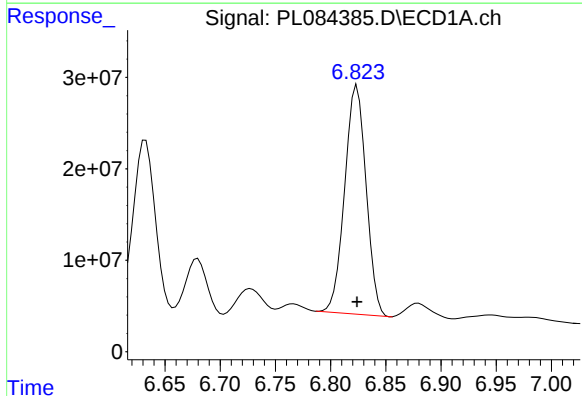


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.000 min
Response: 338124805
Conc: 500.00 ng/ml

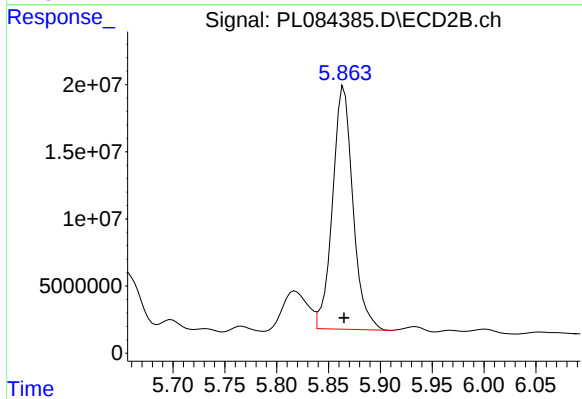

#27 Chlordane-5


R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 247914930
Conc: 500.00 ng/ml

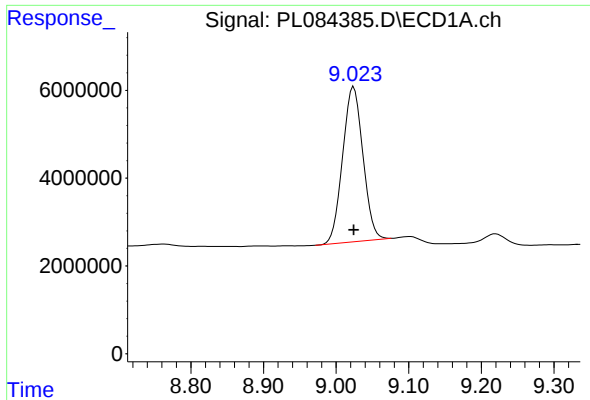

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 68598979
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

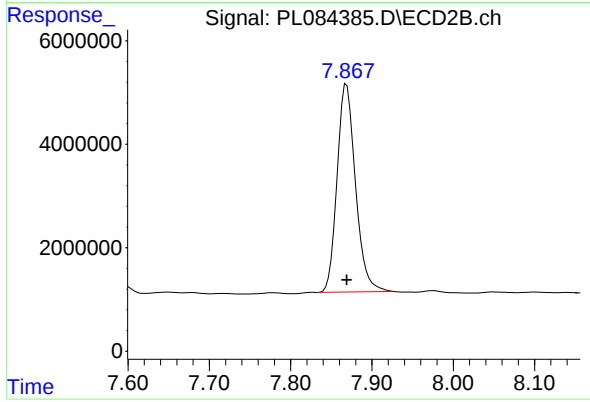

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: 0.000 min
Response: 63238050
Conc: 50.00 ng/ml