

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 16:55
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 17:18:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:17:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.682	56699139	95989224	26.123	25.580
28)	SA Decachlor...	9.024	7.870	37845453	34587053	27.585	27.347
Target Compounds							
23)	Chlordane-1	4.644	3.689	245.2E6	97814056	253.543	252.276
24)	Chlordane-2	5.177	4.270	232.2E6	109.1E6	264.829	266.296
25)	Chlordane-3	5.890	4.904	993.5E6	357.0E6	253.899	263.655
26)	Chlordane-4	5.973	4.966	1154.6E6	373.1E6	256.322	263.460
27)	Chlordane-5	6.824	5.865	172.6E6	127.4E6	255.244	256.854



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 16:55
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 17:18:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:17:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

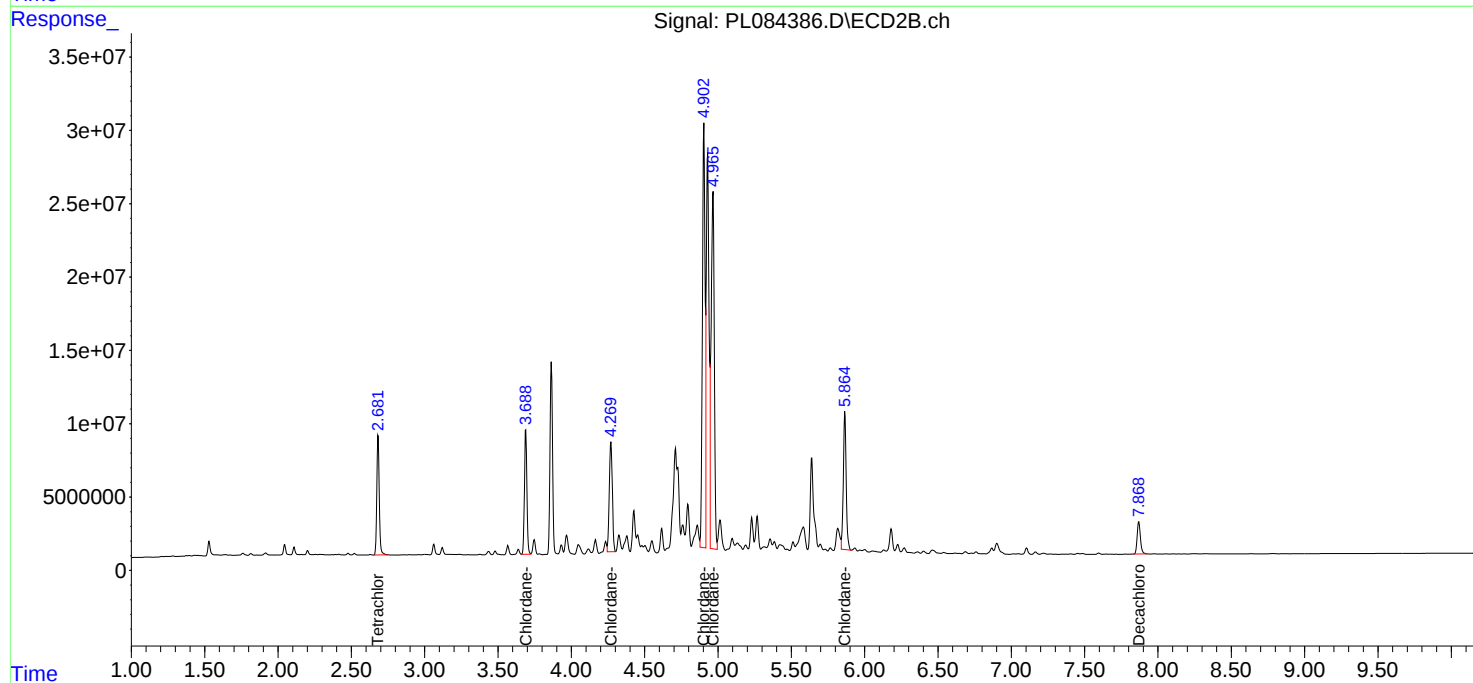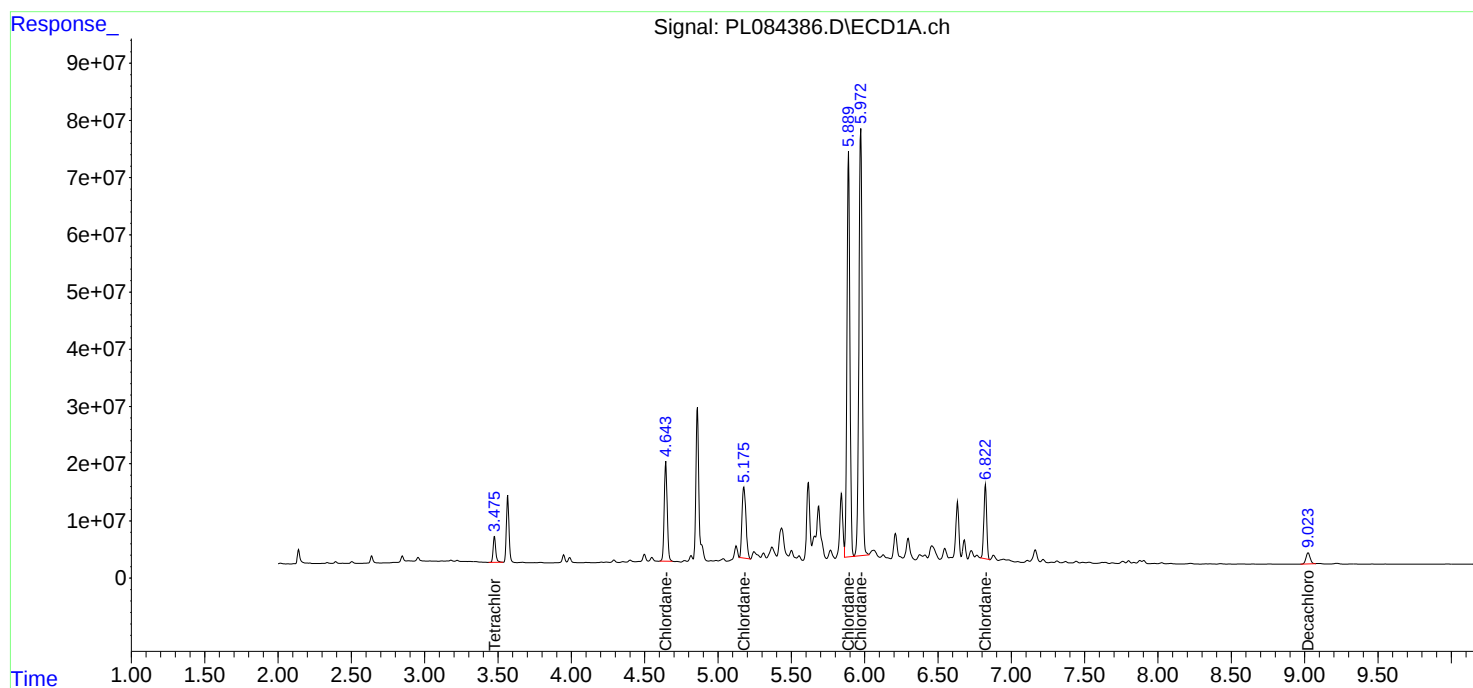


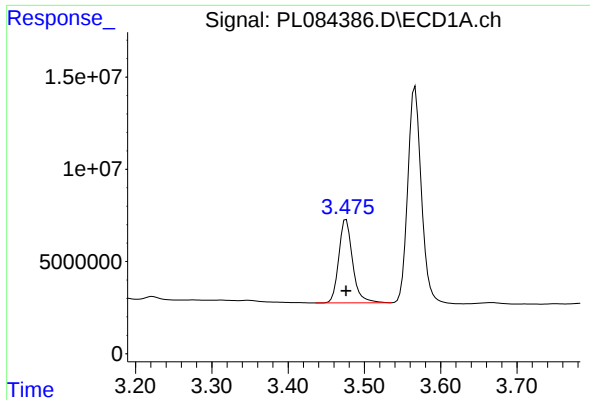

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 56699139
Conc: 26.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

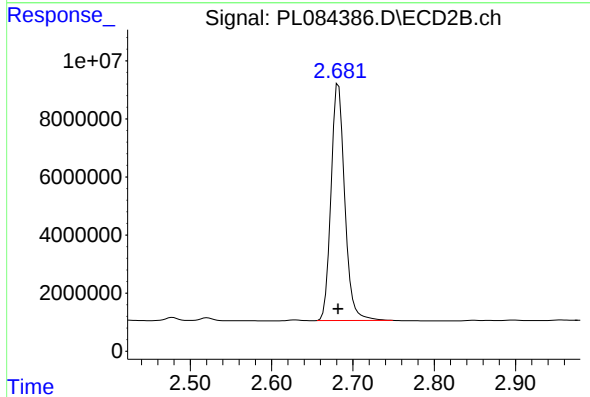


#1 Tetrachloro-m-xylene

R.T.: 2.682 min
Delta R.T.: 0.000 min
Response: 95989224
Conc: 25.58 ng/ml

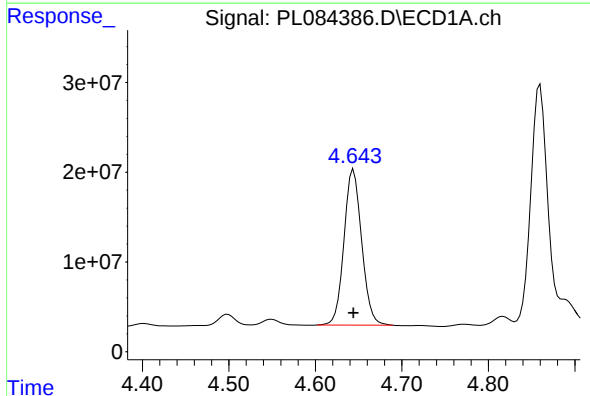


#23 Chlordane-1

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 245173825
Conc: 253.54 ng/ml

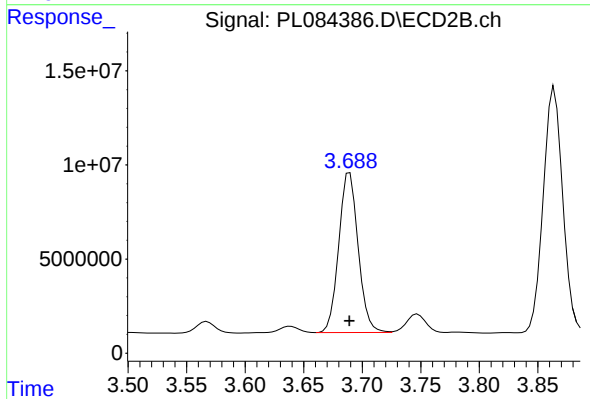

#23 Chlordane-1


R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 97814056
Conc: 252.28 ng/ml

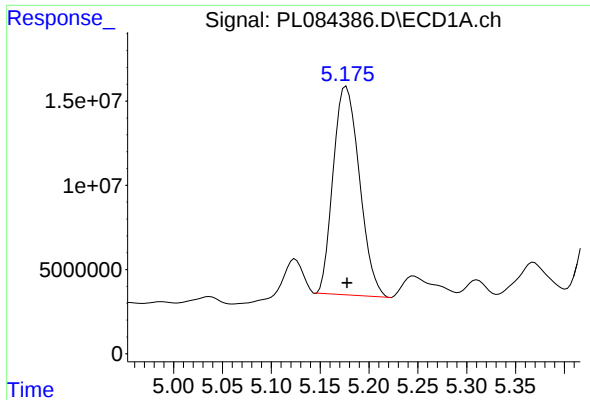

#24 Chlordane-2


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 232232844
Conc: 264.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

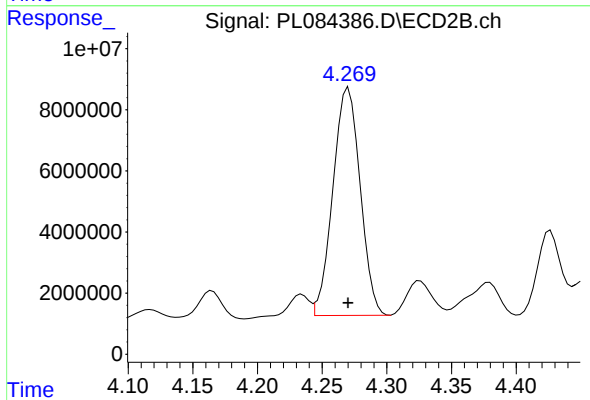


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 109120670
Conc: 266.30 ng/ml

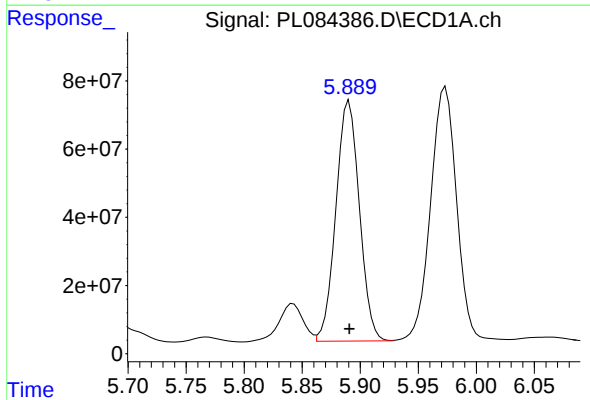


#25 Chlordane-3

R.T.: 5.890 min
Delta R.T.: 0.000 min
Response: 993464976
Conc: 253.90 ng/ml

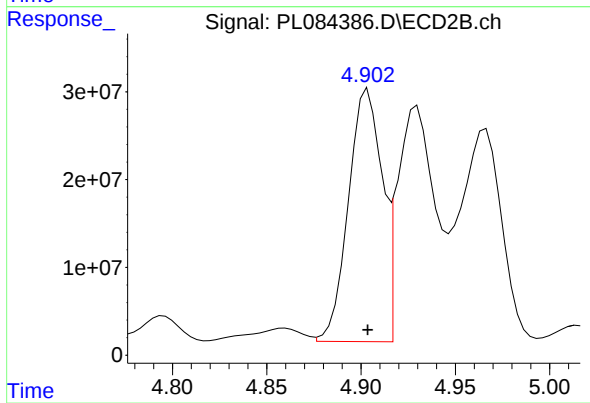

#25 Chlordane-3


R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 356981401
Conc: 263.65 ng/ml

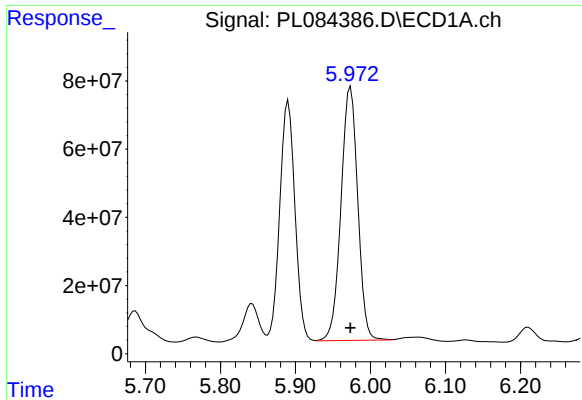

#26 Chlordane-4


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 1154629019
Conc: 256.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

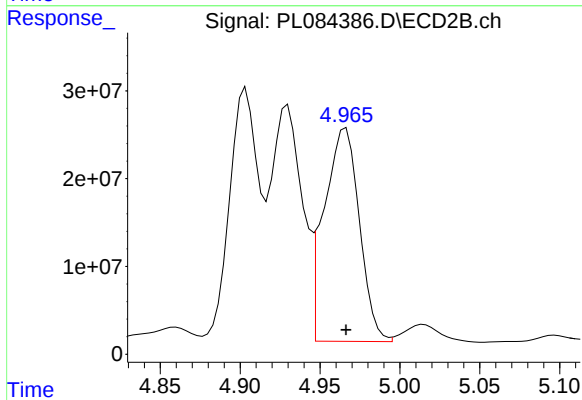


#26 Chlordane-4

R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 373078326
Conc: 263.46 ng/ml

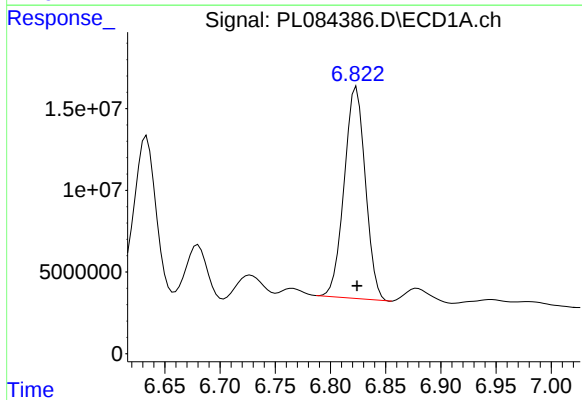


#27 Chlordane-5

R.T.: 6.824 min
Delta R.T.: 0.000 min
Response: 172608869
Conc: 255.24 ng/ml

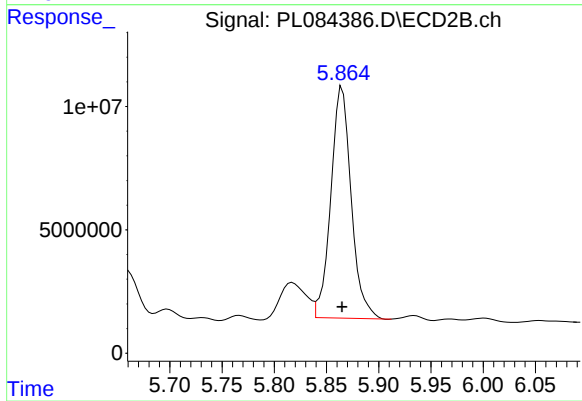

#27 Chlordane-5


R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 127356062
Conc: 256.85 ng/ml

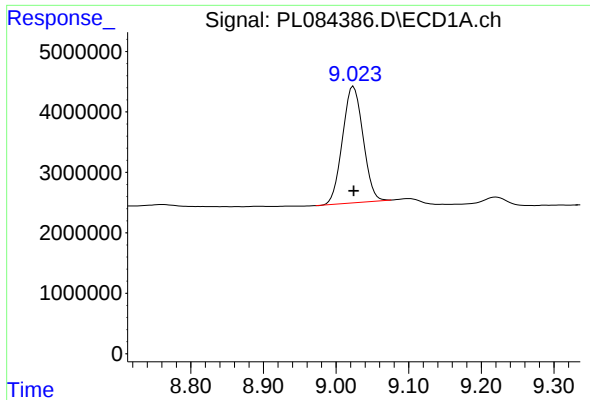

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 37845453
Conc: 27.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

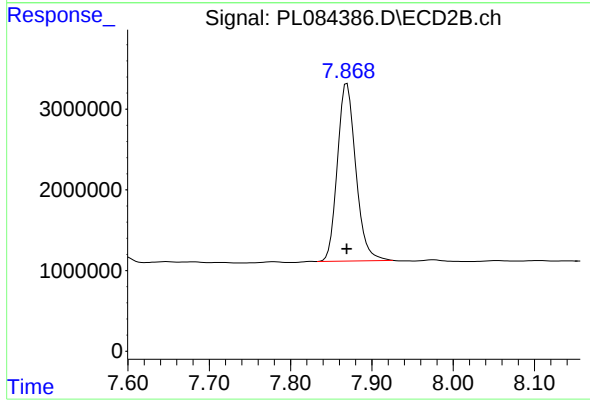

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: 0.000 min
Response: 34587053
Conc: 27.35 ng/ml