

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 23:11
 Operator : AR\AJ
 Sample : 03815-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUP-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/01/2023
 Supervised By : Ankita Jodhani 08/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 05:35:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:26:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.475	2.687	16539611	6637695	7.158m	6.071m
2) SA Decachlor...	9.032	7.868	14527065	9848113	9.459m	8.054
Target Compounds						
8) B Heptachlo...	5.631	4.643	3124613	1530179	1.021	1.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 23:11
Operator : AR\AJ
Sample : 03815-03
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/01/2023
Supervised By : Ankita Jodhani 08/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 05:35:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:26:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

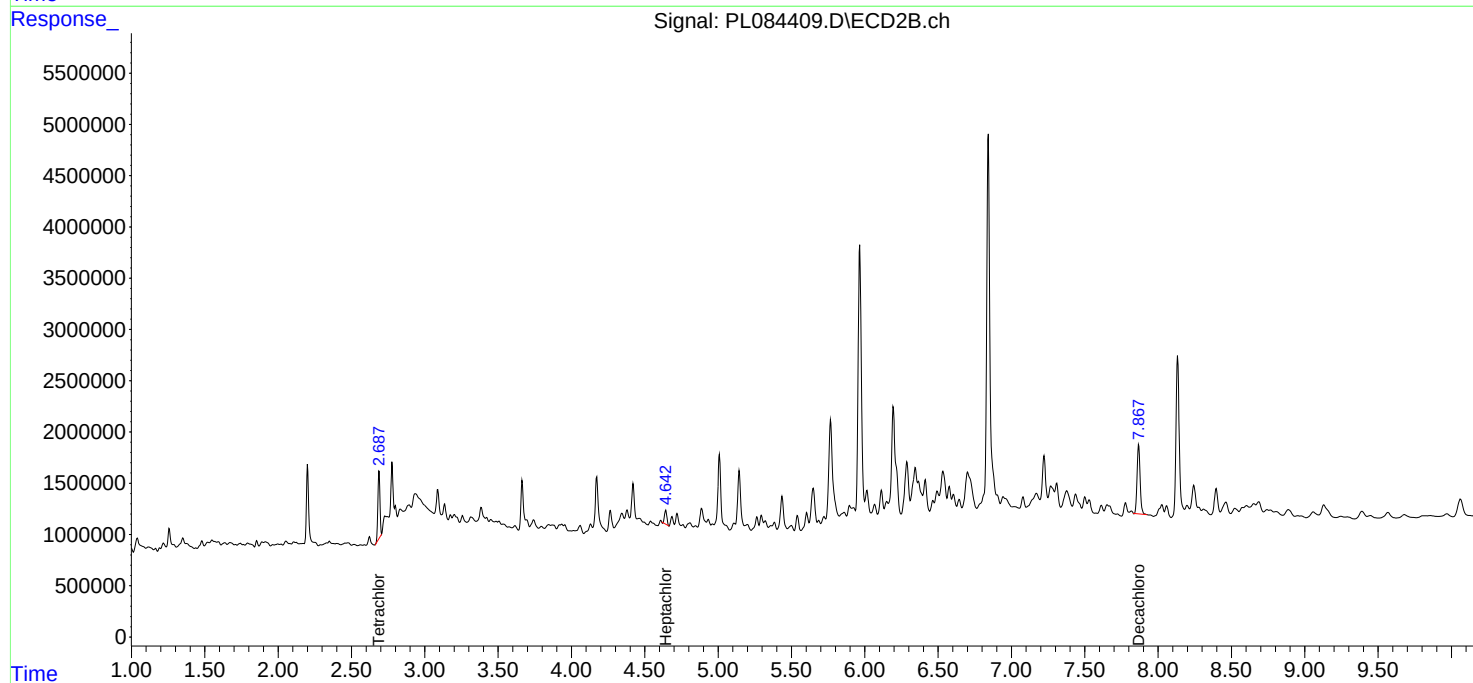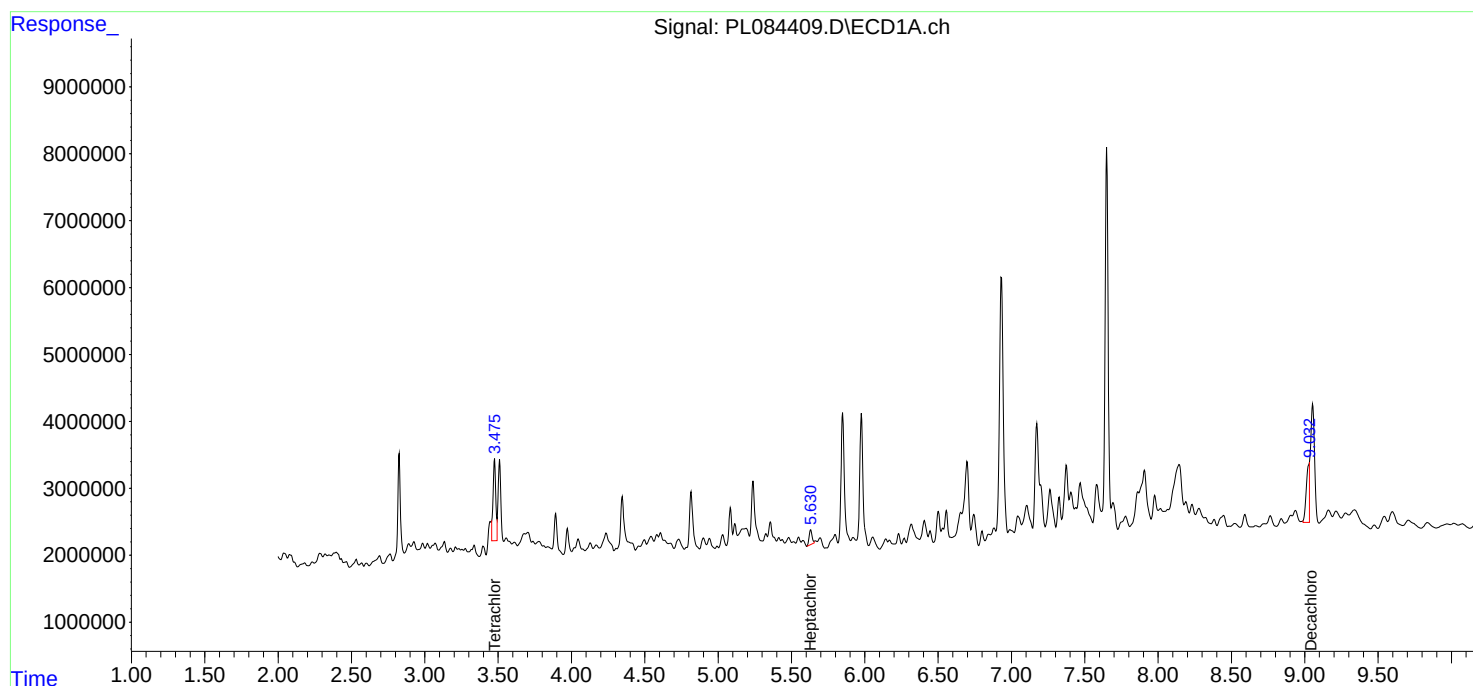

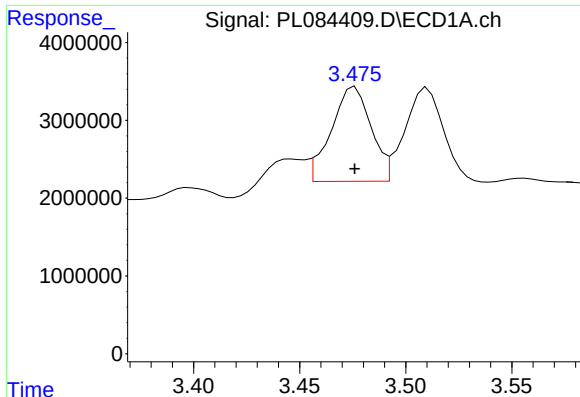


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: -0.001 min
Response: 16539611
Conc: 7.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

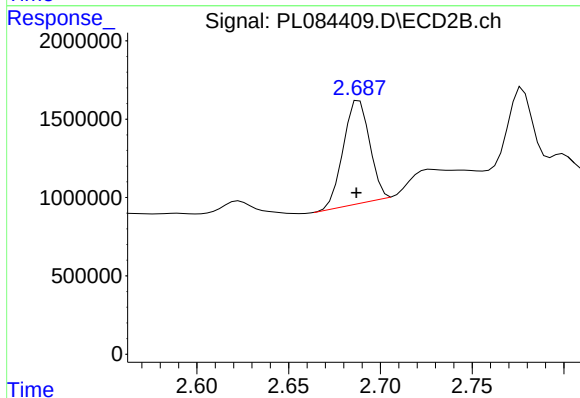


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 6637695
Conc: 6.07 ng/ml m

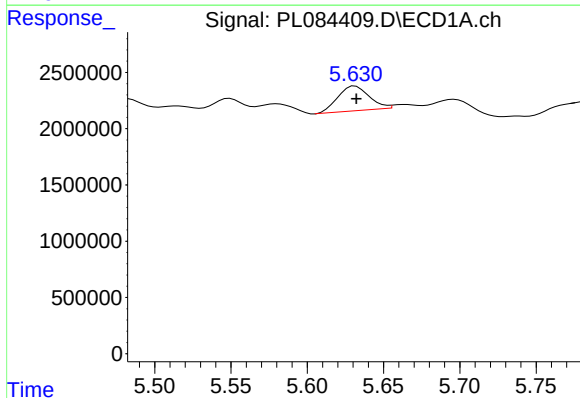


#8 Heptachlor epoxide

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 3124613
Conc: 1.02 ng/ml

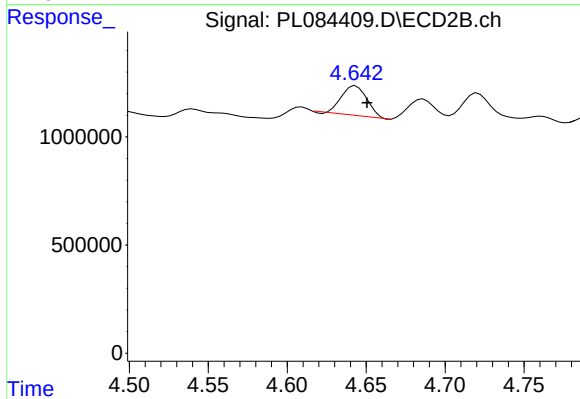

#8 Heptachlor epoxide

R.T.: 4.643 min
Delta R.T.: -0.007 min
Response: 1530179
Conc: 1.12 ng/ml

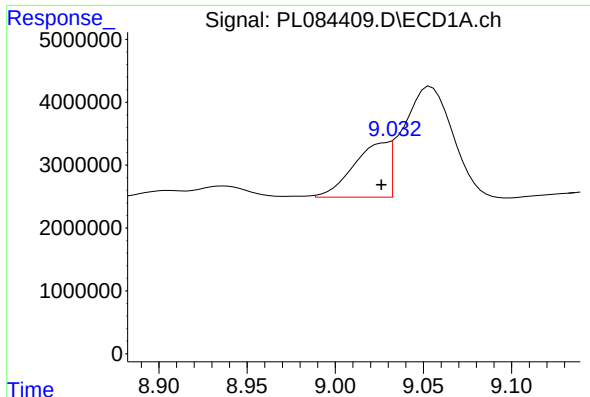


#28 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: 0.006 min
Response: 14527065
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

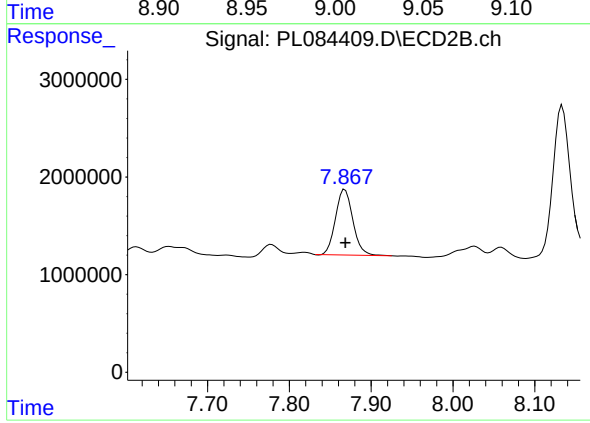

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 9848113
Conc: 8.05 ng/ml