

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
 Data File : PL084411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2023 23:39
 Operator : AR\AJ
 Sample : 03815-05
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUILDING-B-7-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 05:36:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 31 17:26:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.686	24714593	11582430	10.696	10.594
28)	SA Decachlor...	9.023	7.867	15421329	10913482	10.041	8.925

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080123\
Data File : PL084411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2023 23:39
Operator : AR\AJ
Sample : 03815-05
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-7-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 05:36:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Mon Jul 31 17:26:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

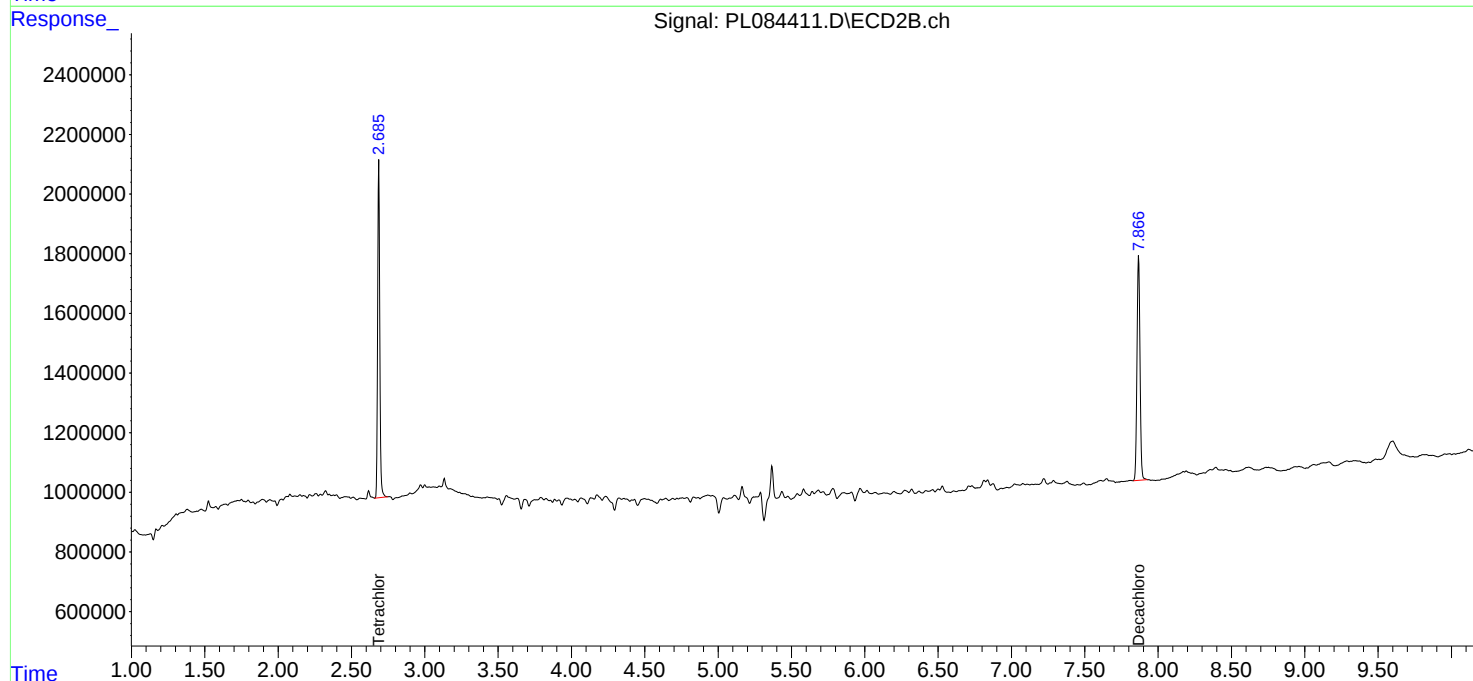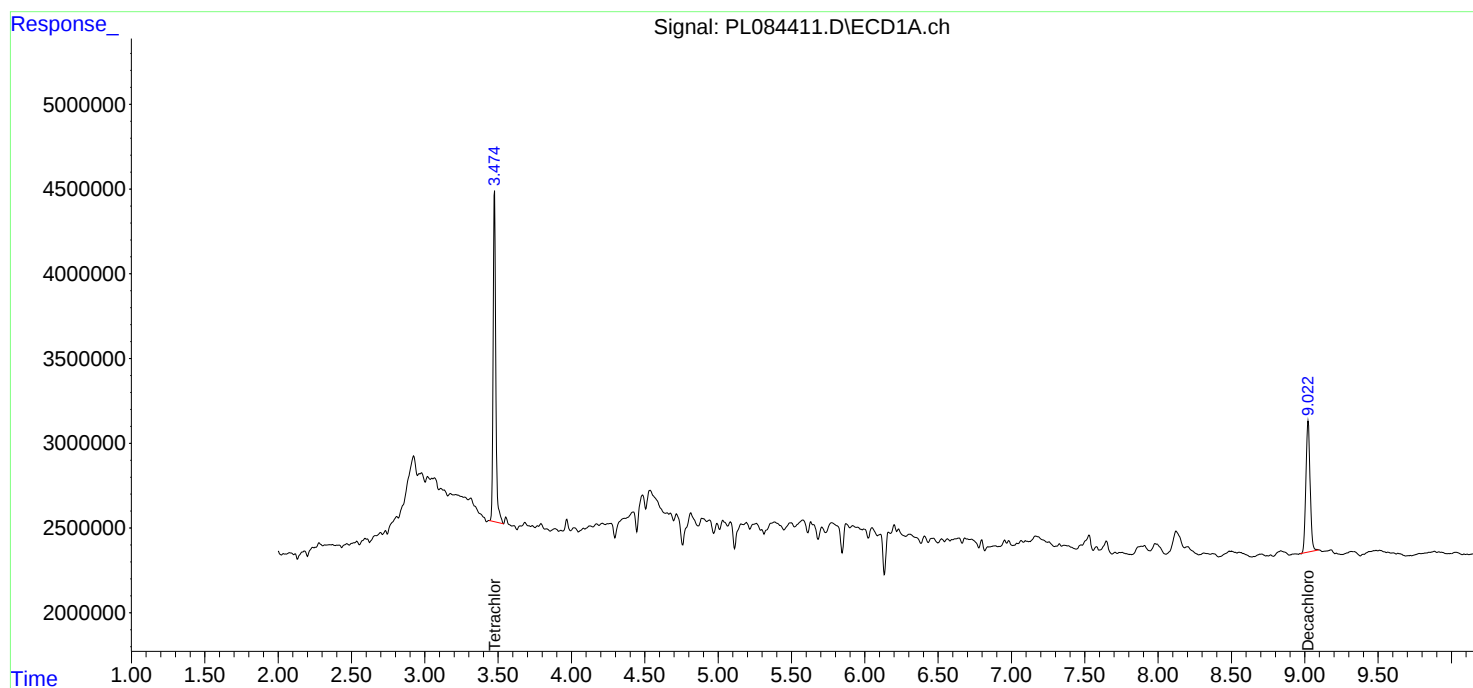


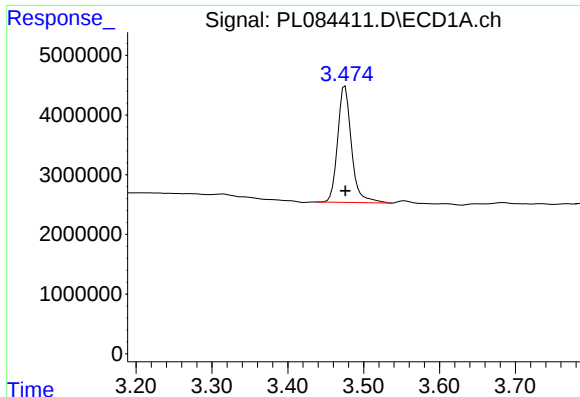

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 24714593
Conc: 10.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-7-(0-5)

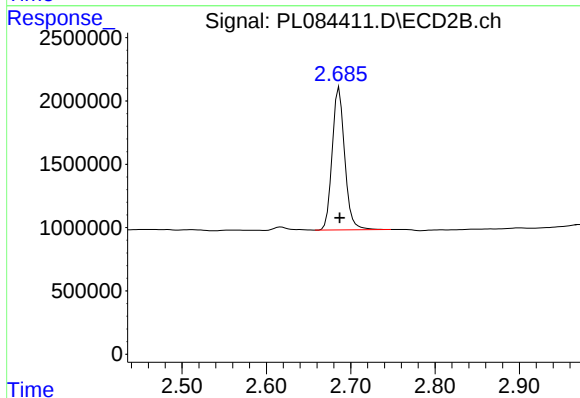


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 11582430
Conc: 10.59 ng/ml

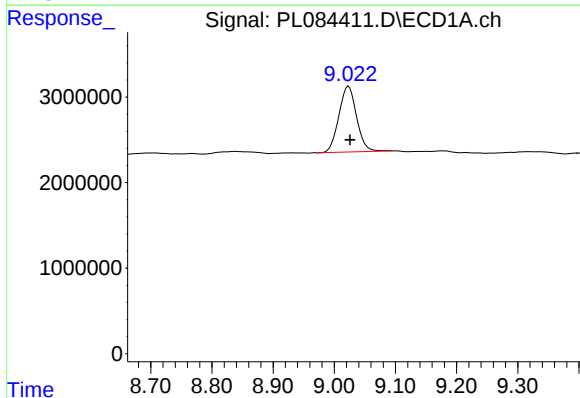

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: -0.003 min
Response: 15421329
Conc: 10.04 ng/ml

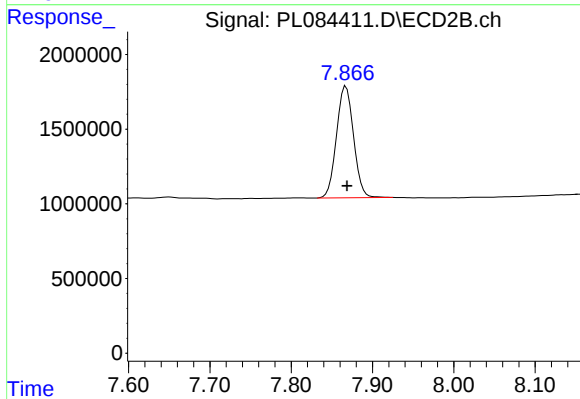

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: -0.001 min
Response: 10913482
Conc: 8.92 ng/ml