

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080218\
 Data File : PL038806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2018 11:11
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 00:45:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.240f	0.000	14007043	0	2.967	N.D.	#
7) B	delta-BHC	0.000	4.957	0	2373880	N.D.	0.716	#
8) B	Heptachlo...	4.944f	5.771	9088403	2359165	0.964	0.830	
12) B	4,4'-DDE	0.000	6.295f	0	2501644	N.D.	0.936	#
15) B	Endosulfa...	0.000	6.827	0	280418	N.D.	0.117	#
16) A	4,4'-DDD	0.000	6.680f	0	16707097	N.D.	7.806	#
19) B	Endosulfa...	6.538f	0.000	49993809	0	6.619	N.D.	#
23)	Chlordane-1	4.106	4.957	13778257	2373880	39.793	20.485	#
27)	Chlordane-5	0.000	6.827	0	280418	N.D.	3.130	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080218\
Data File : PL038806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2018 11:11
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 00:45:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

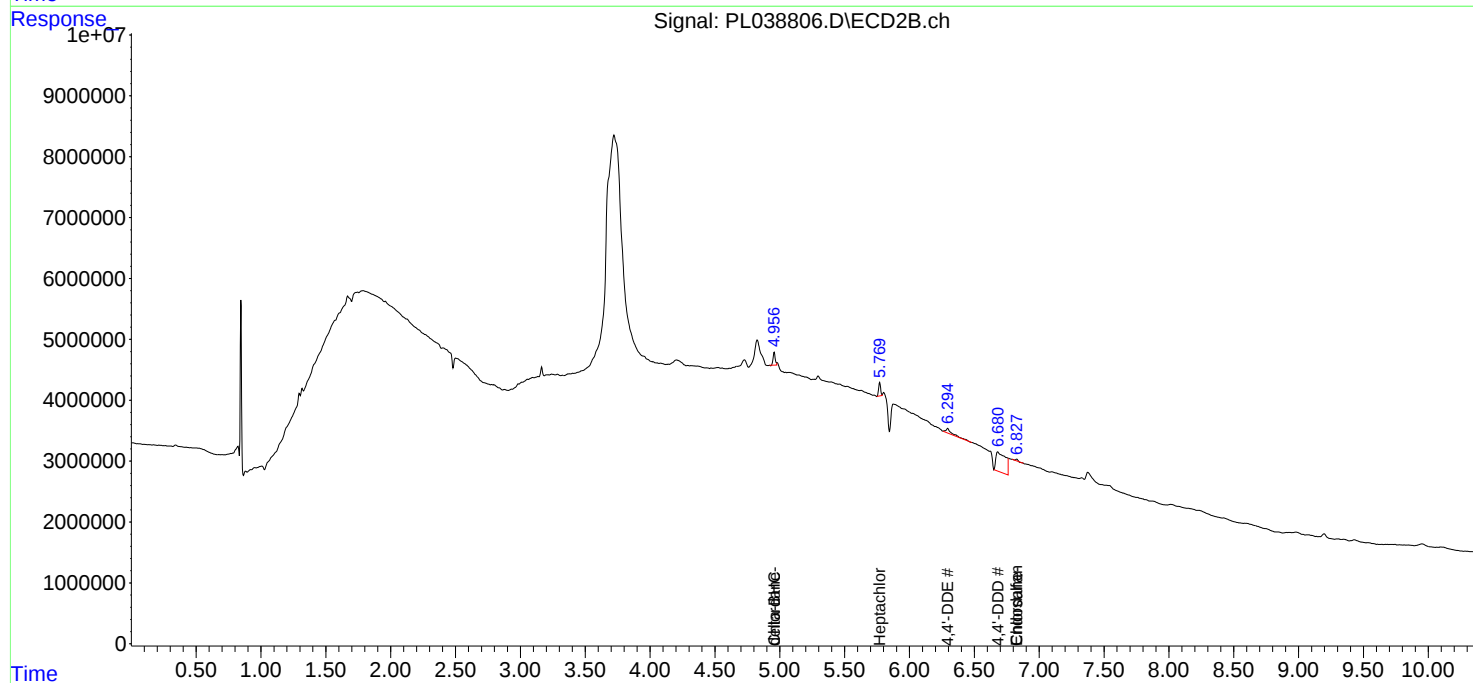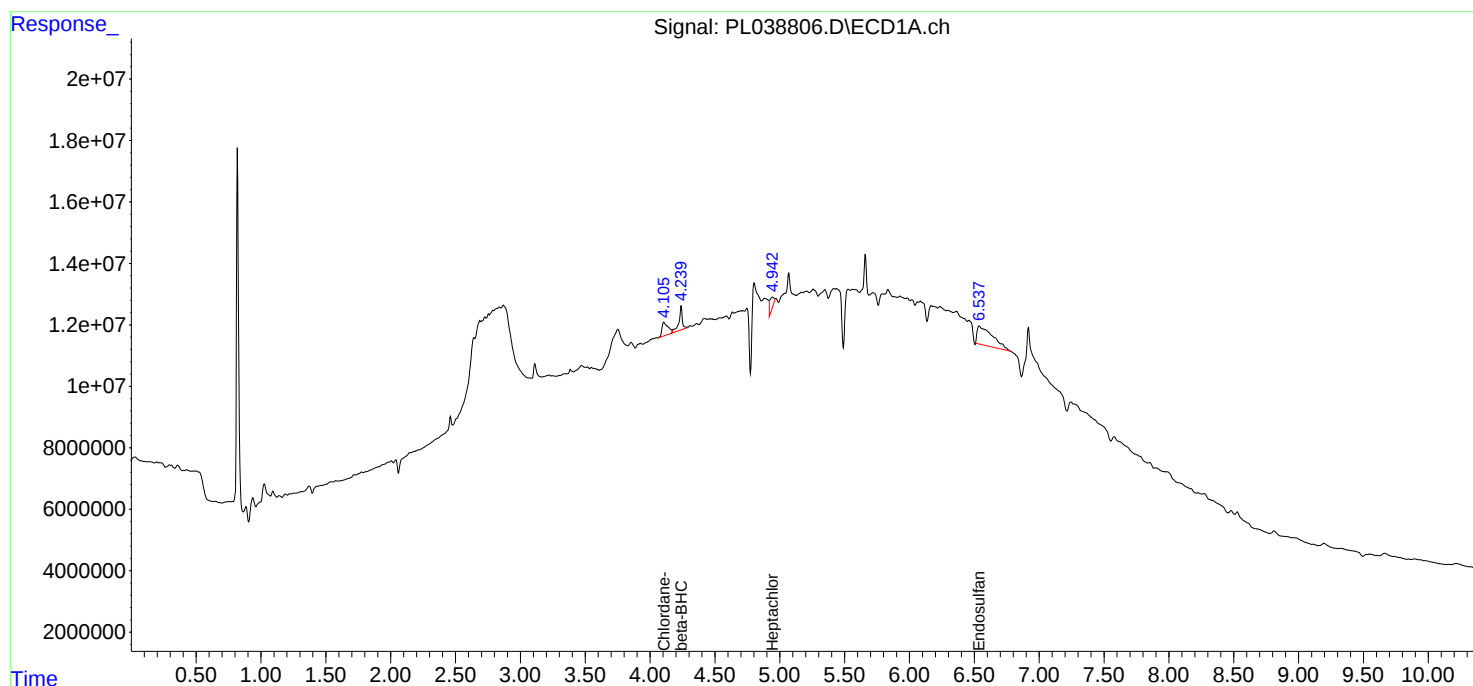


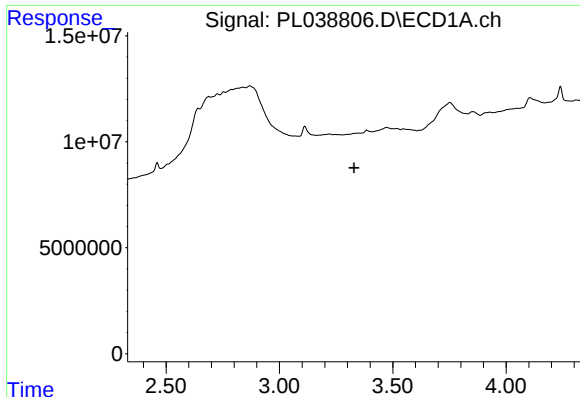

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

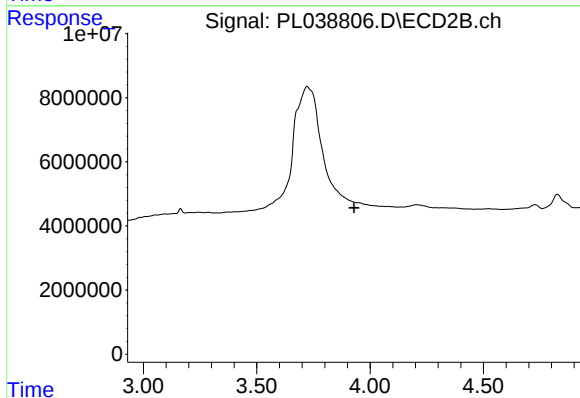


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.930 min
Response: 0
Conc: N.D.

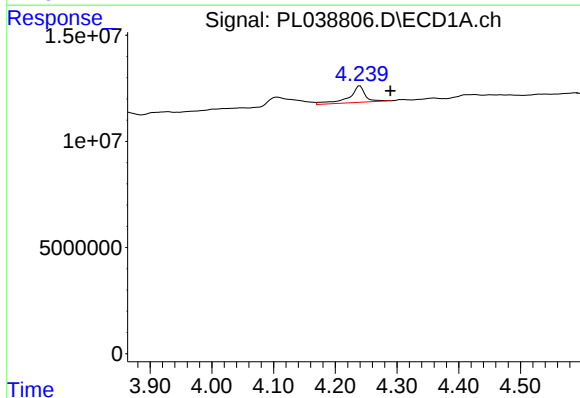


#6 beta-BHC

R.T.: 4.240 min
Delta R.T.: -0.049 min
Response: 14007043
Conc: 2.97 ng/ml

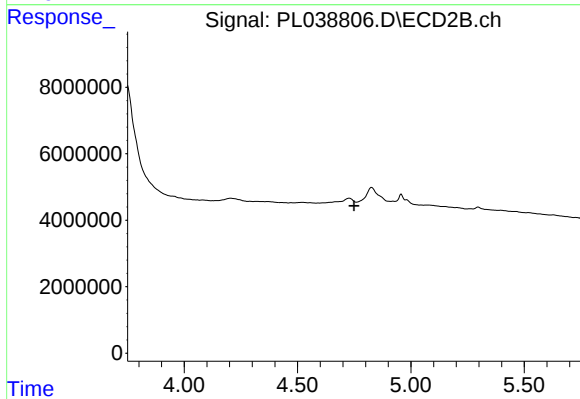

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

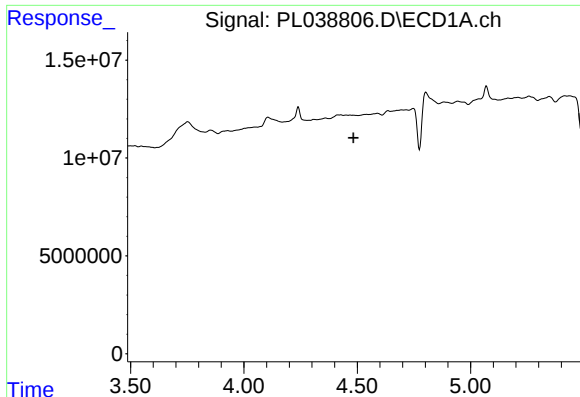

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

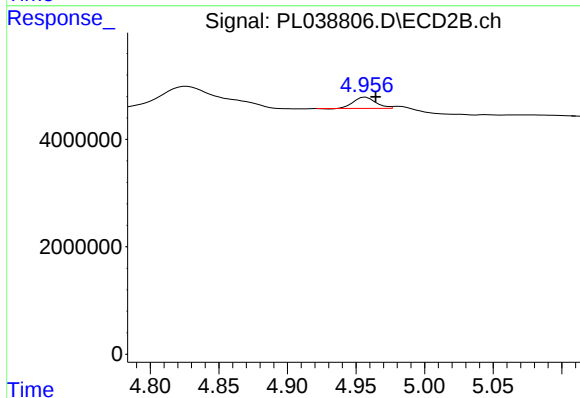


#7 delta-BHC

R.T.: 4.957 min
Delta R.T.: -0.007 min
Response: 2373880
Conc: 0.72 ng/ml

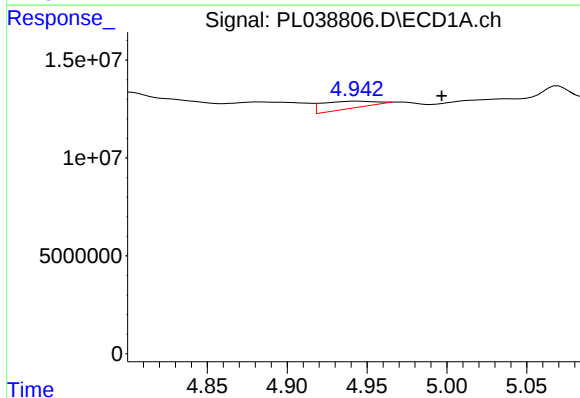


#8 Heptachlor epoxide

R.T.: 4.944 min
Delta R.T.: -0.053 min
Response: 9088403
Conc: 0.96 ng/ml

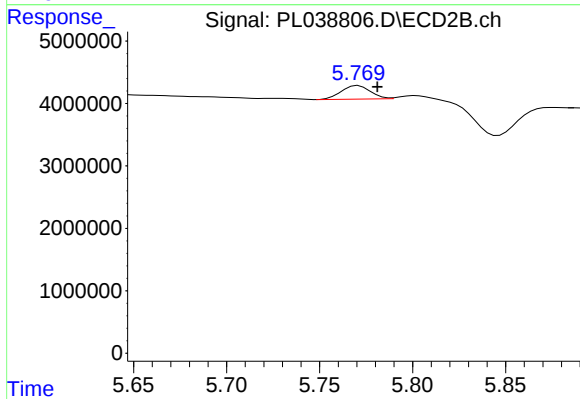

#8 Heptachlor epoxide


R.T.: 5.771 min
Delta R.T.: -0.010 min
Response: 2359165
Conc: 0.83 ng/ml

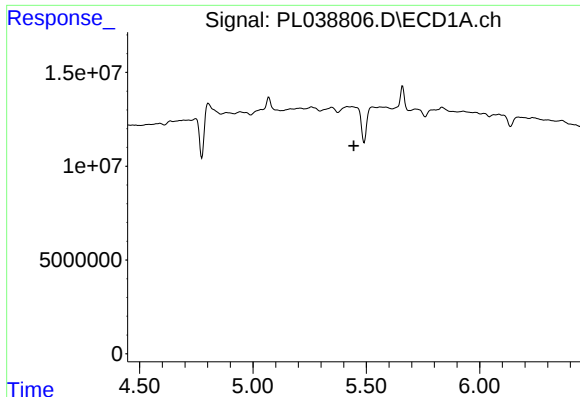

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

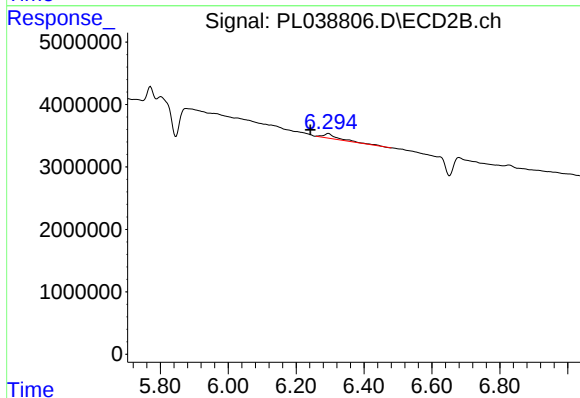


#12 4,4'-DDE

R.T.: 6.295 min
Delta R.T.: 0.053 min
Response: 2501644
Conc: 0.94 ng/ml

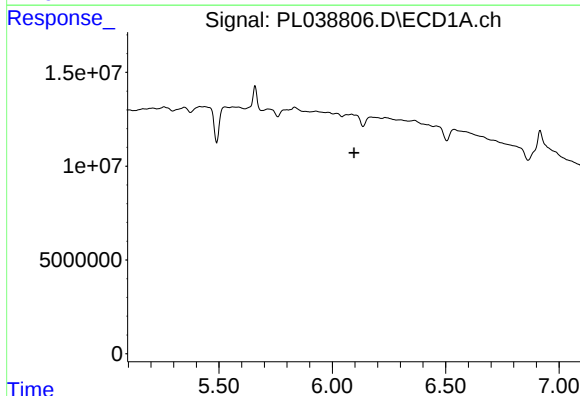


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

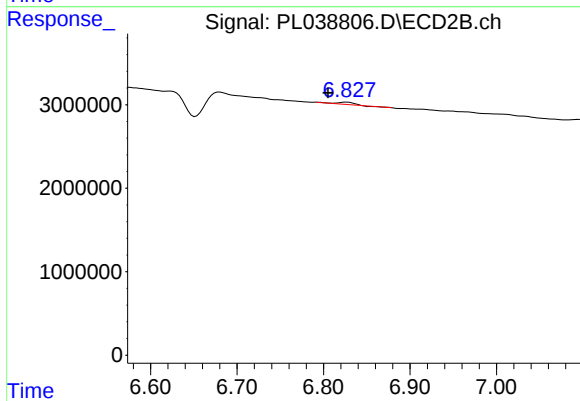

#15 Endosulfan II


R.T.: 6.827 min
Delta R.T.: 0.022 min
Response: 280418
Conc: 0.12 ng/ml

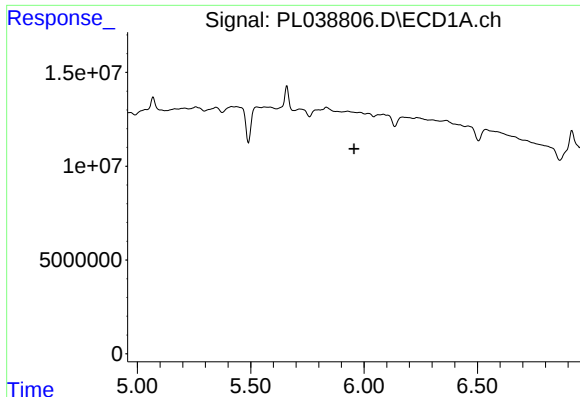

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

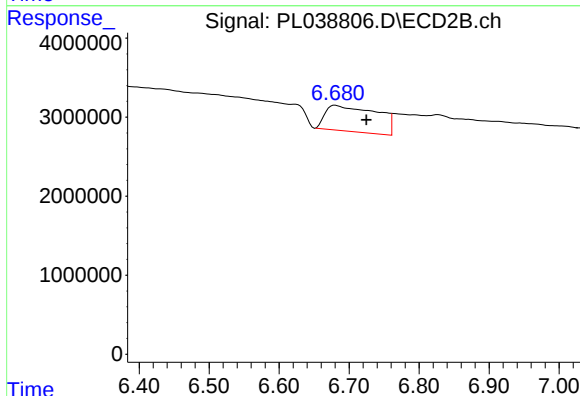


#16 4,4'-DDD

R.T.: 6.680 min
Delta R.T.: -0.044 min
Response: 16707097
Conc: 7.81 ng/ml

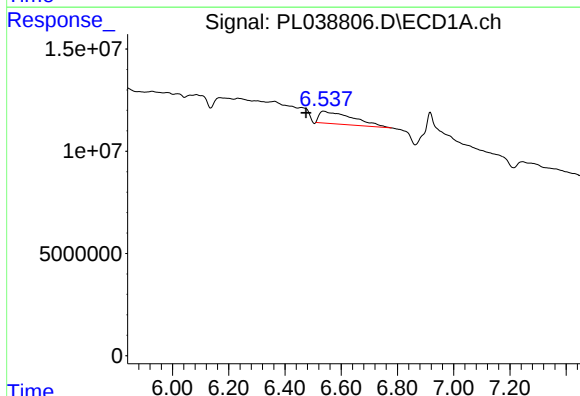


#19 Endosulfan Sulfate

R.T.: 6.538 min
Delta R.T.: 0.063 min
Response: 49993809
Conc: 6.62 ng/ml

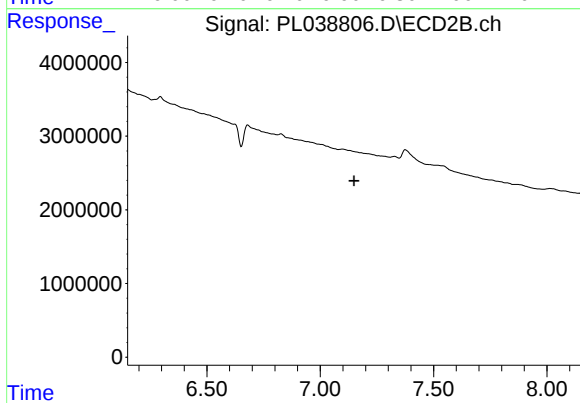

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

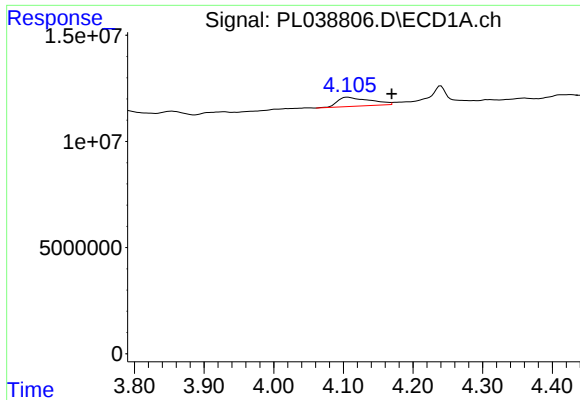

#23 Chlordane-1


R.T.: 4.106 min
Delta R.T.: -0.063 min
Response: 13778257
Conc: 39.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

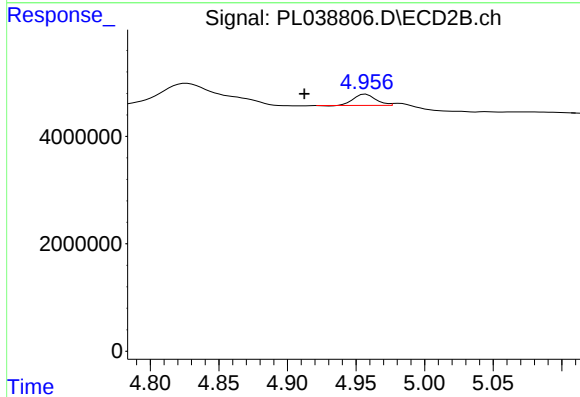


#23 Chlordane-1

R.T.: 4.957 min
Delta R.T.: 0.045 min
Response: 2373880
Conc: 20.48 ng/ml

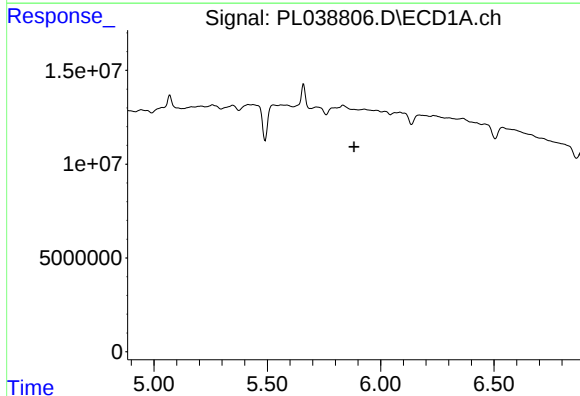


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

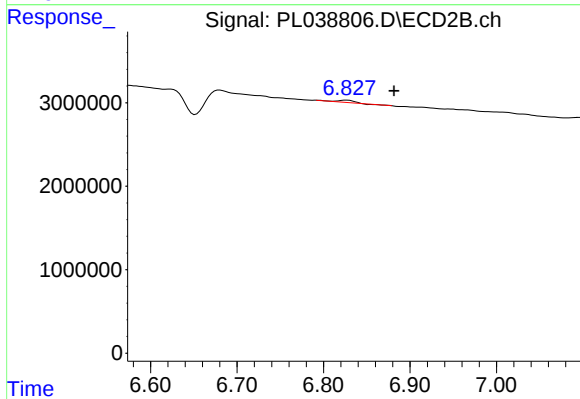

#27 Chlordane-5

R.T.: 6.827 min
Delta R.T.: -0.055 min
Response: 280418
Conc: 3.13 ng/ml

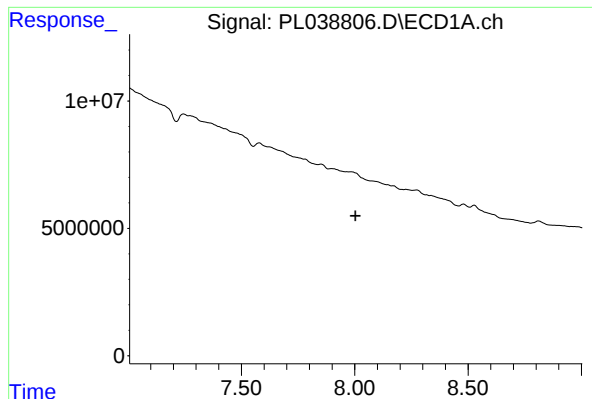

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T. : 8.004 min

Response: 0

Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

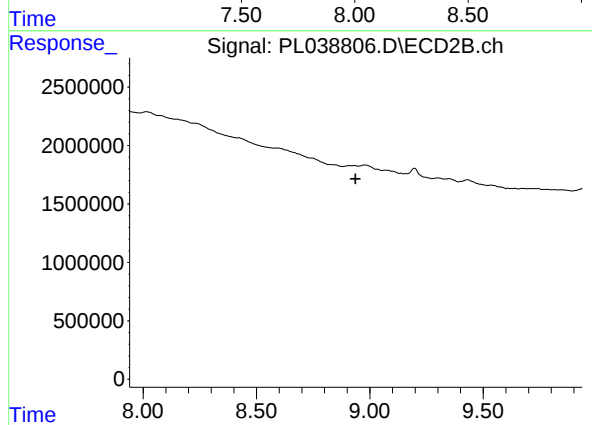

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 8.937 min

Response: 0

Conc: N.D.