

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080218\
 Data File : PL038870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2018 04:09
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 05:06:12 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.928	140.0E6	56872892	18.804	21.666
28)	SA Decachlor...	7.991	8.934	118.4E6	39436390	15.613	16.133
Target Compounds							
2)	A alpha-BHC	0.000	4.327	0	850690	N.D.	0.220 #
7)	B delta-BHC	0.000	4.957	0	1378912	N.D.	0.416 #
8)	B Heptachlo...	0.000	5.770	0	2019043	N.D.	0.710 #
13)	MA Dieldrin	5.520f	0.000	2763253	0	0.288	N.D. #
14)	MA Endrin	0.000	6.627	0	2563465	N.D.	1.073 #
16)	A 4,4'-DDD	0.000	6.677f	0	3195167	N.D.	1.493 #
20)	A Methoxychlor	0.000	7.547f	0	1425794	N.D.	1.252 #
21)	B Endrin ke...	6.914f	7.547f	8303391	1425794	1.058	0.598 #
23)	Chlordane-1	4.237	4.957	15487870	1378912	44.730	11.899 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080218\
Data File : PL038870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2018 04:09
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 05:06:12 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

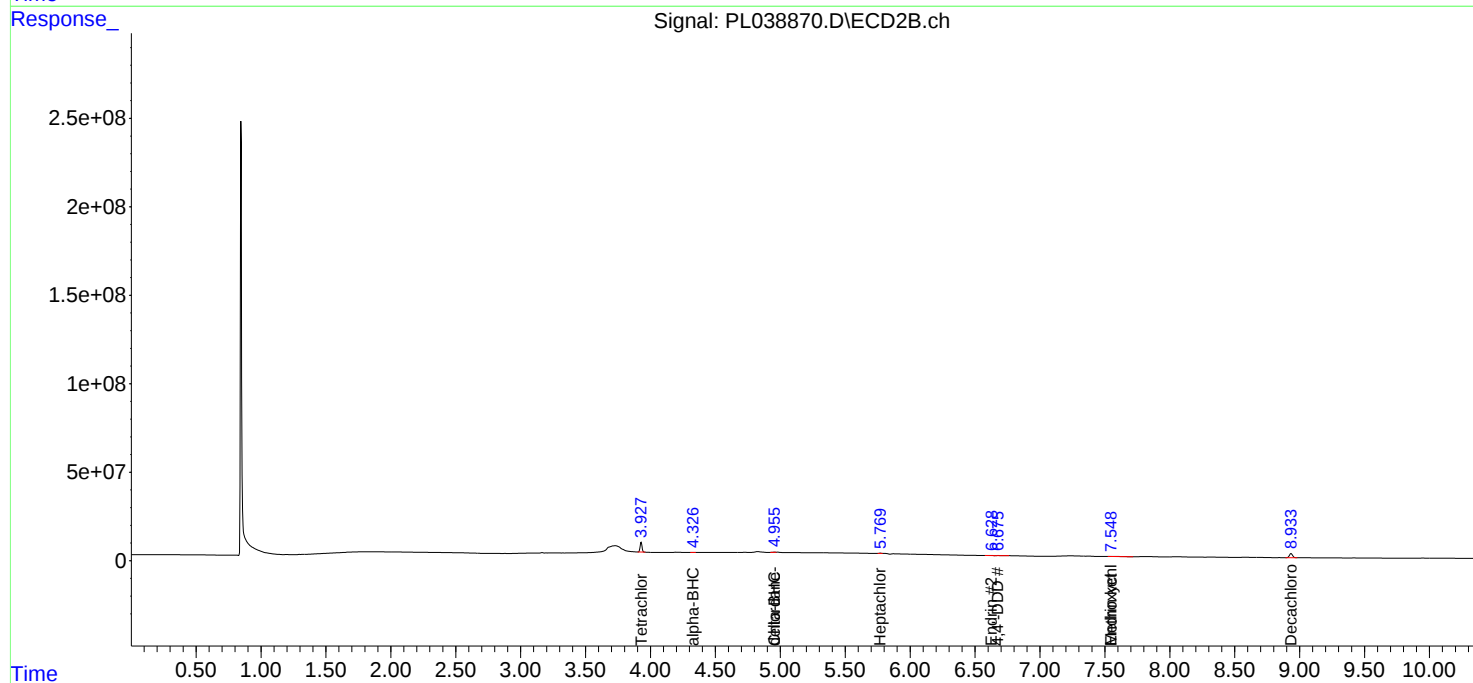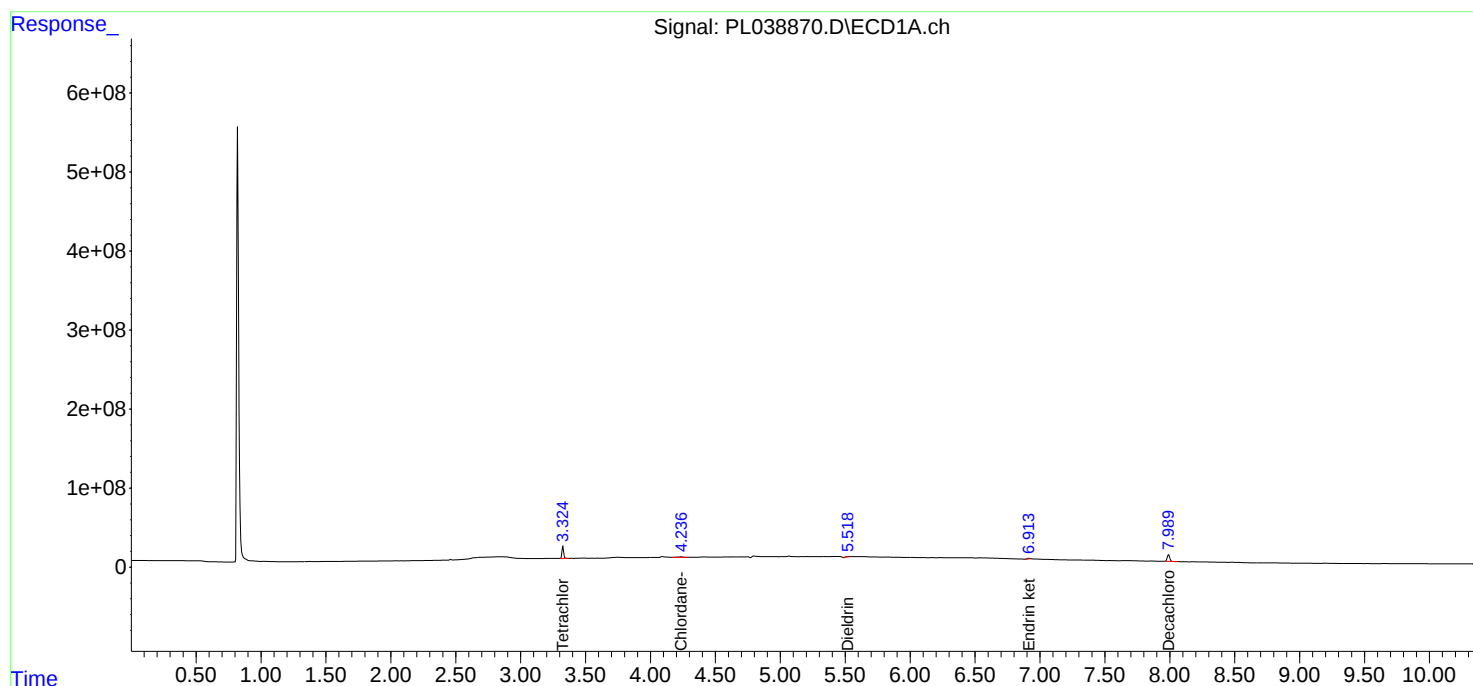


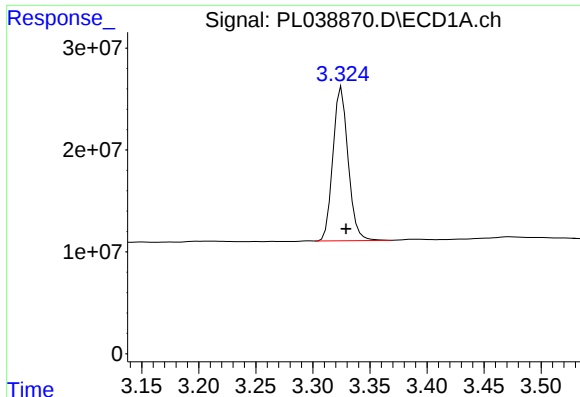

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 140021123
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

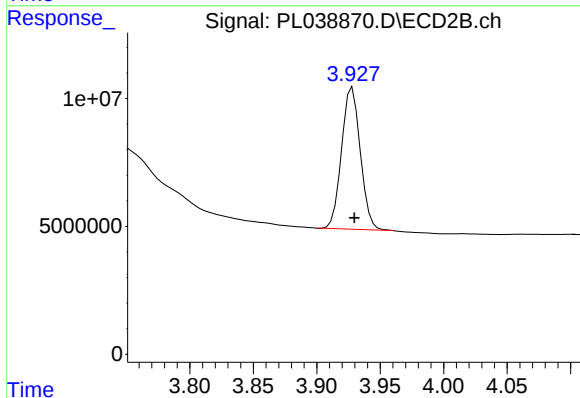


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 56872892
Conc: 21.67 ng/ml

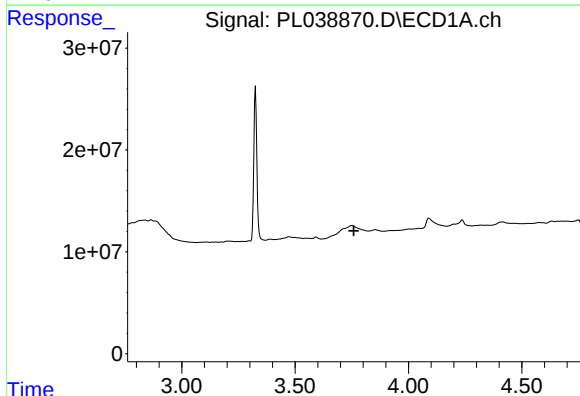


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

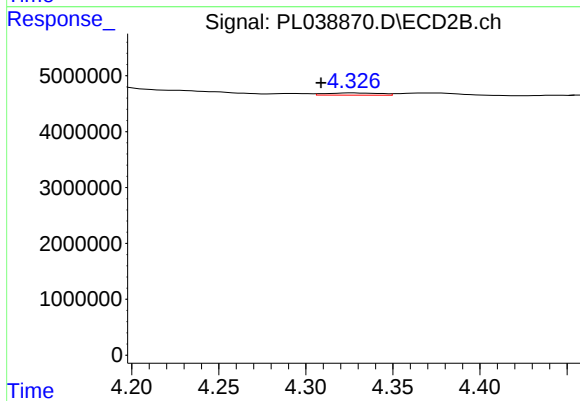

#2 alpha-BHC


R.T.: 4.327 min
Delta R.T.: 0.019 min
Response: 850690
Conc: 0.22 ng/ml

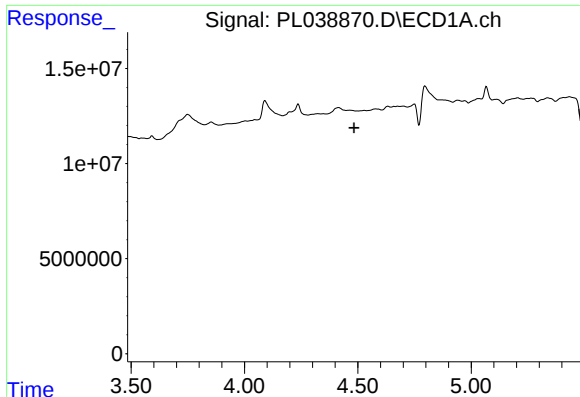

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

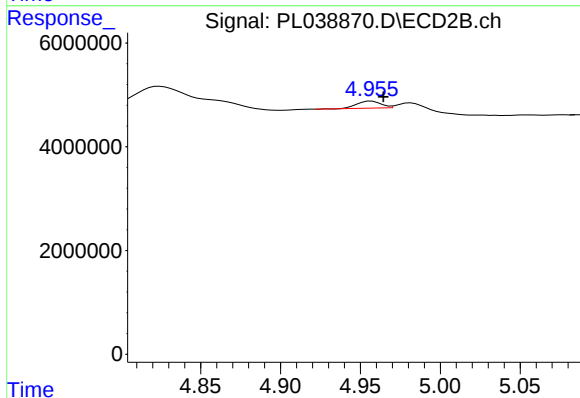


#7 delta-BHC

R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 1378912
Conc: 0.42 ng/ml

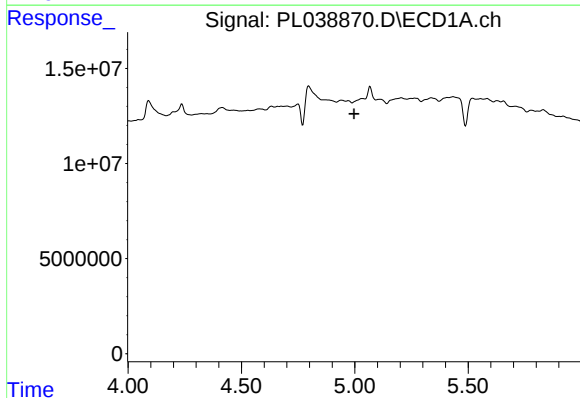


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

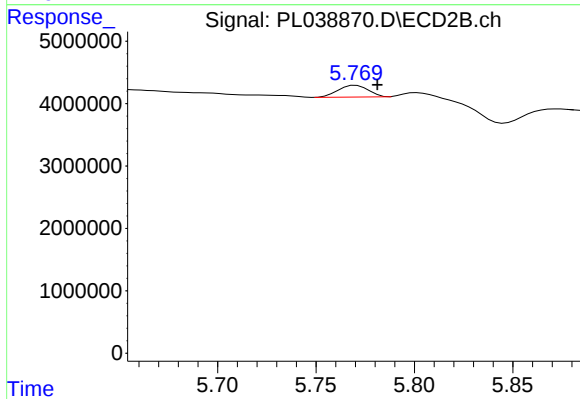

#8 Heptachlor epoxide


R.T.: 5.770 min
Delta R.T.: -0.011 min
Response: 2019043
Conc: 0.71 ng/ml

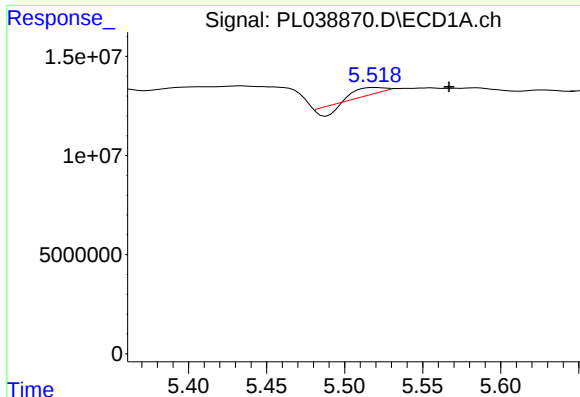

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: -0.047 min
Response: 2763253
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

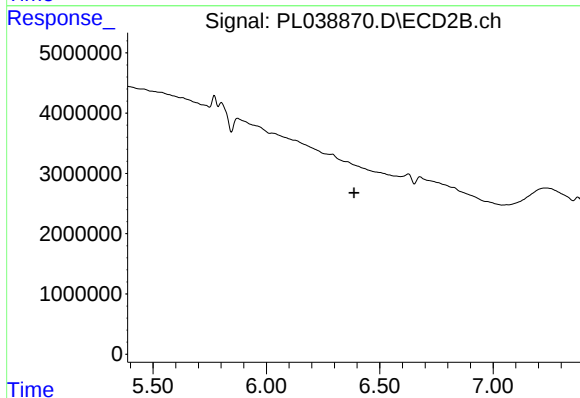


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.387 min
Response: 0
Conc: N.D.

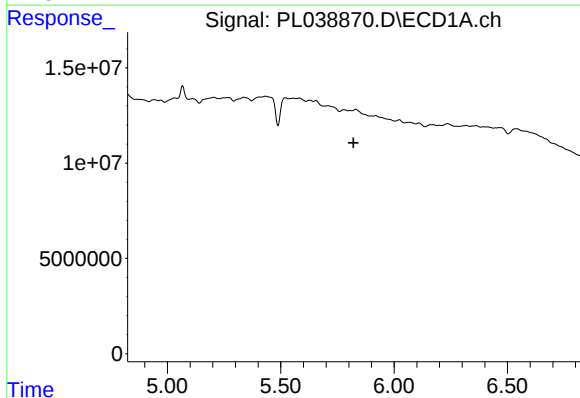


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.821 min
Response: 0
Conc: N.D.

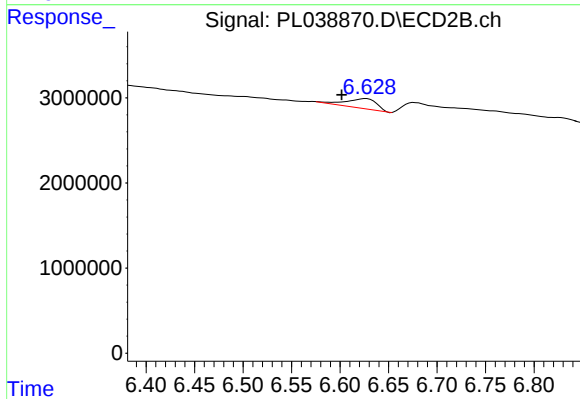

#14 Endrin


R.T.: 6.627 min
Delta R.T.: 0.025 min
Response: 2563465
Conc: 1.07 ng/ml

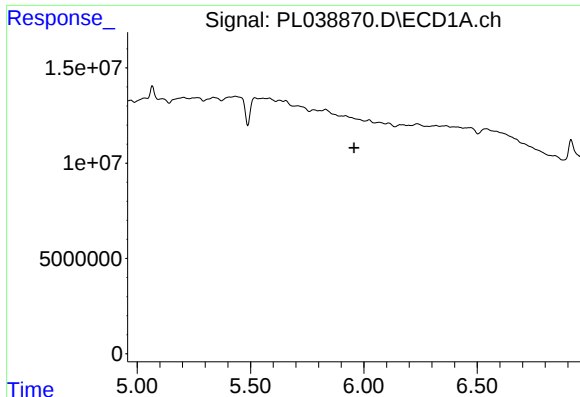

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

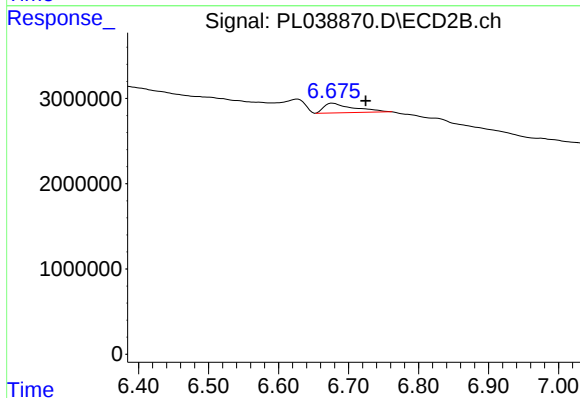


#16 4,4'-DDD

R.T.: 6.677 min
Delta R.T.: -0.048 min
Response: 3195167
Conc: 1.49 ng/ml

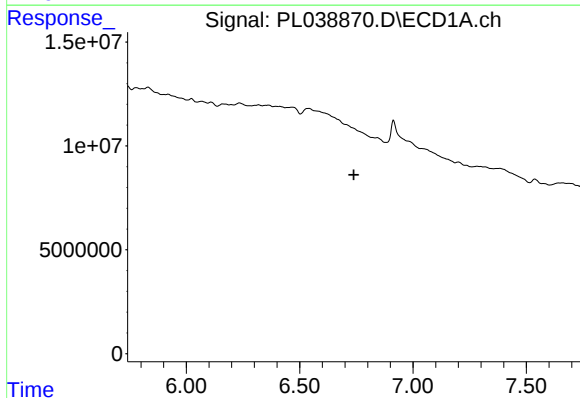


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.739 min
Response: 0
Conc: N.D.

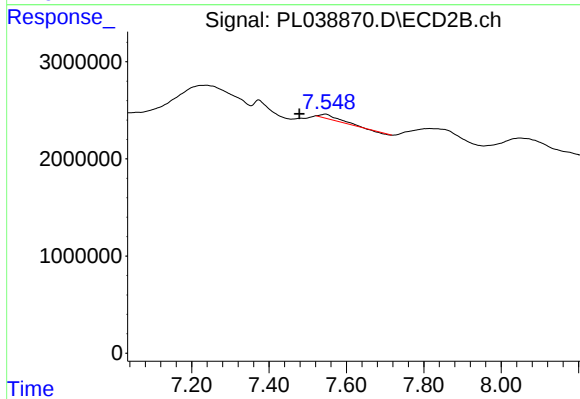

#20 Methoxychlor


R.T.: 7.547 min
Delta R.T.: 0.068 min
Response: 1425794
Conc: 1.25 ng/ml

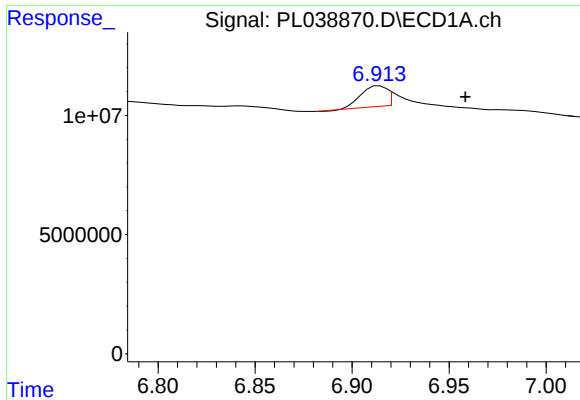

#21 Endrin ketone


R.T.: 6.914 min
Delta R.T.: -0.044 min
Response: 8303391
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

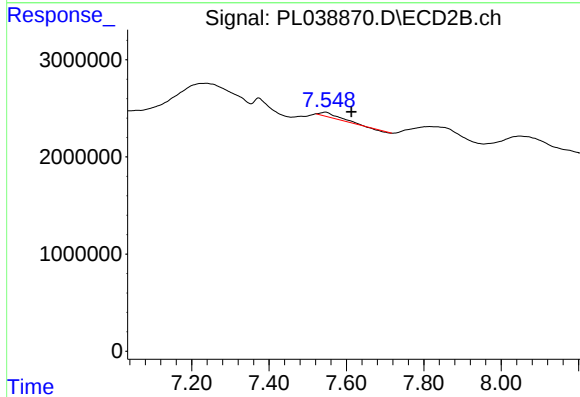


#21 Endrin ketone

R.T.: 7.547 min
Delta R.T.: -0.067 min
Response: 1425794
Conc: 0.60 ng/ml

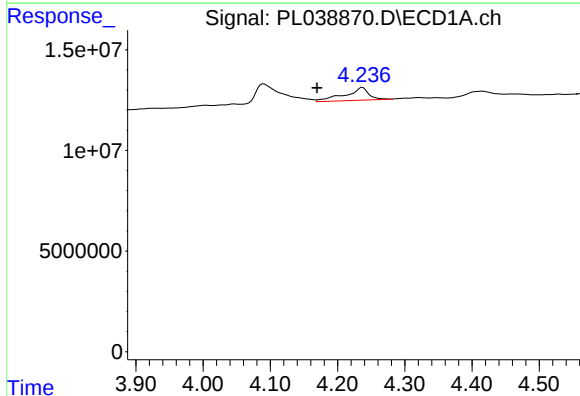


#23 Chlordane-1

R.T.: 4.237 min
Delta R.T.: 0.068 min
Response: 15487870
Conc: 44.73 ng/ml

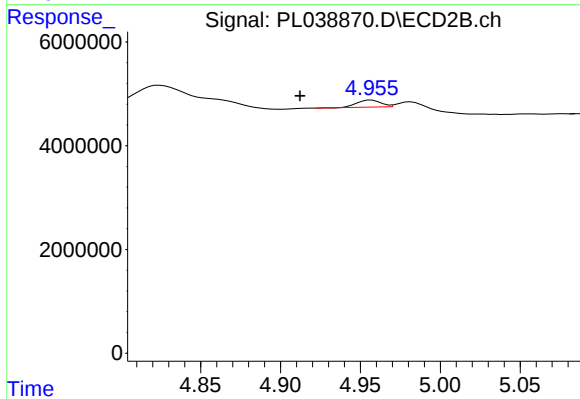

#23 Chlordane-1


R.T.: 4.957 min
Delta R.T.: 0.045 min
Response: 1378912
Conc: 11.90 ng/ml

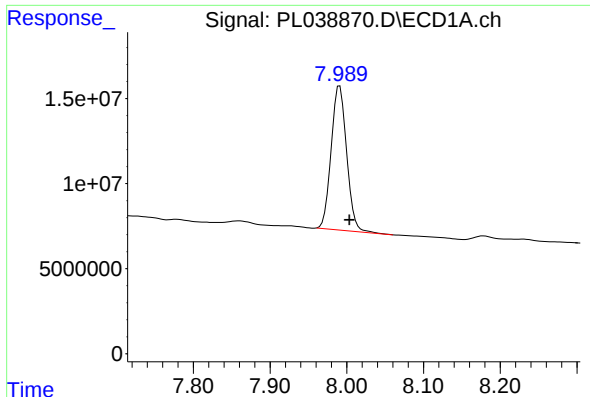

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.013 min
Response: 118437757
Conc: 15.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

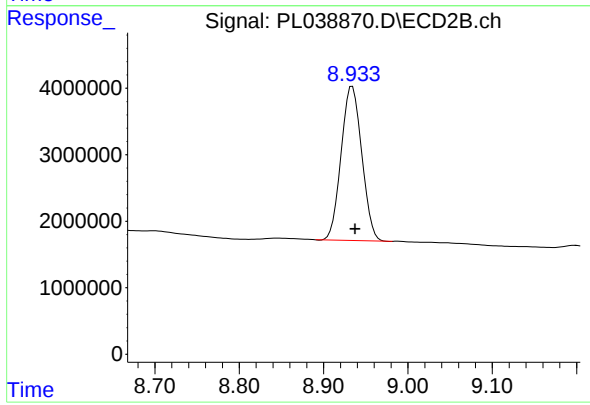

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 39436390
Conc: 16.13 ng/ml