

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
 Data File : PL050978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2019 10:40
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:45:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.759	0.000	2806855	0	0.167	N.D. #
11) B	alpha-Chl...	5.272	0.000	1827807	0	0.120	N.D. #
13) MA	Dieldrin	5.541	0.000	3150359	0	0.203	N.D. #
16) A	4,4'-DDD	5.941	0.000	9691223	0	0.809	N.D. #
17) MA	4,4'-DDT	6.179	0.000	96735295	0	7.810	N.D. #
18) B	Endrin al...	6.258	0.000	16009292	0	1.388	N.D. #
20) A	Methoxychlor	6.731f	0.000	12737676	0	2.042	N.D. #
21) B	Endrin ke...	6.935	0.000	8533781	0	0.624	N.D. #
26)	Chlordane-4	5.272	0.000	1827807	0	1.386	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
Data File : PL050978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2019 10:40
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:45:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

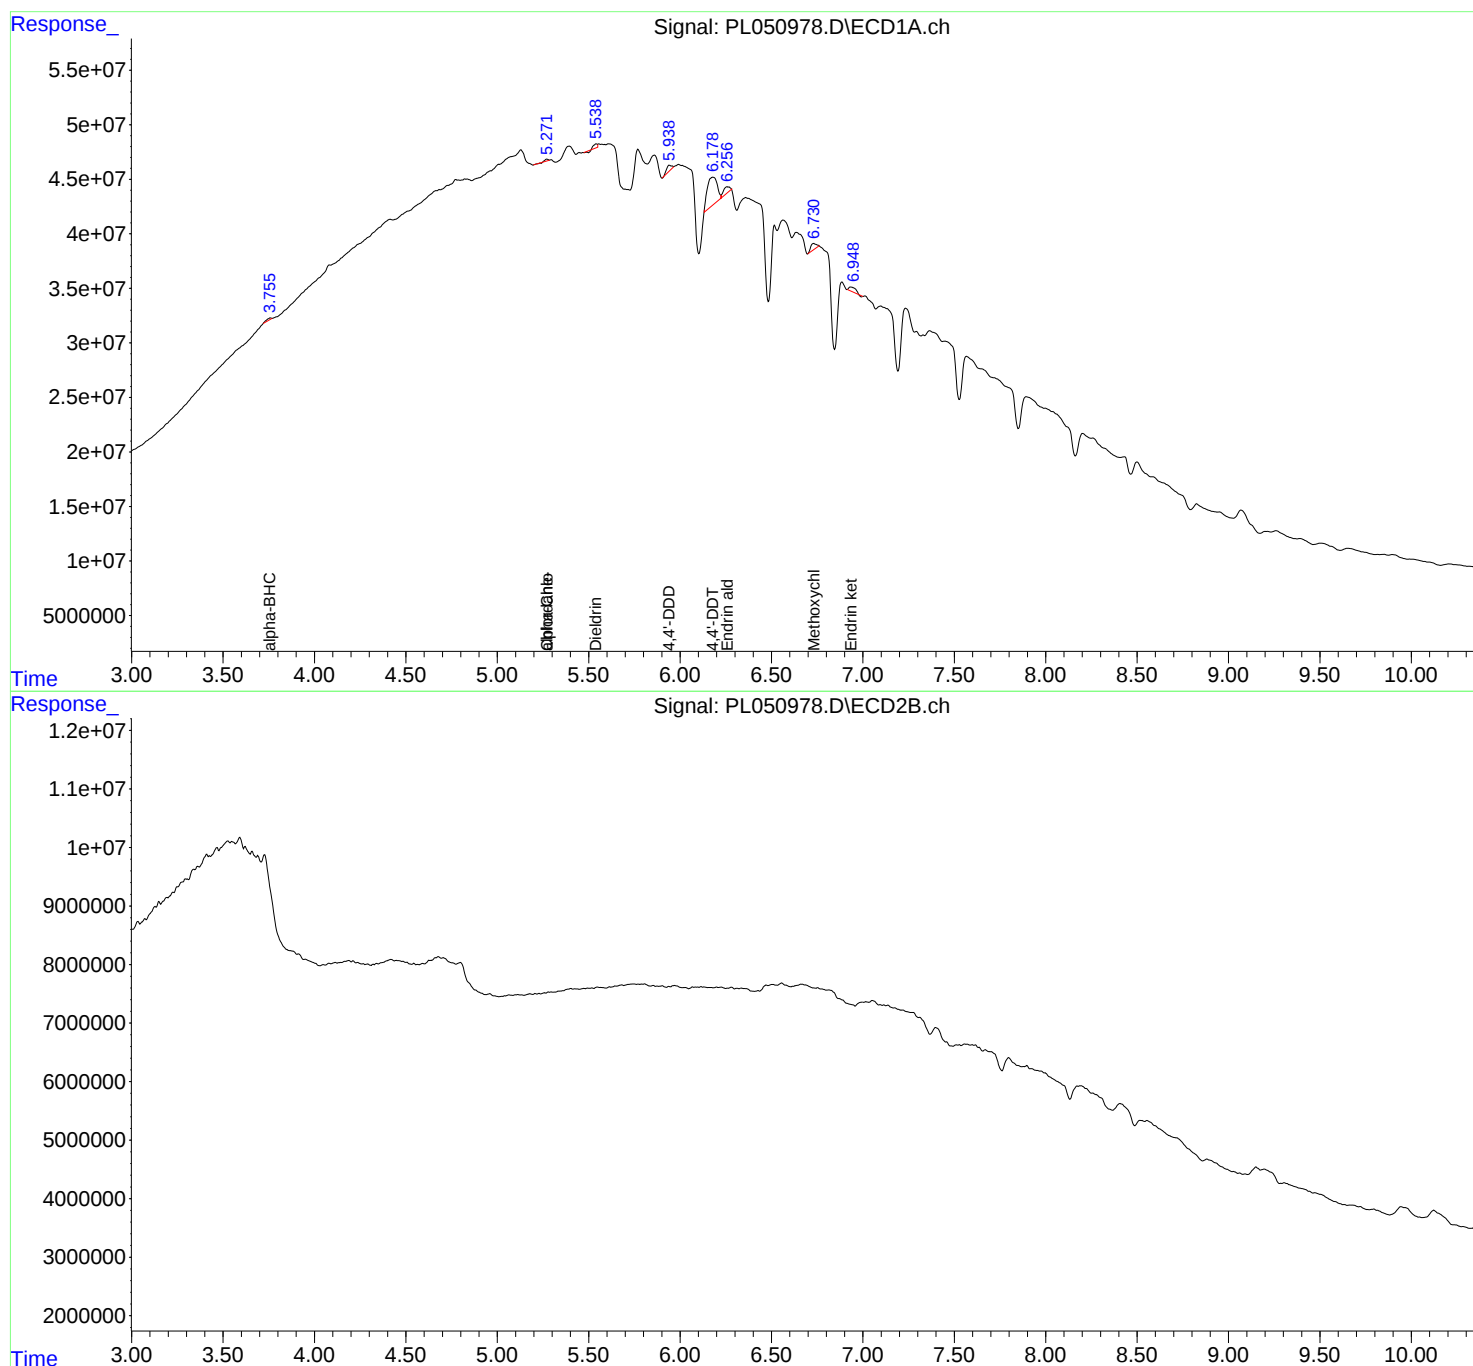


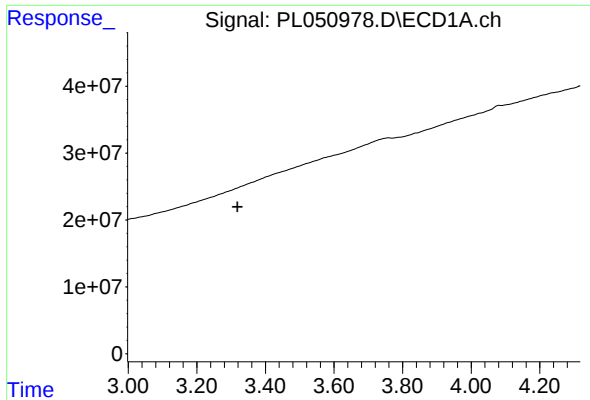

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

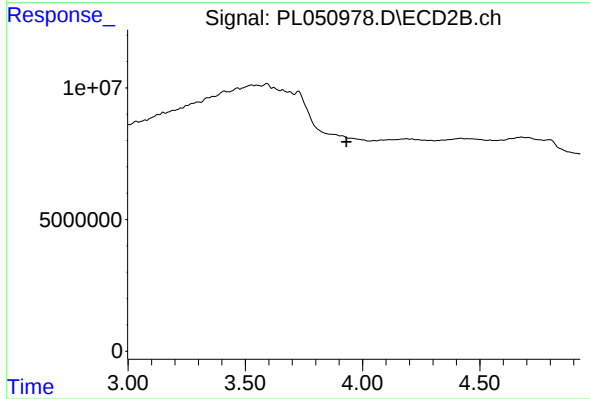


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

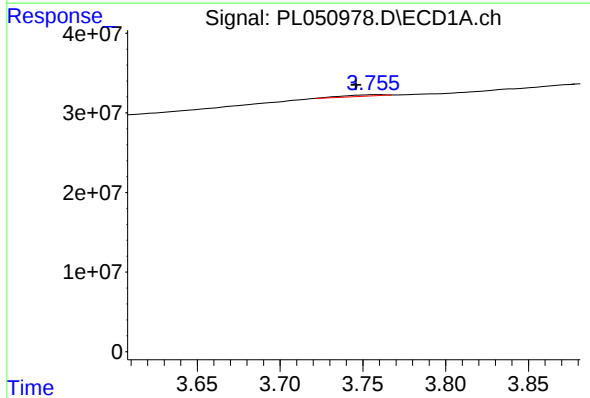


#2 alpha-BHC

R.T.: 3.759 min
Delta R.T.: 0.013 min
Response: 2806855
Conc: 0.17 ng/ml

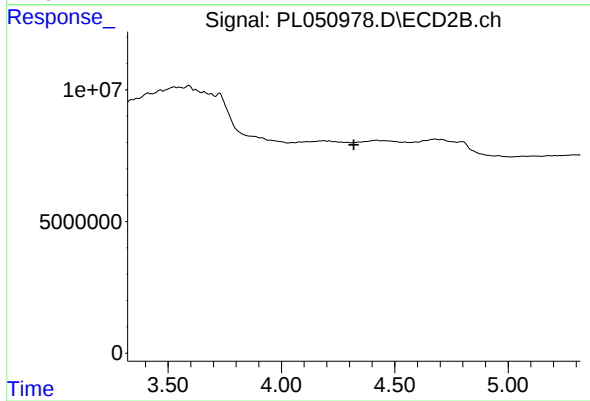

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

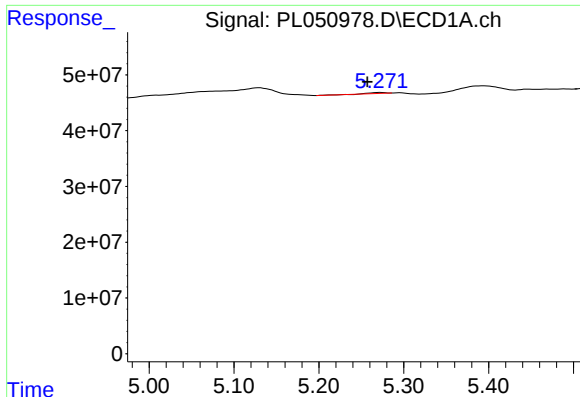

#11 alpha-Chlordane


R.T.: 5.272 min
Delta R.T.: 0.014 min
Response: 1827807
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

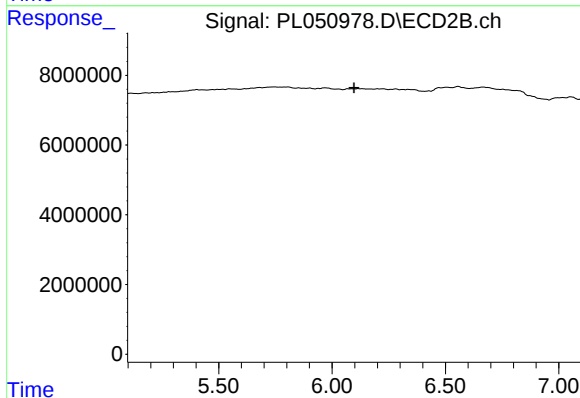


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

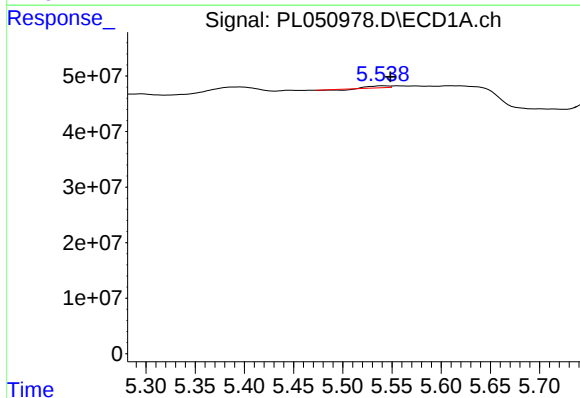


#13 Dieldrin

R.T.: 5.541 min
Delta R.T.: -0.007 min
Response: 3150359
Conc: 0.20 ng/ml

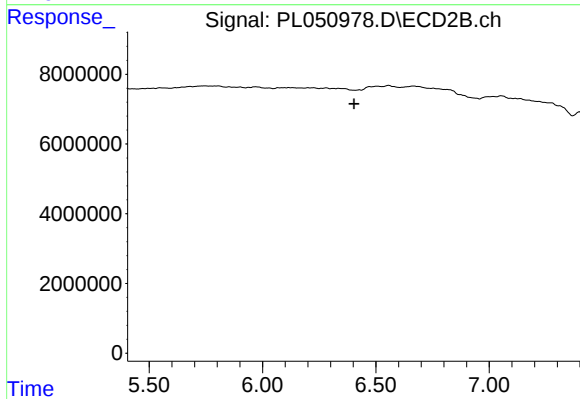

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

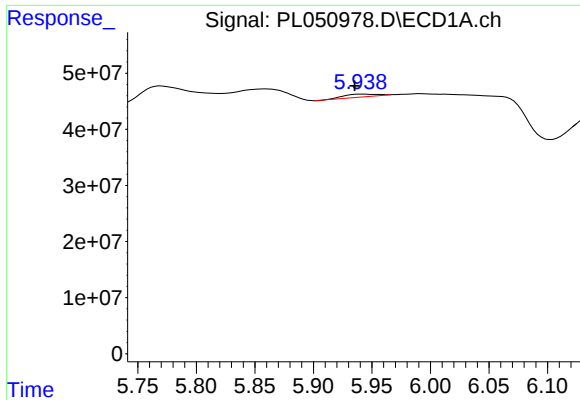

#16 4,4'-DDD


R.T.: 5.941 min
Delta R.T.: 0.006 min
Response: 9691223
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

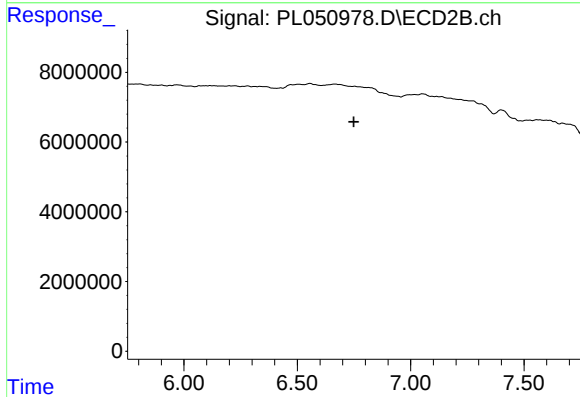


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

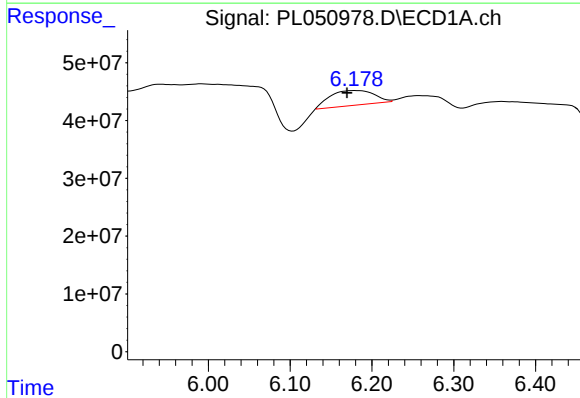


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: 0.010 min
Response: 96735295
Conc: 7.81 ng/ml

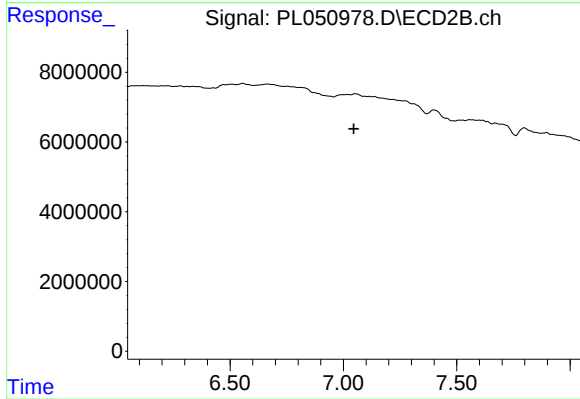

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

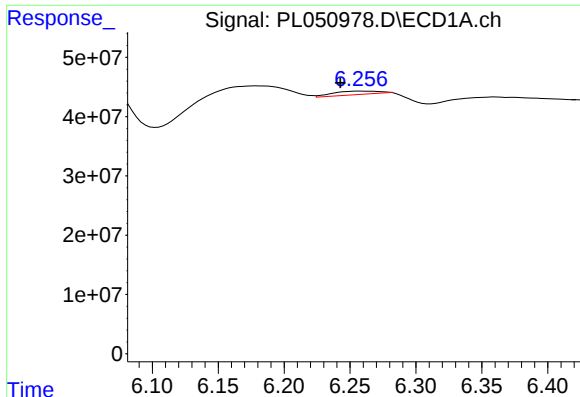

#18 Endrin aldehyde


R.T.: 6.258 min
Delta R.T.: 0.015 min
Response: 16009292
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

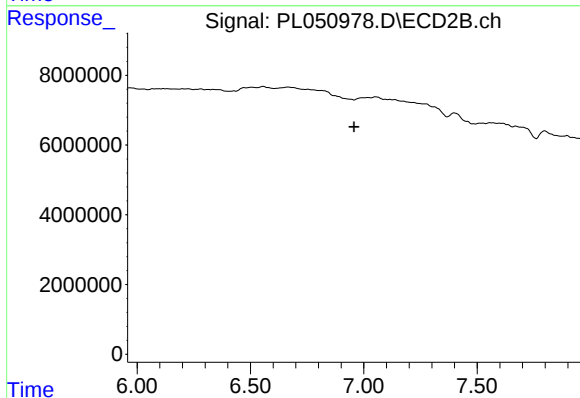


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

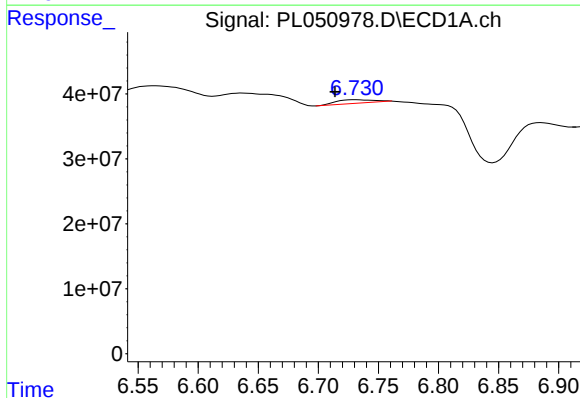


#20 Methoxychlor

R.T.: 6.731 min
Delta R.T.: 0.017 min
Response: 12737676
Conc: 2.04 ng/ml

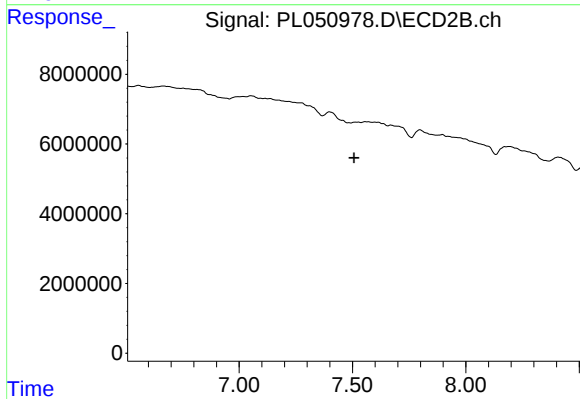

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

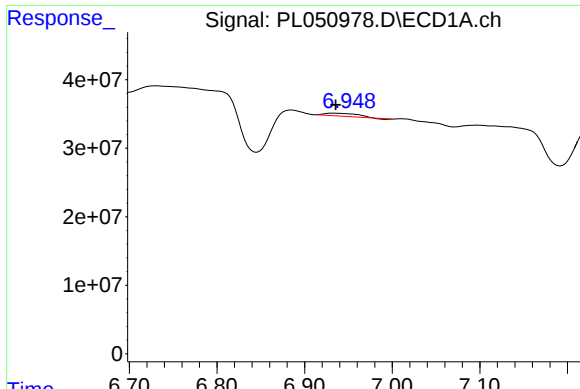

#21 Endrin ketone


R.T.: 6.935 min
Delta R.T.: -0.001 min
Response: 8533781
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

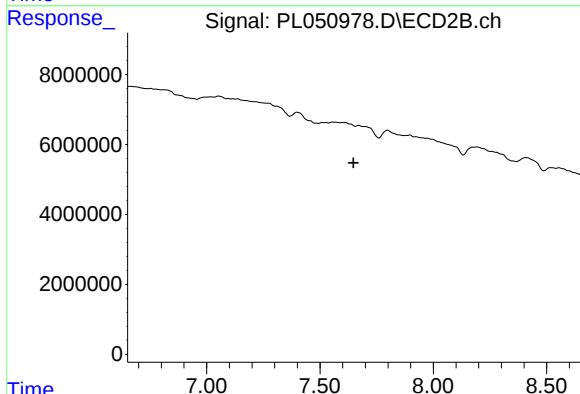


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.648 min
Response: 0
Conc: N.D.

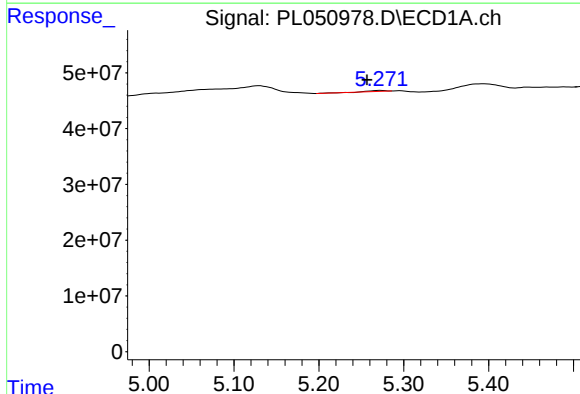


#26 Chlordane-4

R.T.: 5.272 min
Delta R.T.: 0.015 min
Response: 1827807
Conc: 1.39 ng/ml

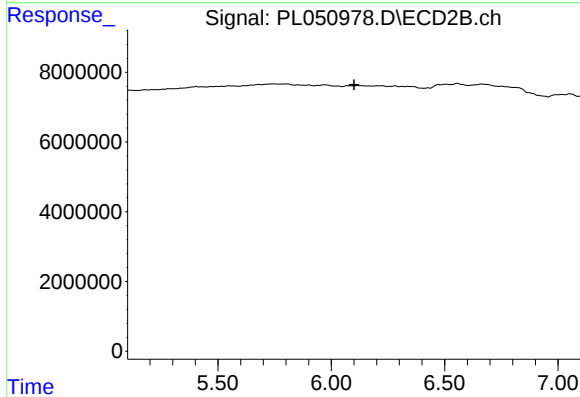

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

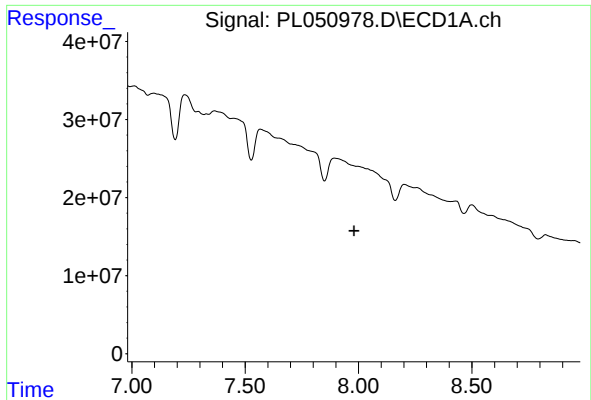

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

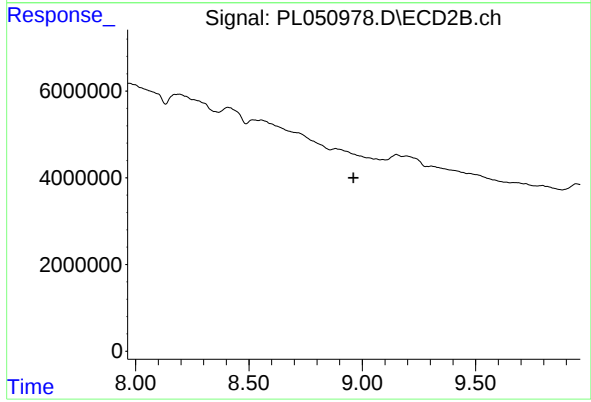

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.