

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
 Data File : PL050995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2019 17:52
 Operator : SM\AJ
 Sample : K4130-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:49:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.927	129.2E6	34437540	12.855	12.070
28)	SA Decachlor...	7.978	8.955	130.4E6	35140611	12.879	12.426
Target Compounds							
6)	B beta-BHC	0.000	4.797f	0	7807624	N.D.	4.516 #
8)	B Heptachlo...	0.000	5.804	0	5330781	N.D.	1.394 #
10)	B gamma-Chl...	5.218f	0.000	13270630	0	0.841	N.D. #
13)	MA Dieldrin	5.556	0.000	42977240	0	2.773	N.D. #
23)	Chlordane-1	4.164	0.000	7460817	0	20.277	N.D. #
25)	Chlordane-3	5.218f	0.000	13270630	0	9.480	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
Data File : PL050995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2019 17:52
Operator : SM\AJ
Sample : K4130-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:49:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

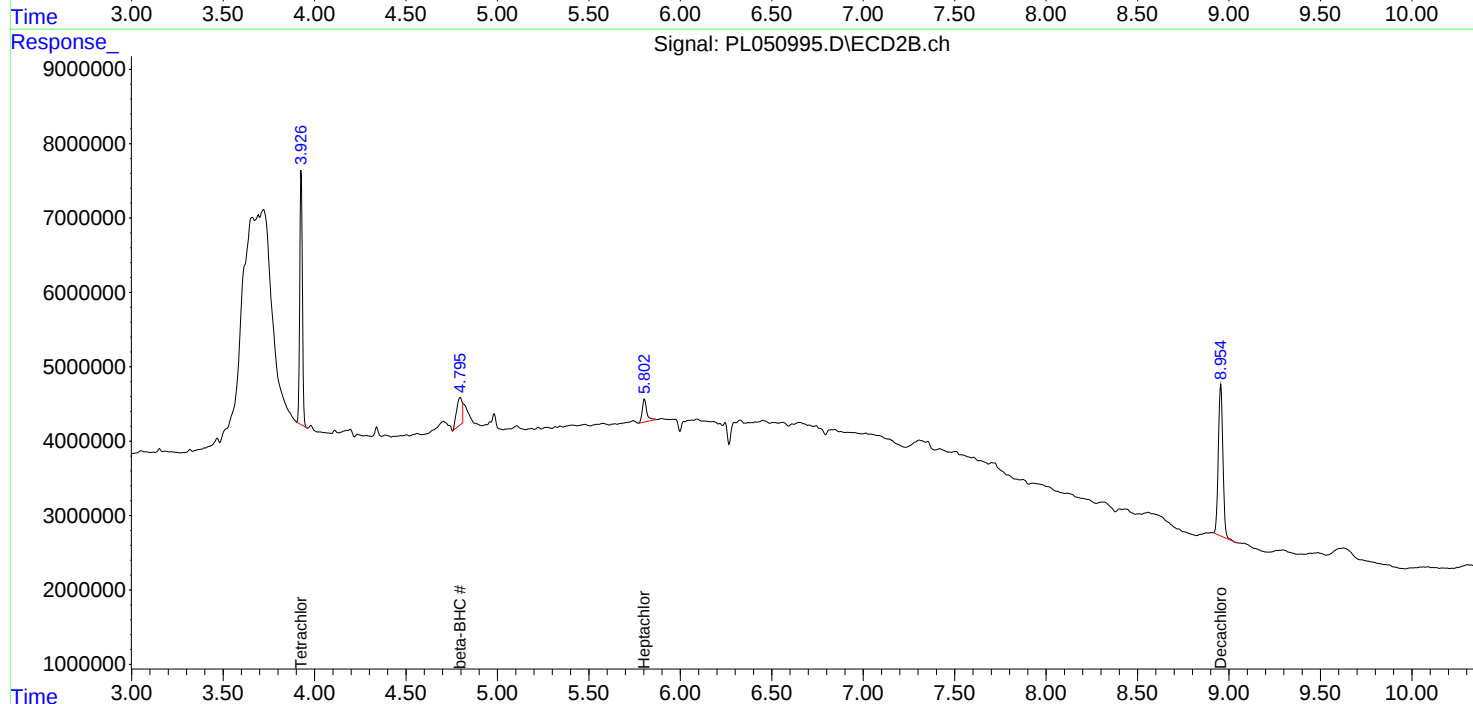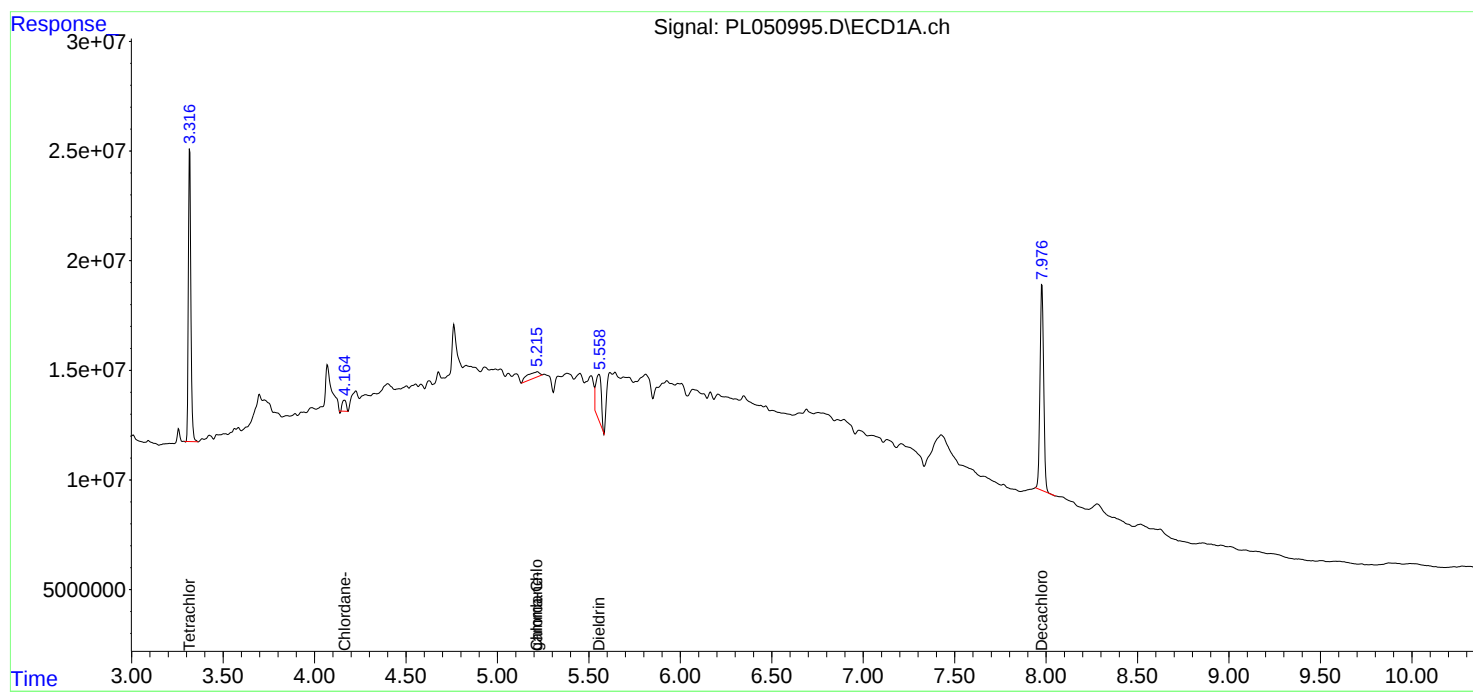


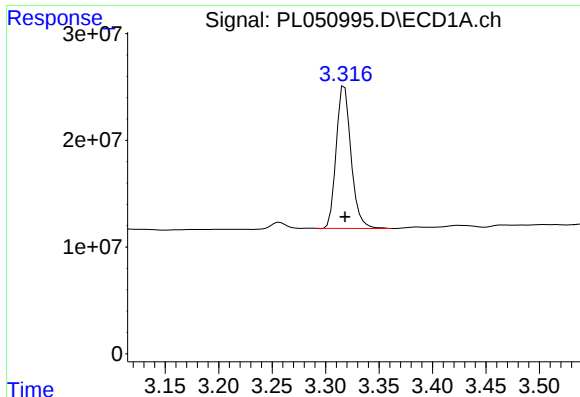

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 129161517
Conc: 12.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

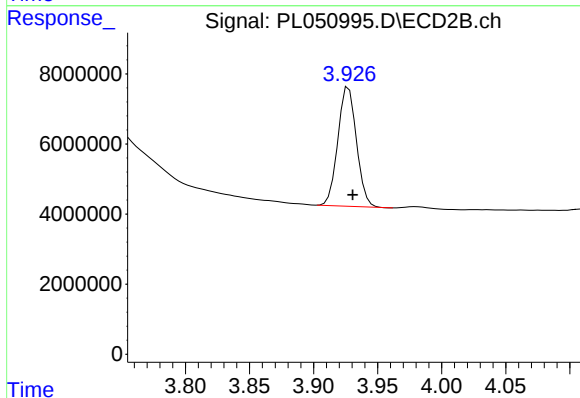


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 34437540
Conc: 12.07 ng/ml

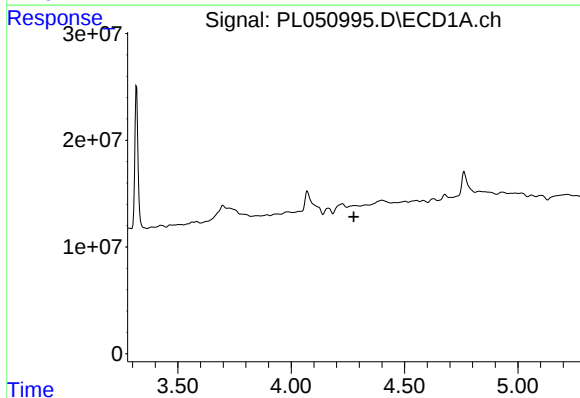


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

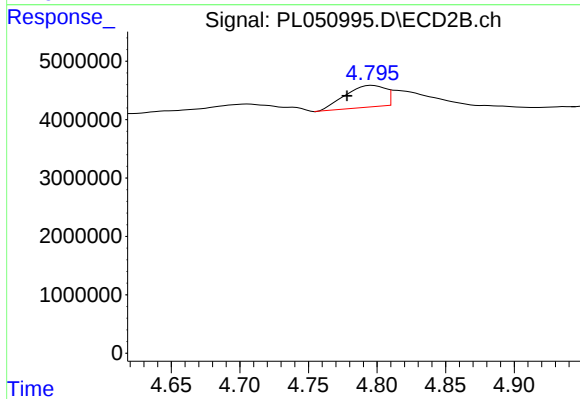

#6 beta-BHC


R.T.: 4.797 min
Delta R.T.: 0.019 min
Response: 7807624
Conc: 4.52 ng/ml

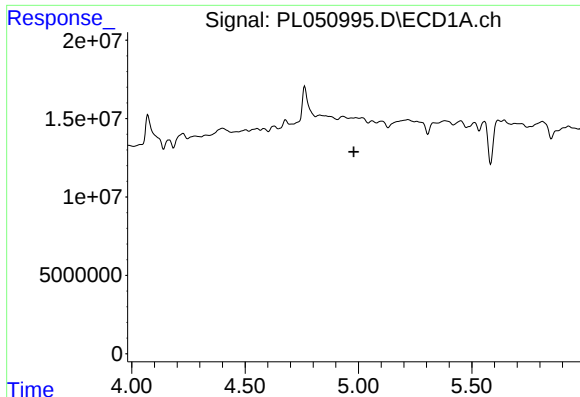

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

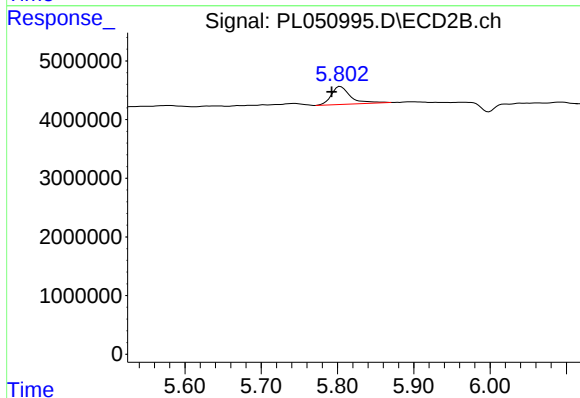


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.011 min
Response: 5330781
Conc: 1.39 ng/ml

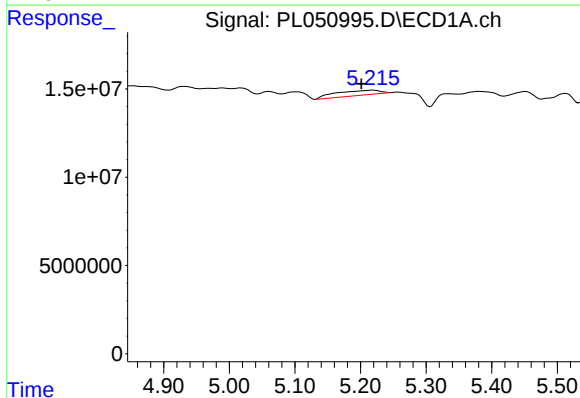


#10 gamma-Chlordane

R.T.: 5.218 min
Delta R.T.: 0.017 min
Response: 13270630
Conc: 0.84 ng/ml

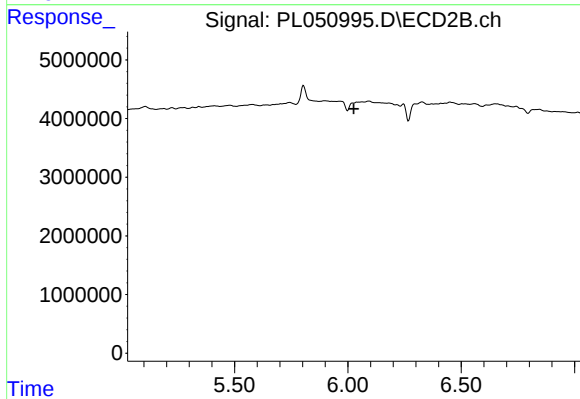

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

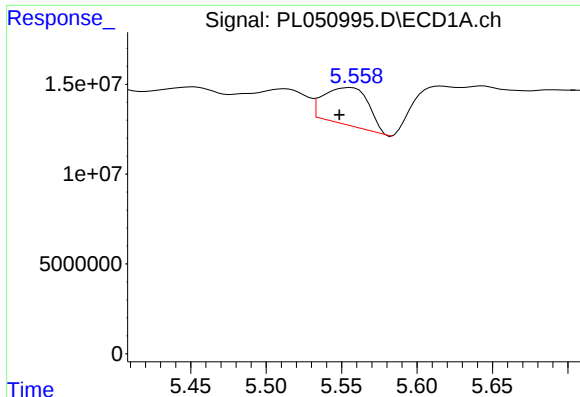

#13 Dieldrin


R.T.: 5.556 min
Delta R.T.: 0.007 min
Response: 42977240
Conc: 2.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

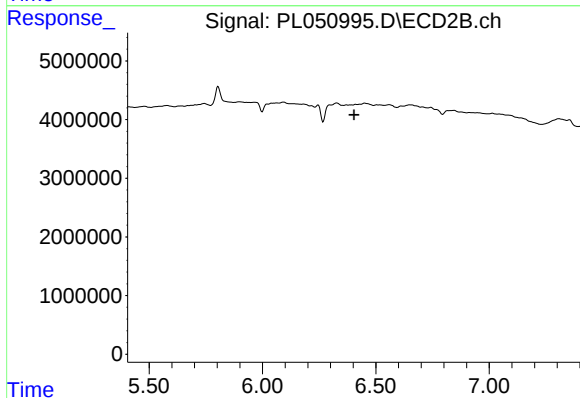


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

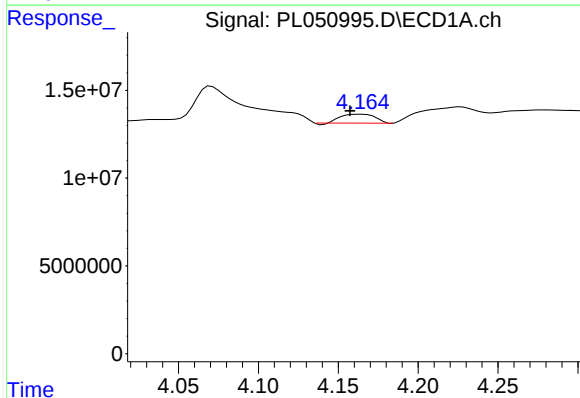


#23 Chlordane-1

R.T.: 4.164 min
Delta R.T.: 0.007 min
Response: 7460817
Conc: 20.28 ng/ml

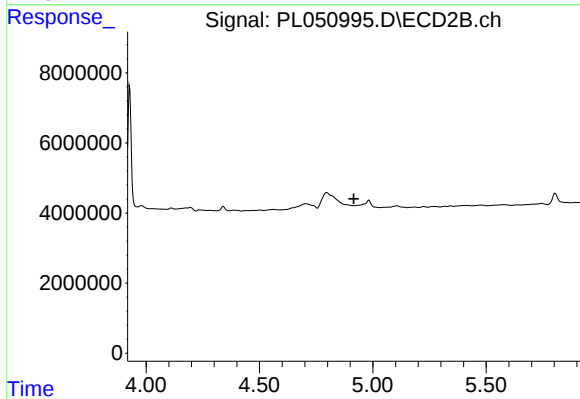

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

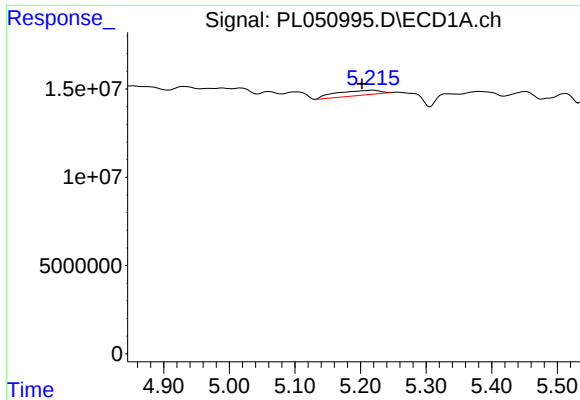

#25 Chlordane-3


R.T.: 5.218 min
Delta R.T.: 0.016 min
Response: 13270630
Conc: 9.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

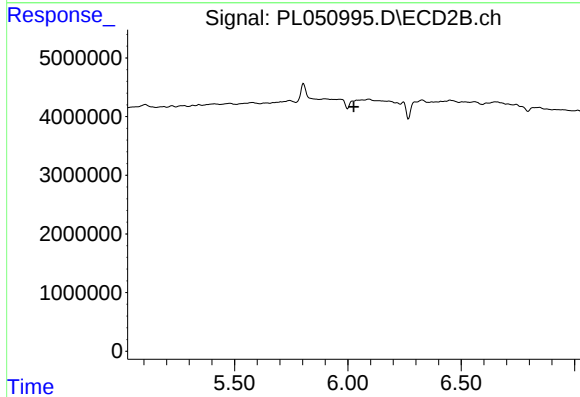


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

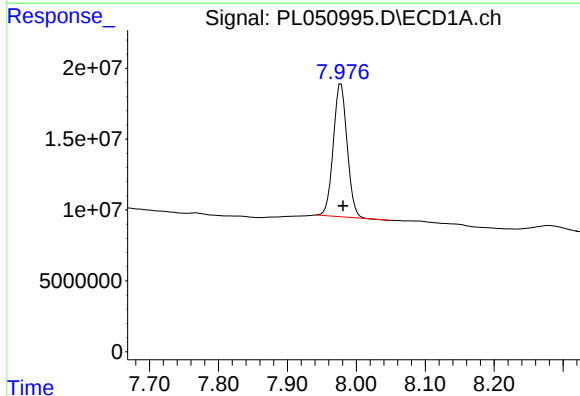

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 130400644
Conc: 12.88 ng/ml

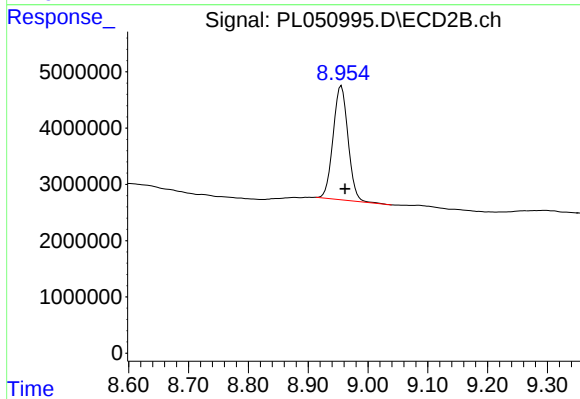

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 35140611
Conc: 12.43 ng/ml