

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
 Data File : PL050989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2019 16:21
 Operator : SM\AJ
 Sample : K4124-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15

Manual Integrations
 APPROVED

Ankita
 8/5/2019 2:39:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:48:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.927	120.8E6	32701414	12.021	11.461
28)	SA Decachlor...	7.978	8.956	106.3E6	30109183	10.501	10.647
Target Compounds							
10)	B gamma-Chl...	5.200	6.022	5017215	2986338	0.318m	0.808 #
11)	B alpha-Chl...	5.254	6.095	14921089	6959560	0.978m	1.899 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
Data File : PL050989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2019 16:21
Operator : SM\AJ
Sample : K4124-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 22:48:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

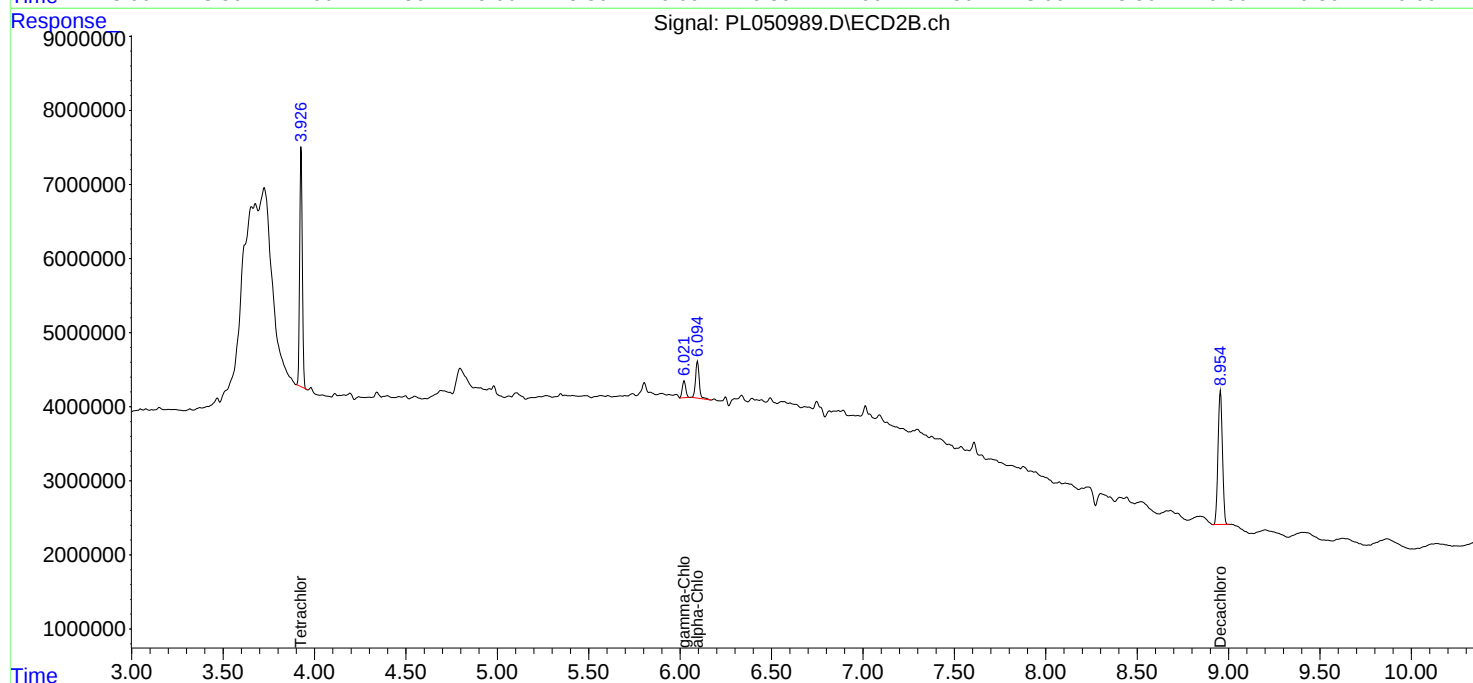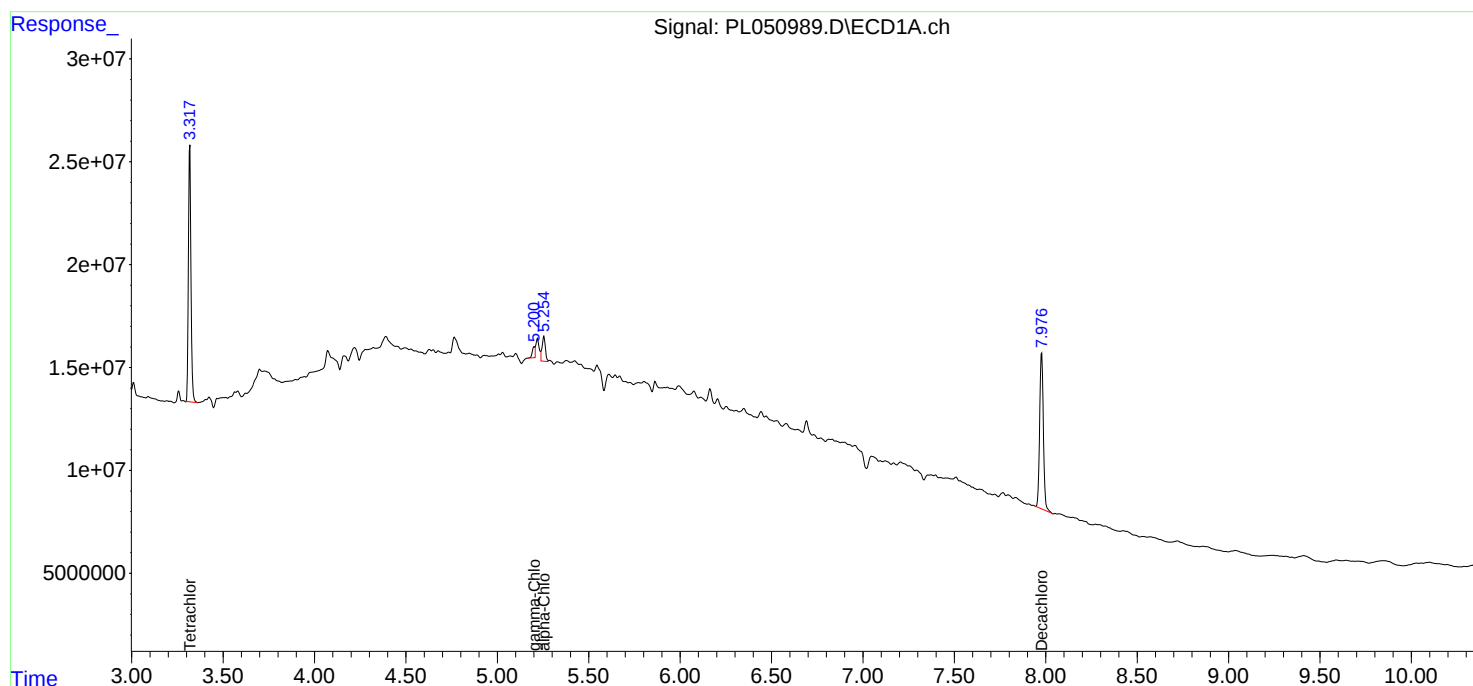

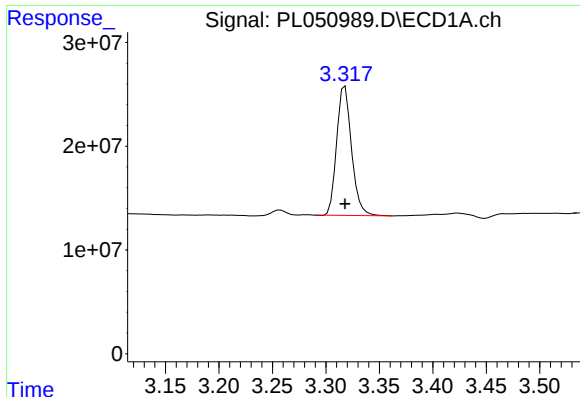


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 120784459
Conc: 12.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:09 PM

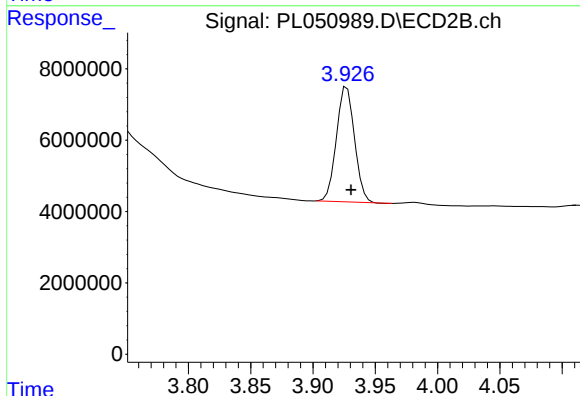


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 32701414
Conc: 11.46 ng/ml

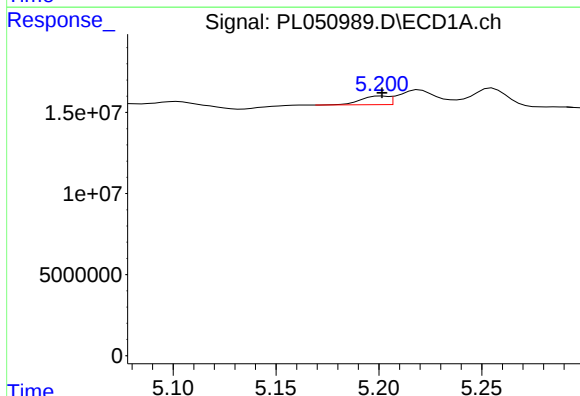


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 5017215
Conc: 0.32 ng/ml m

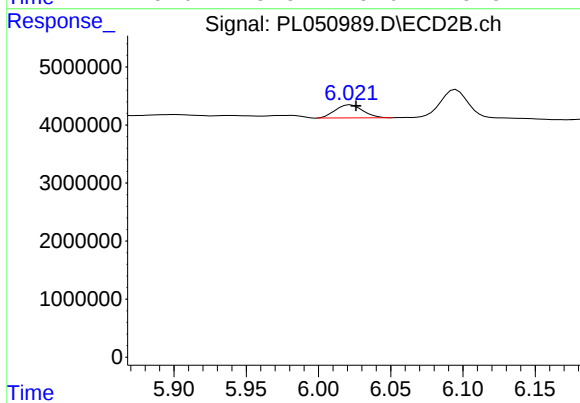

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.004 min
Response: 2986338
Conc: 0.81 ng/ml

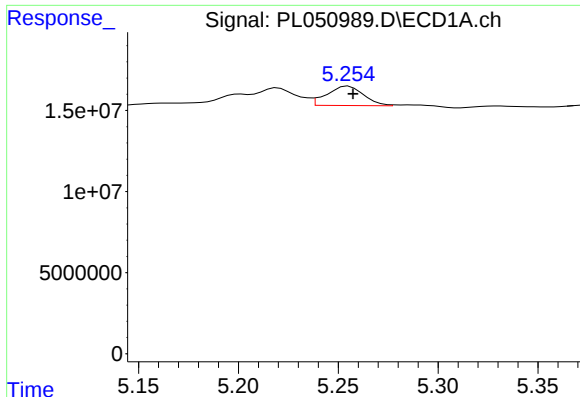


#11 alpha-Chlordane

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 14921089
Conc: 0.98 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-15


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:09 PM

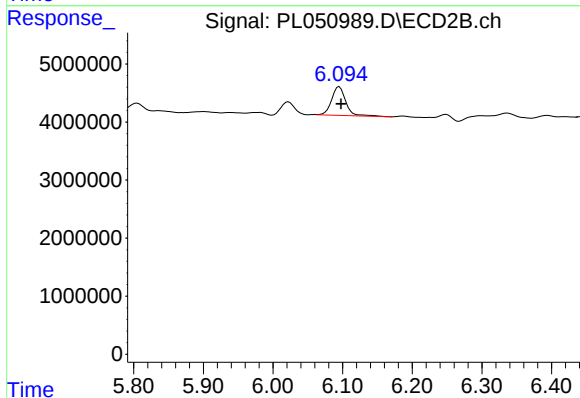


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 6959560
Conc: 1.90 ng/ml

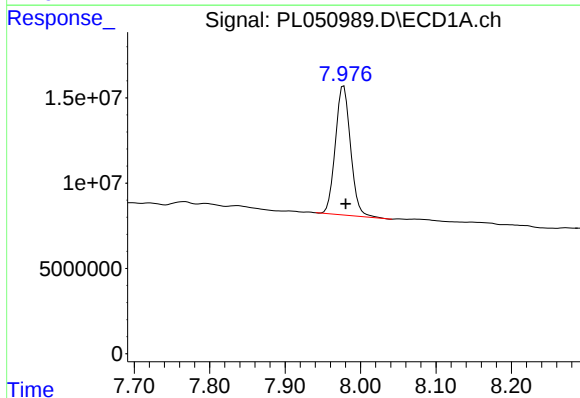

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 106323399
Conc: 10.50 ng/ml

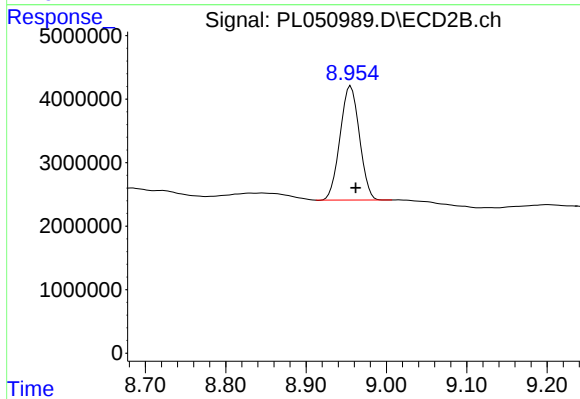

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.006 min
Response: 30109183
Conc: 10.65 ng/ml