

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
 Data File : PL051007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2019 20:54
 Operator : SM\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Ankita
 8/5/2019 2:39:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:52:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	566.4E6	149.1E6	56.370	52.255
28)	SA Decachlor...	7.977	8.955	534.9E6	144.7E6	52.824	51.158
Target Compounds							
2)	A alpha-BHC	3.745	4.316	952.2E6	222.5E6	56.824	53.926
3)	MA gamma-BHC...	4.021	4.599	887.7E6	210.4E6	57.708	54.326
4)	MA Heptachlor	4.304	5.100	926.9E6	219.5E6	56.494	52.934
5)	MB Aldrin	4.542	5.402	881.0E6	203.0E6	56.869	53.865
6)	B beta-BHC	4.275	4.775	365.0E6	97917634	55.680	56.637
7)	B delta-BHC	4.468	4.989	923.6E6	208.9E6	56.284	54.016
8)	B Heptachlo...	4.978	5.789	805.3E6	193.4E6	54.512	50.566
9)	A Endosulfan I	5.308	6.143	749.0E6	178.8E6	51.502	51.993
10)	B gamma-Chl...	5.200	6.022	831.4E6	196.4E6	52.674	53.160
11)	B alpha-Chl...	5.256	6.093	799.5E6	193.1E6	52.408	52.693
12)	B 4,4'-DDE	5.423	6.254	760.8E6	188.6E6	50.769	52.348
13)	MA Dieldrin	5.547	6.399	832.0E6	187.1E6	53.686	52.844
14)	MA Endrin	5.799	6.617	777.8E6	156.3E6	52.840	50.393
15)	B Endosulfa...	6.074	6.828	713.0E6	165.6E6	50.944	52.083
16)	A 4,4'-DDD	5.934	6.745	657.7E6	140.5E6	54.881	52.771
17)	MA 4,4'-DDT	6.168	7.041	630.1E6	141.4E6	50.876	52.395
18)	B Endrin al...	6.241	6.951	566.8E6	139.9E6	49.135	51.468m
19)	B Endosulfa...	6.452	7.176	633.6E6	152.0E6	49.733	52.621
20)	A Methoxychlor	6.712	7.502	306.4E6	78973886	49.114	53.824
21)	B Endrin ke...	6.934	7.644	702.3E6	157.3E6	51.345	54.422
22)	Mirex	7.107	8.092	470.6E6	118.8E6	48.003	51.709

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080219\
 Data File : PL051007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2019 20:54
 Operator : SM\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1



Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050


Manual Integrations
 APPROVED

Ankita
 8/5/2019 2:39:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 22:52:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

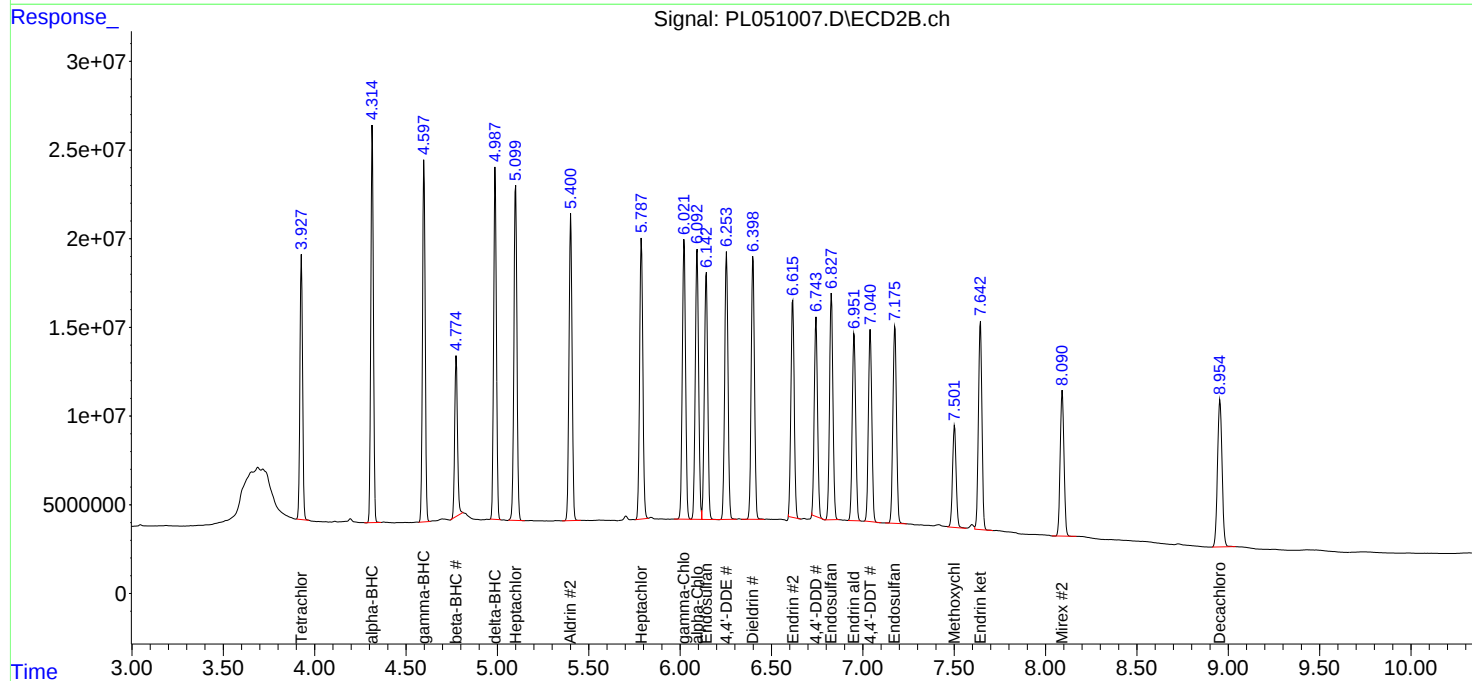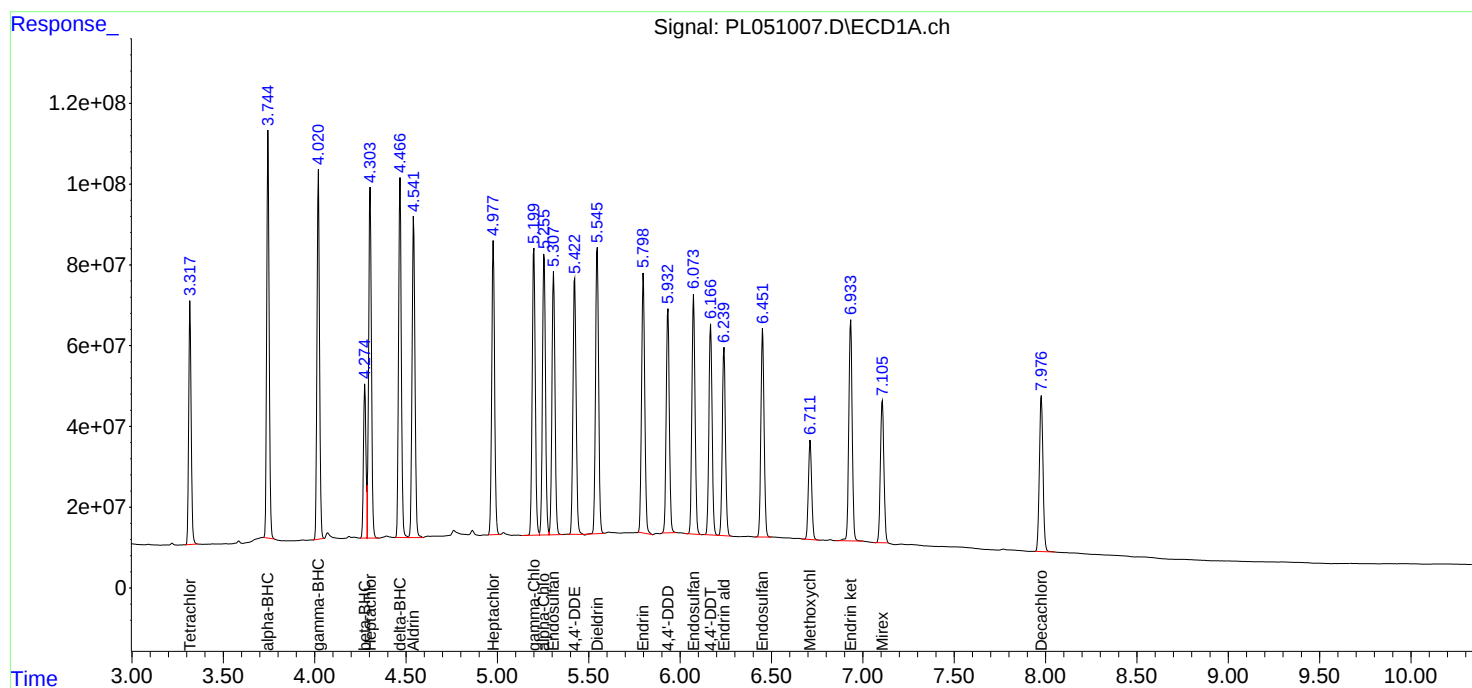

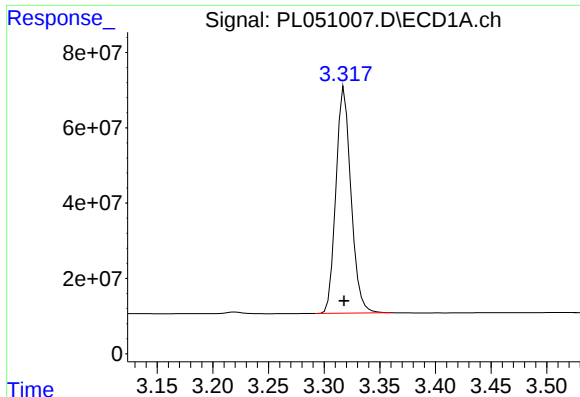


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 566399681
Conc: 56.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

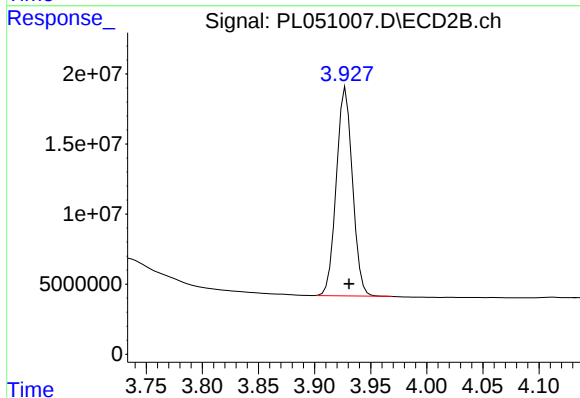


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 149093377
Conc: 52.25 ng/ml

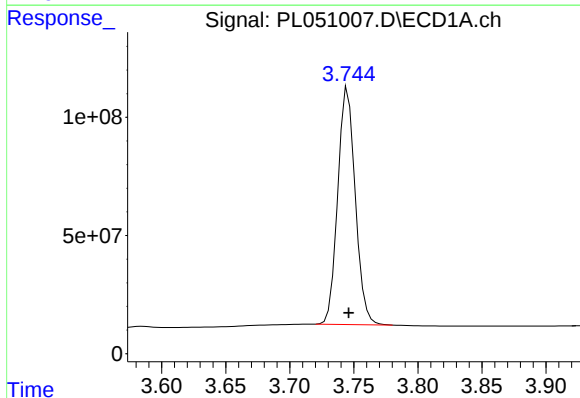


#2 alpha-BHC

R.T.: 3.745 min
Delta R.T.: 0.000 min
Response: 952247969
Conc: 56.82 ng/ml

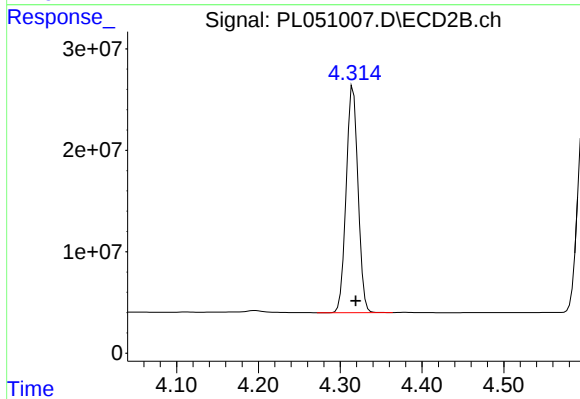

#2 alpha-BHC

R.T.: 4.316 min
Delta R.T.: -0.003 min
Response: 222496431
Conc: 53.93 ng/ml

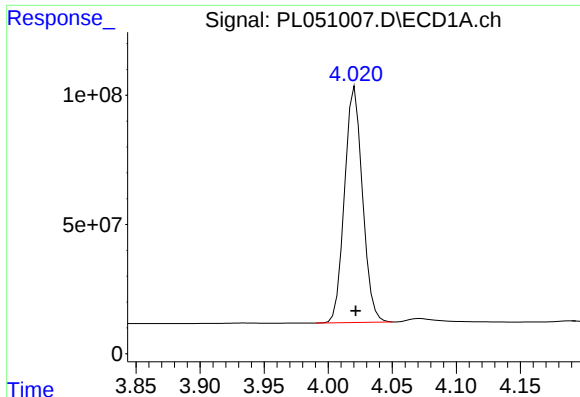


#3 gamma-BHC (Lindane)

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 887650747
Conc: 57.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

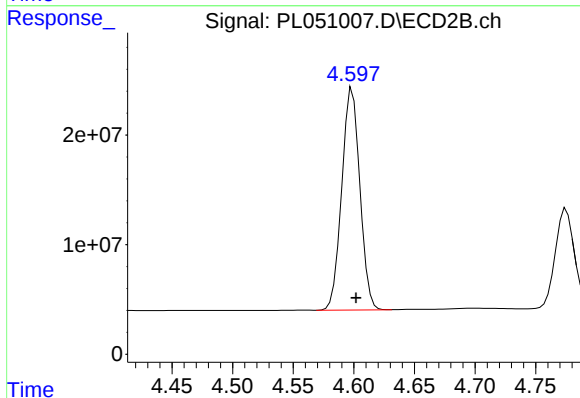


#3 gamma-BHC (Lindane)

R.T.: 4.599 min
Delta R.T.: -0.003 min
Response: 210415041
Conc: 54.33 ng/ml

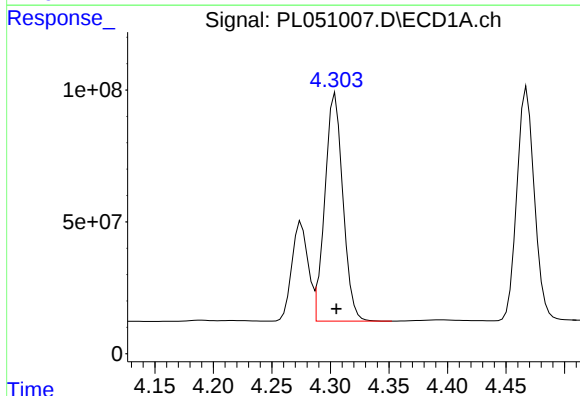


#4 Heptachlor

R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 926947296
Conc: 56.49 ng/ml

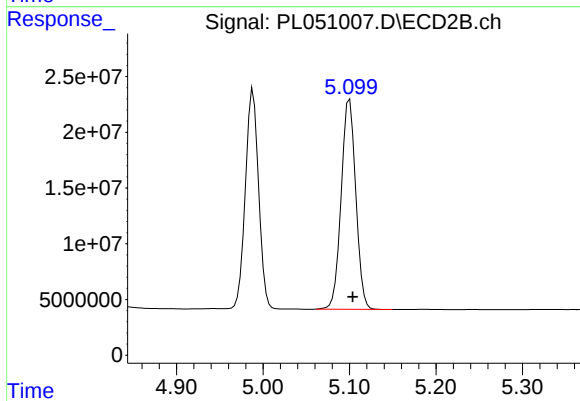

#4 Heptachlor

R.T.: 5.100 min
Delta R.T.: -0.004 min
Response: 219500212
Conc: 52.93 ng/ml

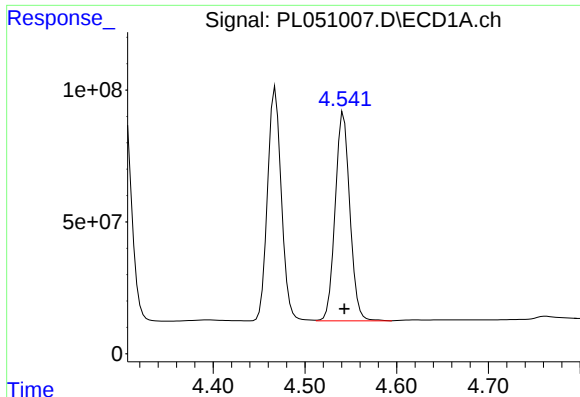


#5 Aldrin

R.T.: 4.542 min
Delta R.T.: 0.000 min
Response: 880984186
Conc: 56.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

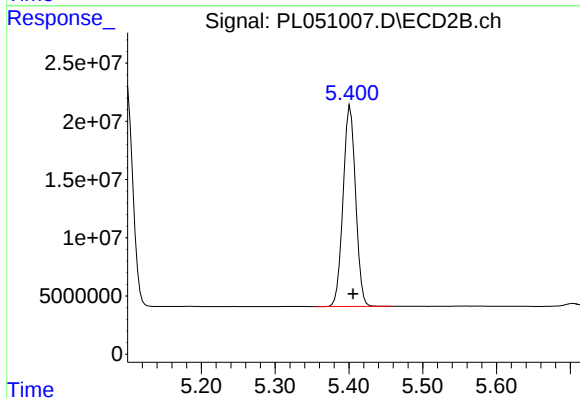


#5 Aldrin

R.T.: 5.402 min
Delta R.T.: -0.004 min
Response: 202980401
Conc: 53.86 ng/ml

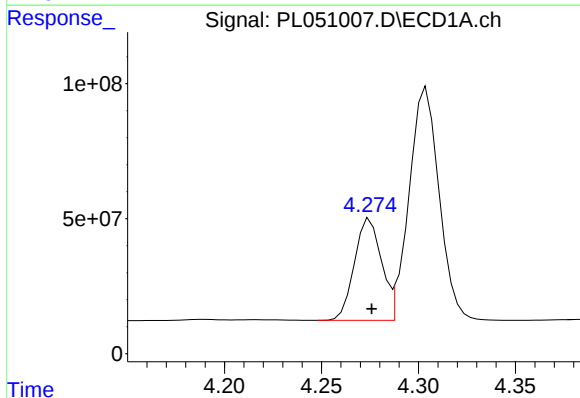


#6 beta-BHC

R.T.: 4.275 min
Delta R.T.: 0.000 min
Response: 365031545
Conc: 55.68 ng/ml

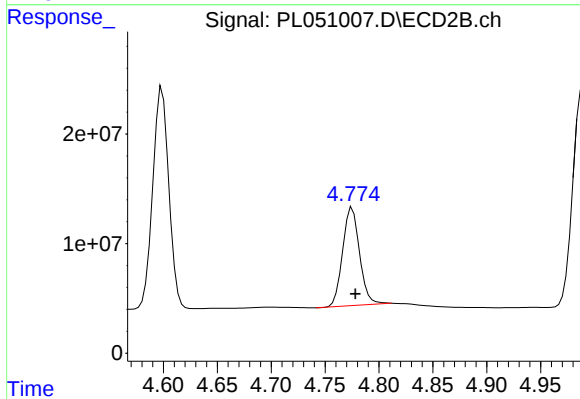

#6 beta-BHC

R.T.: 4.775 min
Delta R.T.: -0.003 min
Response: 97917634
Conc: 56.64 ng/ml

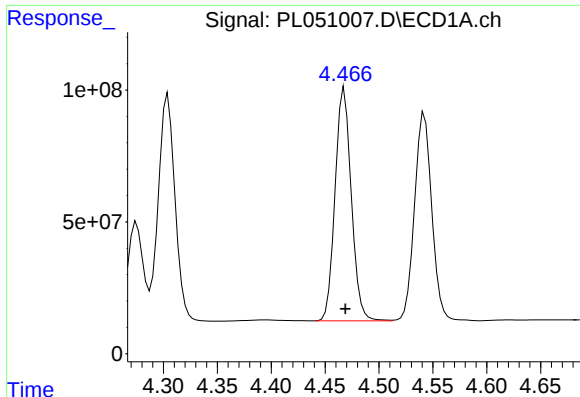


#7 delta-BHC

R.T.: 4.468 min
Delta R.T.: -0.001 min
Response: 923554044
Conc: 56.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

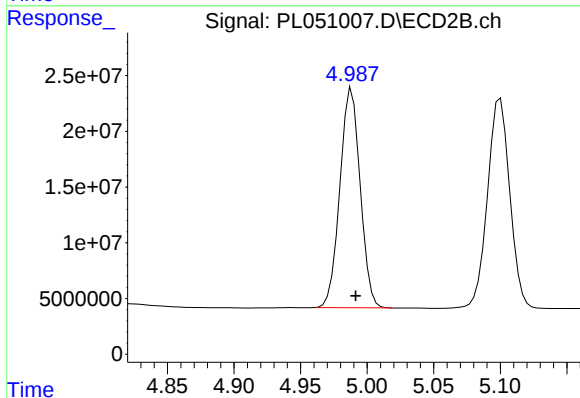


#7 delta-BHC

R.T.: 4.989 min
Delta R.T.: -0.003 min
Response: 208913224
Conc: 54.02 ng/ml

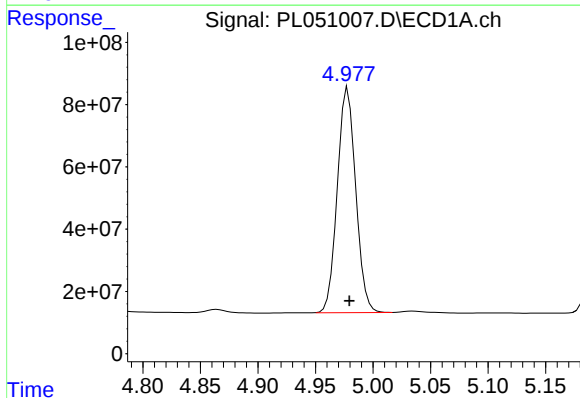


#8 Heptachlor epoxide

R.T.: 4.978 min
Delta R.T.: -0.001 min
Response: 805335529
Conc: 54.51 ng/ml

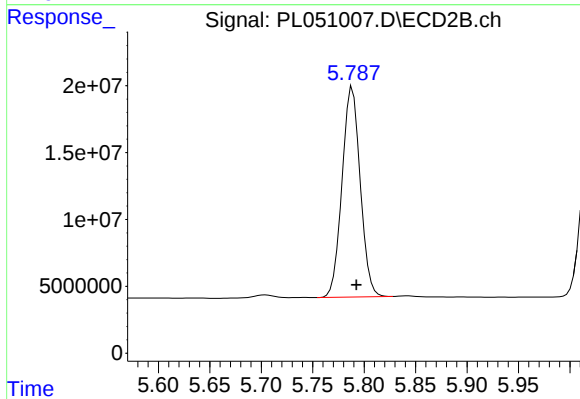

#8 Heptachlor epoxide

R.T.: 5.789 min
Delta R.T.: -0.004 min
Response: 193407663
Conc: 50.57 ng/ml

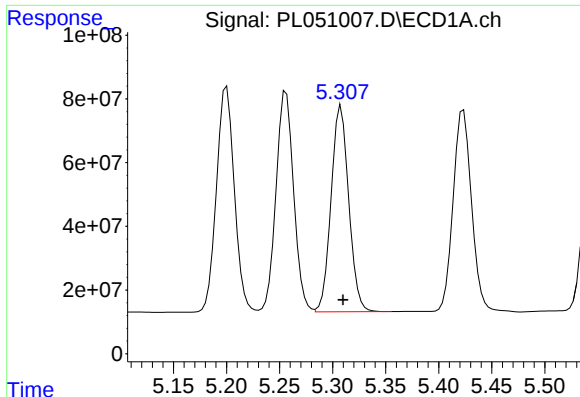


#9 Endosulfan I

R.T.: 5.308 min
Delta R.T.: -0.002 min
Response: 749044451
Conc: 51.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

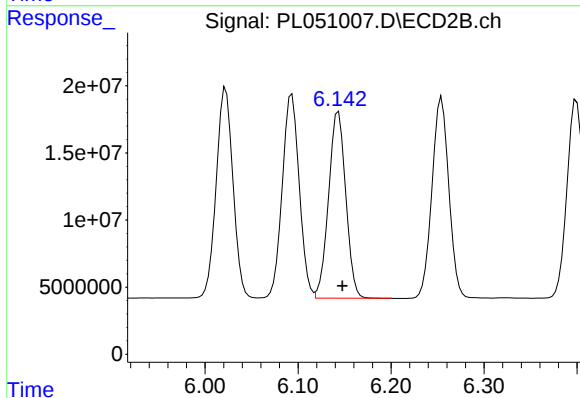


#9 Endosulfan I

R.T.: 6.143 min
Delta R.T.: -0.004 min
Response: 178797098
Conc: 51.99 ng/ml

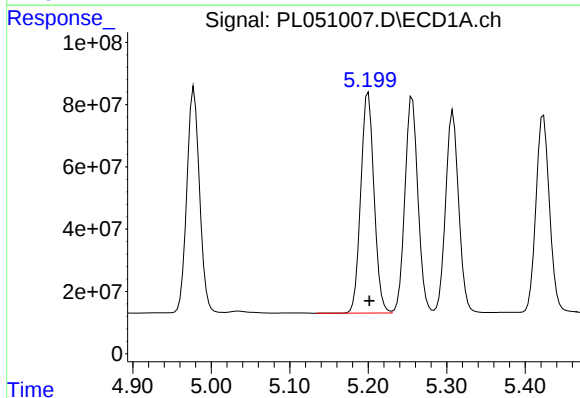


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 831364951
Conc: 52.67 ng/ml

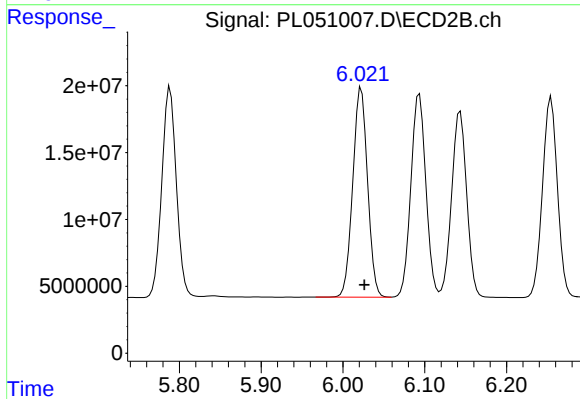

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.004 min
Response: 196442931
Conc: 53.16 ng/ml

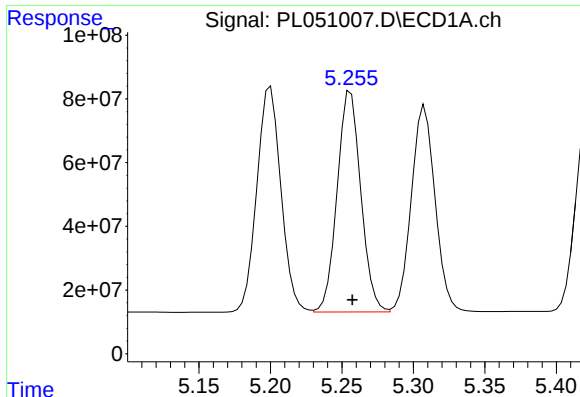


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 799538301
Conc: 52.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

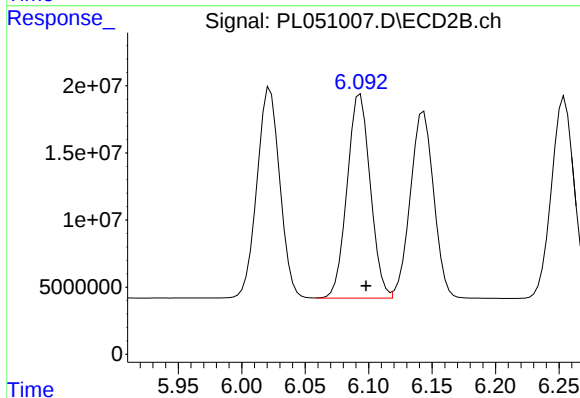


#11 alpha-Chlordane

R.T.: 6.093 min
Delta R.T.: -0.004 min
Response: 193128150
Conc: 52.69 ng/ml

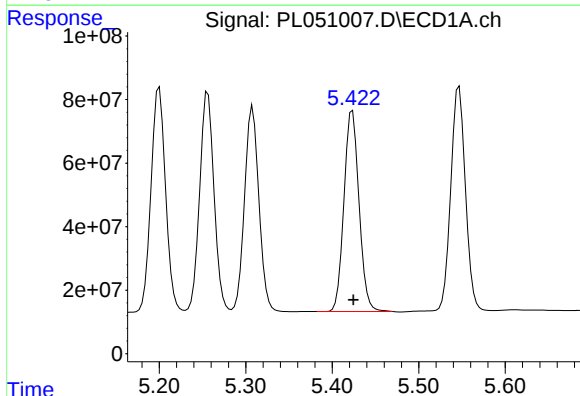


#12 4,4'-DDE

R.T.: 5.423 min
Delta R.T.: -0.001 min
Response: 760811113
Conc: 50.77 ng/ml

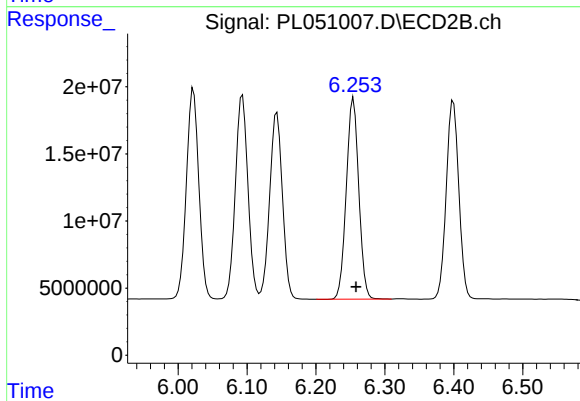

#12 4,4'-DDE

R.T.: 6.254 min
Delta R.T.: -0.004 min
Response: 188631248
Conc: 52.35 ng/ml

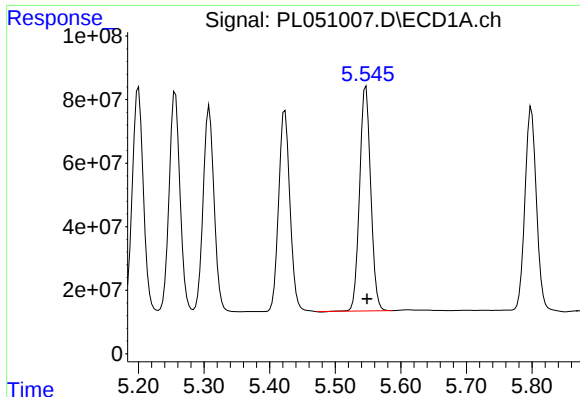


#13 Dieldrin

R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 831963858
Conc: 53.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

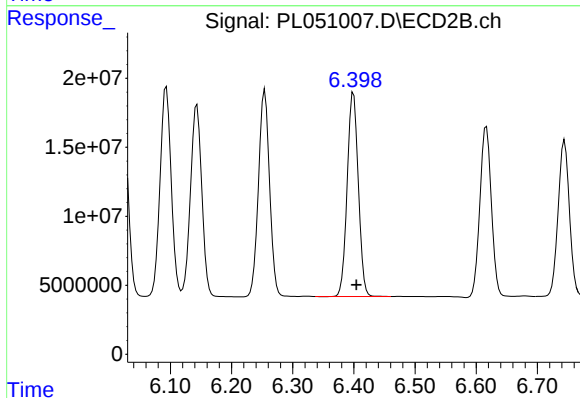


#13 Dieldrin

R.T.: 6.399 min
Delta R.T.: -0.005 min
Response: 187127799
Conc: 52.84 ng/ml

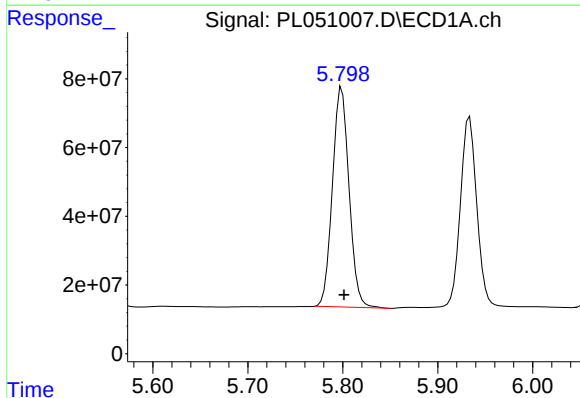


#14 Endrin

R.T.: 5.799 min
Delta R.T.: -0.002 min
Response: 777824194
Conc: 52.84 ng/ml

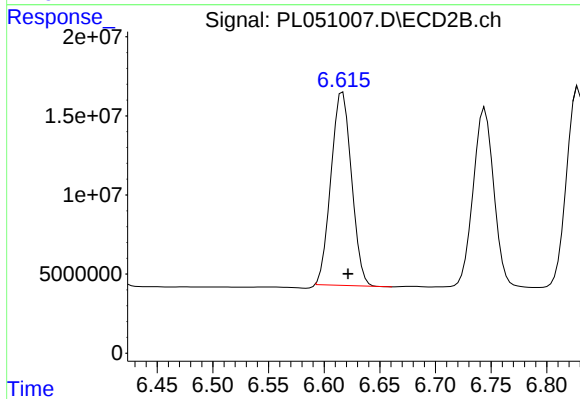

#14 Endrin

R.T.: 6.617 min
Delta R.T.: -0.005 min
Response: 156289805
Conc: 50.39 ng/ml

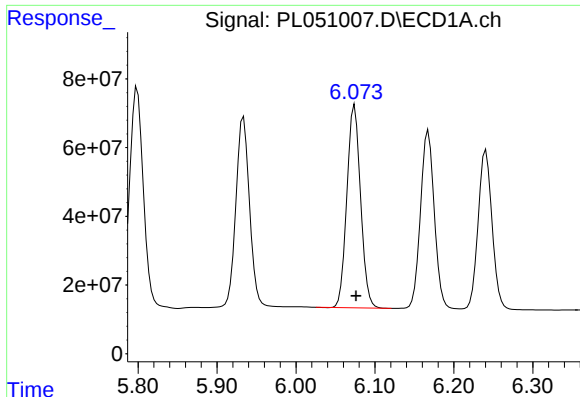


#15 Endosulfan II

R.T.: 6.074 min
Delta R.T.: -0.002 min
Response: 712959132
Conc: 50.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

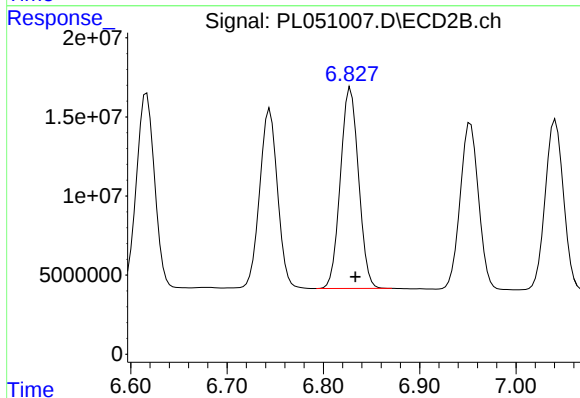


#15 Endosulfan II

R.T.: 6.828 min
Delta R.T.: -0.005 min
Response: 165582311
Conc: 52.08 ng/ml

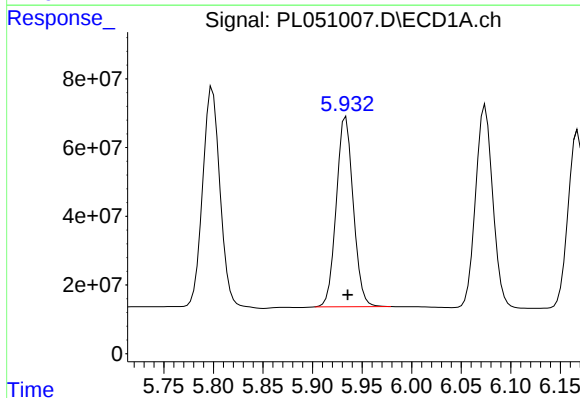


#16 4,4'-DDD

R.T.: 5.934 min
Delta R.T.: -0.002 min
Response: 657683433
Conc: 54.88 ng/ml

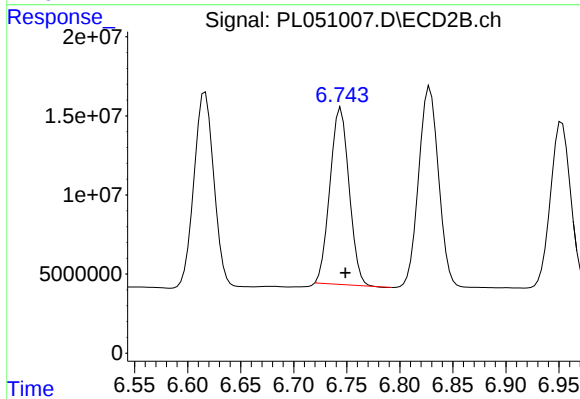

#16 4,4'-DDD

R.T.: 6.745 min
Delta R.T.: -0.004 min
Response: 140522812
Conc: 52.77 ng/ml

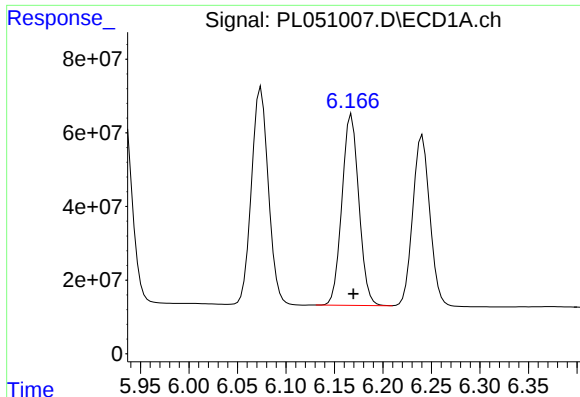


#17 4,4'-DDT

R.T.: 6.168 min
Delta R.T.: -0.002 min
Response: 630132182
Conc: 50.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

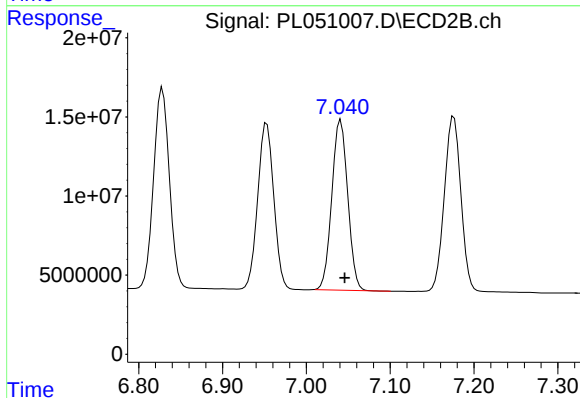


#17 4,4'-DDT

R.T.: 7.041 min
Delta R.T.: -0.005 min
Response: 141446243
Conc: 52.40 ng/ml

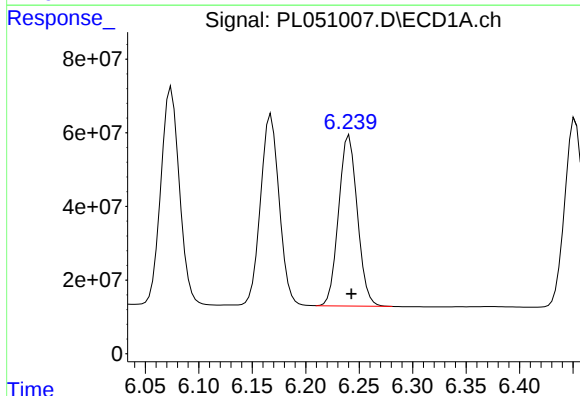


#18 Endrin aldehyde

R.T.: 6.241 min
Delta R.T.: -0.002 min
Response: 566843407
Conc: 49.14 ng/ml

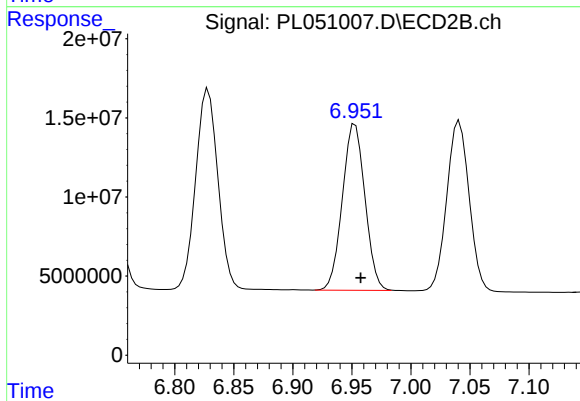

#18 Endrin aldehyde

R.T.: 6.951 min
Delta R.T.: -0.006 min
Response: 139871120
Conc: 51.47 ng/ml m

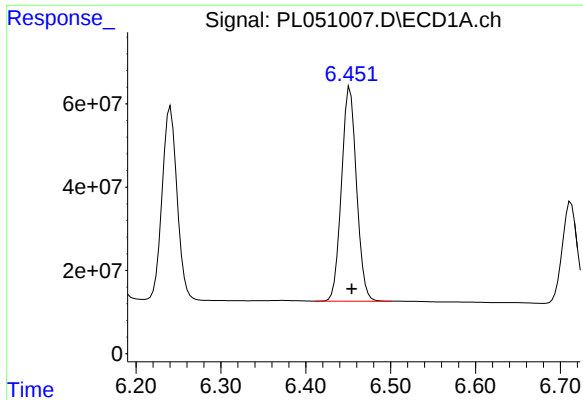


#19 Endosulfan Sulfate

R.T.: 6.452 min
Delta R.T.: -0.002 min
Response: 633581082
Conc: 49.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

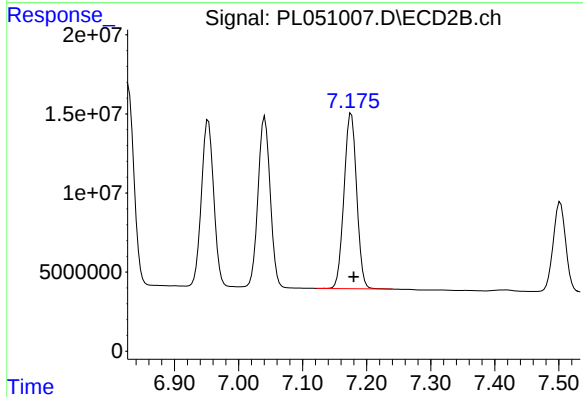


#19 Endosulfan Sulfate

R.T.: 7.176 min
Delta R.T.: -0.004 min
Response: 151983021
Conc: 52.62 ng/ml

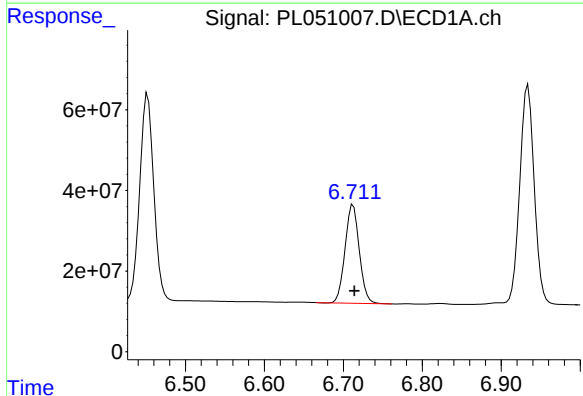


#20 Methoxychlor

R.T.: 6.712 min
Delta R.T.: -0.002 min
Response: 306419124
Conc: 49.11 ng/ml

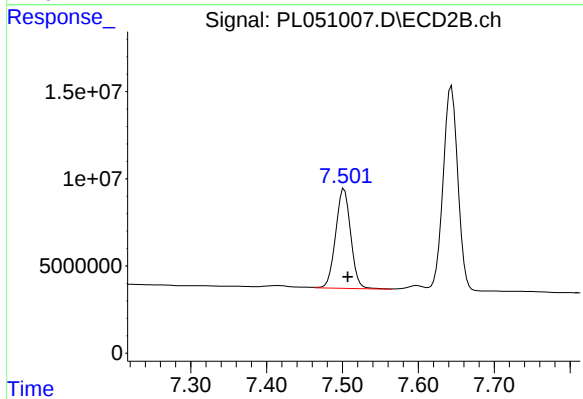

#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: -0.005 min
Response: 78973886
Conc: 53.82 ng/ml

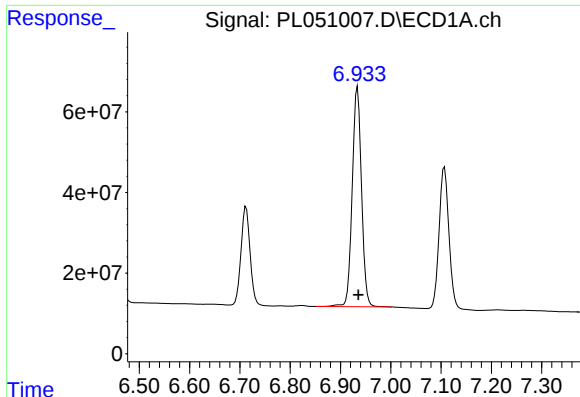


#21 Endrin ketone

R.T.: 6.934 min
Delta R.T.: -0.002 min
Response: 702269883
Conc: 51.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

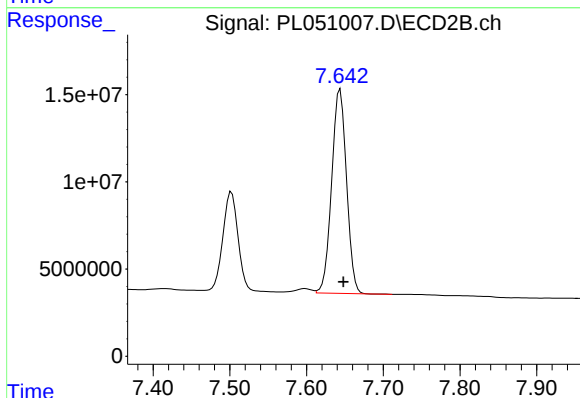


#21 Endrin ketone

R.T.: 7.644 min
Delta R.T.: -0.004 min
Response: 157348724
Conc: 54.42 ng/ml

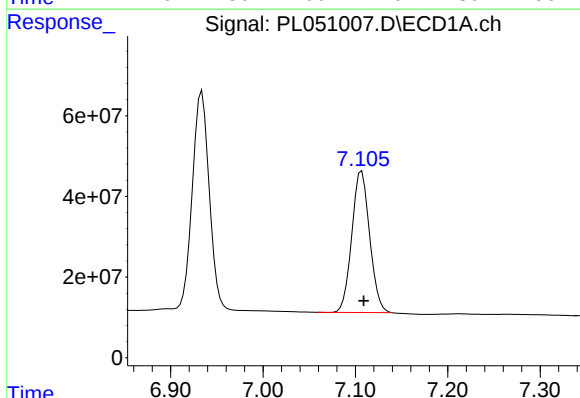


#22 Mirex

R.T.: 7.107 min
Delta R.T.: -0.002 min
Response: 470633675
Conc: 48.00 ng/ml

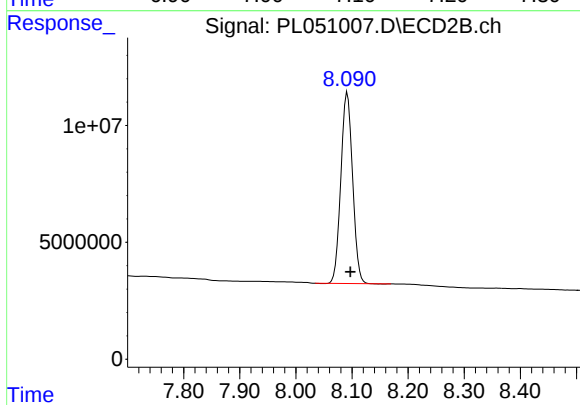

#22 Mirex

R.T.: 8.092 min
Delta R.T.: -0.005 min
Response: 118775580
Conc: 51.71 ng/ml

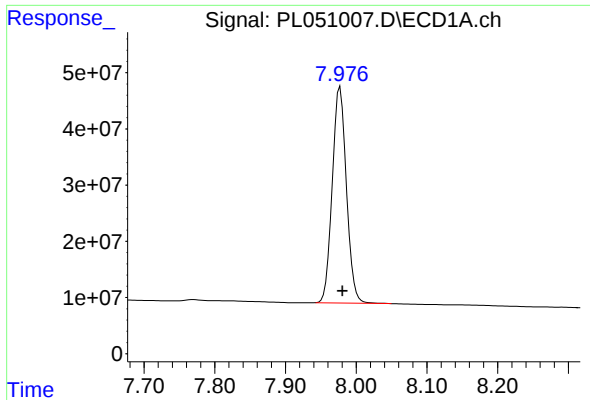


#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 534858394
Conc: 52.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Manual Integrations
APPROVED

Ankita
8/5/2019 2:39:23 PM

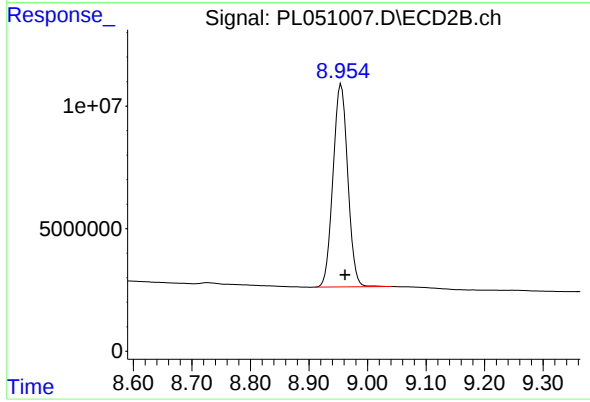

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.007 min
Response: 144669904
Conc: 51.16 ng/ml