

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080221\
 Data File : PL068629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2021 08:40
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 01:27:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	6.161f	0.000	1033703	0	1.696	N.D.	#
6) B	beta-BHC	6.161	0.000	1033703	0	3.533	N.D.	#
8) B	Heptachlo...	0.000	8.040	0	49813	N.D.	0.044	#
9) A	Endosulfan I	0.000	8.467f	0	104677	N.D.	0.102	#
14) MA	Endrin	0.000	8.983f	0	212899	N.D.	0.238	#
15) B	Endosulfa...	0.000	9.222f	0	79901	N.D.	0.088	#
17) MA	4,4'-DDT	0.000	9.434	0	50899	N.D.	0.054	#
22)	Mirex	0.000	10.530	0	49634	N.D.	0.064	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080221\
Data File : PL068629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2021 08:40
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 01:27:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

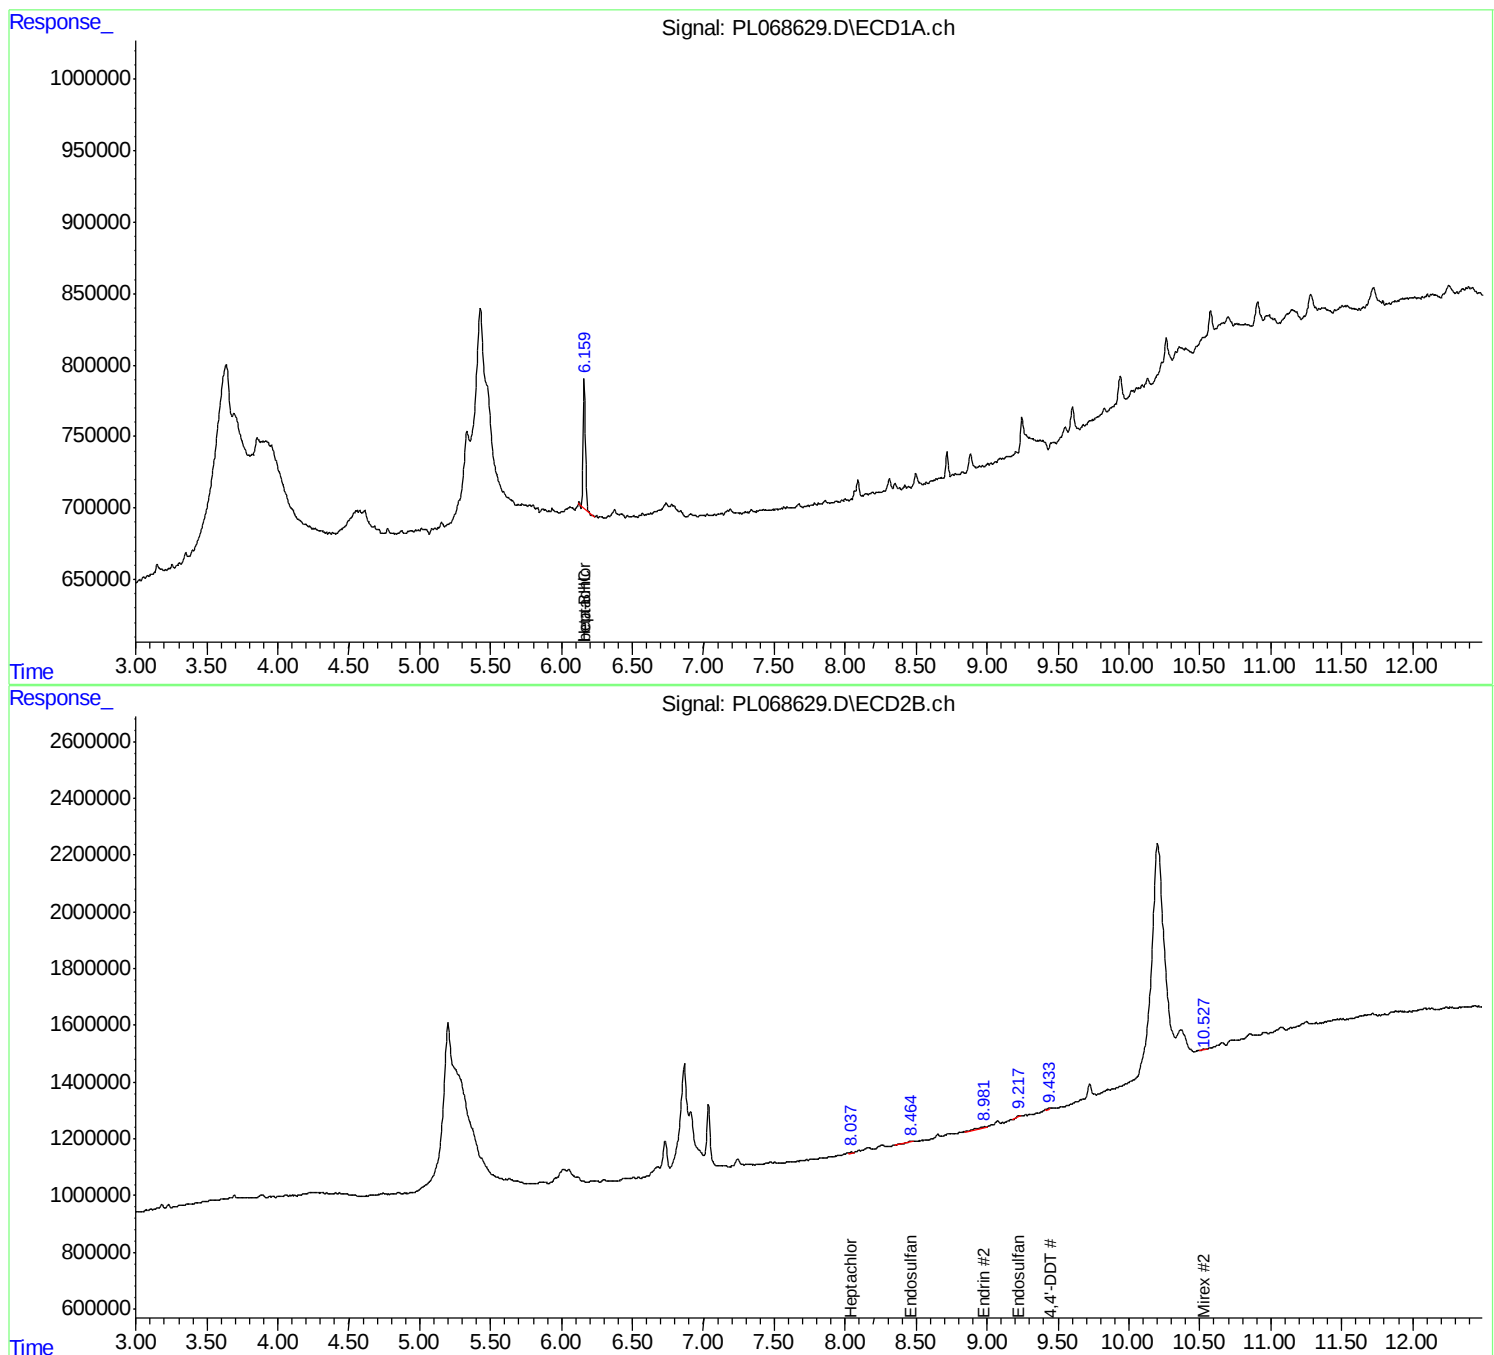


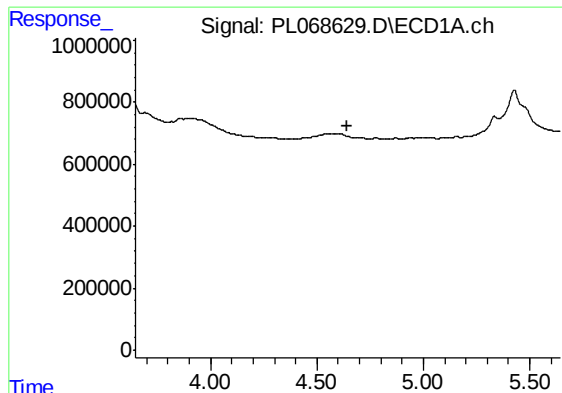

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

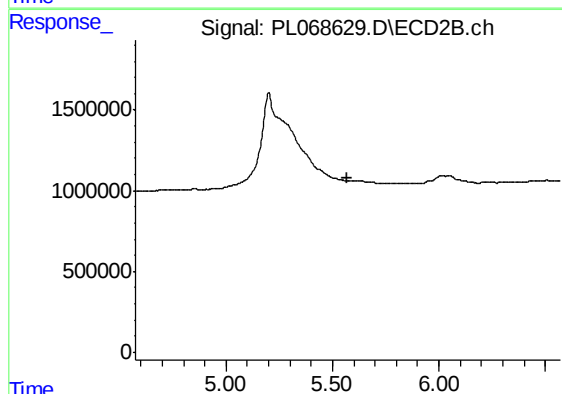


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

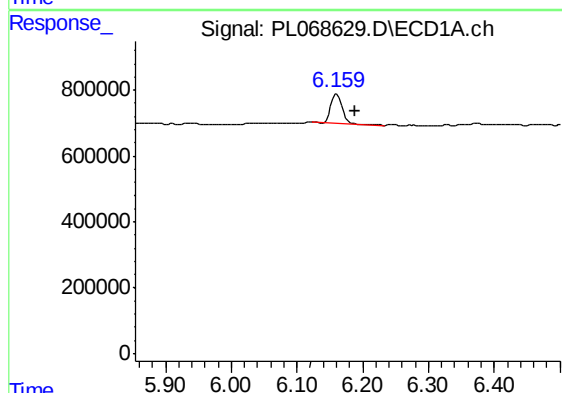


#4 Heptachlor

R.T.: 6.161 min
Delta R.T.: -0.028 min
Response: 1033703
Conc: 1.70 ng/ml

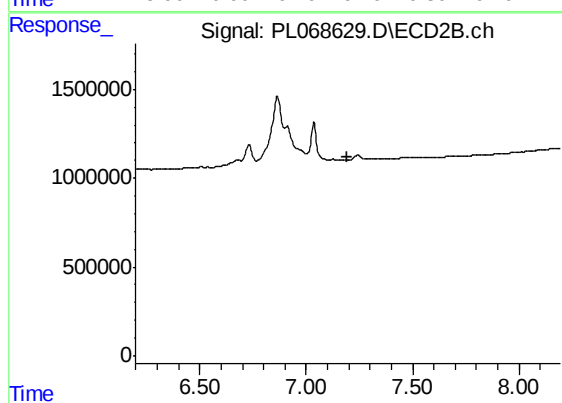

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 7.195 min
Response: 0
Conc: N.D.

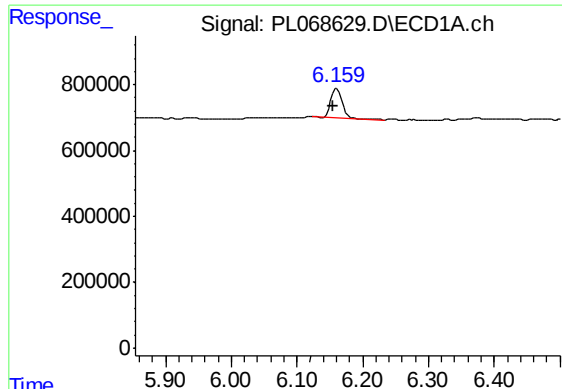

#6 beta-BHC


R.T.: 6.161 min
Delta R.T.: 0.006 min
Response: 1033703
Conc: 3.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

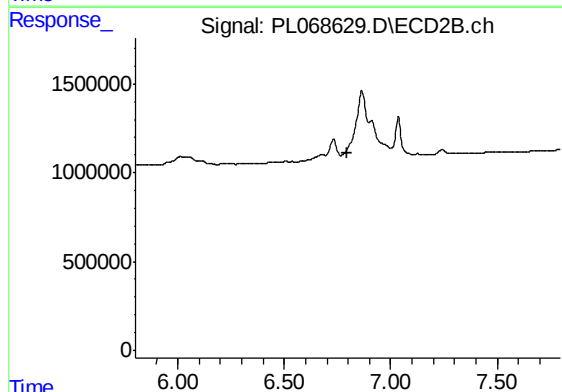


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

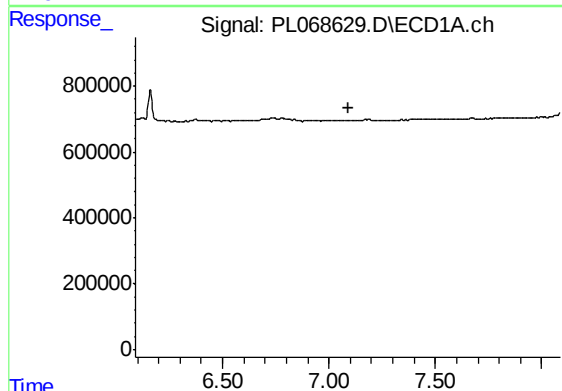


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

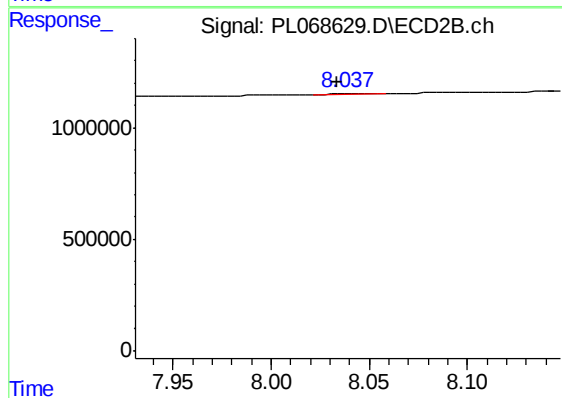

#8 Heptachlor epoxide


R.T.: 8.040 min
Delta R.T.: 0.006 min
Response: 49813
Conc: 0.04 ng/ml

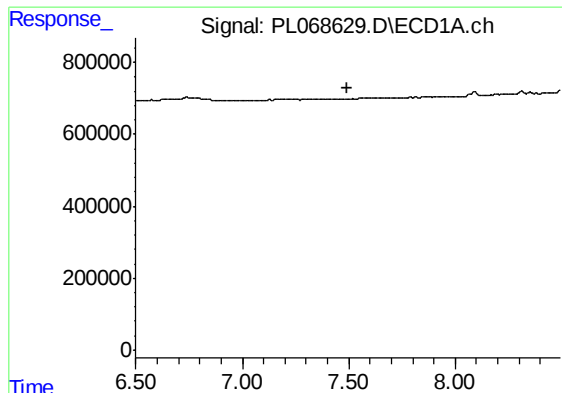

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

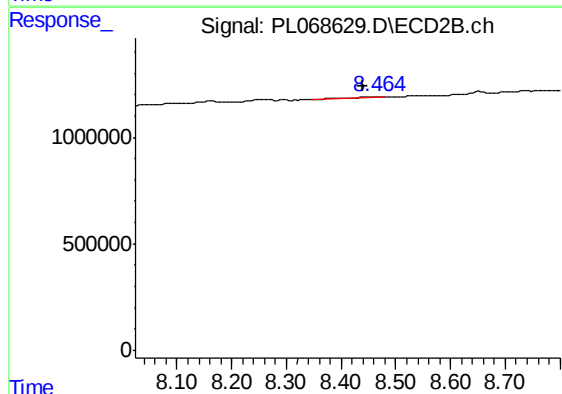


#9 Endosulfan I

R.T.: 8.467 min
Delta R.T.: 0.028 min
Response: 104677
Conc: 0.10 ng/ml

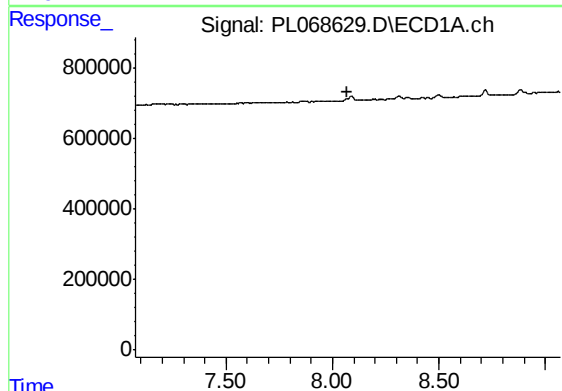


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

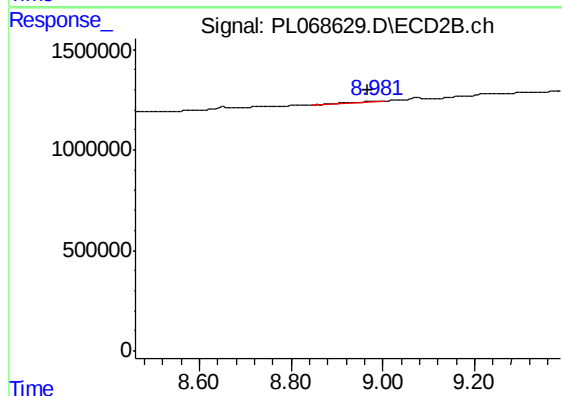

#14 Endrin


R.T.: 8.983 min
Delta R.T.: 0.016 min
Response: 212899
Conc: 0.24 ng/ml

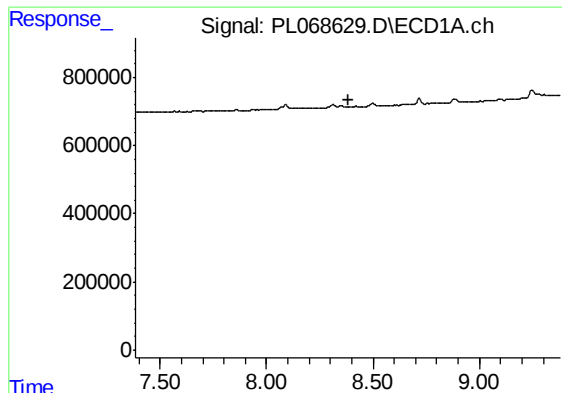

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

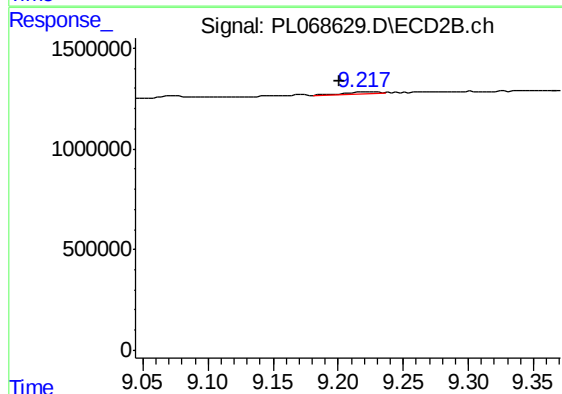


#15 Endosulfan II

R.T.: 9.222 min
Delta R.T.: 0.021 min
Response: 79901
Conc: 0.09 ng/ml

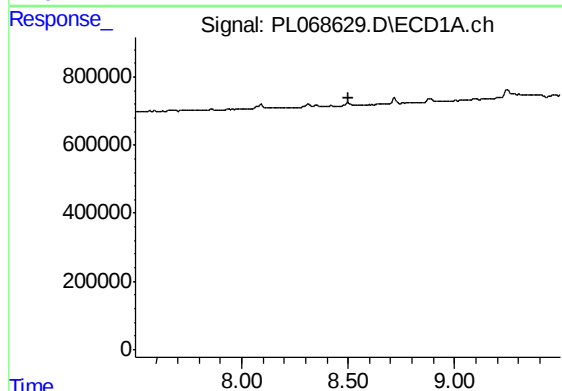


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.501 min
Response: 0
Conc: N.D.

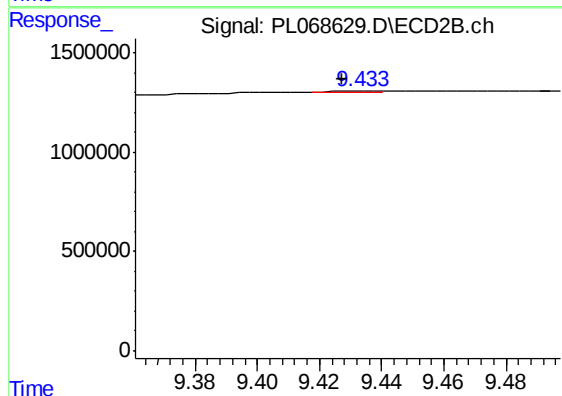

#17 4,4'-DDT


R.T.: 9.434 min
Delta R.T.: 0.007 min
Response: 50899
Conc: 0.05 ng/ml

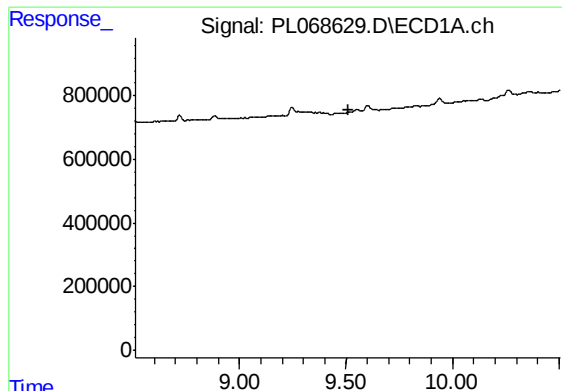

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

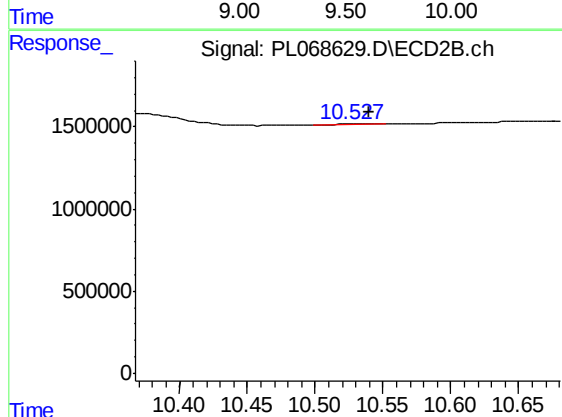


#22 Mirex

R.T.: 10.530 min
Delta R.T.: -0.009 min
Response: 49634
Conc: 0.06 ng/ml

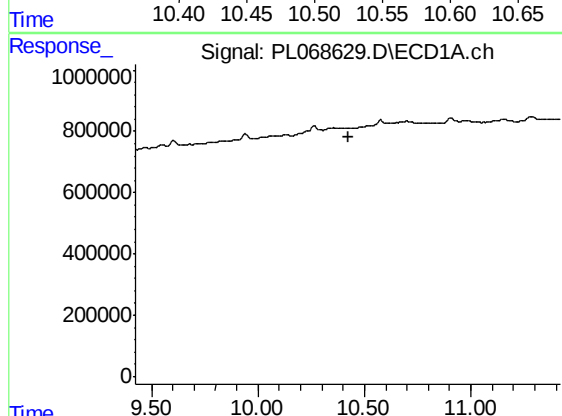

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

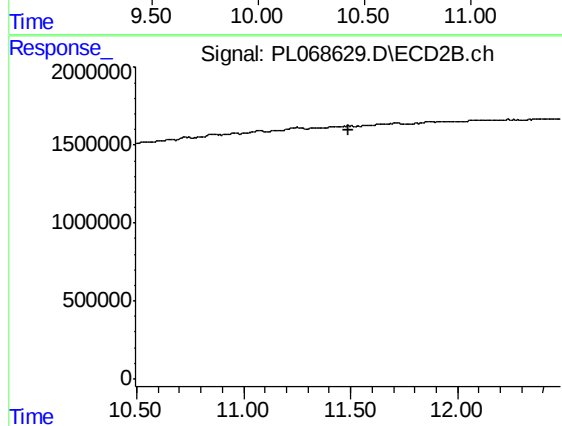

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.