

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080222\
 Data File : PL076844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Aug 2022 14:48
 Operator : AR\AJ
 Sample : N3995-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 03 04:56:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.640	11198441	28112492	11.763	12.180
28)	SA Decachlor...	8.912	7.748	8420413	20731957	10.596	10.783
Target Compounds							
4)	MA Heptachlor	4.821f	0.000	185779	0	0.152	N.D. #
9)	A Endosulfan I	0.000	4.946	0	211752	N.D.	0.100 #
16)	A 4,4'-DDD	0.000	5.618	0	218643	N.D.	0.117 #
23)	Chlordane-1	0.000	3.609	0	501823	N.D.	6.290 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080222\
Data File : PL076844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Aug 2022 14:48
Operator : AR\AJ
Sample : N3995-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 03 04:56:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

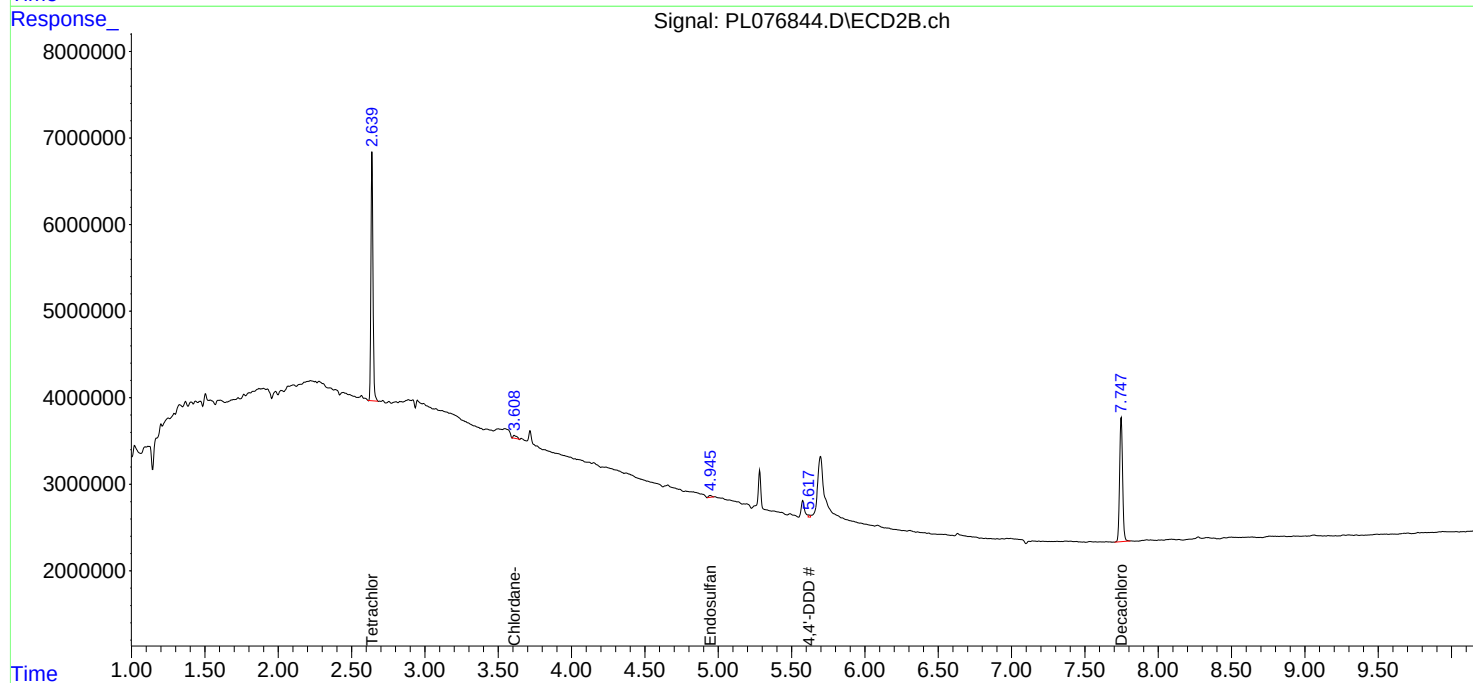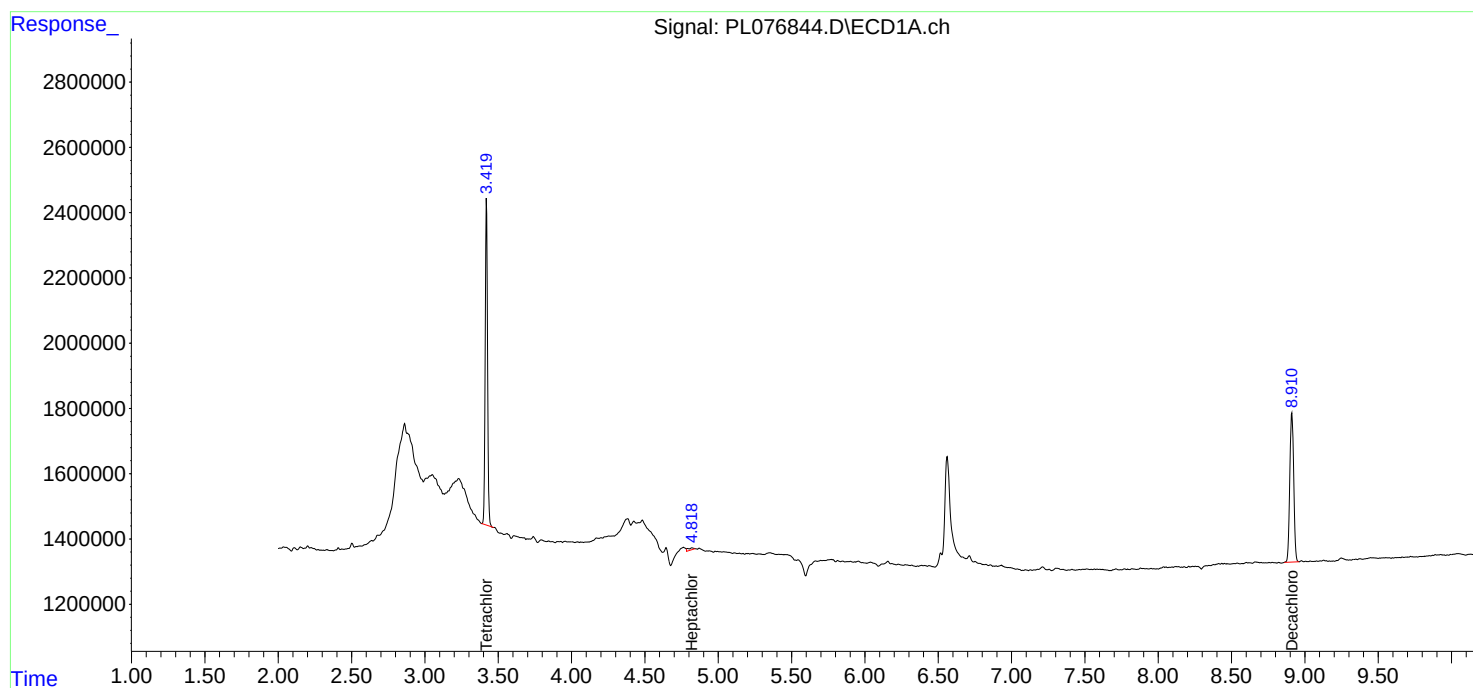


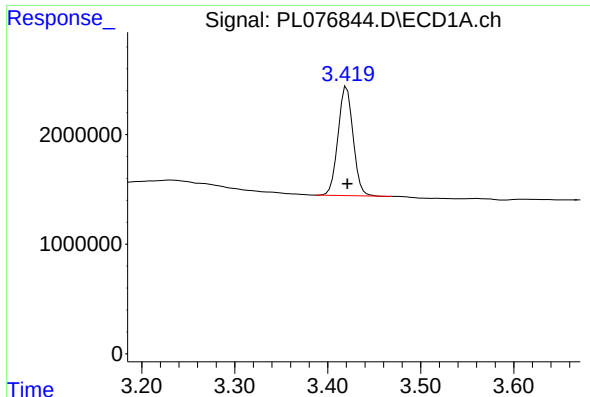

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 11198441
Conc: 11.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

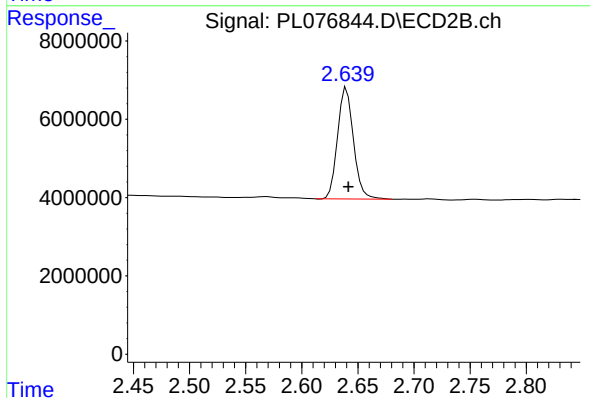


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.001 min
Response: 28112492
Conc: 12.18 ng/ml

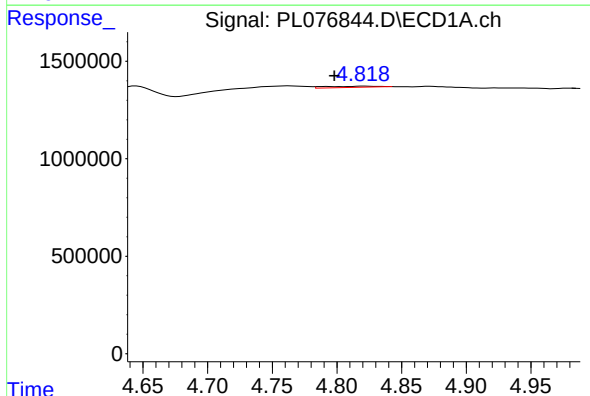


#4 Heptachlor

R.T.: 4.821 min
Delta R.T.: 0.023 min
Response: 185779
Conc: 0.15 ng/ml

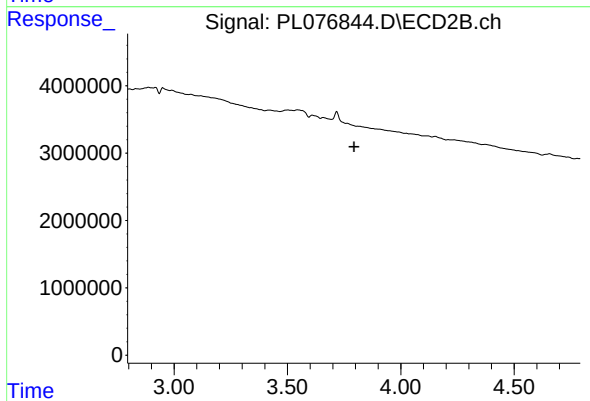

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.794 min
Response: 0
Conc: N.D.

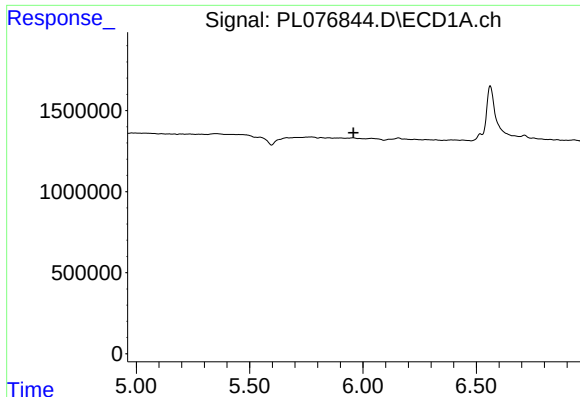

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.958 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

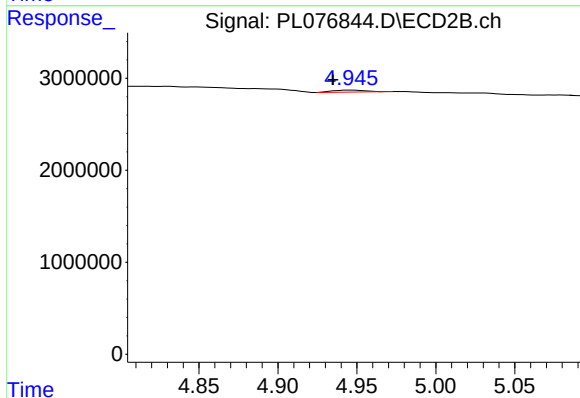


#9 Endosulfan I

R.T.: 4.946 min
Delta R.T.: 0.011 min
Response: 211752
Conc: 0.10 ng/ml

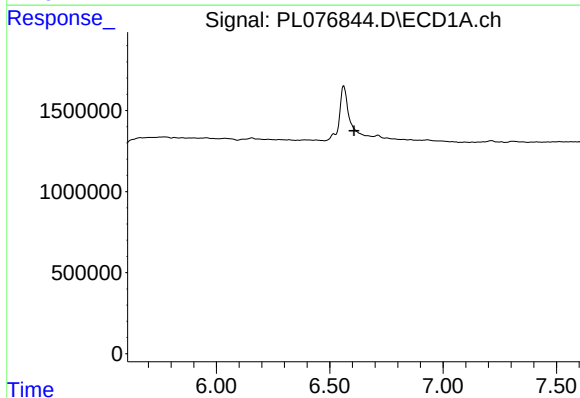


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.608 min
Response: 0
Conc: N.D.

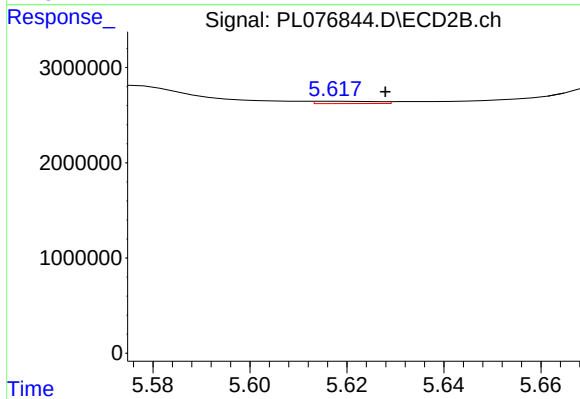

#16 4,4'-DDD


R.T.: 5.618 min
Delta R.T.: -0.010 min
Response: 218643
Conc: 0.12 ng/ml

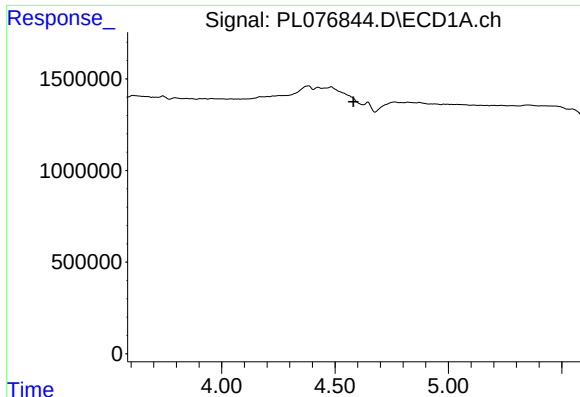

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.581 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

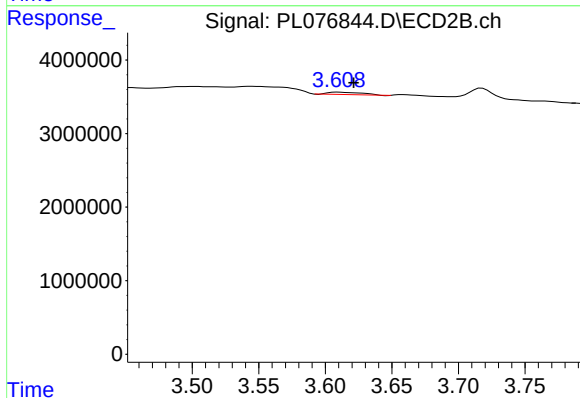


#23 Chlordane-1

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 501823
Conc: 6.29 ng/ml

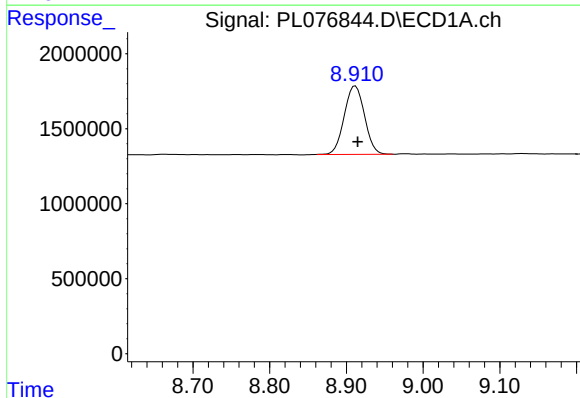

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: -0.003 min
Response: 8420413
Conc: 10.60 ng/ml

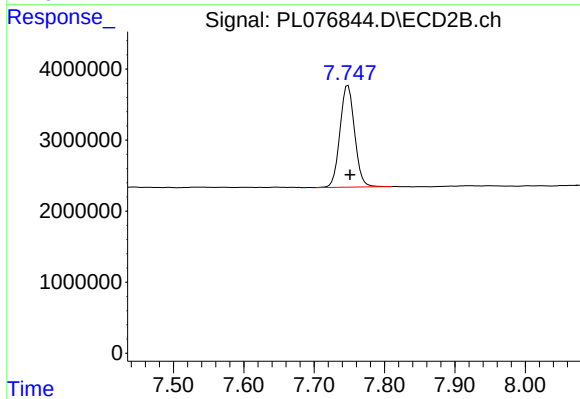

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 20731957
Conc: 10.78 ng/ml