

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080223\
 Data File : PL084442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2023 16:41
 Operator : AR\AJ
 Sample : 03840-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUILDING-B-19-(0-5)

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/02/2023
 Supervised By :Ankita Jodhani 08/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 21:39:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 01 05:59:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.687	34848996	16552781	15.083	15.140
2) SA Decachlor...	9.021	7.868	18368099	15331943	11.960m	12.538
Target Compounds						
17) MA 4,4'-DDT	6.985	5.972	2746711	1670094	1.542	1.402

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080223\
Data File : PL084442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2023 16:41
Operator : AR\AJ
Sample : 03840-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BUILDING-B-19-(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/02/2023
Supervised By :Ankita Jodhani 08/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 21:39:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080123.M
Quant Title : GC Extractables
QLast Update : Tue Aug 01 05:59:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

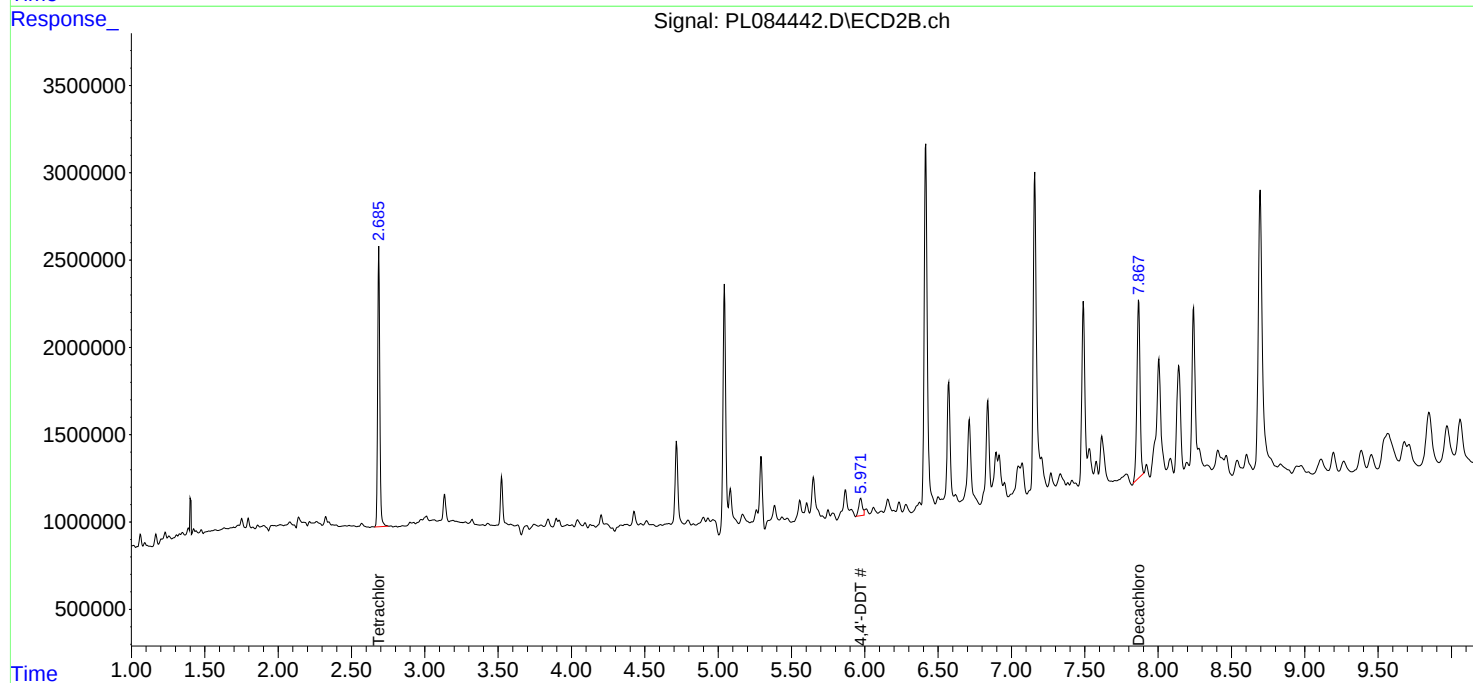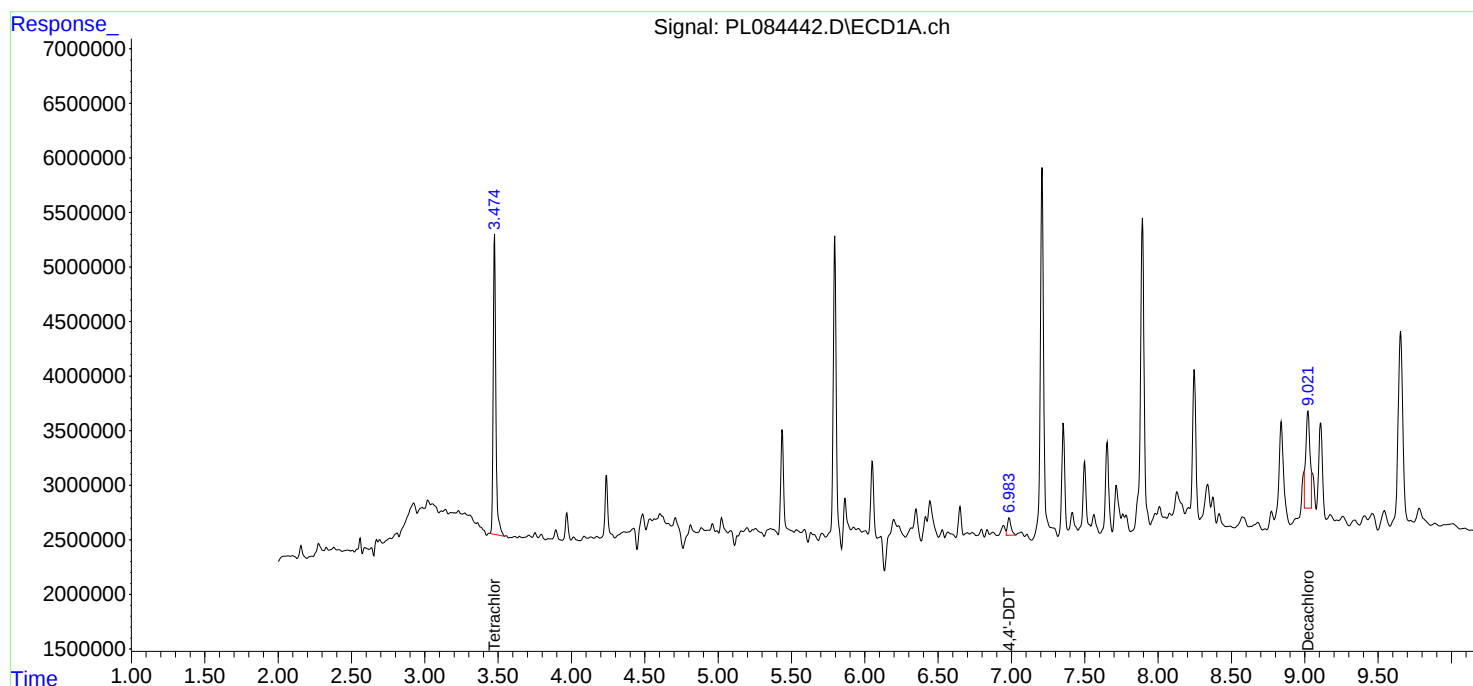

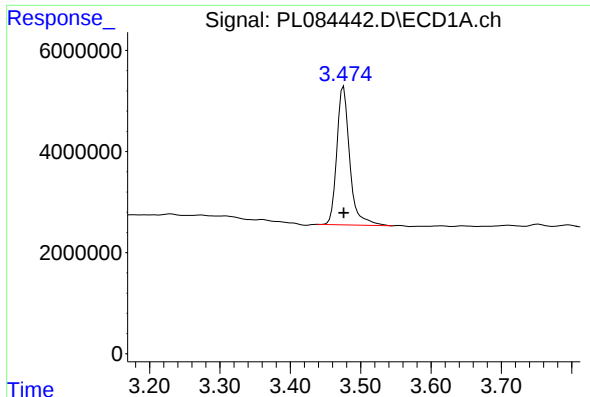


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 34848996
Conc: 15.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-19-(0-5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/02/2023
Supervised By :Ankita Jodhani 08/02/2023

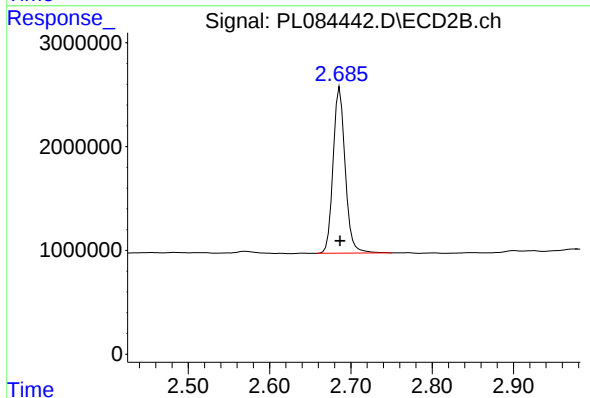


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 16552781
Conc: 15.14 ng/ml

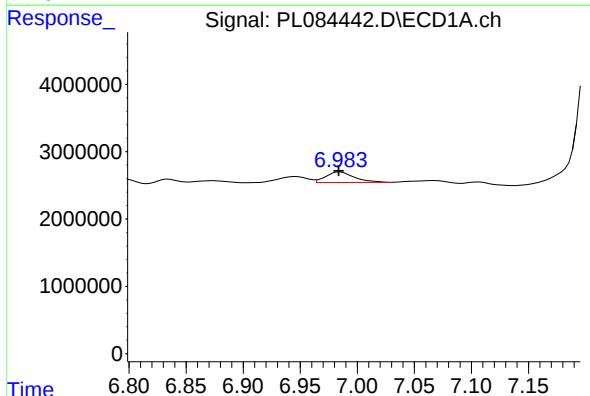


#17 4,4'-DDT

R.T.: 6.985 min
Delta R.T.: 0.000 min
Response: 2746711
Conc: 1.54 ng/ml

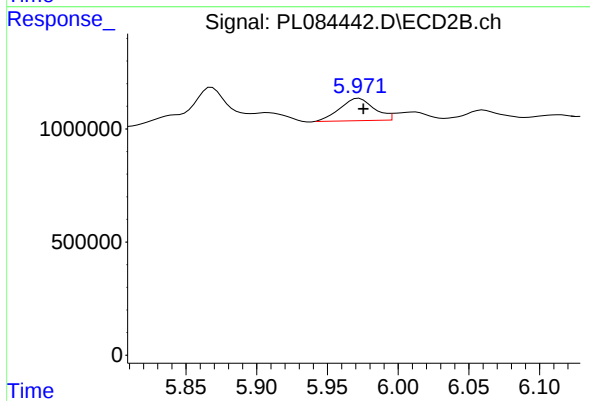

#17 4,4'-DDT

R.T.: 5.972 min
Delta R.T.: -0.003 min
Response: 1670094
Conc: 1.40 ng/ml

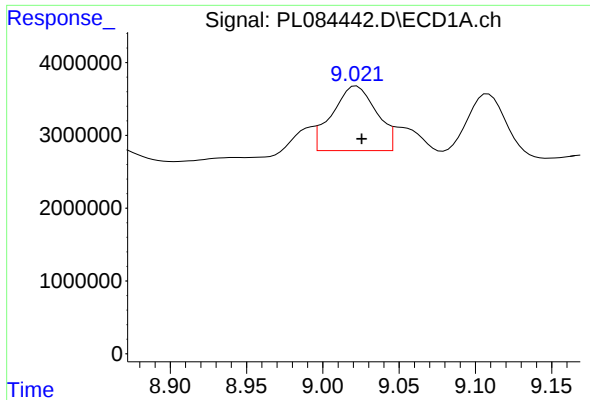


#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: -0.005 min
Response: 18368099
Conc: 11.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-B-19-(0-5)

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/02/2023
Supervised By :Ankita Jodhani 08/02/2023

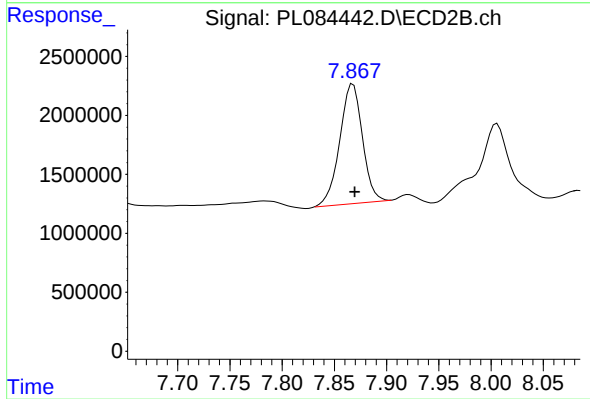

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: -0.002 min
Response: 15331943
Conc: 12.54 ng/ml