

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
 Data File : PL038895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2018 18:17
 Operator : AJ\SJ
 Sample : J4310-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 00:09:32 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	154.1E6	59442251	20.699	22.645
28)	SA Decachlor...	7.989	8.933	145.9E6	52059784	19.239	21.297
Target Compounds							
2)	A alpha-BHC	0.000	4.324	0	557979	N.D.	0.144 #
3)	MA gamma-BHC...	4.076f	0.000	22677800	0	2.163	N.D. #
4)	MA Heptachlor	0.000	5.164f	0	2429645	N.D.	0.760 #
7)	B delta-BHC	0.000	4.958	0	10825507	N.D.	3.264 #
8)	B Heptachlo...	4.939f	5.799	3755883	1451434	0.398	0.511 #
15)	B Endosulfa...	0.000	6.826	0	1310074	N.D.	0.546 #
16)	A 4,4'-DDD	0.000	6.673f	0	1102635	N.D.	0.515 #
23)	Chlordane-1	4.238	4.912	19280511	38417	55.684	0.332 #
27)	Chlordane-5	0.000	6.826	0	1310074	N.D.	14.625 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
Data File : PL038895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2018 18:17
Operator : AJ\SJ
Sample : J4310-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 00:09:32 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

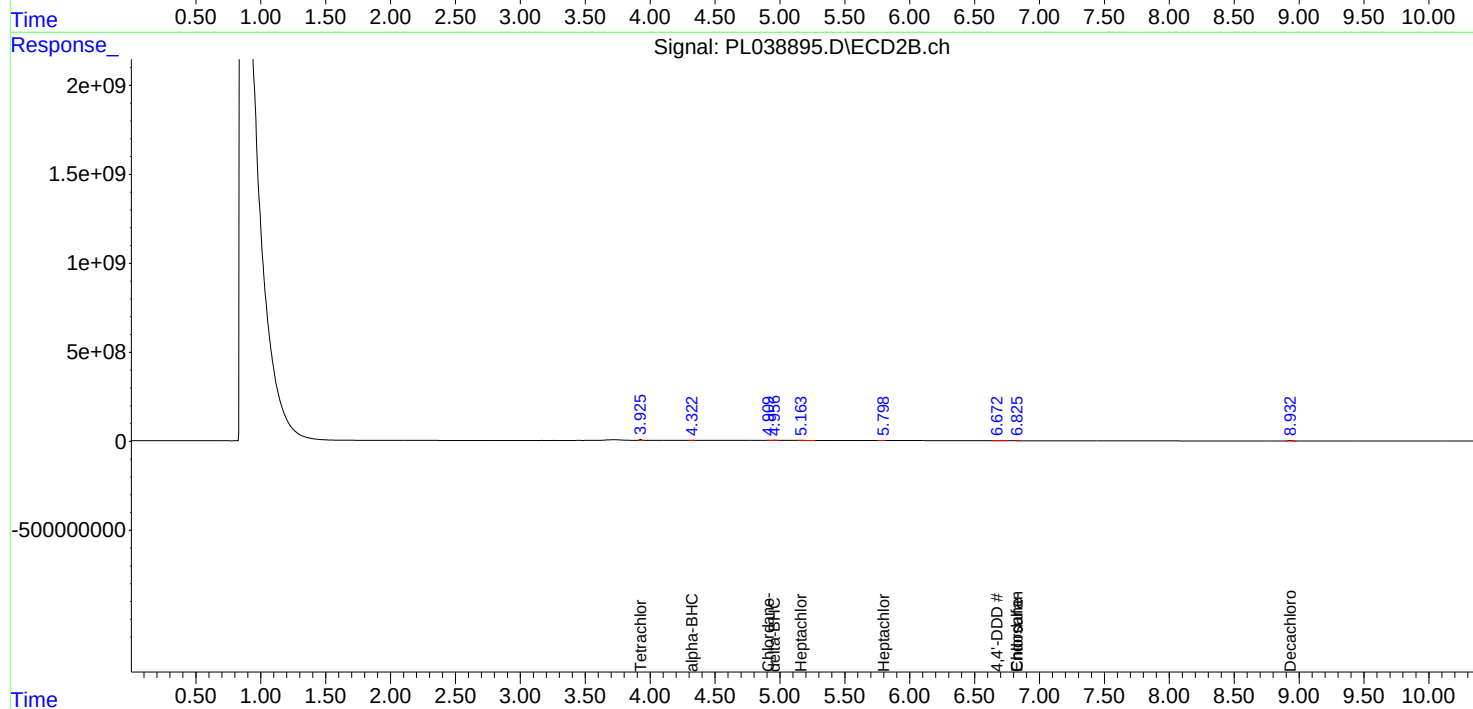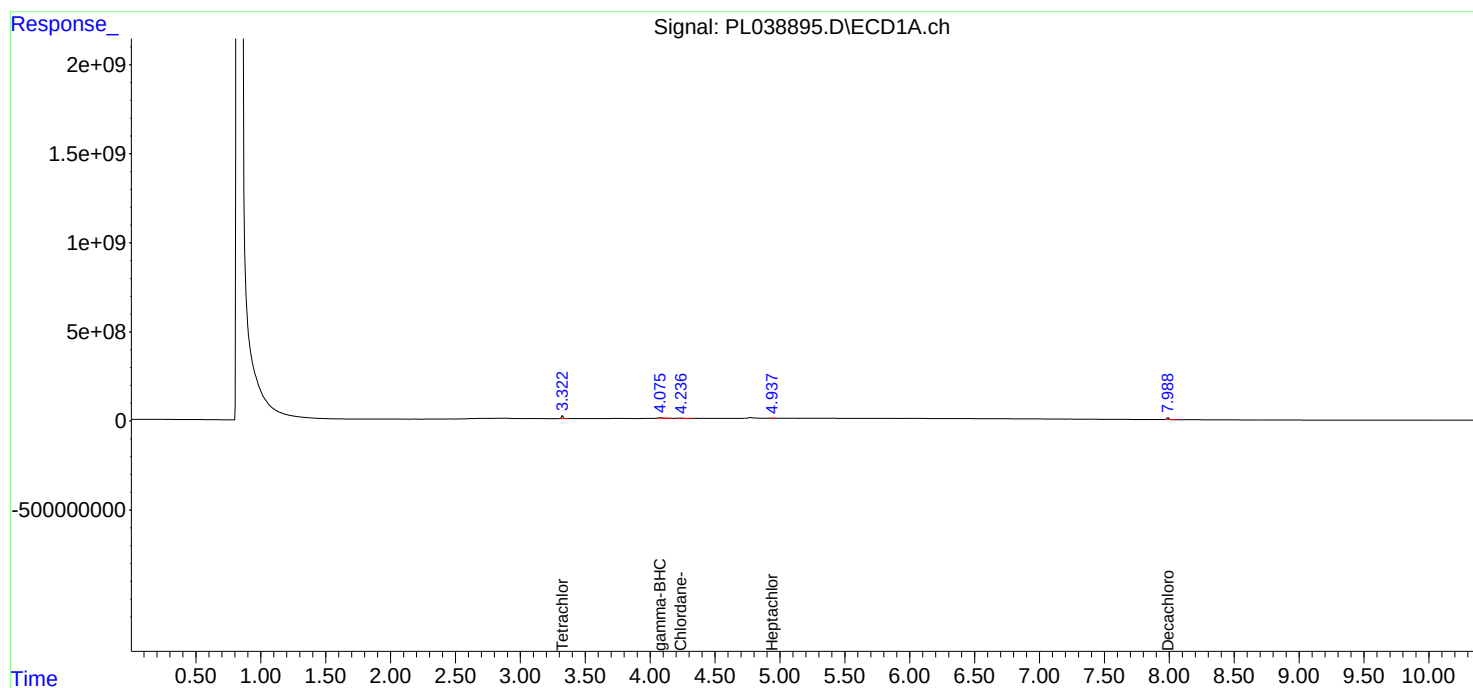


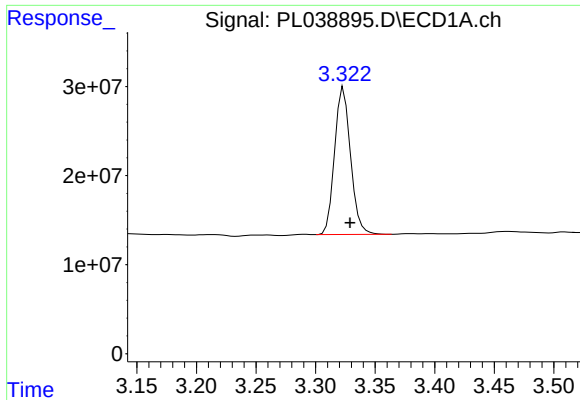

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 154133591
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

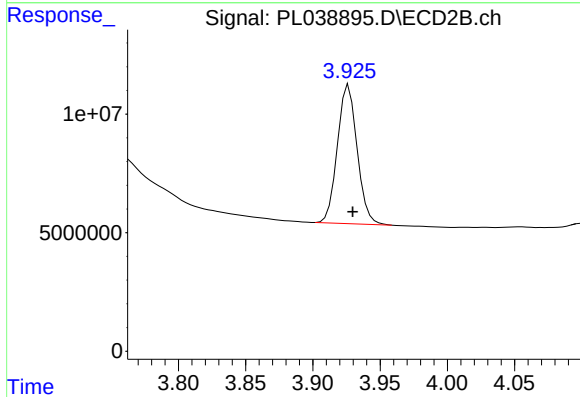


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 59442251
Conc: 22.65 ng/ml

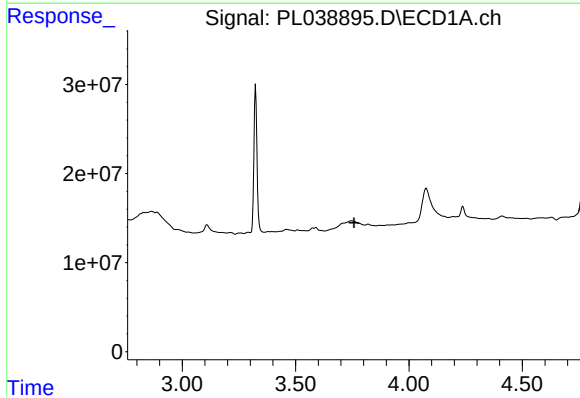


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

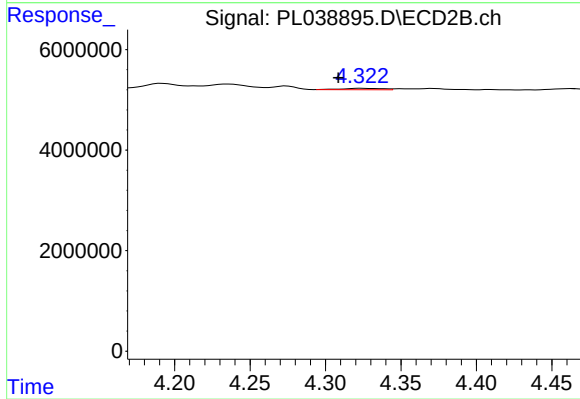

#2 alpha-BHC


R.T.: 4.324 min
Delta R.T.: 0.015 min
Response: 557979
Conc: 0.14 ng/ml

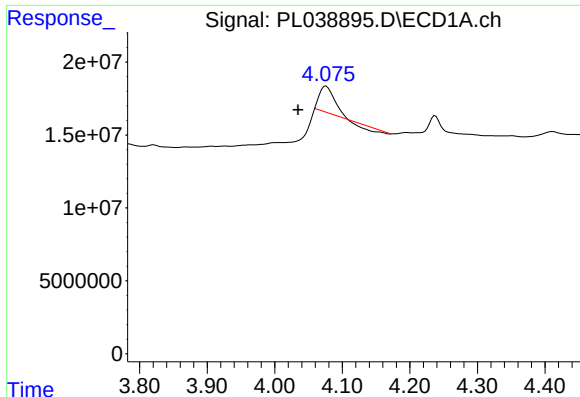

#3 gamma-BHC (Lindane)


R.T.: 4.076 min
Delta R.T.: 0.041 min
Response: 22677800
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

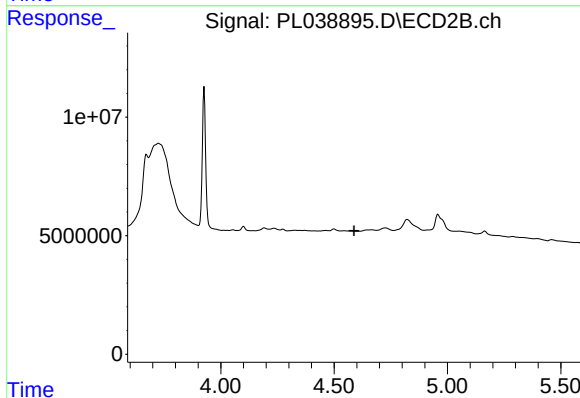


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.588 min
Response: 0
Conc: N.D.

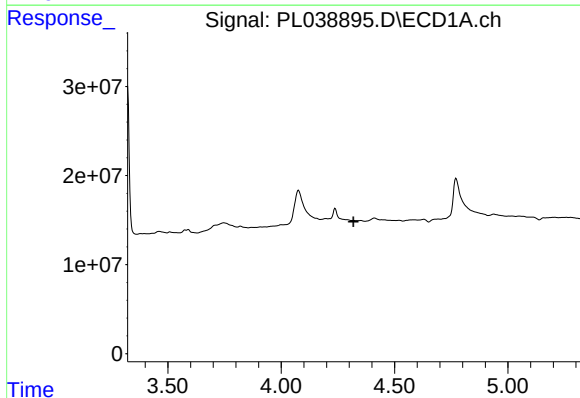


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

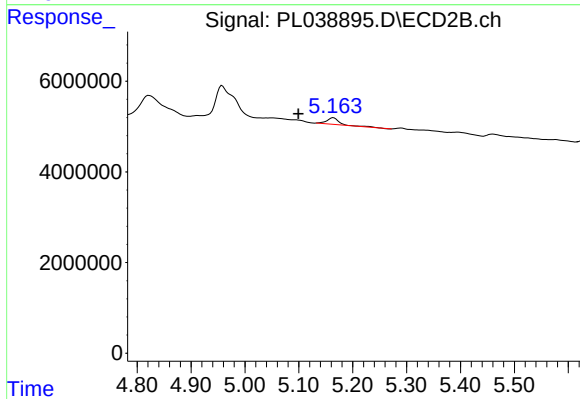

#4 Heptachlor


R.T.: 5.164 min
Delta R.T.: 0.065 min
Response: 2429645
Conc: 0.76 ng/ml

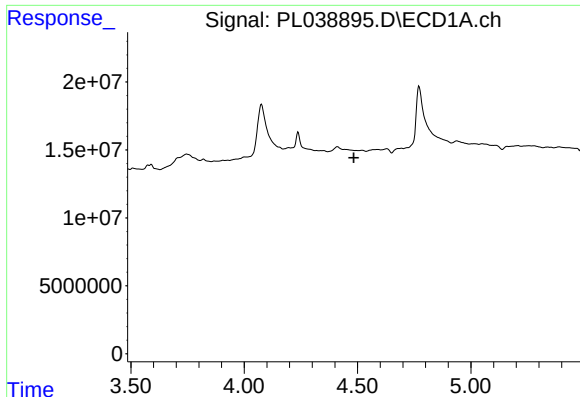

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

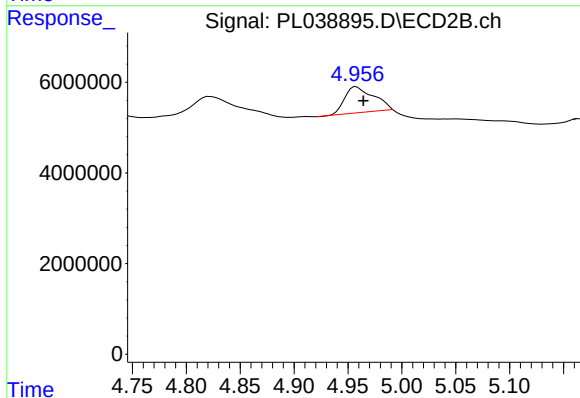


#7 delta-BHC

R.T.: 4.958 min
Delta R.T.: -0.007 min
Response: 10825507
Conc: 3.26 ng/ml

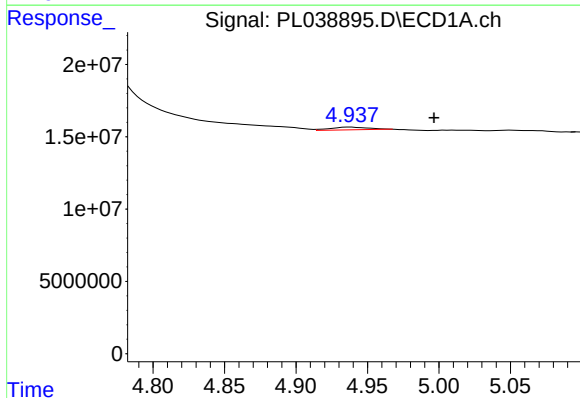


#8 Heptachlor epoxide

R.T.: 4.939 min
Delta R.T.: -0.058 min
Response: 3755883
Conc: 0.40 ng/ml

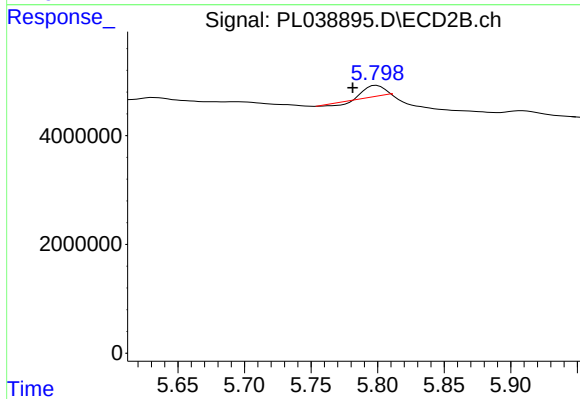

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: 0.018 min
Response: 1451434
Conc: 0.51 ng/ml

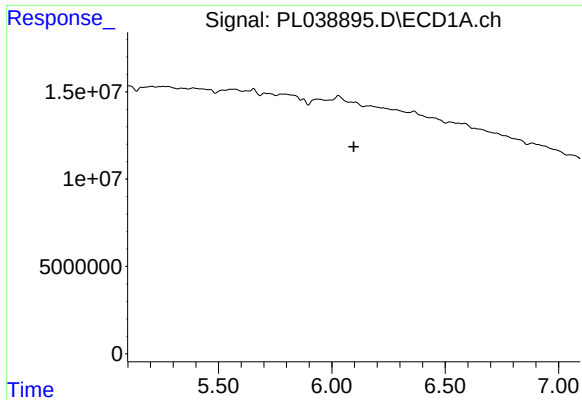

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

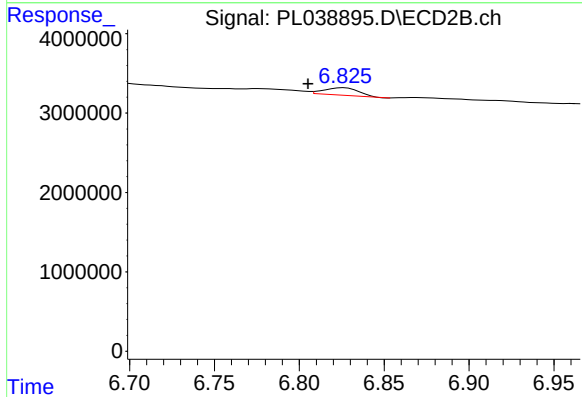


#15 Endosulfan II

R.T.: 6.826 min
Delta R.T.: 0.021 min
Response: 1310074
Conc: 0.55 ng/ml

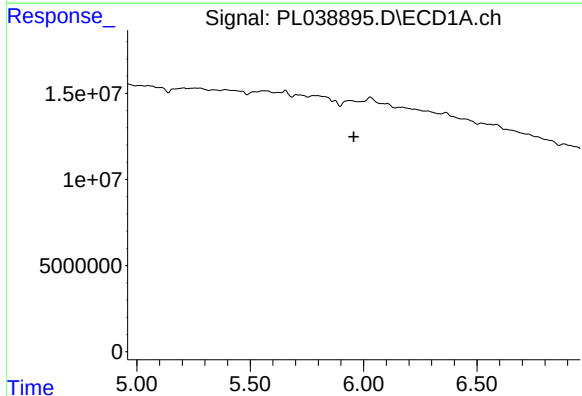


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

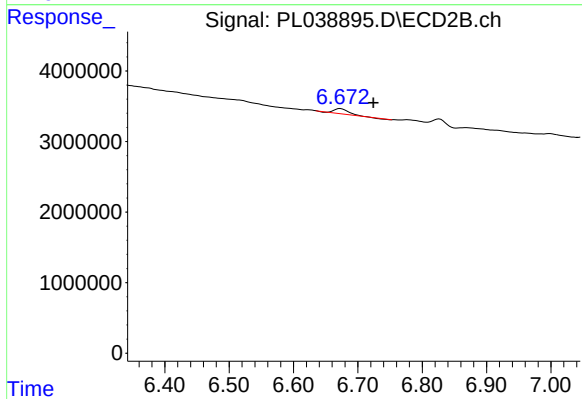

#16 4,4'-DDD


R.T.: 6.673 min
Delta R.T.: -0.052 min
Response: 1102635
Conc: 0.52 ng/ml

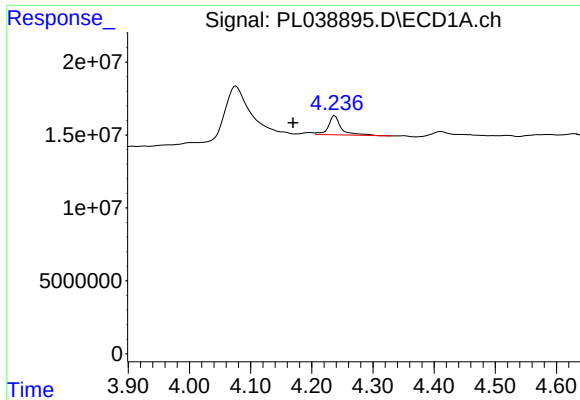

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 19280511
Conc: 55.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

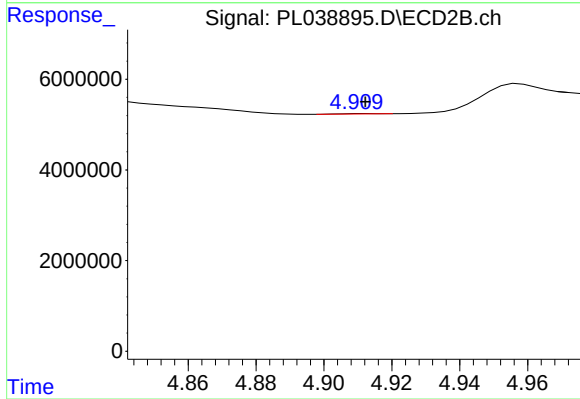


#23 Chlordane-1

R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 38417
Conc: 0.33 ng/ml

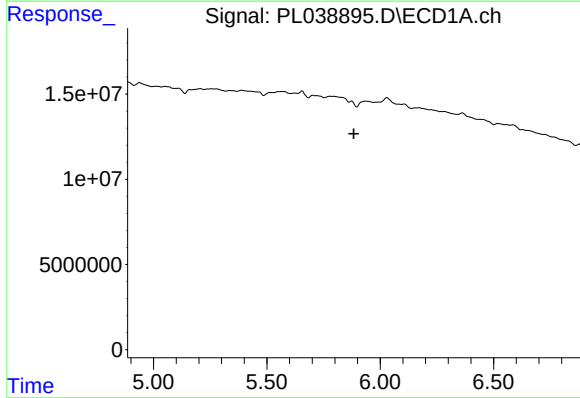


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

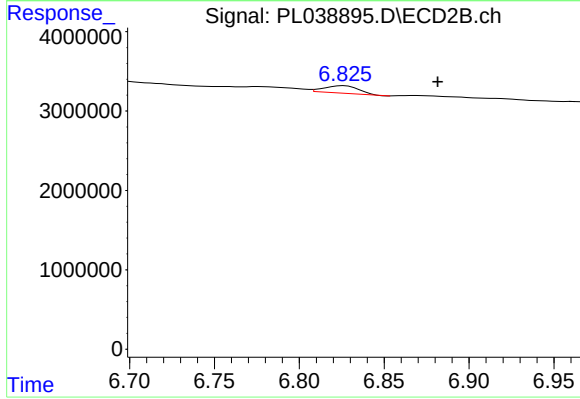

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.055 min
Response: 1310074
Conc: 14.62 ng/ml

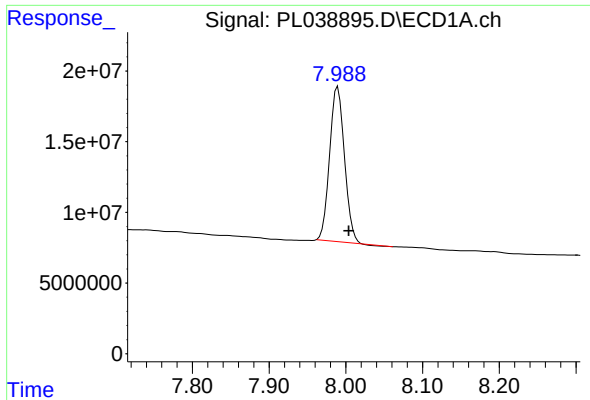

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.014 min
Response: 145948445
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

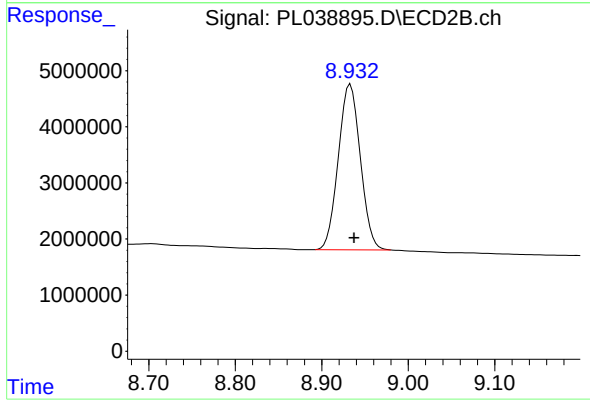

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 52059784
Conc: 21.30 ng/ml