

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
 Data File : PL038900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2018 19:27
 Operator : AJ\SJ
 Sample : J4313-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 00:11:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	152.0E6	58904789	20.410	22.440
28)	SA Decachlor...	7.990	8.933	145.4E6	51054447	19.170	20.886
Target Compounds							
2)	A alpha-BHC	0.000	4.324	0	1210762	N.D.	0.313 #
3)	MA gamma-BHC...	4.079f	4.547f	40798938	1371248	3.892	0.380 #
4)	MA Heptachlor	0.000	5.158f	0	1237468	N.D.	0.387 #
7)	B delta-BHC	0.000	4.958	0	10391660	N.D.	3.133 #
8)	B Heptachlo...	4.939f	5.799	3790791	1600222	0.402	0.563 #
15)	B Endosulfa...	0.000	6.827	0	1485496	N.D.	0.619 #
16)	A 4,4'-DDD	0.000	6.673f	0	268268	N.D.	0.125 #
23)	Chlordane-1	4.238	4.913	17988743	60598	51.953	0.523 #
27)	Chlordane-5	0.000	6.827	0	1485496	N.D.	16.583 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
Data File : PL038900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2018 19:27
Operator : AJ\SJ
Sample : J4313-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 00:11:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

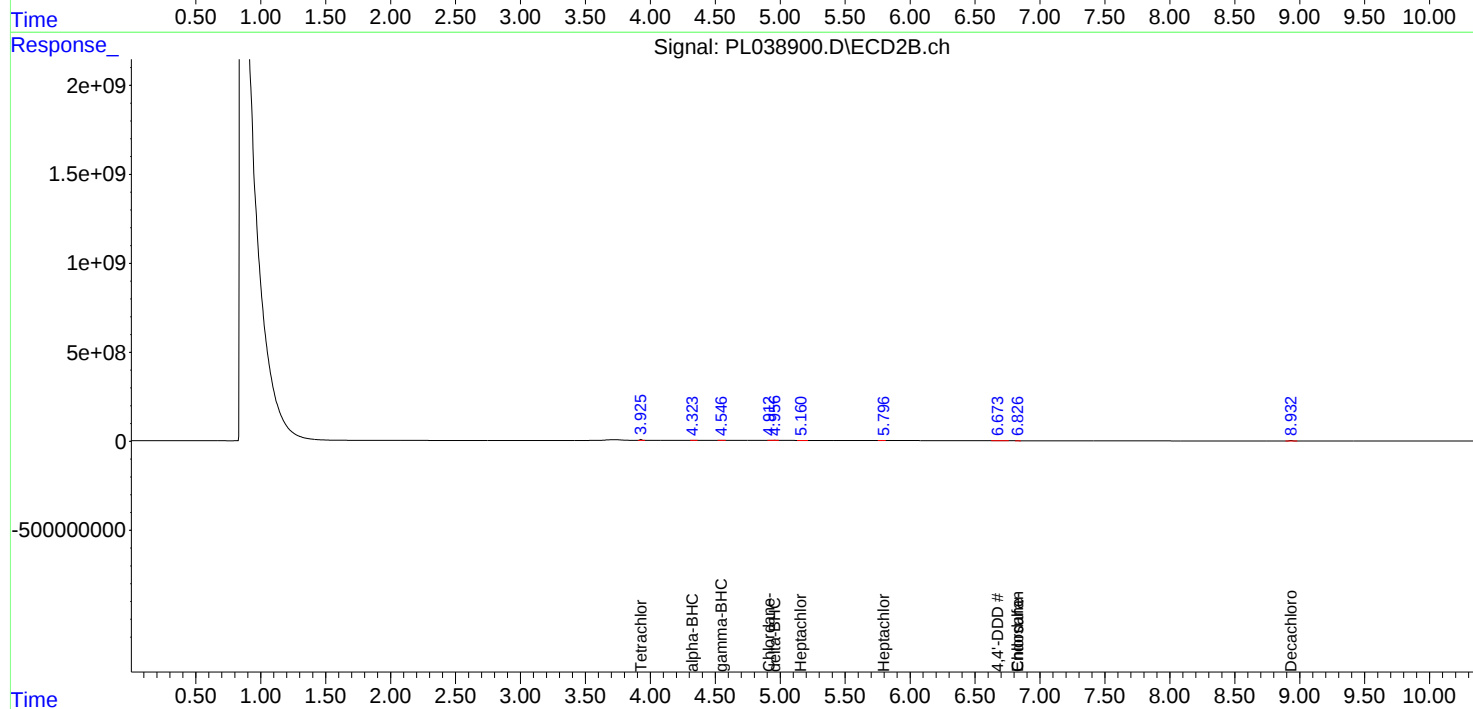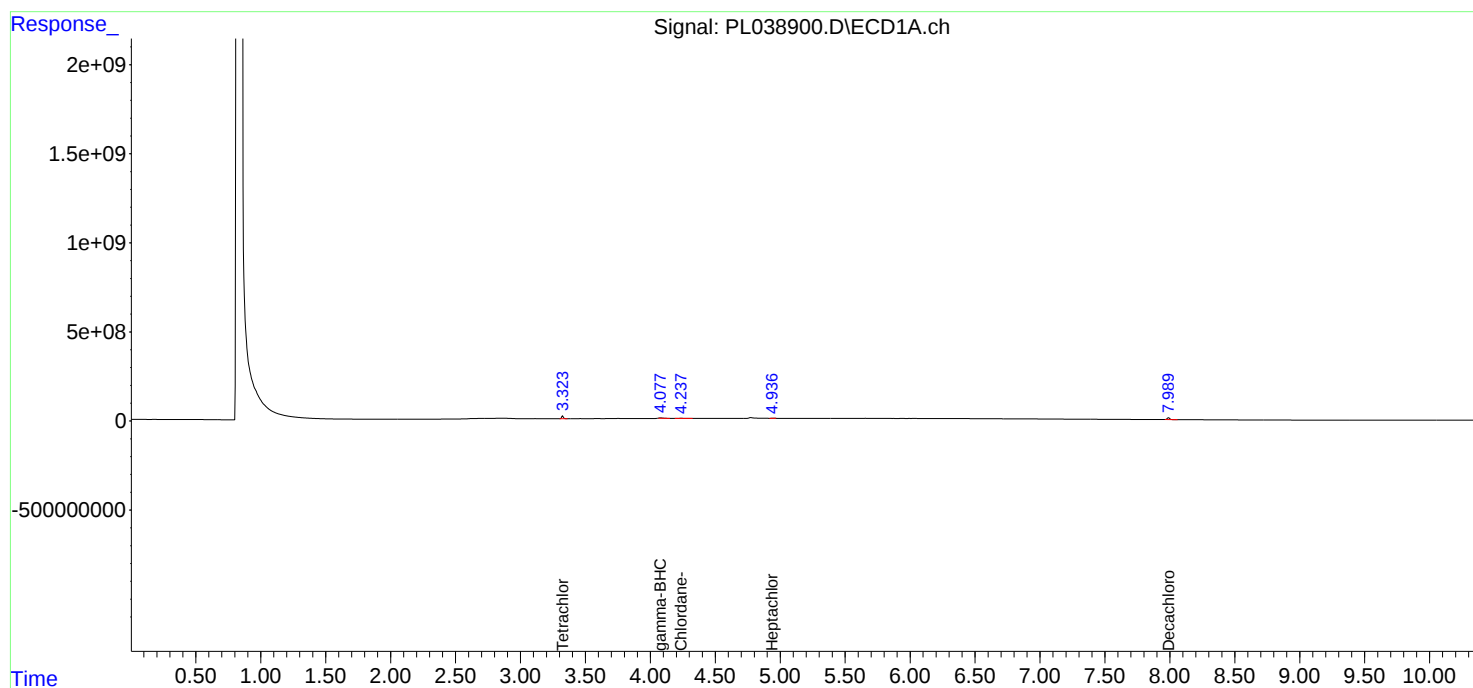


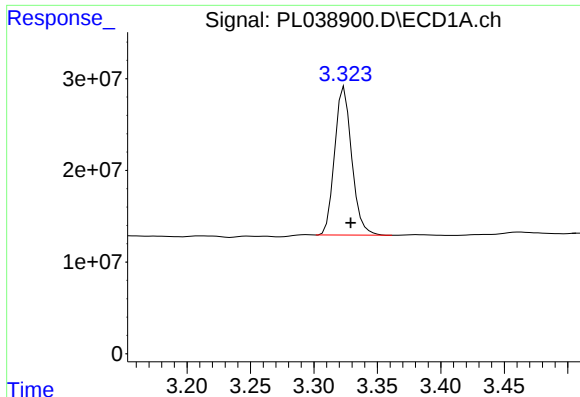

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 151982623
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

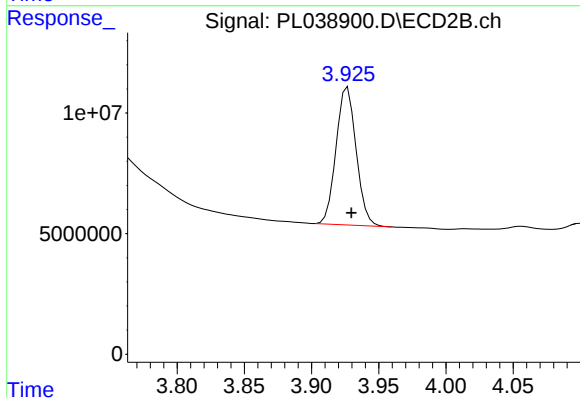


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 58904789
Conc: 22.44 ng/ml

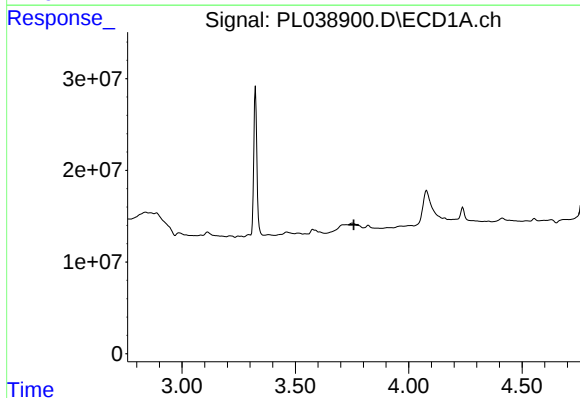


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

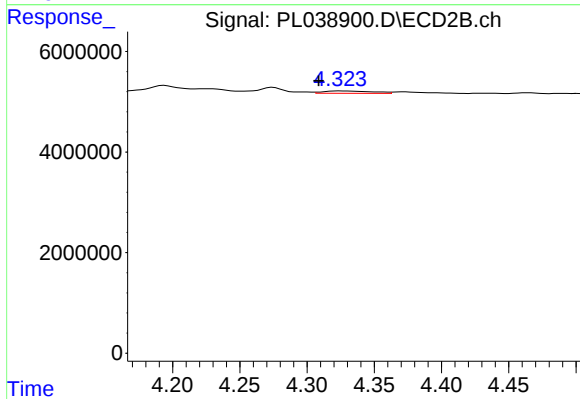

#2 alpha-BHC


R.T.: 4.324 min
Delta R.T.: 0.015 min
Response: 1210762
Conc: 0.31 ng/ml

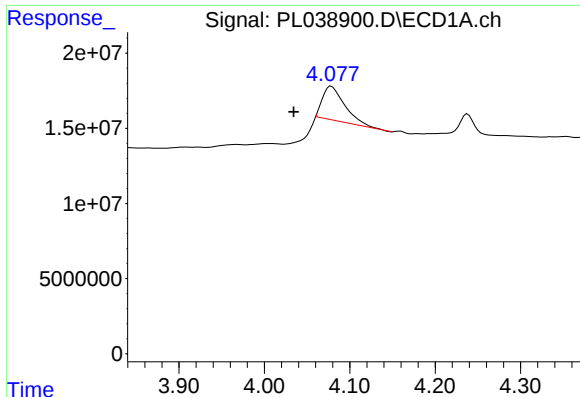

#3 gamma-BHC (Lindane)


R.T.: 4.079 min
Delta R.T.: 0.044 min
Response: 40798938
Conc: 3.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

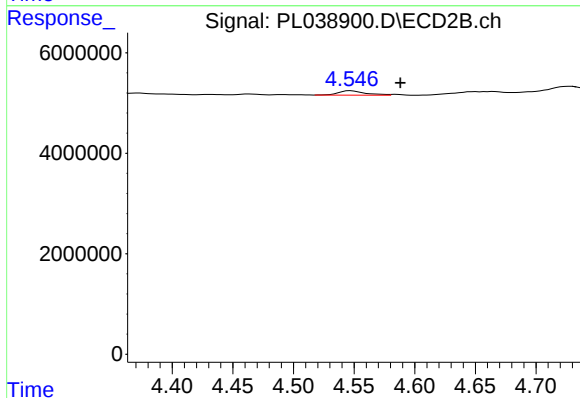


#3 gamma-BHC (Lindane)

R.T.: 4.547 min
Delta R.T.: -0.041 min
Response: 1371248
Conc: 0.38 ng/ml

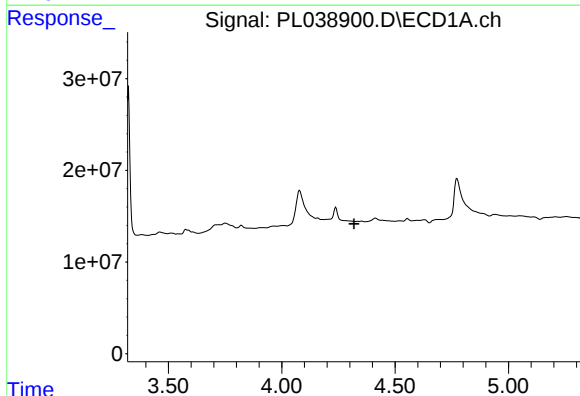


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

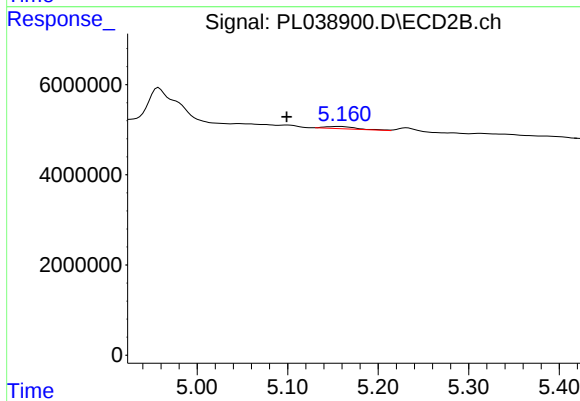

#4 Heptachlor


R.T.: 5.158 min
Delta R.T.: 0.059 min
Response: 1237468
Conc: 0.39 ng/ml

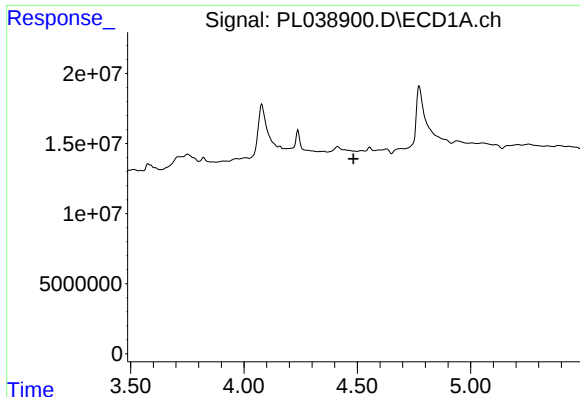

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

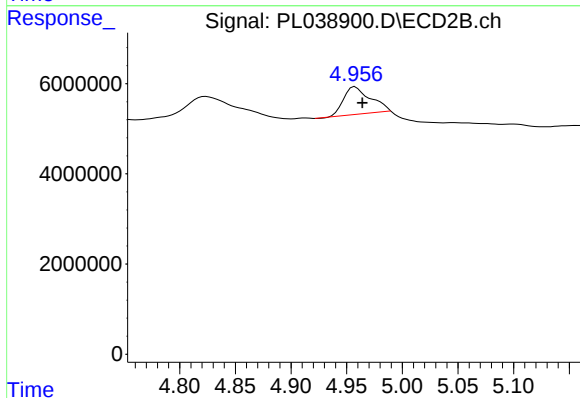


#7 delta-BHC

R.T.: 4.958 min
Delta R.T.: -0.007 min
Response: 10391660
Conc: 3.13 ng/ml

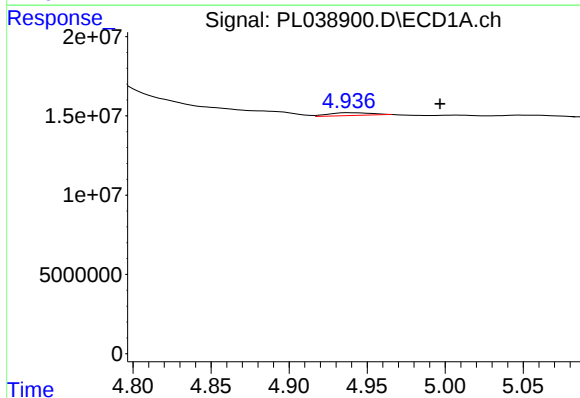


#8 Heptachlor epoxide

R.T.: 4.939 min
Delta R.T.: -0.058 min
Response: 3790791
Conc: 0.40 ng/ml

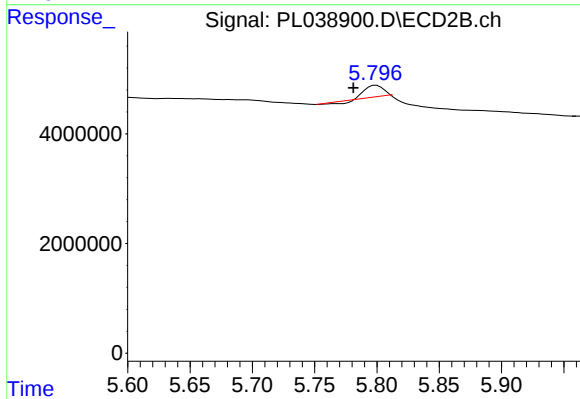

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: 0.018 min
Response: 1600222
Conc: 0.56 ng/ml

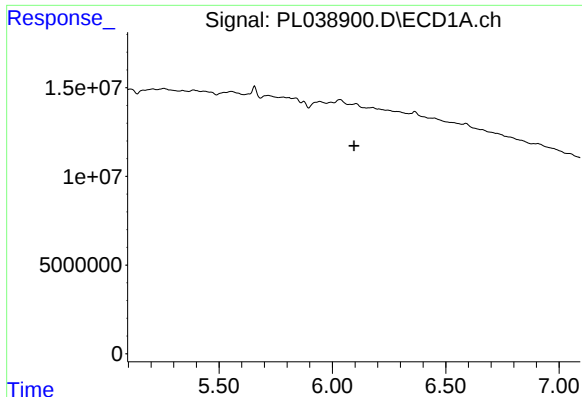

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

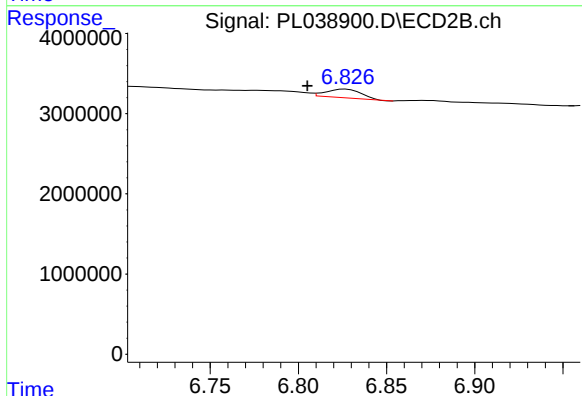


#15 Endosulfan II

R.T.: 6.827 min
Delta R.T.: 0.022 min
Response: 1485496
Conc: 0.62 ng/ml

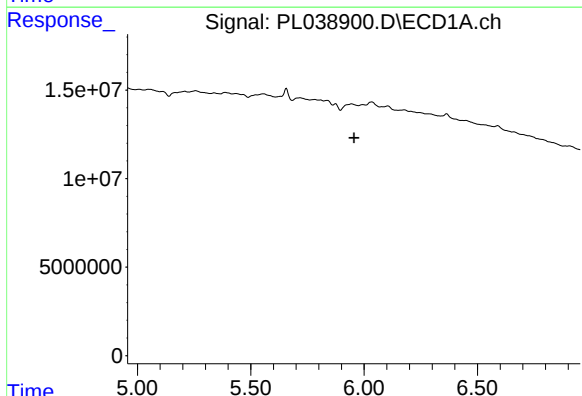


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

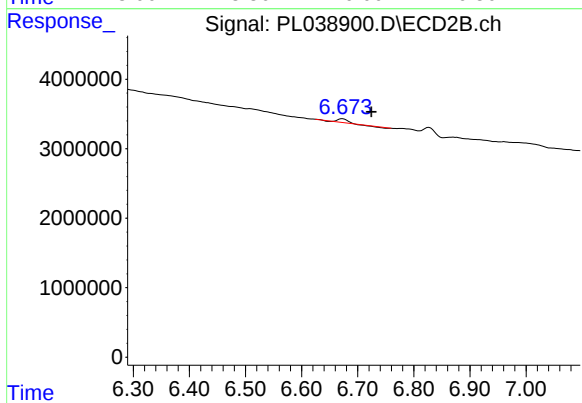

#16 4,4'-DDD


R.T.: 6.673 min
Delta R.T.: -0.051 min
Response: 268268
Conc: 0.13 ng/ml

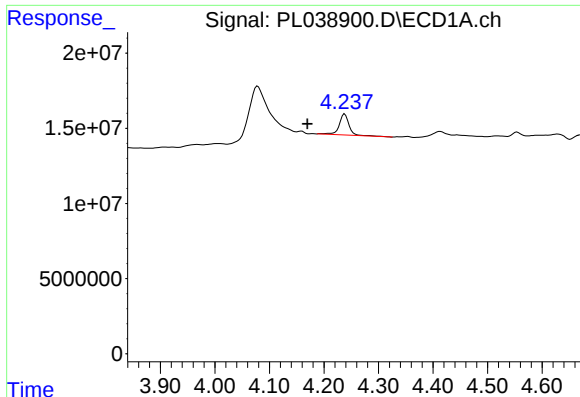

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.069 min
Response: 17988743
Conc: 51.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

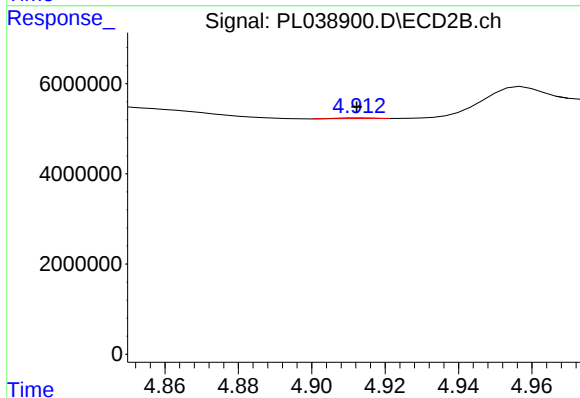


#23 Chlordane-1

R.T.: 4.913 min
Delta R.T.: 0.001 min
Response: 60598
Conc: 0.52 ng/ml

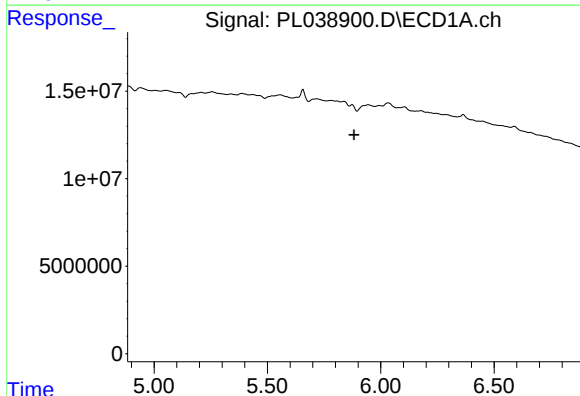


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

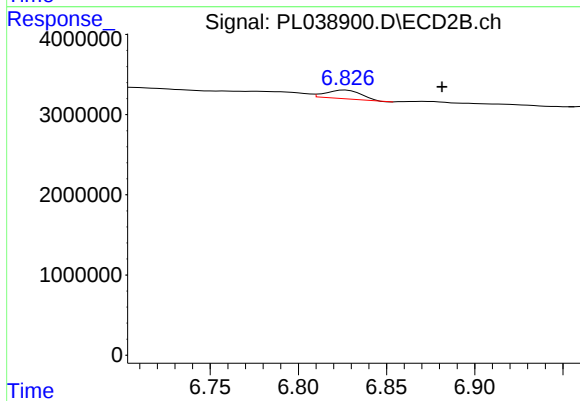

#27 Chlordane-5


R.T.: 6.827 min
Delta R.T.: -0.055 min
Response: 1485496
Conc: 16.58 ng/ml

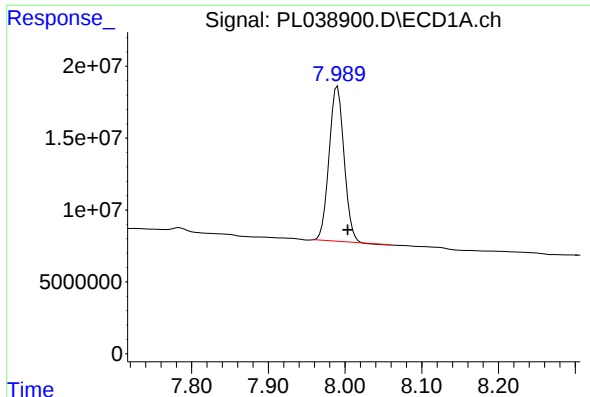

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 145418996
Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

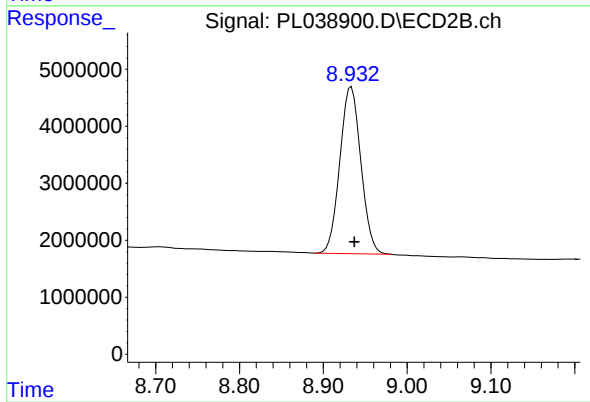

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 51054447
Conc: 20.89 ng/ml