

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
 Data File : PL038908.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2018 23:29
 Operator : AJ\SJ
 Sample : J4316-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 T40-CLAY-1

Manual Integrations
 APPROVED

Sohil
 8/4/2018 10:52:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 00:14:13 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.325	3.926	186.6E6	71202942	25.056	27.126
28)	SA Decachlor...	7.992	8.933	158.4E6	53243479	20.884	21.781
Target Compounds							
17)	MA 4,4'-DDT	6.181	7.018	15474914	4491703	2.083	2.107m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080318\
Data File : PL038908.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2018 23:29
Operator : AJ\SJ
Sample : J4316-05
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
T40-CLAY-1


Manual Integrations
APPROVED

Sohil
8/4/2018 10:52:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 00:14:13 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

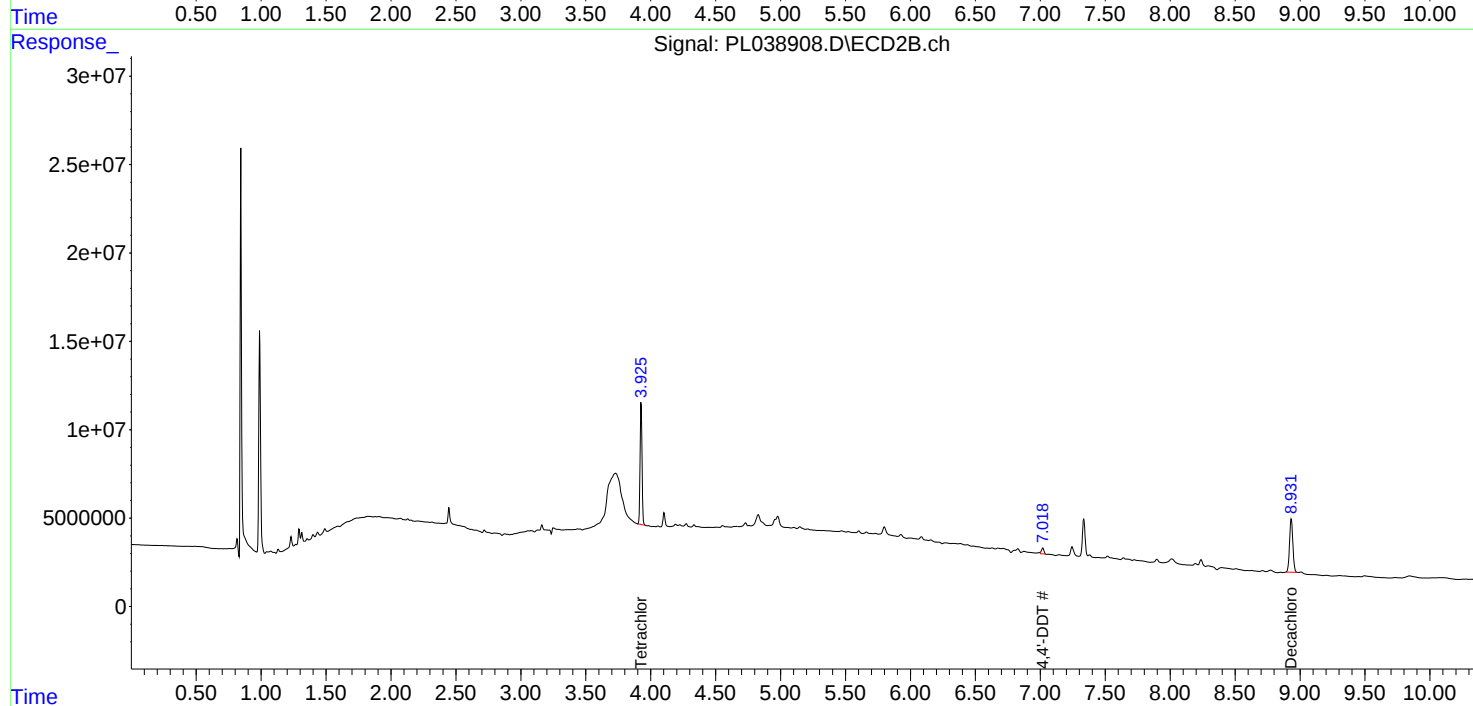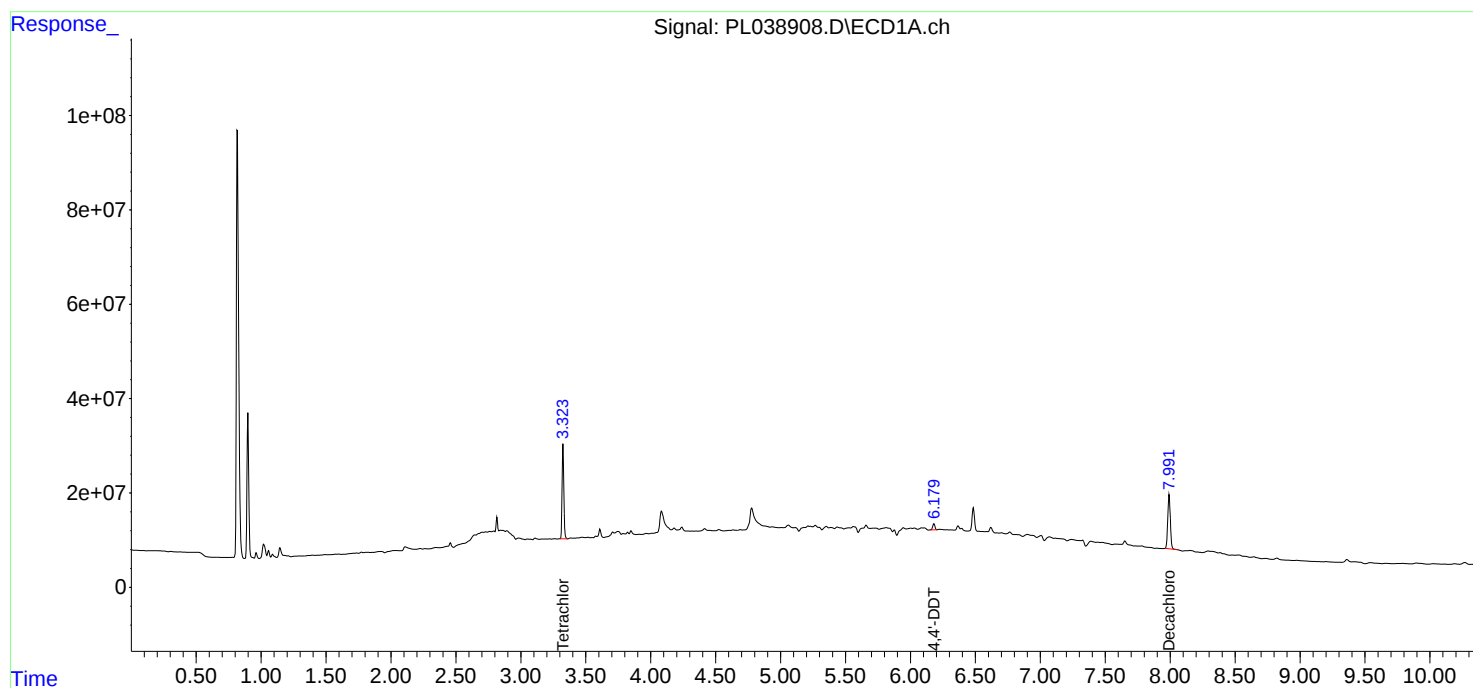

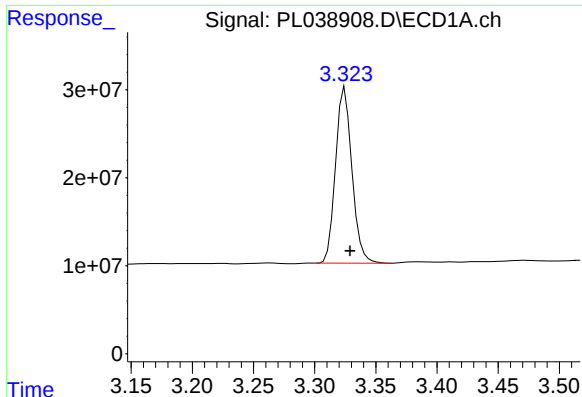


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.004 min
Response: 186580118
Conc: 25.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
T40-CLAY-1


Manual Integrations
APPROVED

Sohil
8/4/2018 10:52:51 AM

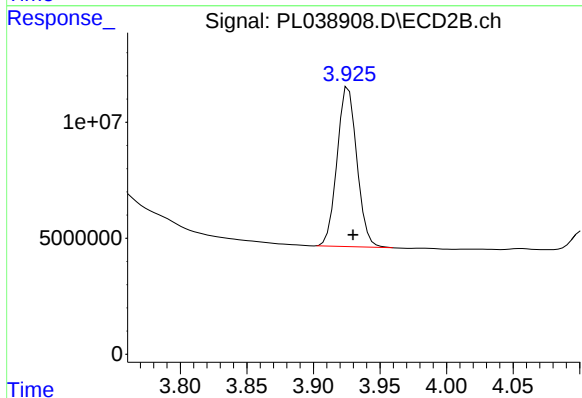


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 71202942
Conc: 27.13 ng/ml

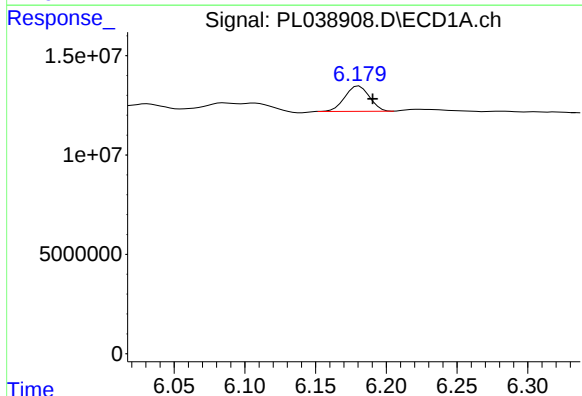


#17 4,4'-DDT

R.T.: 6.181 min
Delta R.T.: -0.010 min
Response: 15474914
Conc: 2.08 ng/ml

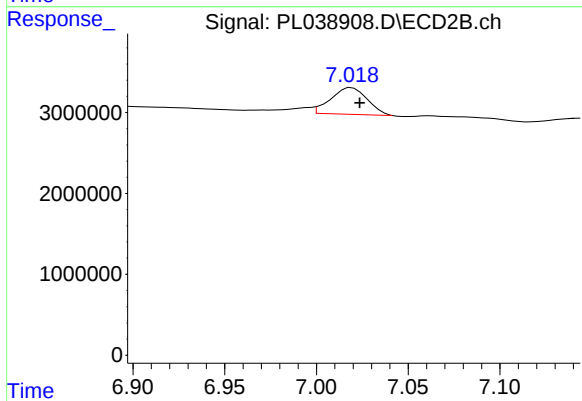

#17 4,4'-DDT

R.T.: 7.018 min
Delta R.T.: -0.006 min
Response: 4491703
Conc: 2.11 ng/ml m

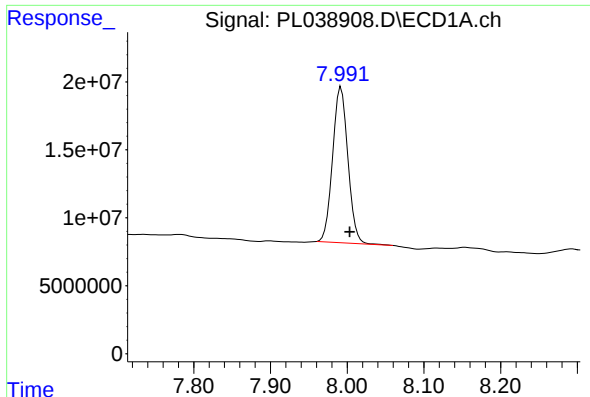


#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.012 min
Response: 158424116
Conc: 20.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
T40-CLAY-1

Manual Integrations
APPROVED

Sohil
8/4/2018 10:52:51 AM

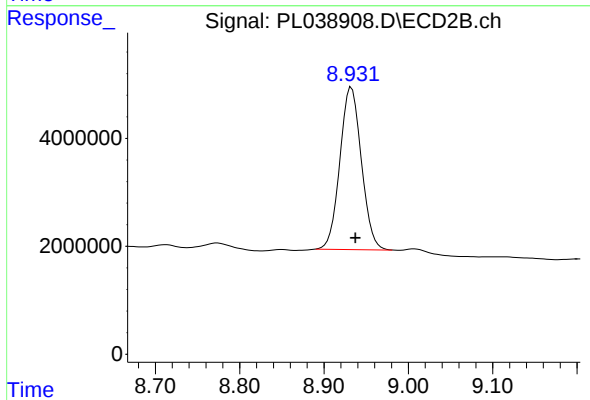

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.005 min
Response: 53243479
Conc: 21.78 ng/ml