

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080321\
 Data File : PL068658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2021 16:56
 Operator : AR\AJ
 Sample : PB138174TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138174TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 01:46:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.570	8612870	20771984	20.068	20.356
28)	SA Decachlor...	10.413	11.491	12100054	18826644	21.514	21.106
Target Compounds							
11)	B alpha-Chl...	0.000	8.405f	0	32784	N.D.	0.029 #
13)	MA Dieldrin	0.000	8.734	0	76017	N.D.	0.072 #
14)	MA Endrin	0.000	8.986f	0	5690	N.D.	0.006 #
15)	B Endosulfa...	0.000	9.219f	0	212346	N.D.	0.234 #
21)	B Endrin ke...	0.000	10.095f	0	188029	N.D.	0.189 #
22)	Mirex	0.000	10.560f	0	37612	N.D.	0.049 #
23)	Chlordane-1	0.000	6.974f	0	379144	N.D.	9.359 #
26)	Chlordane-4	0.000	8.405f	0	32784	N.D.	0.175 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080321\
Data File : PL068658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2021 16:56
Operator : AR\AJ
Sample : PB138174TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB138174TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 01:46:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

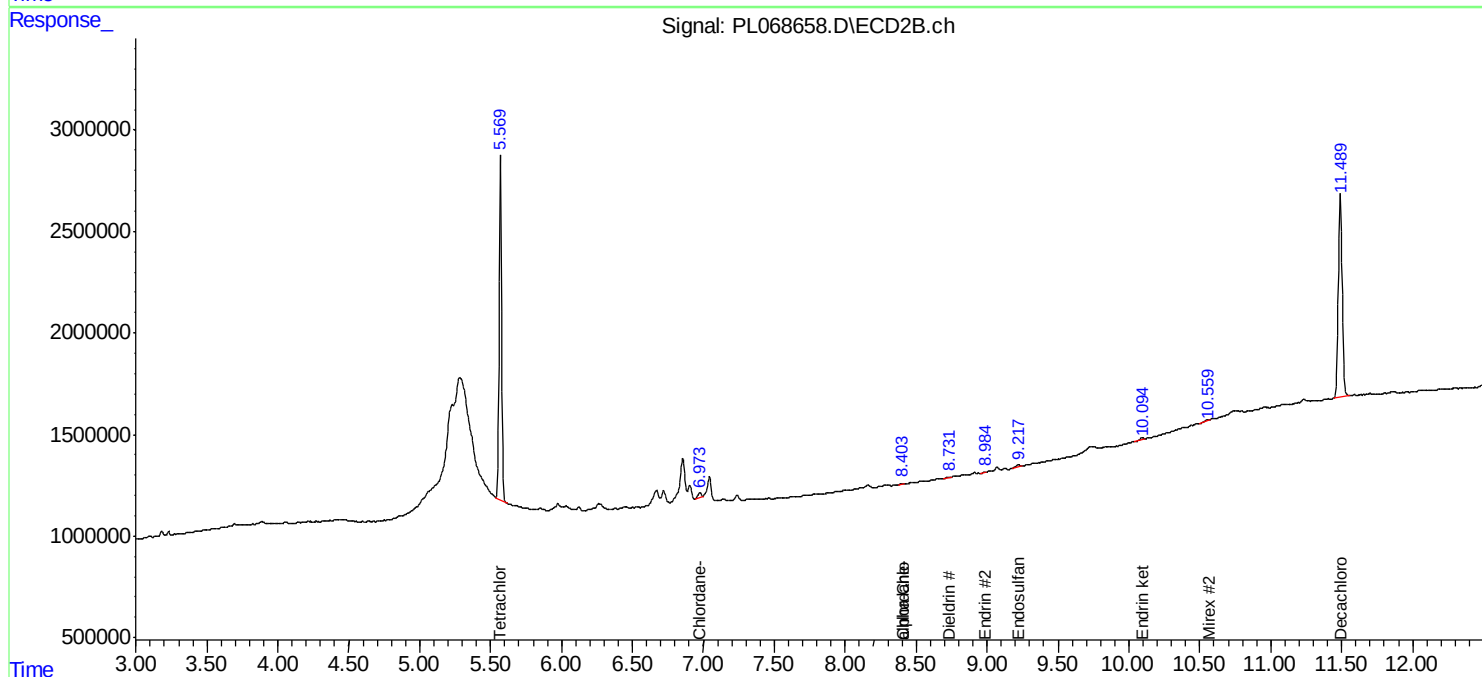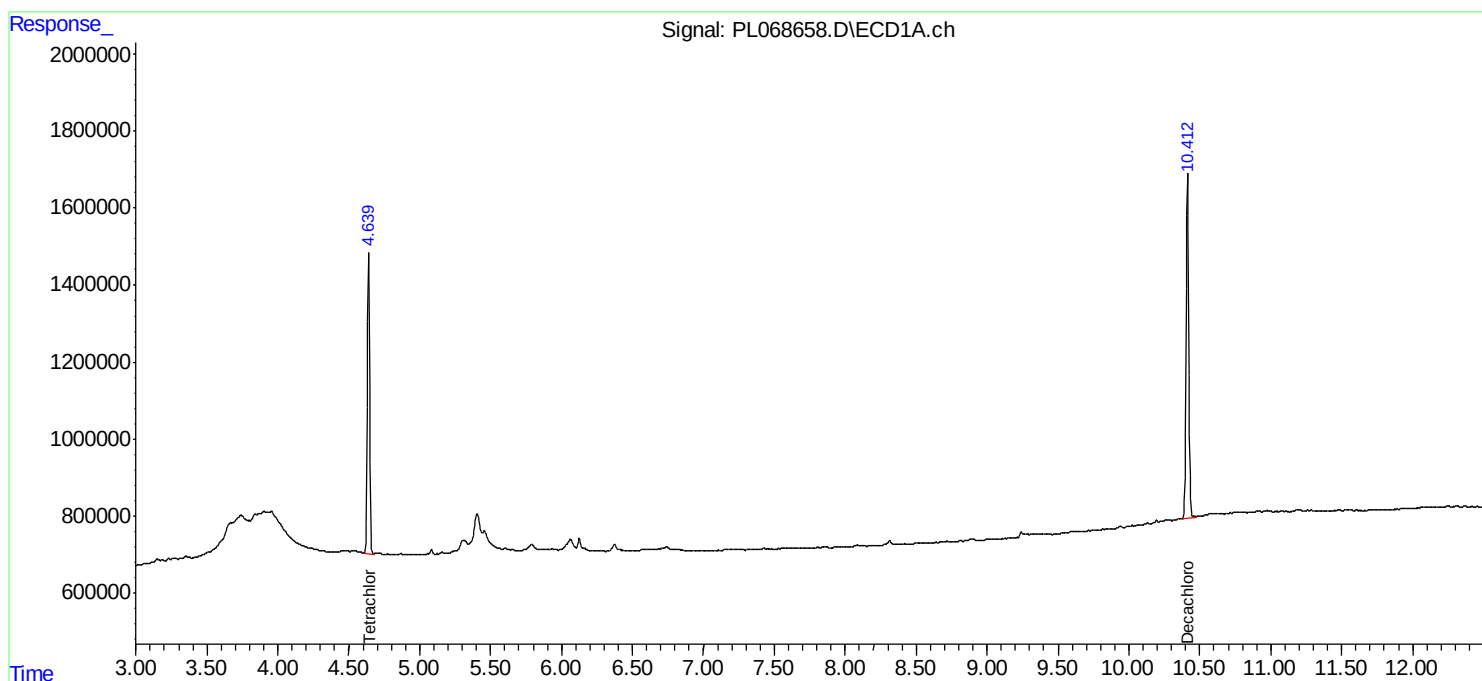


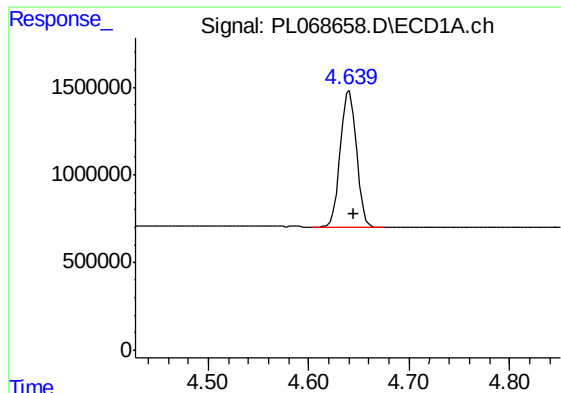

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 8612870
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138174TB

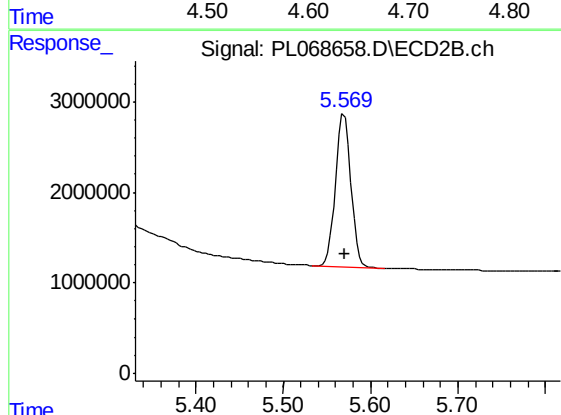


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 20771984
Conc: 20.36 ng/ml

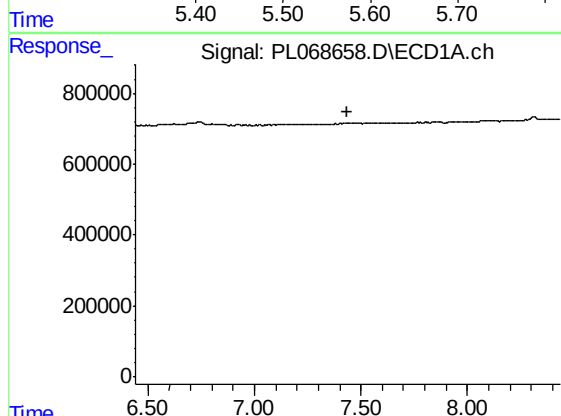


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

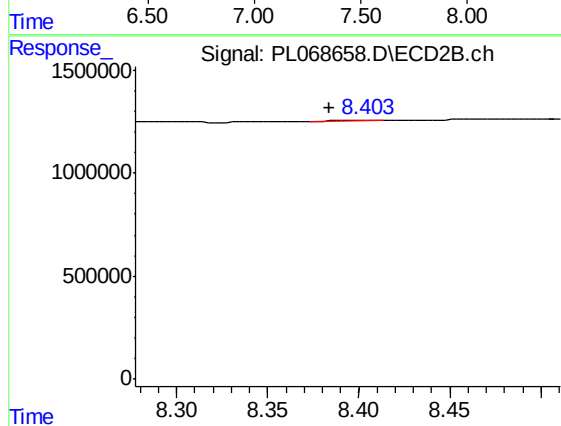

#11 alpha-Chlordane


R.T.: 8.405 min
Delta R.T.: 0.021 min
Response: 32784
Conc: 0.03 ng/ml

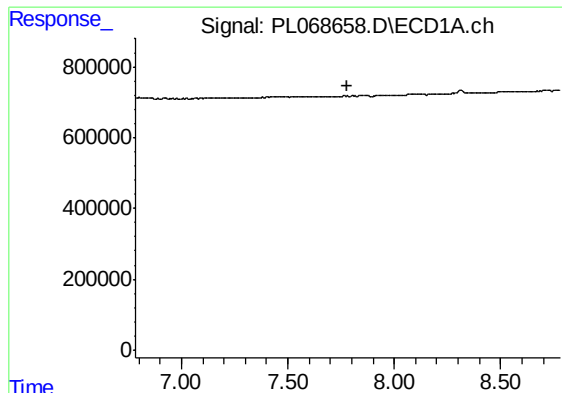

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 7.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138174TB

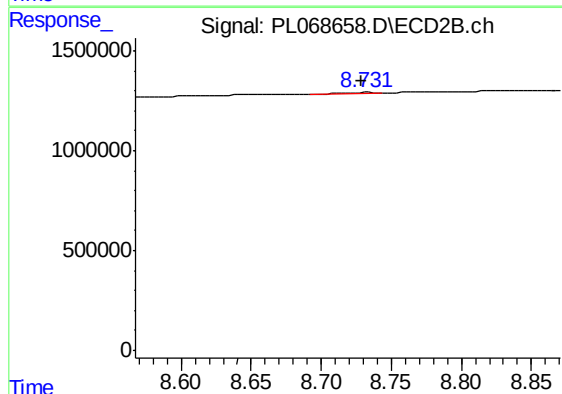


#13 Dielldrin

R.T.: 8.734 min
Delta R.T.: 0.005 min
Response: 76017
Conc: 0.07 ng/ml

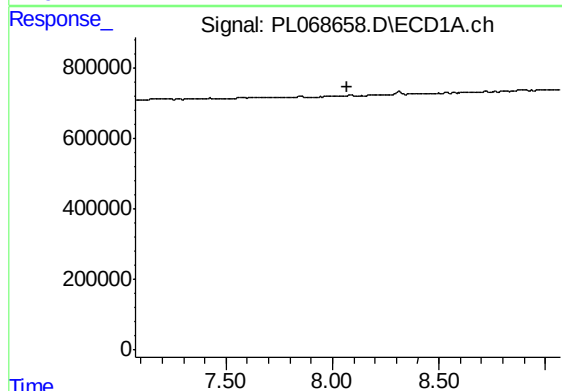


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

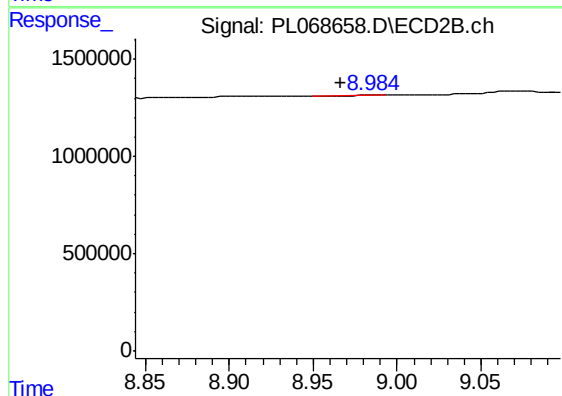

#14 Endrin


R.T.: 8.986 min
Delta R.T.: 0.019 min
Response: 5690
Conc: 0.01 ng/ml

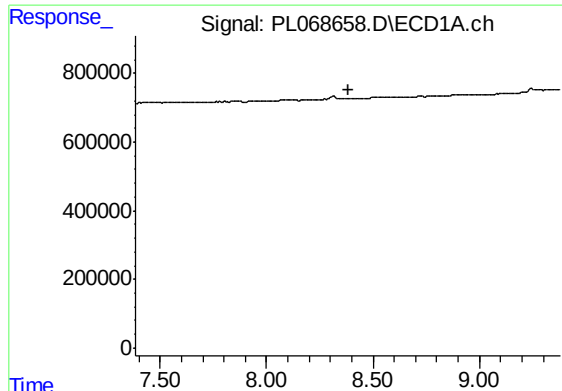

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138174TB

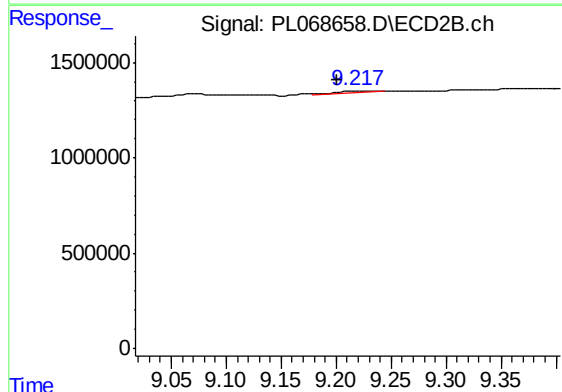


#15 Endosulfan II

R.T.: 9.219 min
Delta R.T.: 0.019 min
Response: 212346
Conc: 0.23 ng/ml

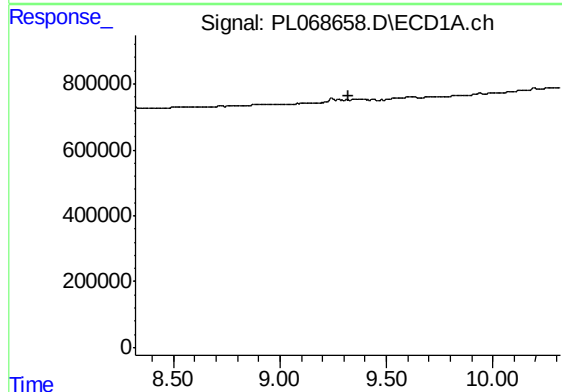


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.320 min
Response: 0
Conc: N.D.

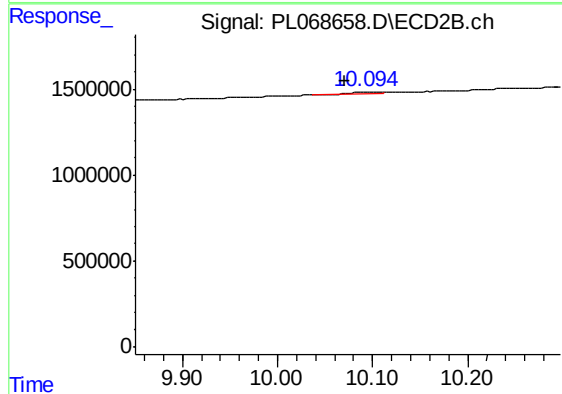

#21 Endrin ketone


R.T.: 10.095 min
Delta R.T.: 0.024 min
Response: 188029
Conc: 0.19 ng/ml

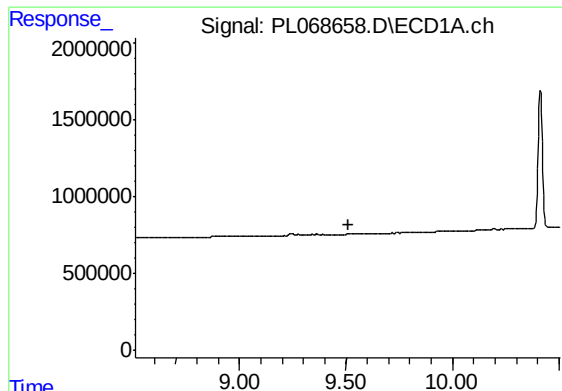

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138174TB

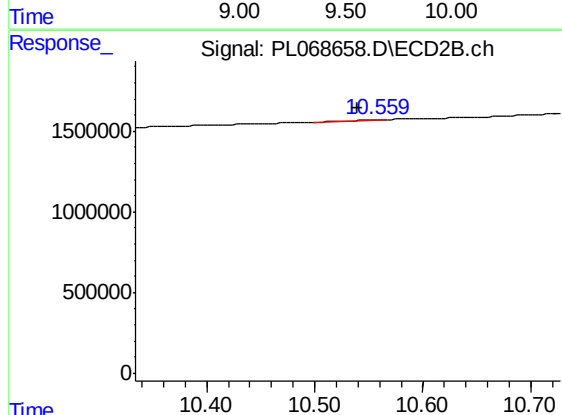


#22 Mirex

R.T.: 10.560 min
Delta R.T.: 0.021 min
Response: 37612
Conc: 0.05 ng/ml

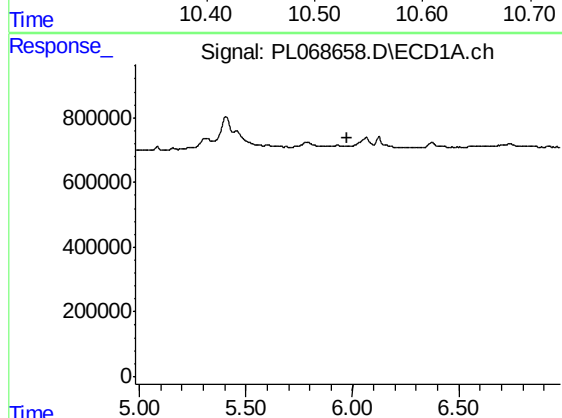


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

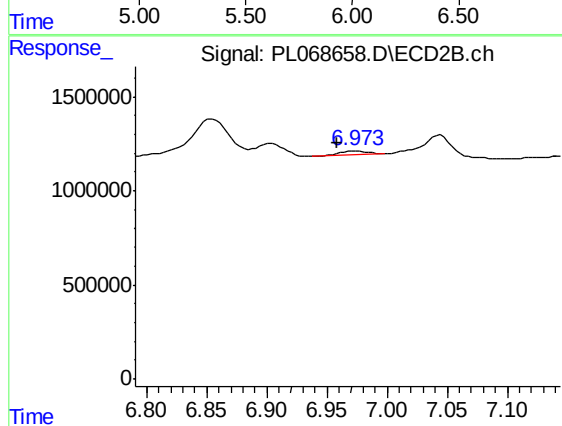

#23 Chlordane-1


R.T.: 6.974 min
Delta R.T.: 0.016 min
Response: 379144
Conc: 9.36 ng/ml

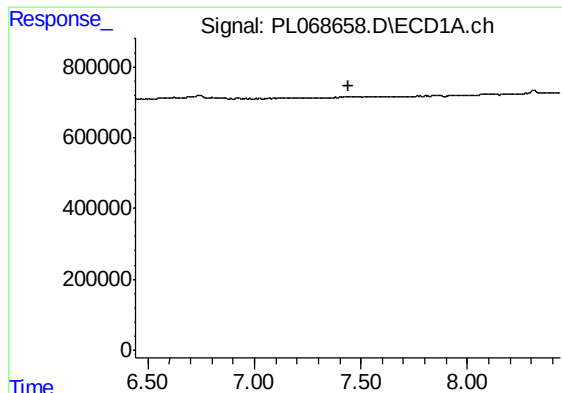

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138174TB

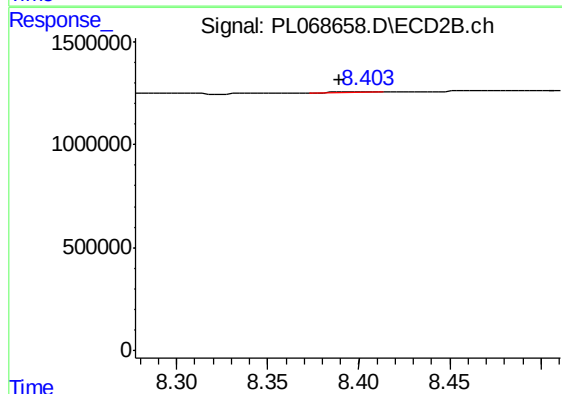


#26 Chlordane-4

R.T.: 8.405 min
Delta R.T.: 0.015 min
Response: 32784
Conc: 0.17 ng/ml

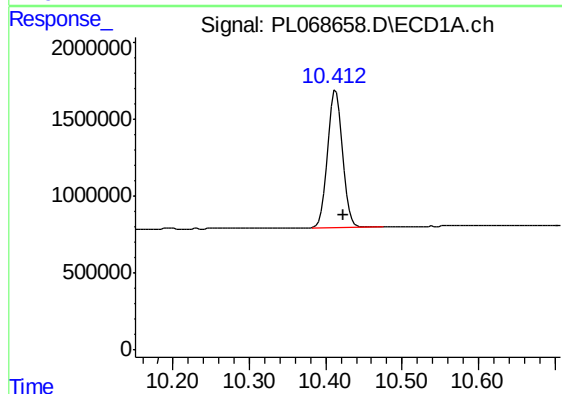

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: -0.011 min
Response: 12100054
Conc: 21.51 ng/ml

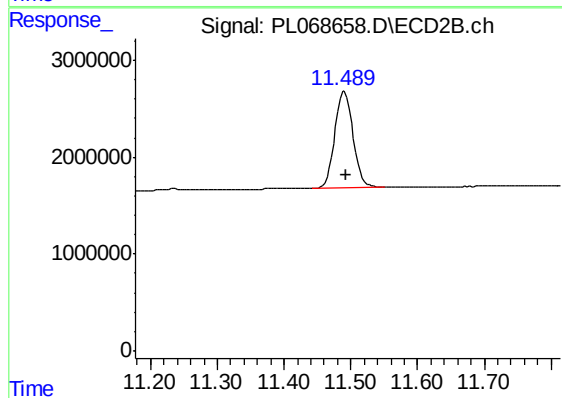

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 18826644
Conc: 21.11 ng/ml