

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080322\
 Data File : PL076857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Aug 2022 11:40
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 00:09:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 01 16:34:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) MA	gamma-BHC...	4.233	0.000	423384	0	0.334	N.D. #
4) MA	Heptachlor	4.805	3.782	117807	124204	0.096	0.043 #
5) MB	Aldrin	0.000	4.042f	0	4767865	N.D.	1.715 #
6) B	beta-BHC	0.000	3.782f	0	124204	N.D.	0.102 #
8) B	Heptachlo...	5.580	0.000	5529990	0	5.915	N.D. #
10) B	gamma-Chl...	0.000	4.806	0	213107	N.D.	0.087 #
12) B	4,4'-DDE	0.000	5.083	0	1443222	N.D.	0.620 #
14) MA	Endrin	6.492f	5.494f	793252	4608622	0.861	2.129 #
16) A	4,4'-DDD	0.000	5.654f	0	49050350	N.D.	26.270 #
24)	Chlordane-2	0.000	4.189	0	472445	N.D.	4.797 #
25)	Chlordane-3	0.000	4.806	0	213107	N.D.	0.773 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080322\
Data File : PL076857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Aug 2022 11:40
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 04 00:09:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080122.M
Quant Title : GC Extractables
QLast Update : Mon Aug 01 16:34:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

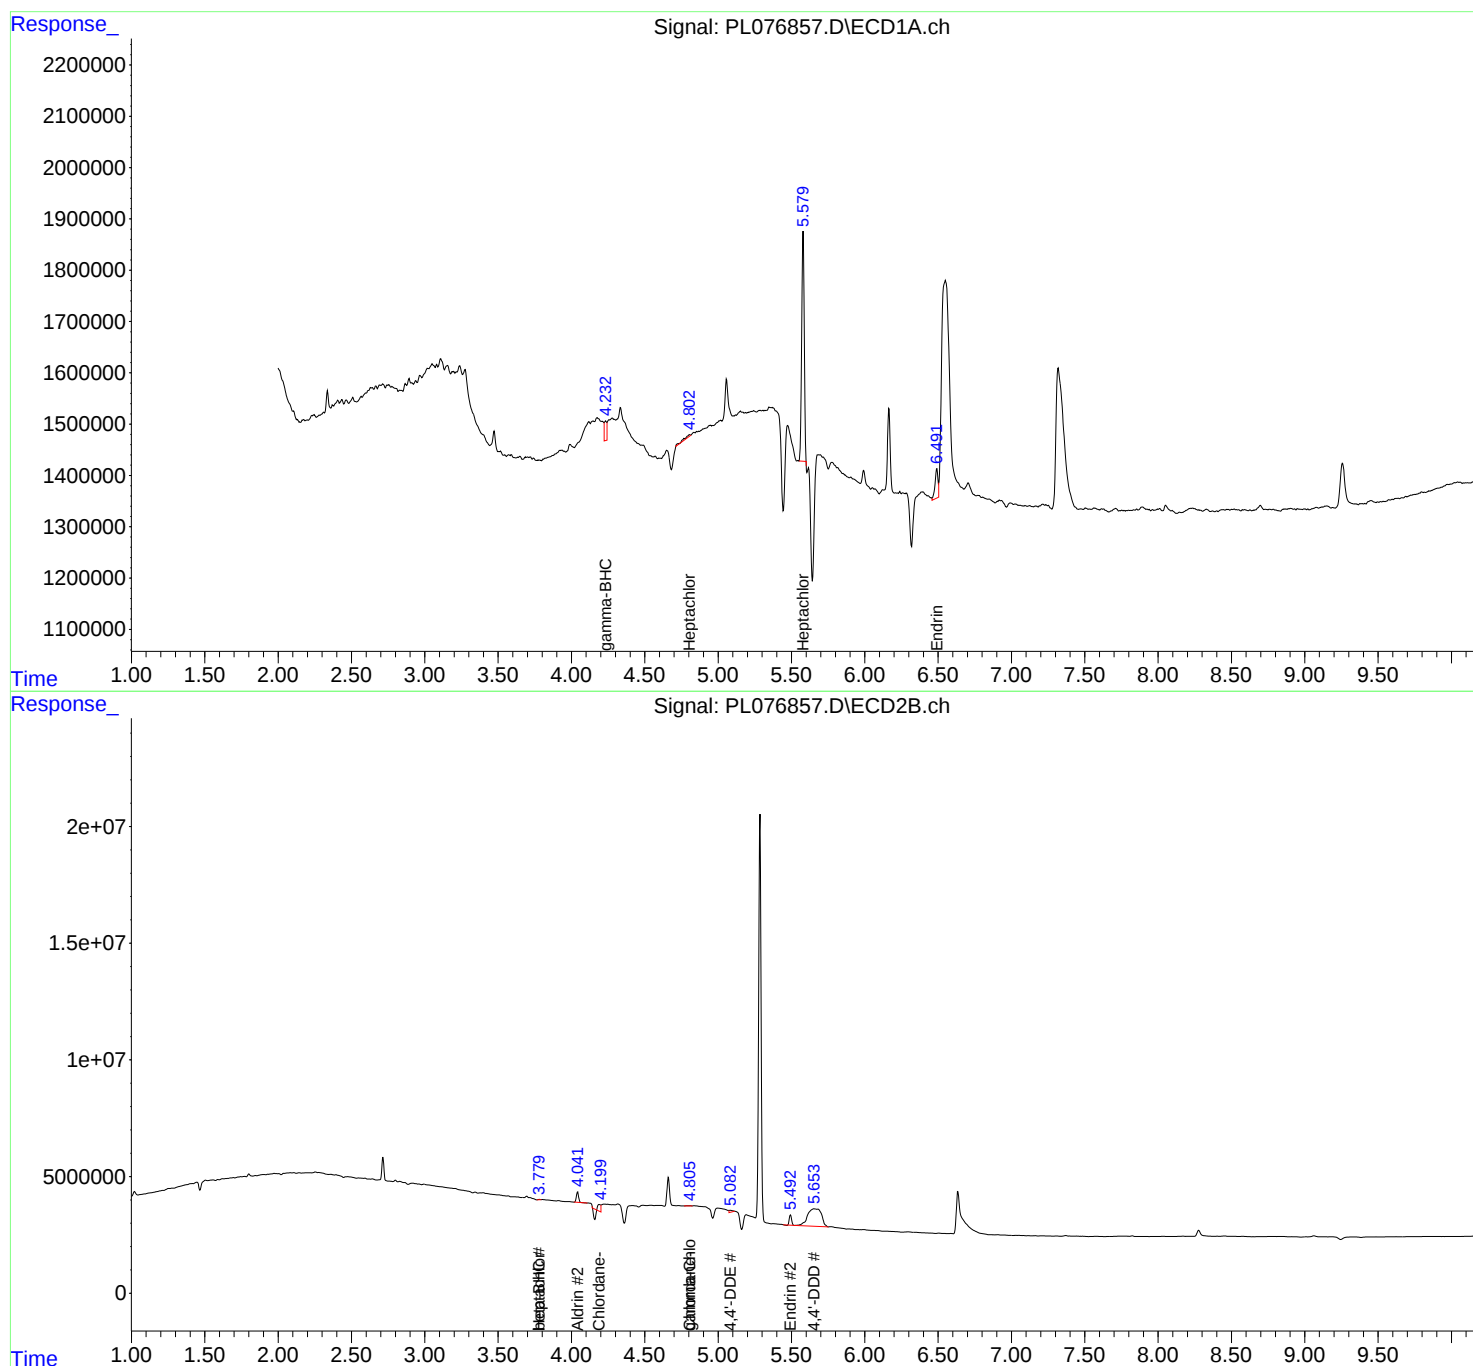


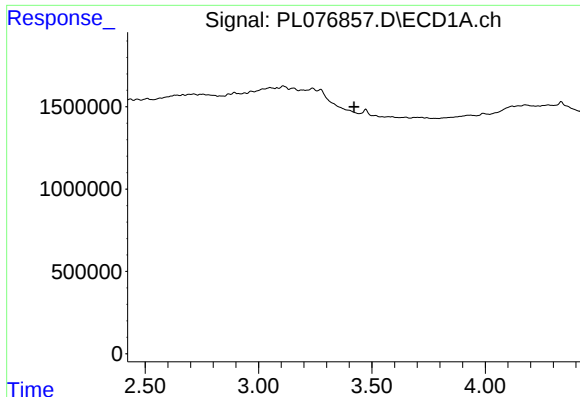

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

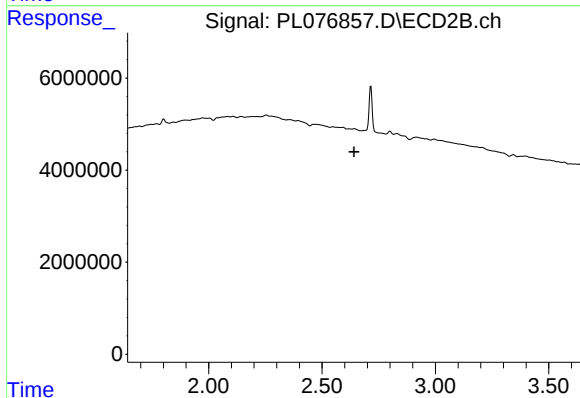


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.642 min
Response: 0
Conc: N.D.

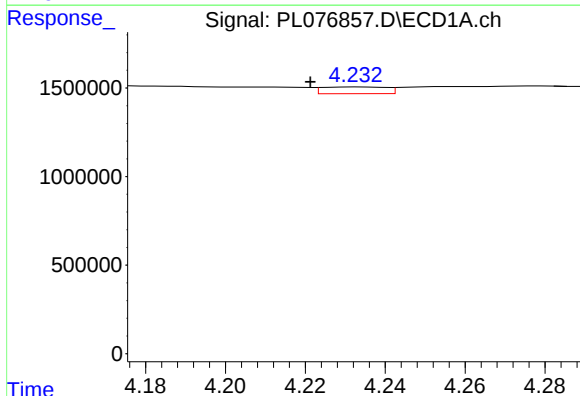


#3 gamma-BHC (Lindane)

R.T.: 4.233 min
Delta R.T.: 0.012 min
Response: 423384
Conc: 0.33 ng/ml

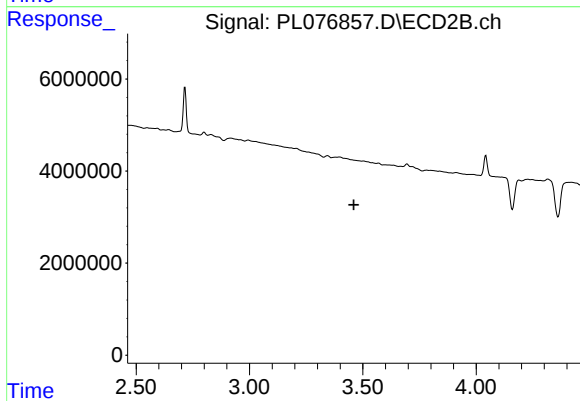

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.460 min
Response: 0
Conc: N.D.

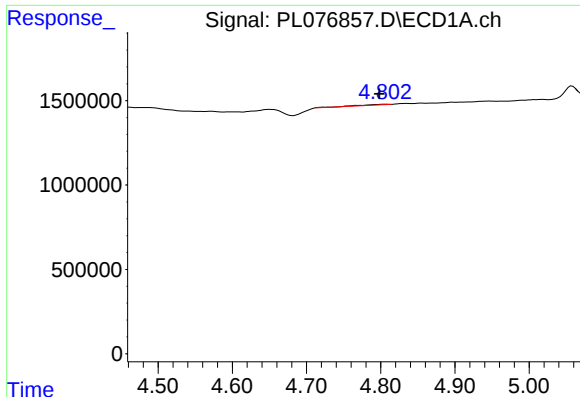

#4 Heptachlor


R.T.: 4.805 min
Delta R.T.: 0.007 min
Response: 117807
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

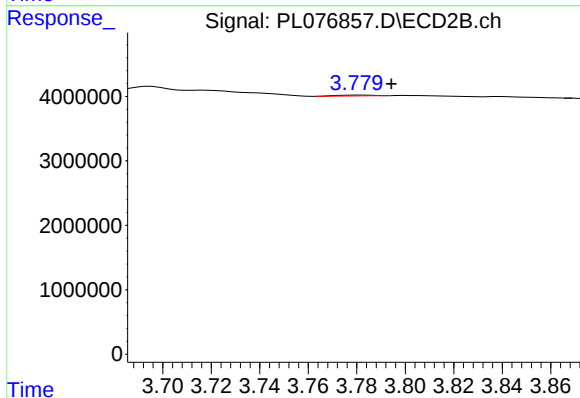


#4 Heptachlor

R.T.: 3.782 min
Delta R.T.: -0.013 min
Response: 124204
Conc: 0.04 ng/ml

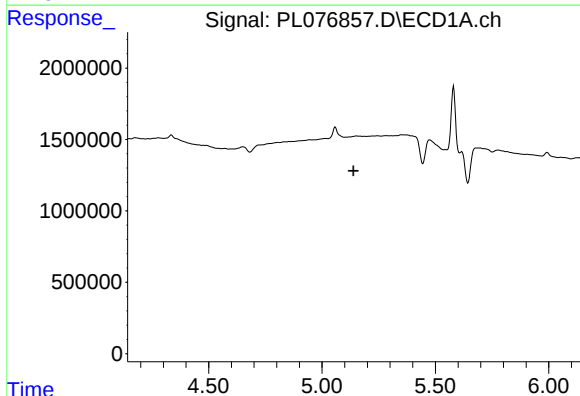


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.139 min
Response: 0
Conc: N.D.

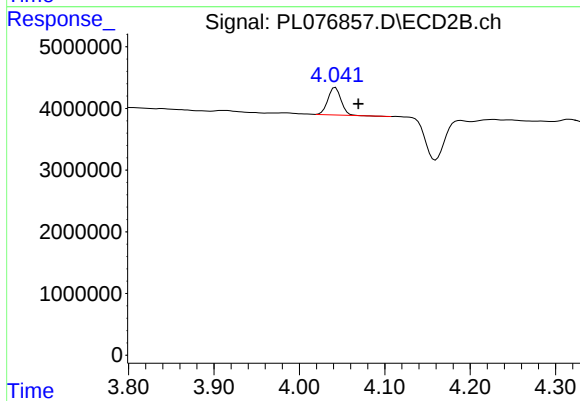

#5 Aldrin


R.T.: 4.042 min
Delta R.T.: -0.027 min
Response: 4767865
Conc: 1.71 ng/ml

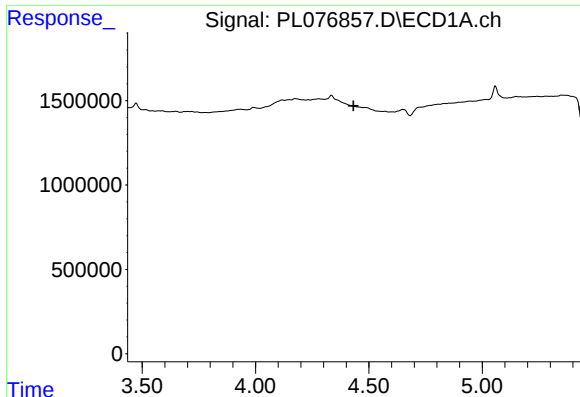

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.433 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

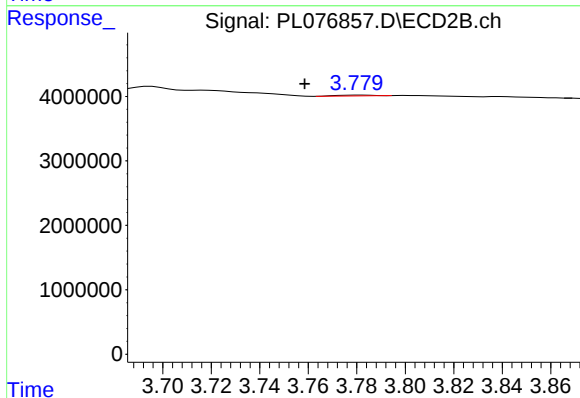


#6 beta-BHC

R.T.: 3.782 min
Delta R.T.: 0.023 min
Response: 124204
Conc: 0.10 ng/ml

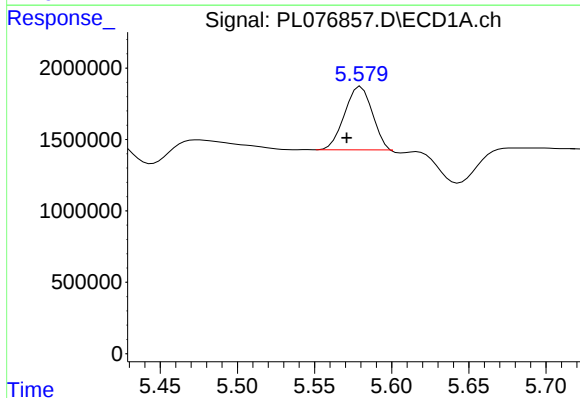


#8 Heptachlor epoxide

R.T.: 5.580 min
Delta R.T.: 0.009 min
Response: 5529990
Conc: 5.92 ng/ml

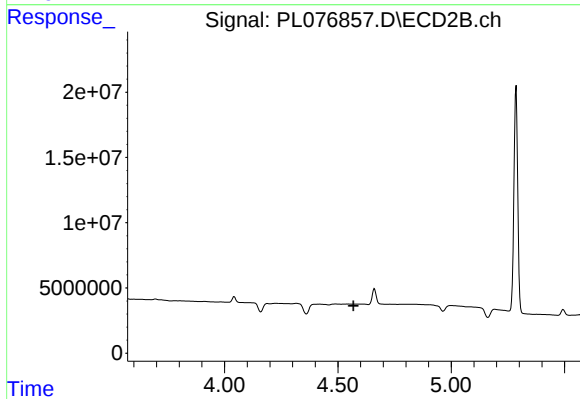

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.569 min
Response: 0
Conc: N.D.

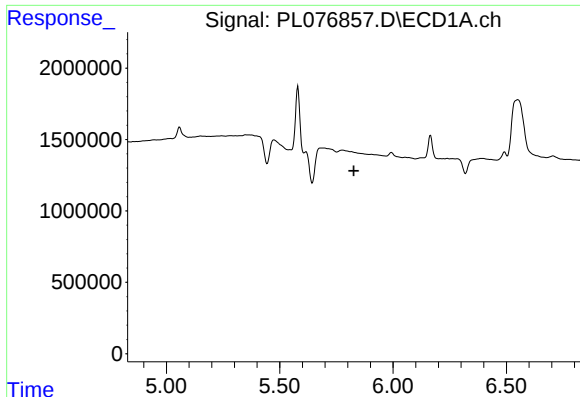

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

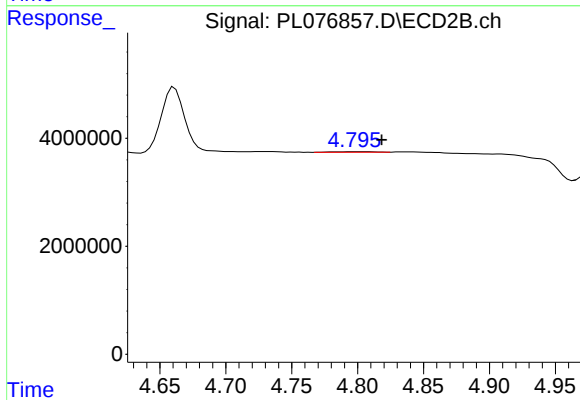


#10 gamma-Chlordane

R.T.: 4.806 min
Delta R.T.: -0.012 min
Response: 213107
Conc: 0.09 ng/ml

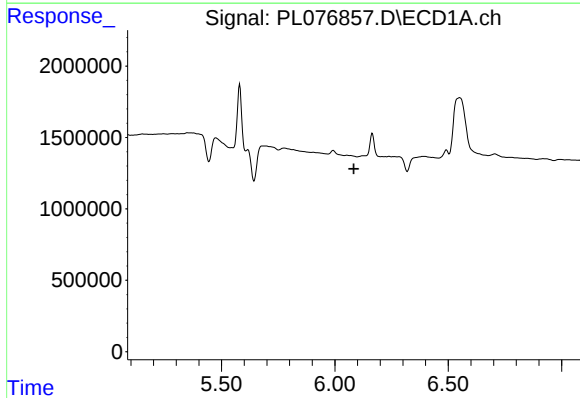


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.083 min
Response: 0
Conc: N.D.

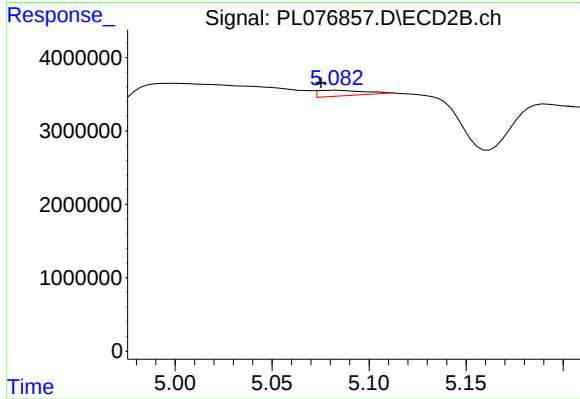

#12 4,4'-DDE


R.T.: 5.083 min
Delta R.T.: 0.008 min
Response: 1443222
Conc: 0.62 ng/ml

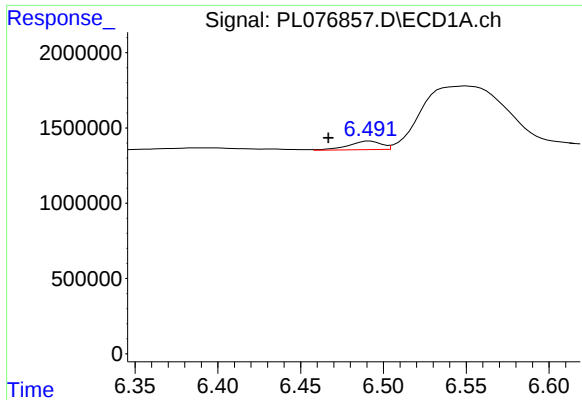

#14 Endrin


R.T.: 6.492 min
Delta R.T.: 0.025 min
Response: 793252
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

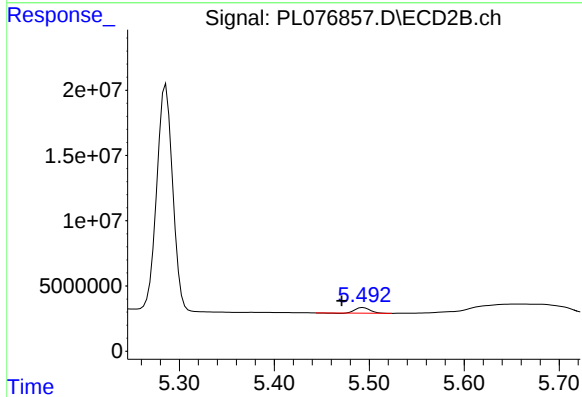


#14 Endrin

R.T.: 5.494 min
Delta R.T.: 0.023 min
Response: 4608622
Conc: 2.13 ng/ml

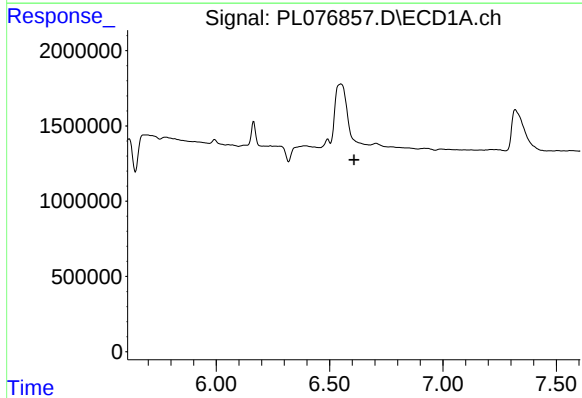


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.608 min
Response: 0
Conc: N.D.

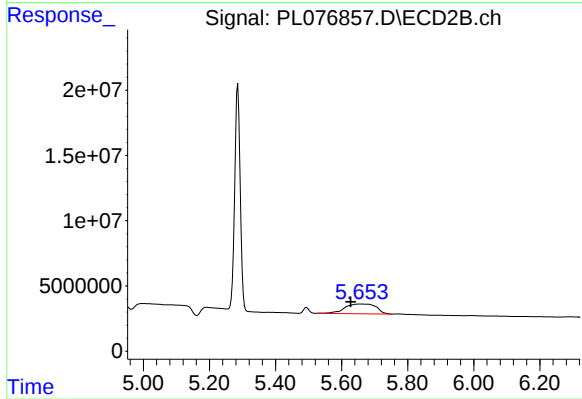

#16 4,4'-DDD


R.T.: 5.654 min
Delta R.T.: 0.026 min
Response: 49050350
Conc: 26.27 ng/ml

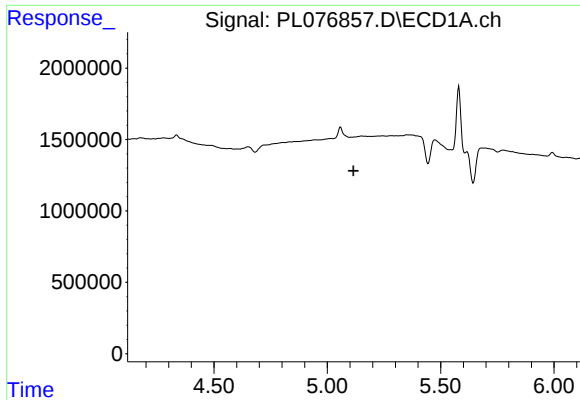

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

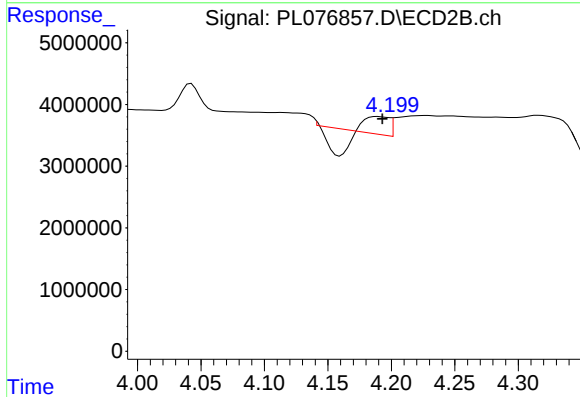


#24 Chlordane-2

R.T.: 4.189 min
Delta R.T.: -0.004 min
Response: 472445
Conc: 4.80 ng/ml

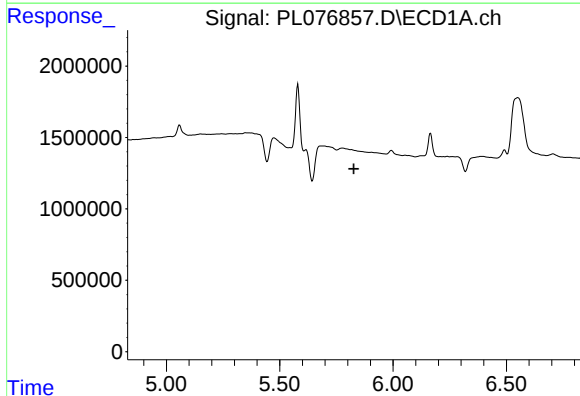


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.827 min
Response: 0
Conc: N.D.

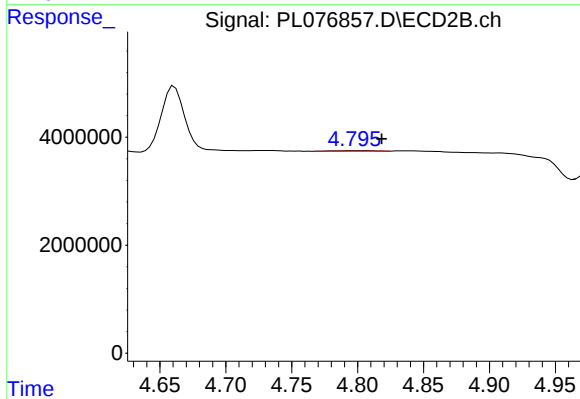

#25 Chlordane-3


R.T.: 4.806 min
Delta R.T.: -0.012 min
Response: 213107
Conc: 0.77 ng/ml

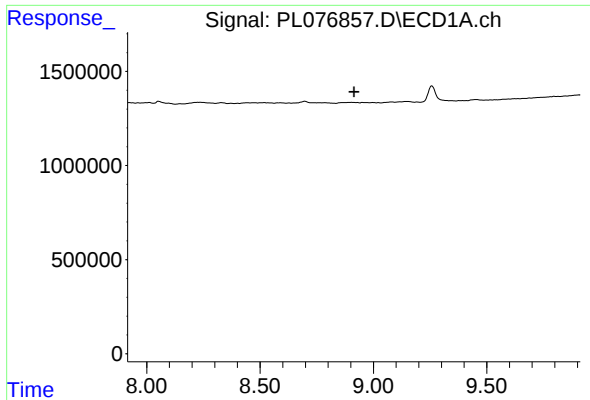

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

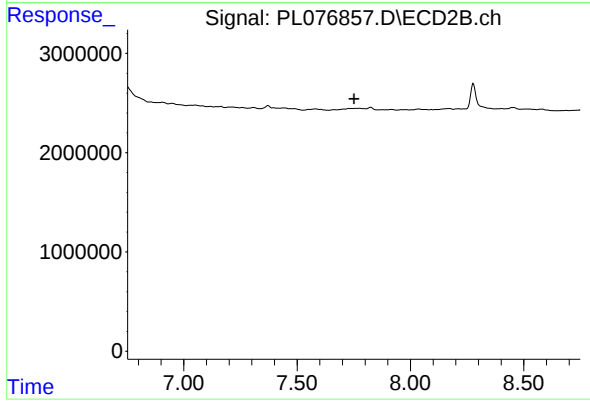

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.751 min
Response: 0
Conc: N.D.